

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
 Data File : PL064713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 18:58
 Operator : AR\AJ
 Sample : M1317-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:11:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.102	58153446	46853415	20.669	21.689
28)	SA Decachlor...	8.148	9.261	48236408	37384690	21.450	19.683
Target Compounds							
16)	A 4,4'-DDD	6.103f	0.000	1033663	0	0.408	N.D. #
17)	MA 4,4'-DDT	0.000	7.270	0	2787088	N.D.	1.828 #
18)	B Endrin al...	6.412f	0.000	1786215	0	0.733	N.D. #
23)	Chlordane-1	4.297	0.000	5841495	0	51.387	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
Data File : PL064713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 18:58
Operator : AR\AJ
Sample : M1317-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:11:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

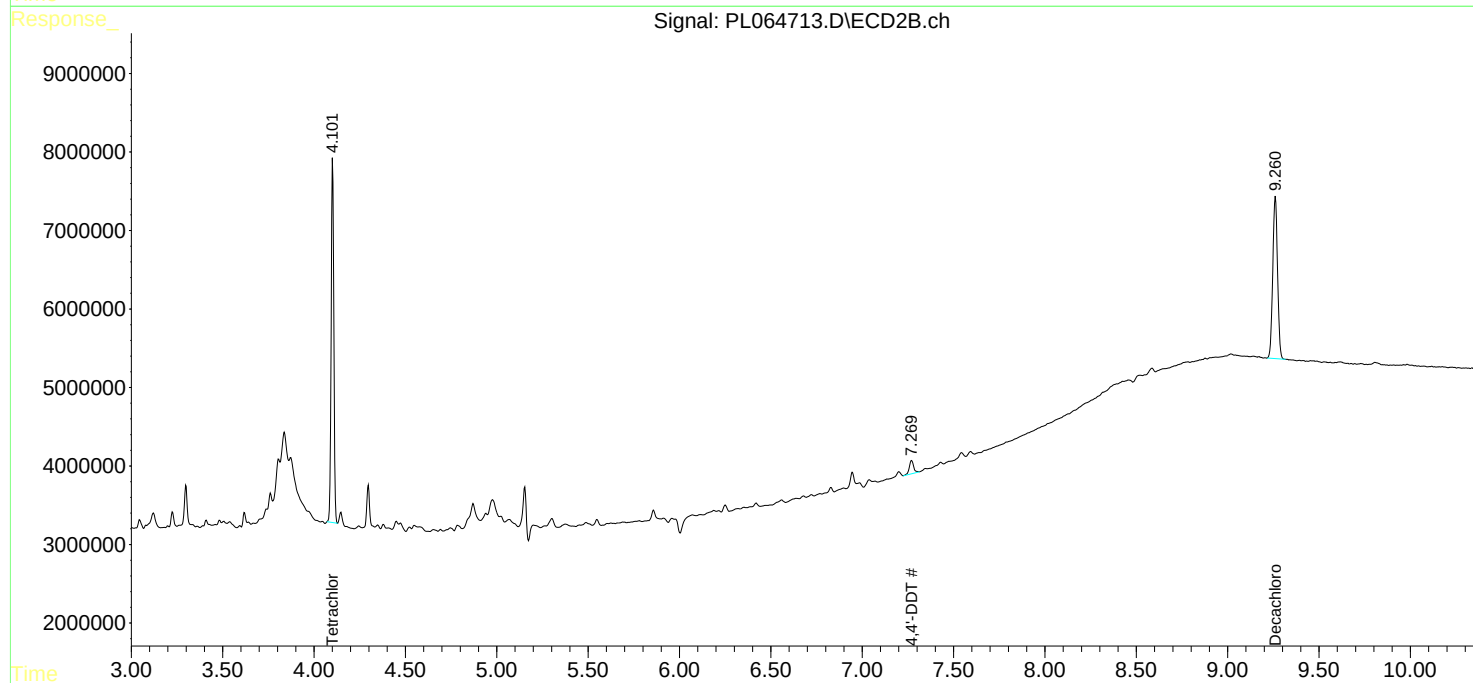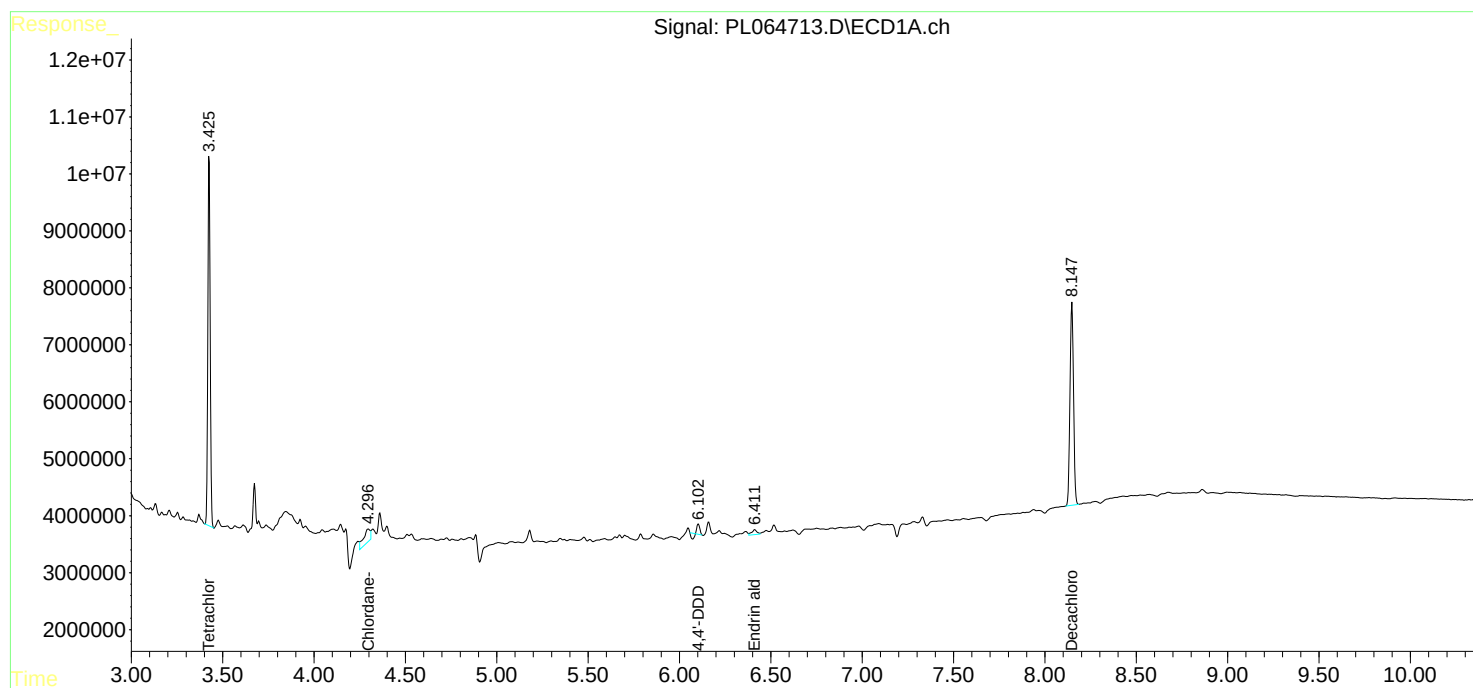


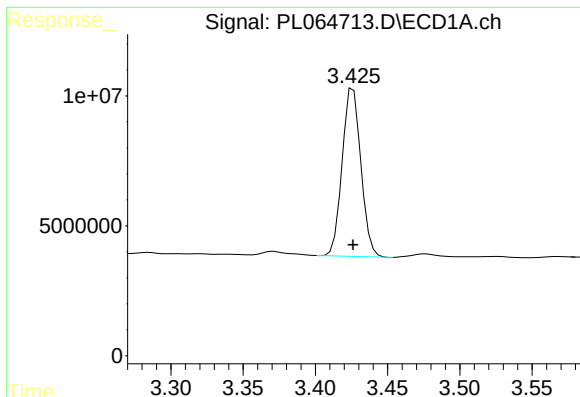

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 58153446
Conc: 20.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

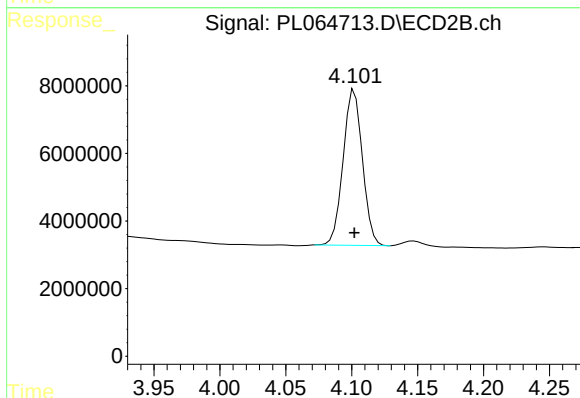


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 46853415
Conc: 21.69 ng/ml

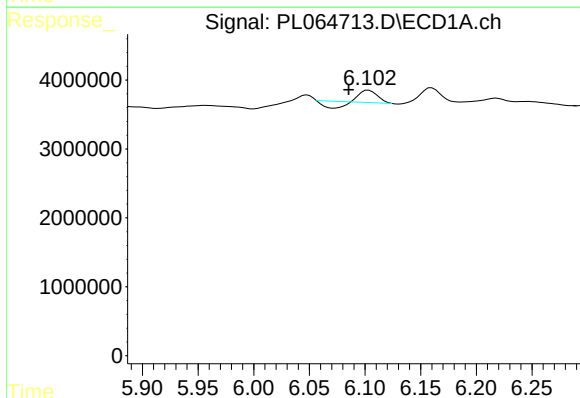


#16 4,4'-DDD

R.T.: 6.103 min
Delta R.T.: 0.018 min
Response: 1033663
Conc: 0.41 ng/ml

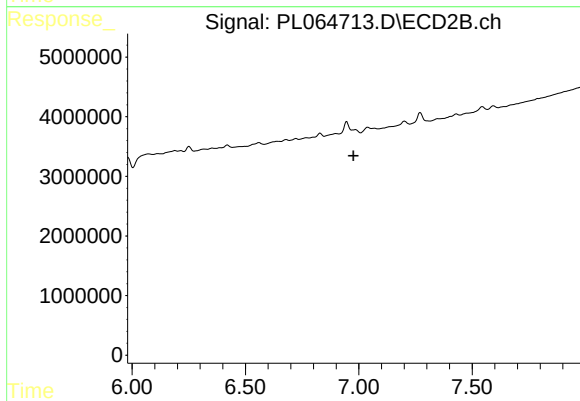

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.977 min
Response: 0
Conc: N.D.

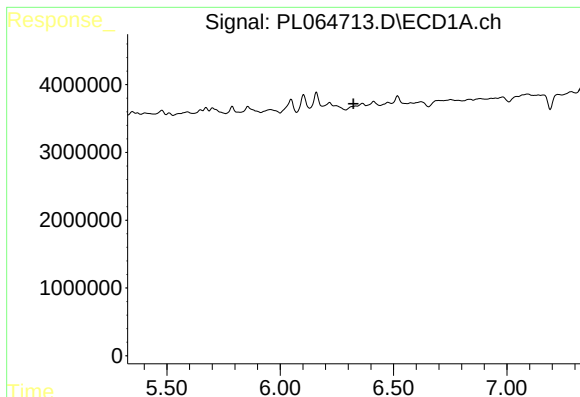

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

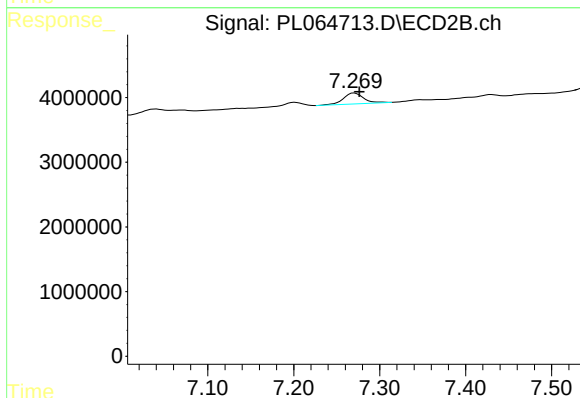


#17 4,4'-DDT

R.T.: 7.270 min
Delta R.T.: -0.006 min
Response: 2787088
Conc: 1.83 ng/ml

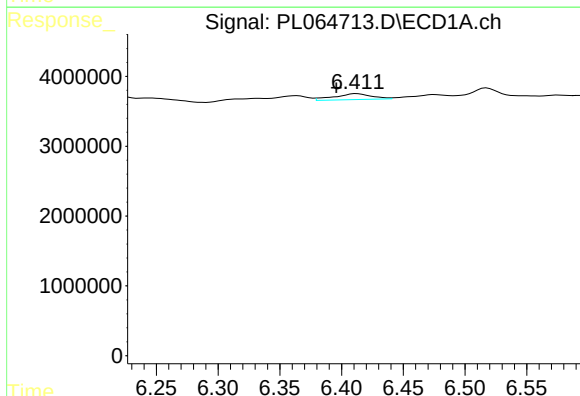


#18 Endrin aldehyde

R.T.: 6.412 min
Delta R.T.: 0.017 min
Response: 1786215
Conc: 0.73 ng/ml

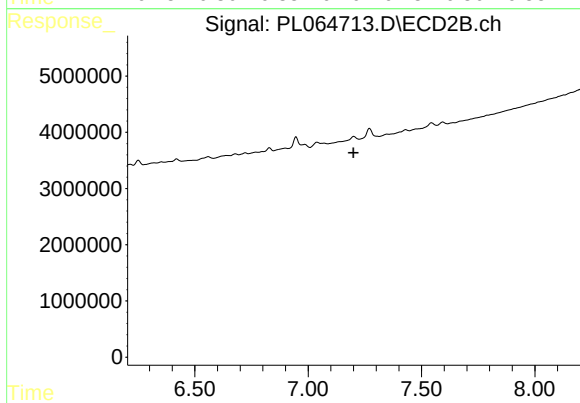

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.200 min
Response: 0
Conc: N.D.

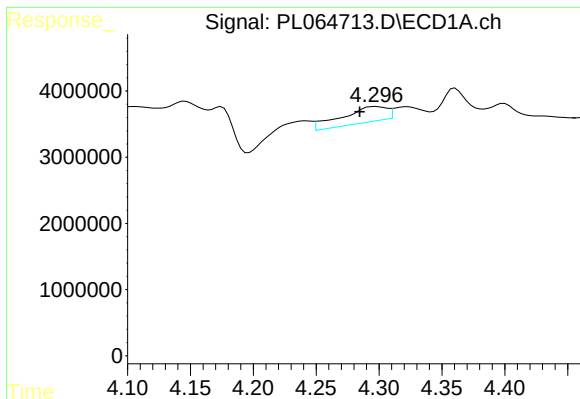

#23 Chlordane-1


R.T.: 4.297 min
Delta R.T.: 0.013 min
Response: 5841495
Conc: 51.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

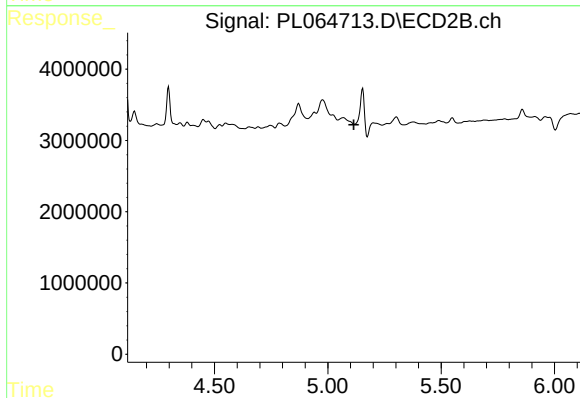


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

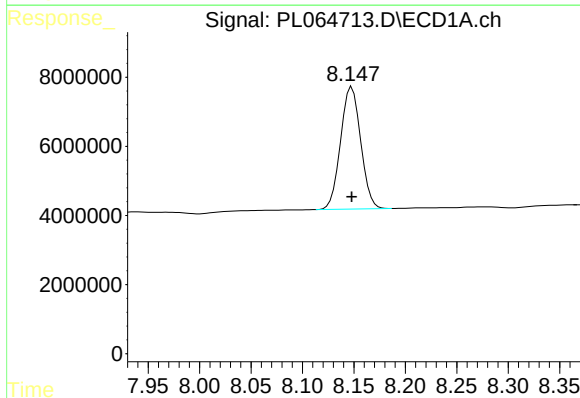

#28 Decachlorobiphenyl

R.T.: 8.148 min
Delta R.T.: 0.000 min
Response: 48236408
Conc: 21.45 ng/ml

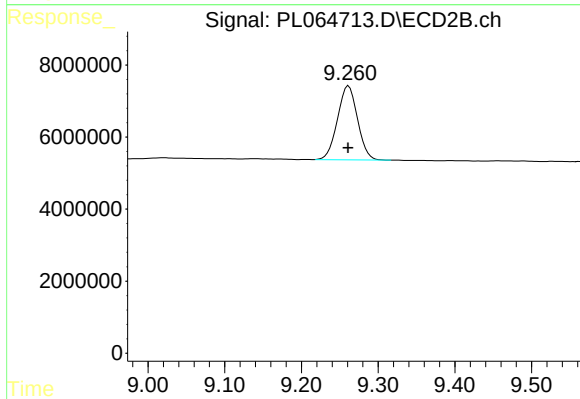

#28 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: 0.000 min
Response: 37384690
Conc: 19.68 ng/ml