

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL020921\  
 Data File : PL064713.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 09 Feb 2021 18:58  
 Operator : AR\AJ  
 Sample : M1317-11  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 R-A

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 10 02:11:07 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL020821.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Feb 09 04:41:29 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|---------|
| -----                       |                 |        |       |          |          |        |         |
| System Monitoring Compounds |                 |        |       |          |          |        |         |
| 1)                          | SA Tetrachlo... | 3.426  | 4.102 | 58153446 | 46853415 | 20.669 | 21.689  |
| 28)                         | SA Decachlor... | 8.148  | 9.261 | 48236408 | 37384690 | 21.450 | 19.683  |
| Target Compounds            |                 |        |       |          |          |        |         |
| 16)                         | A 4,4'-DDD      | 6.103f | 0.000 | 1033663  | 0        | 0.408  | N.D. #  |
| 17)                         | MA 4,4'-DDT     | 0.000  | 7.270 | 0        | 2787088  | N.D.   | 1.828 # |
| 18)                         | B Endrin al...  | 6.412f | 0.000 | 1786215  | 0        | 0.733  | N.D. #  |
| 23)                         | Chlordane-1     | 4.297  | 0.000 | 5841495  | 0        | 51.387 | N.D. #  |
| -----                       |                 |        |       |          |          |        |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL020921\  
Data File : PL064713.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 09 Feb 2021 18:58  
Operator : AR\AJ  
Sample : M1317-11  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampled :  
R-A

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 10 02:11:07 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL020821.M  
Quant Title : GC Extractables  
QLast Update : Tue Feb 09 04:41:29 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

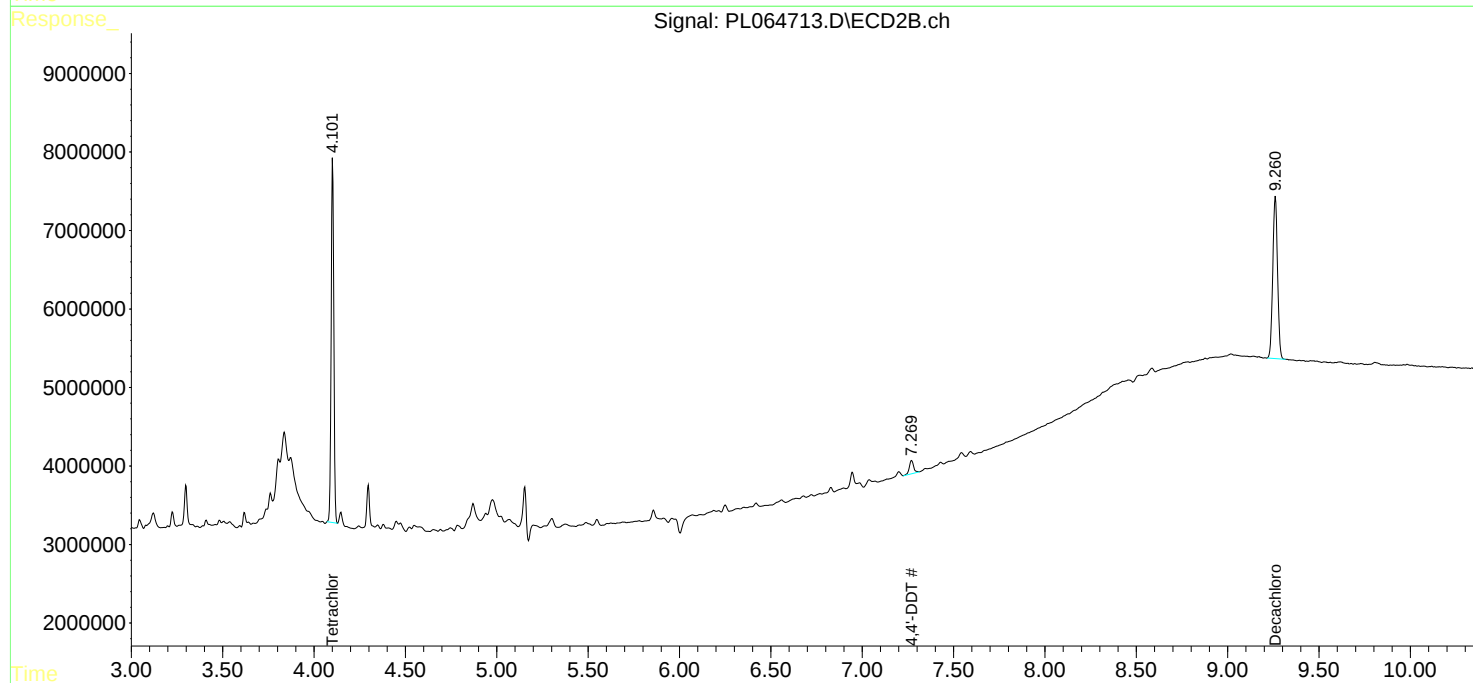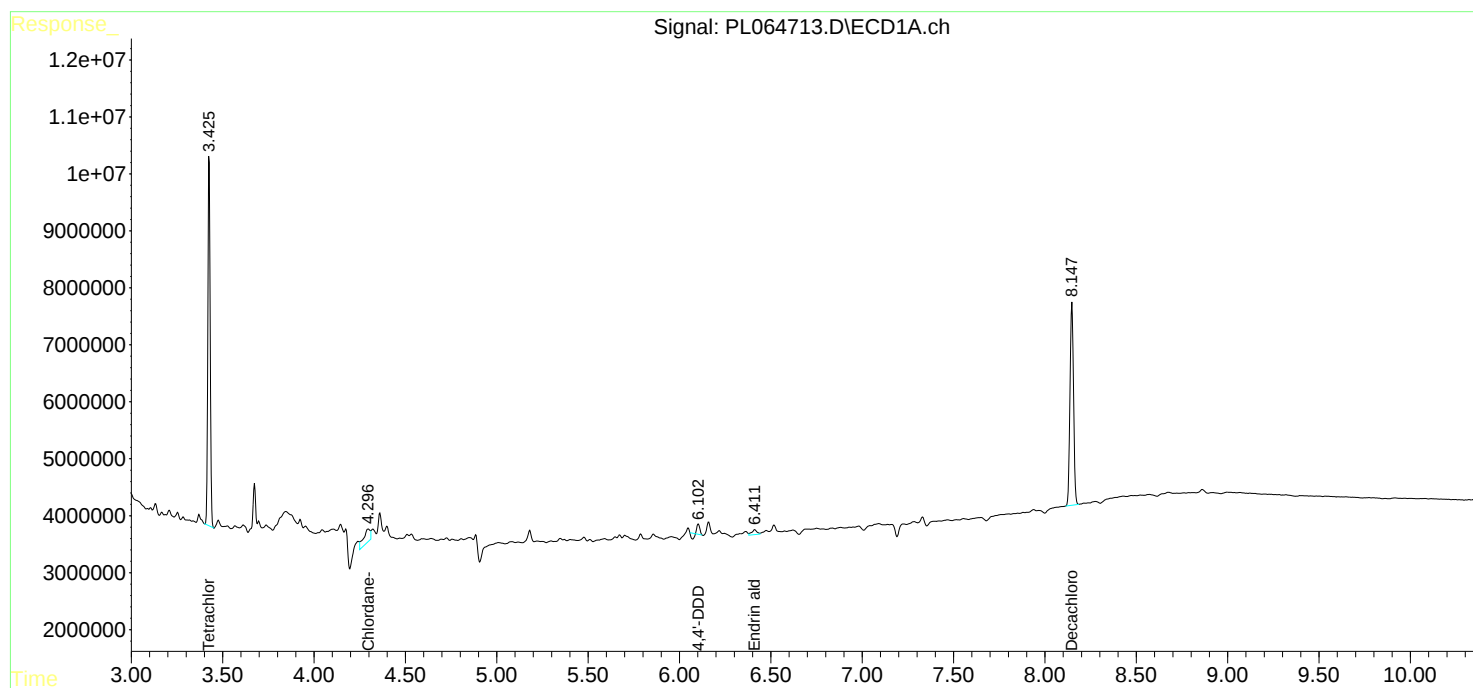


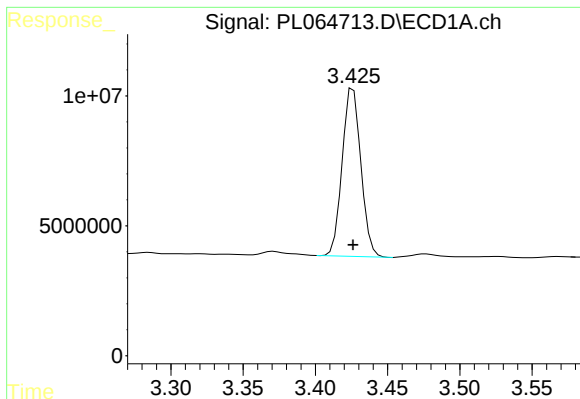

#1 Tetrachloro-m-xylene


R.T.: 3.426 min  
Delta R.T.: 0.000 min  
Response: 58153446  
Conc: 20.67 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
R-A

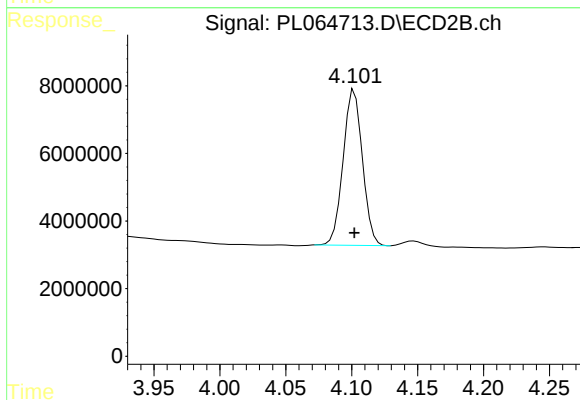


#1 Tetrachloro-m-xylene

R.T.: 4.102 min  
Delta R.T.: 0.000 min  
Response: 46853415  
Conc: 21.69 ng/ml

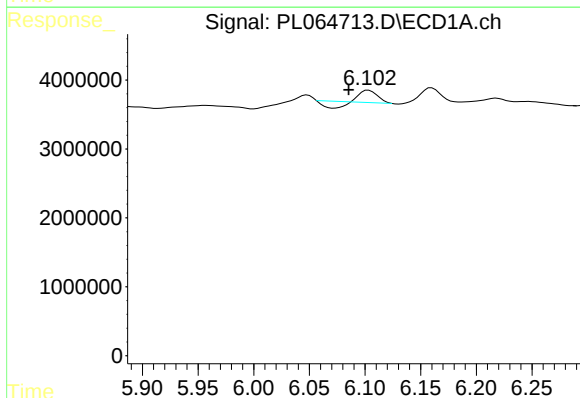


#16 4,4'-DDD

R.T.: 6.103 min  
Delta R.T.: 0.018 min  
Response: 1033663  
Conc: 0.41 ng/ml

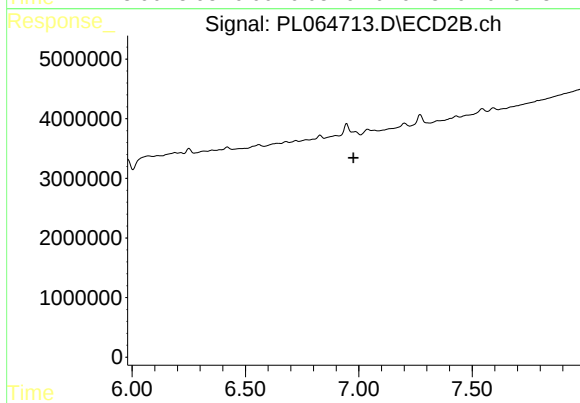

#16 4,4'-DDD


R.T.: 0.000 min  
Exp R.T.: 6.977 min  
Response: 0  
Conc: N.D.

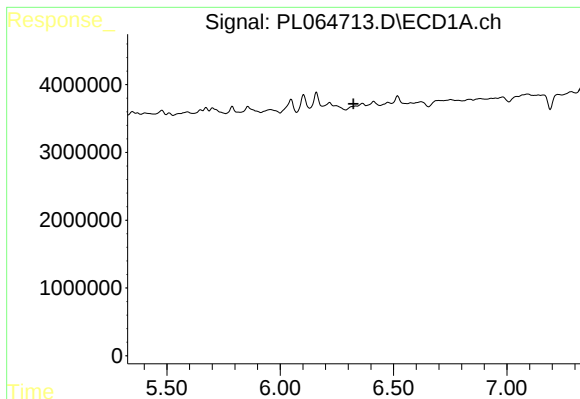

#17 4,4'-DDT


R.T.: 0.000 min  
Exp R.T.: 6.324 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
R-A

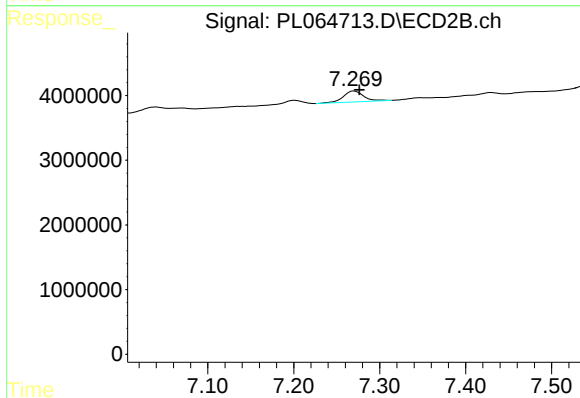


#17 4,4'-DDT

R.T.: 7.270 min  
Delta R.T.: -0.006 min  
Response: 2787088  
Conc: 1.83 ng/ml

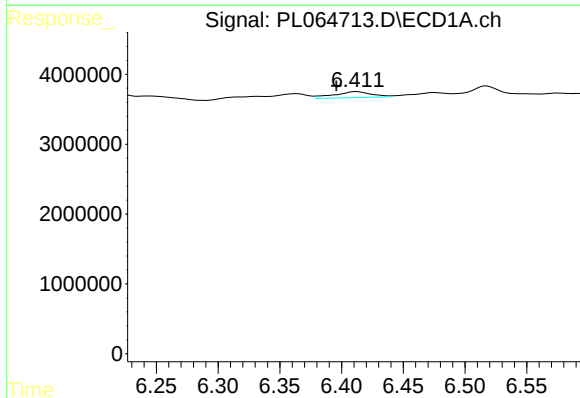


#18 Endrin aldehyde

R.T.: 6.412 min  
Delta R.T.: 0.017 min  
Response: 1786215  
Conc: 0.73 ng/ml

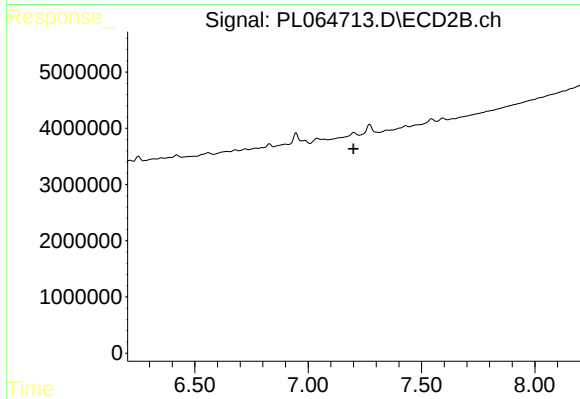

#18 Endrin aldehyde


R.T.: 0.000 min  
Exp R.T.: 7.200 min  
Response: 0  
Conc: N.D.

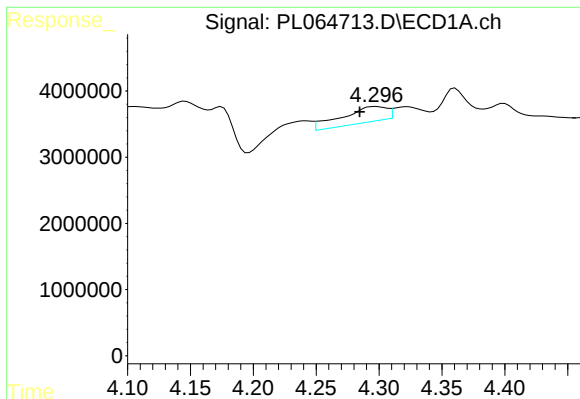

#23 Chlordane-1


R.T.: 4.297 min  
Delta R.T.: 0.013 min  
Response: 5841495  
Conc: 51.39 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
R-A

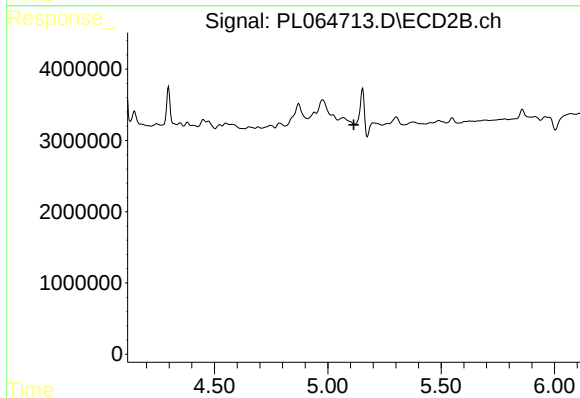


#23 Chlordane-1

R.T.: 0.000 min  
Exp R.T.: 5.114 min  
Response: 0  
Conc: N.D.

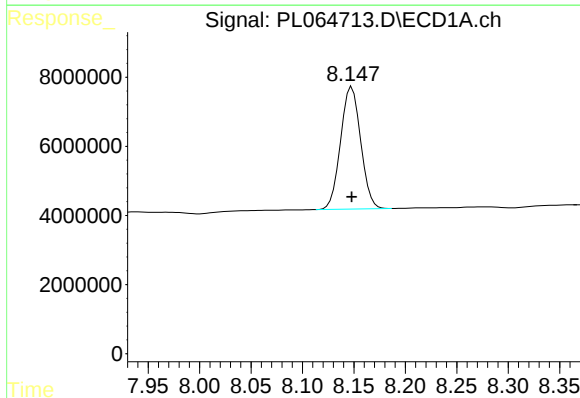

#28 Decachlorobiphenyl

R.T.: 8.148 min  
Delta R.T.: 0.000 min  
Response: 48236408  
Conc: 21.45 ng/ml

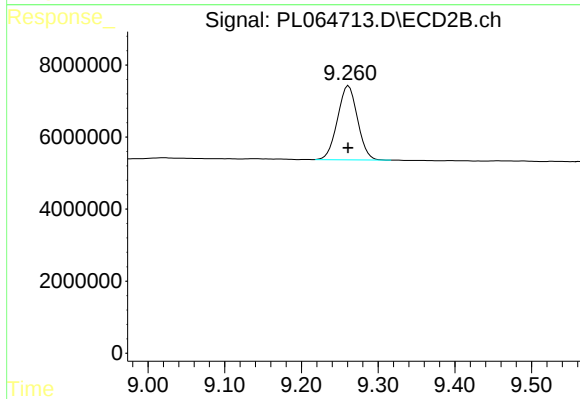

#28 Decachlorobiphenyl

R.T.: 9.261 min  
Delta R.T.: 0.000 min  
Response: 37384690  
Conc: 19.68 ng/ml