

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
 Data File : PL064728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 22:47
 Operator : AR\AJ
 Sample : M1339-07
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-5-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:15:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.102	69656170	55394245	24.758	25.643
28)	SA Decachlor...	8.147	9.259	58494715	44958662	26.012	23.670
Target Compounds							
7)	B delta-BHC	0.000	5.216f	0	3615228	N.D.	1.338 #
9)	A Endosulfan I	5.480f	0.000	3795385	0	1.184	N.D. #
10)	B gamma-Chl...	5.368f	0.000	1077160	0	0.307	N.D. #
13)	MA Dieldrin	5.694	0.000	4558108	0	1.390	N.D. #
15)	B Endosulfa...	6.213f	0.000	1372478	0	0.477	N.D. #
17)	MA 4,4'-DDT	6.318	7.246f	4578081	1460757	2.030	0.958 #
23)	Chlordane-1	4.281	0.000	1875929	0	16.502	N.D. #
25)	Chlordane-3	5.368f	0.000	1077160	0	3.278	N.D. #
27)	Chlordane-5	6.213f	0.000	1372478	0	13.565	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
Data File : PL064728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 22:47
Operator : AR\AJ
Sample : M1339-07
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-5-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:15:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

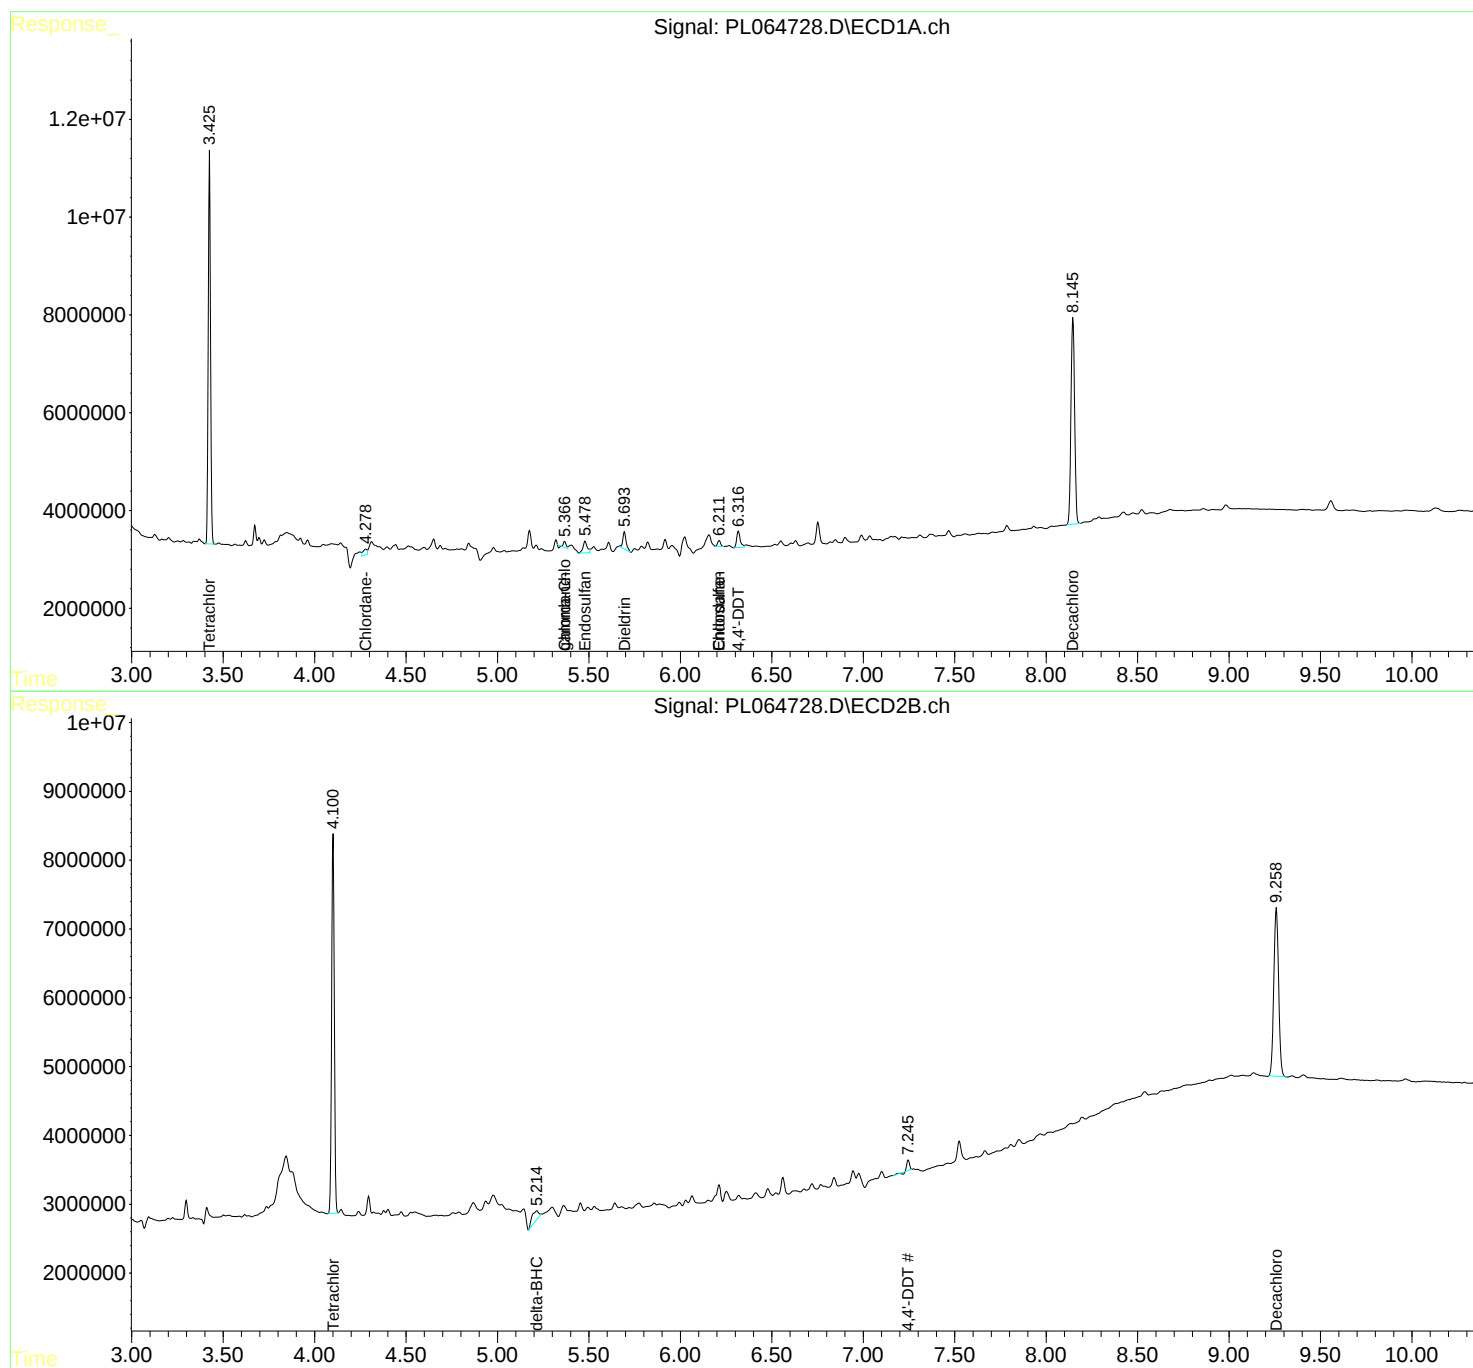


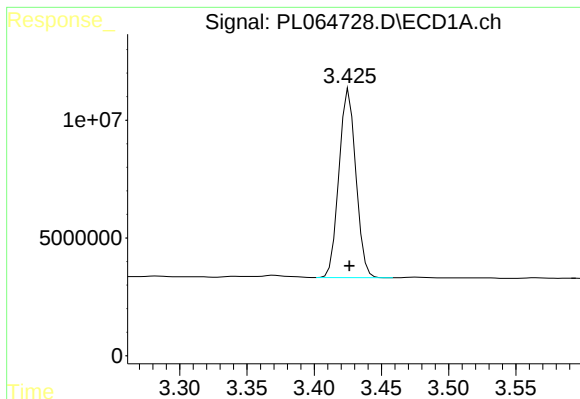

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 69656170
Conc: 24.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-10

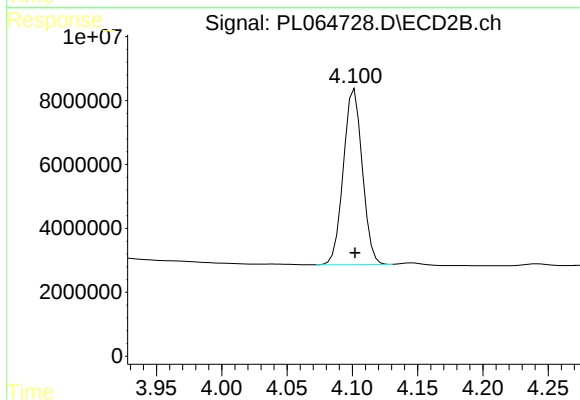


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 55394245
Conc: 25.64 ng/ml

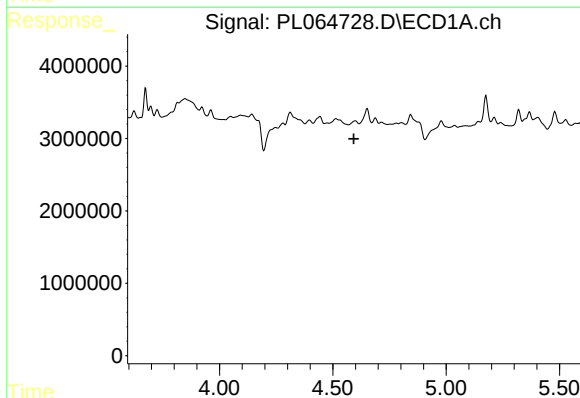


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.593 min
Response: 0
Conc: N.D.

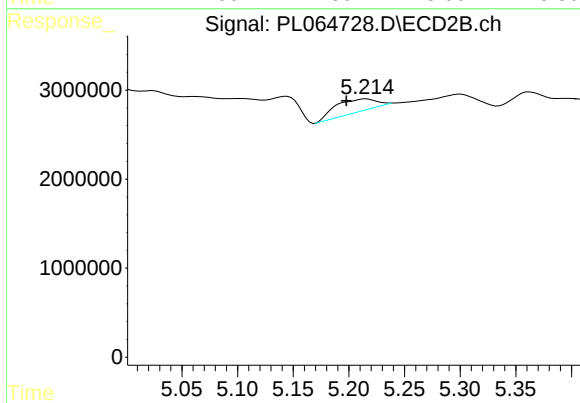

#7 delta-BHC


R.T.: 5.216 min
Delta R.T.: 0.018 min
Response: 3615228
Conc: 1.34 ng/ml

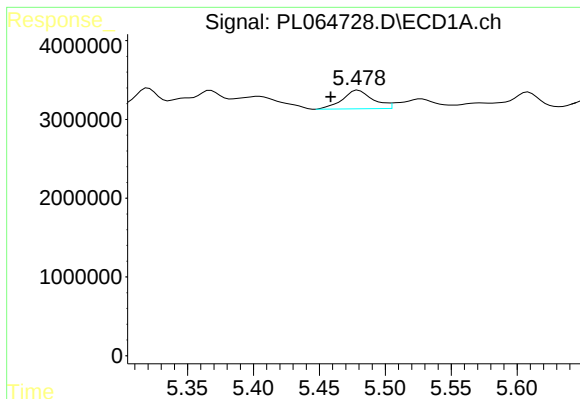

#9 Endosulfan I


R.T.: 5.480 min
Delta R.T.: 0.021 min
Response: 3795385
Conc: 1.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-10

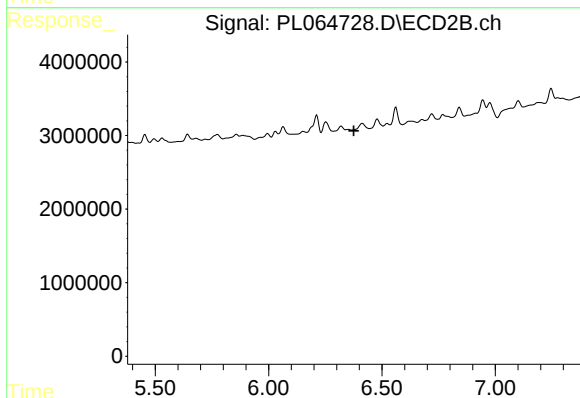


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.376 min
Response: 0
Conc: N.D.

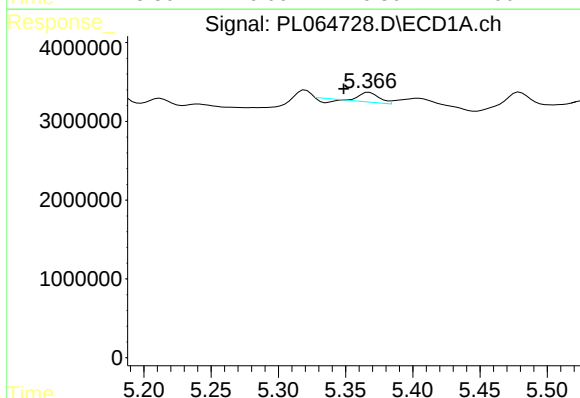


#10 gamma-Chlordane

R.T.: 5.368 min
Delta R.T.: 0.019 min
Response: 1077160
Conc: 0.31 ng/ml

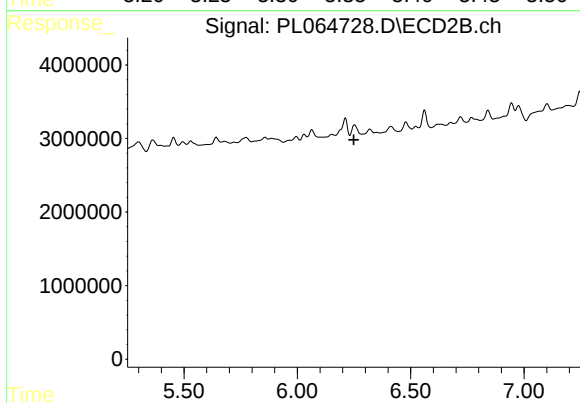

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.249 min
Response: 0
Conc: N.D.

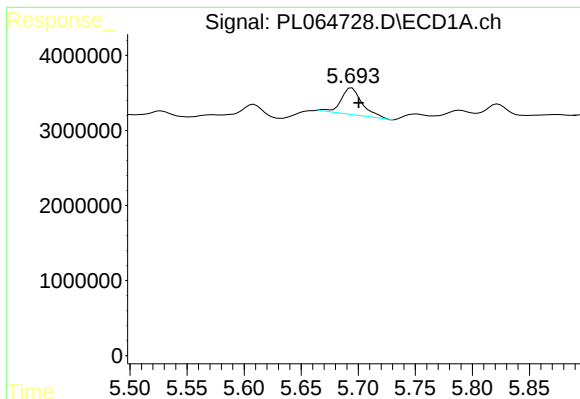

#13 Dieldrin


R.T.: 5.694 min
Delta R.T.: -0.006 min
Response: 4558108
Conc: 1.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-10

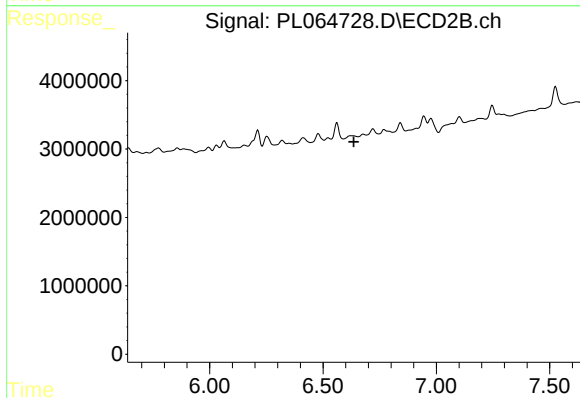


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

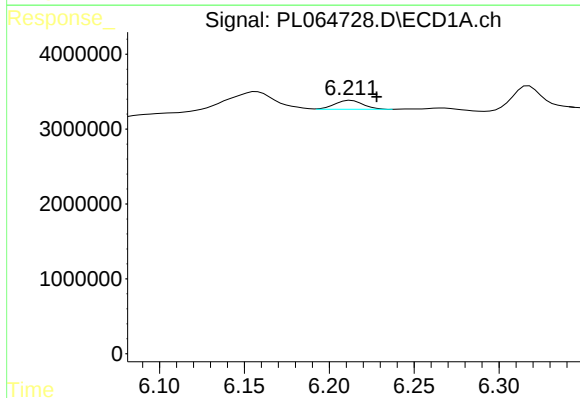


#15 Endosulfan II

R.T.: 6.213 min
Delta R.T.: -0.015 min
Response: 1372478
Conc: 0.48 ng/ml

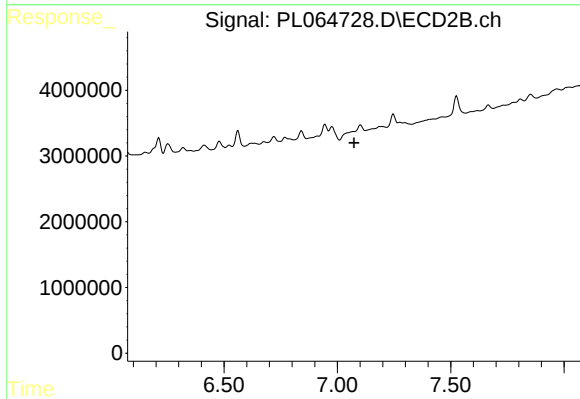

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.073 min
Response: 0
Conc: N.D.

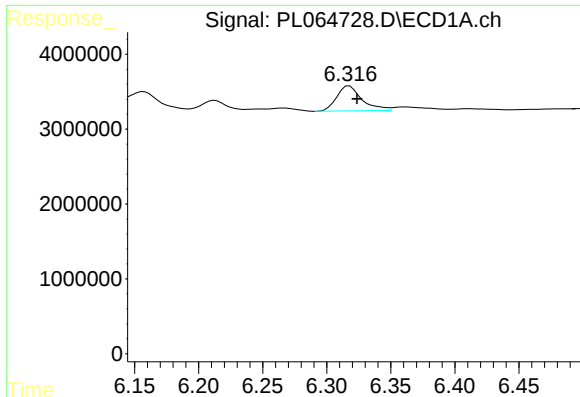

#17 4,4'-DDT


R.T.: 6.318 min
Delta R.T.: -0.006 min
Response: 4578081
Conc: 2.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-10

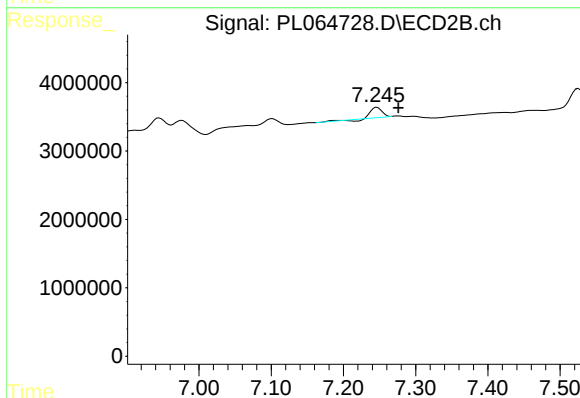


#17 4,4'-DDT

R.T.: 7.246 min
Delta R.T.: -0.030 min
Response: 1460757
Conc: 0.96 ng/ml

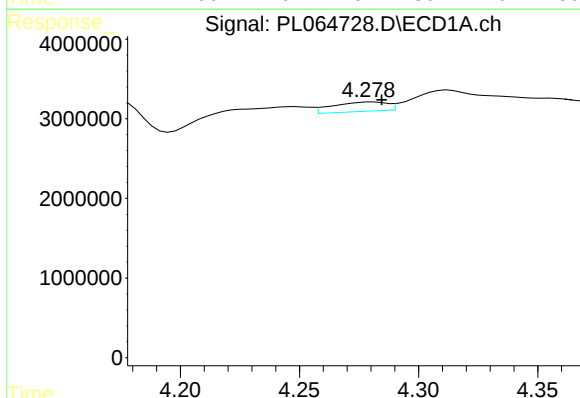


#23 Chlordane-1

R.T.: 4.281 min
Delta R.T.: -0.004 min
Response: 1875929
Conc: 16.50 ng/ml

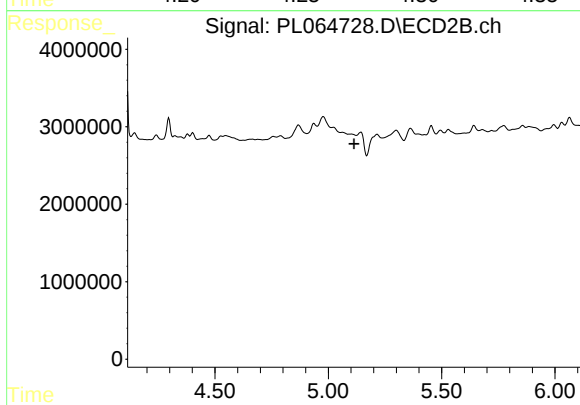

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.114 min
Response: 0
Conc: N.D.

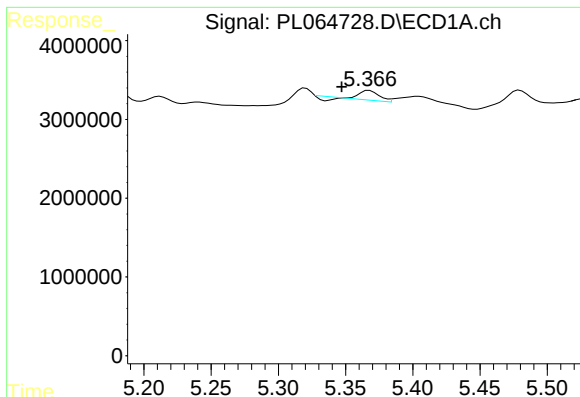

#25 Chlordane-3


R.T.: 5.368 min
Delta R.T.: 0.020 min
Response: 1077160
Conc: 3.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-10

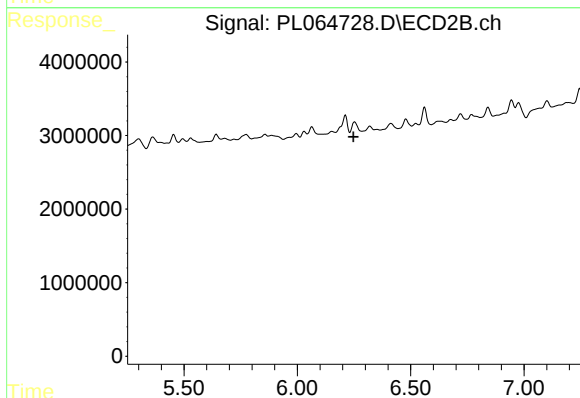


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

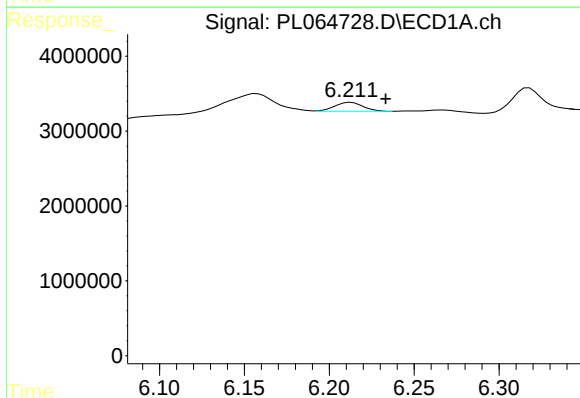


#27 Chlordane-5

R.T.: 6.213 min
Delta R.T.: -0.020 min
Response: 1372478
Conc: 13.56 ng/ml

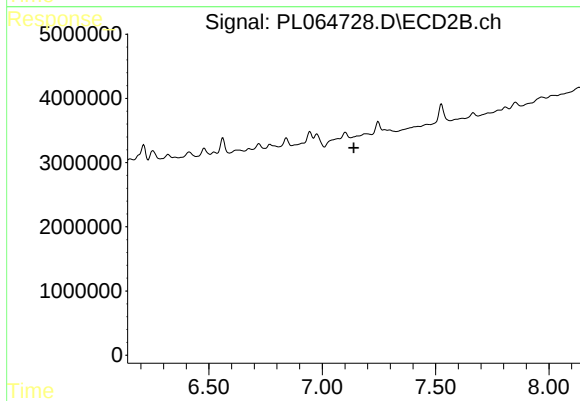

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.139 min
Response: 0
Conc: N.D.

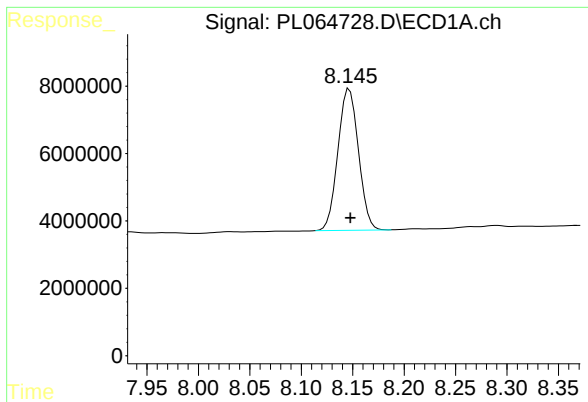

#28 Decachlorobiphenyl

R.T.: 8.147 min
Delta R.T.: 0.000 min
Response: 58494715
Conc: 26.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-10

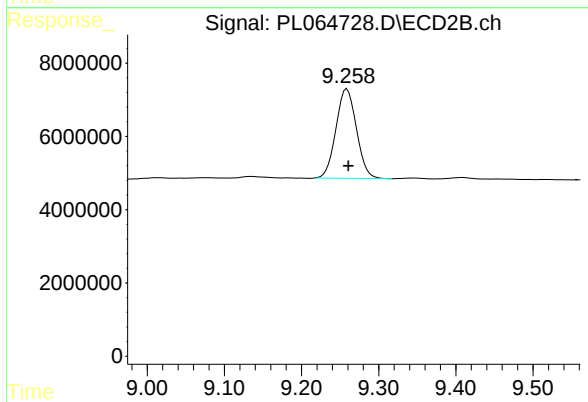

#28 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.002 min
Response: 44958662
Conc: 23.67 ng/ml