

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
 Data File : PL064733.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 23:59
 Operator : AR\AJ
 Sample : M1341-02
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 26572

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:16:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.102	30045987	26005122	10.679	12.038
28)	SA Decachlor...	8.148	9.261	25846156	25283488	11.493	13.311
Target Compounds							
5)	MB Aldrin	4.681	0.000	1253820	0	0.337	N.D. #
10)	B gamma-Chl...	5.370f	0.000	6322643	0	1.803	N.D. #
11)	B alpha-Chl...	5.405	6.321	3331435	5951806	0.962	2.585 #
12)	B 4,4'-DDE	5.571	0.000	2014032	0	0.644	N.D. #
13)	MA Dieldrin	5.694	0.000	2400820	0	0.732	N.D. #
17)	MA 4,4'-DDT	6.318	7.247f	2190071	532855	0.971	0.349 #
23)	Chlordane-1	4.287	0.000	946405	0	8.325	N.D. #
24)	Chlordane-2	4.787	0.000	2635525	0	21.301	N.D. #
25)	Chlordane-3	5.370f	0.000	6322643	0	19.240	N.D. #
26)	Chlordane-4	5.405	6.321	3331435	5951806	12.108	16.065 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
Data File : PL064733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 23:59
Operator : AR\AJ
Sample : M1341-02
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
26572

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:16:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

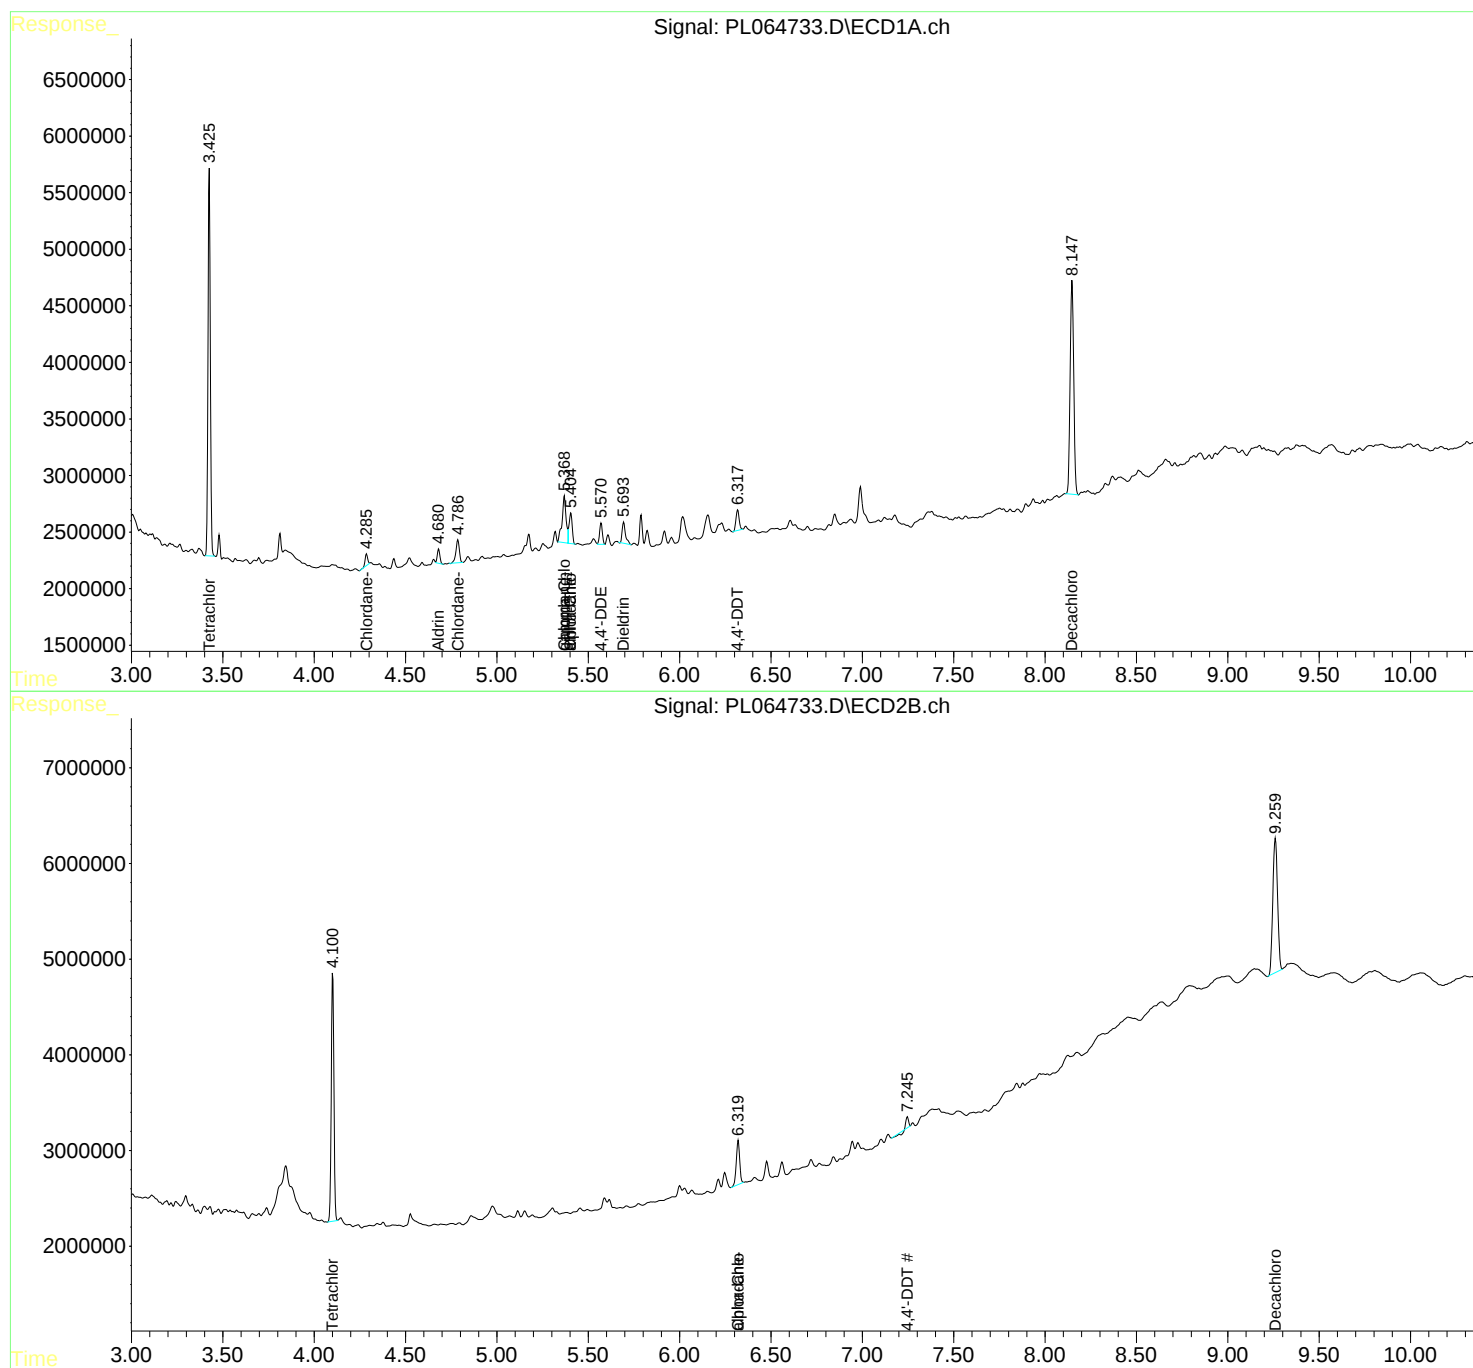


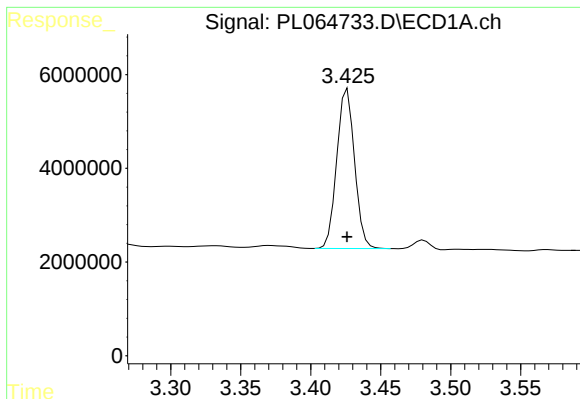

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 30045987
Conc: 10.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
26572

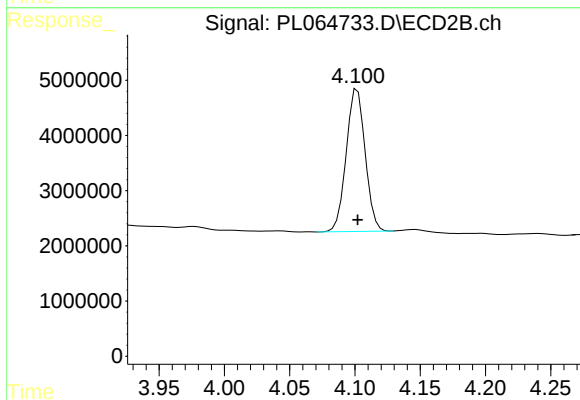


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 26005122
Conc: 12.04 ng/ml

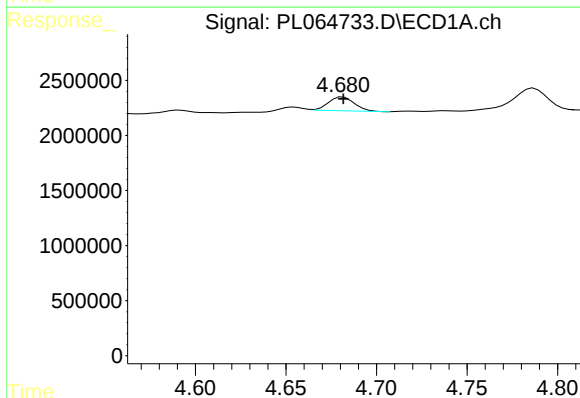


#5 Aldrin

R.T.: 4.681 min
Delta R.T.: 0.000 min
Response: 1253820
Conc: 0.34 ng/ml

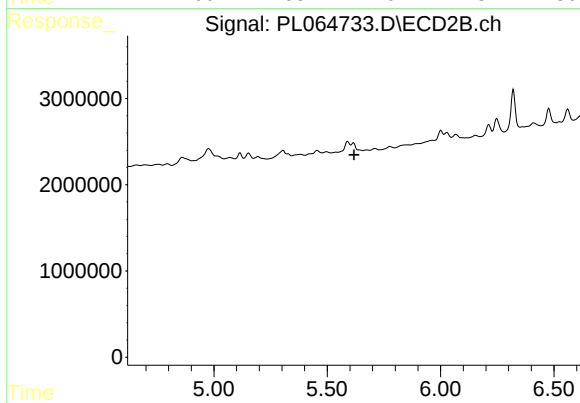

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.618 min
Response: 0
Conc: N.D.

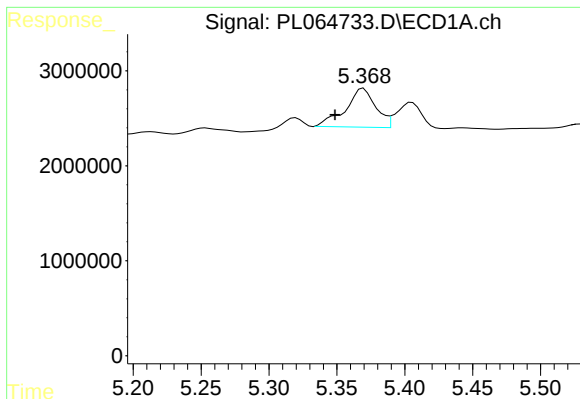

#10 gamma-Chlordane


R.T.: 5.370 min
Delta R.T.: 0.021 min
Response: 6322643
Conc: 1.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
26572

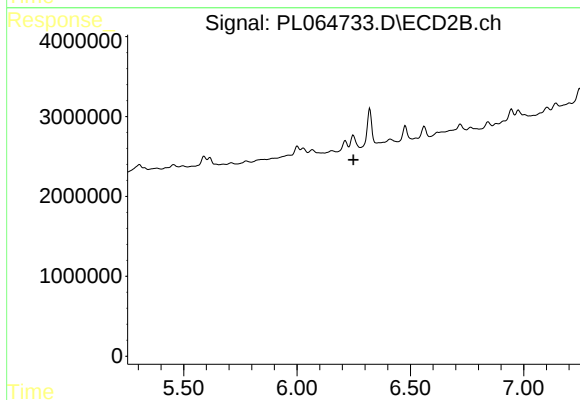


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.249 min
Response: 0
Conc: N.D.

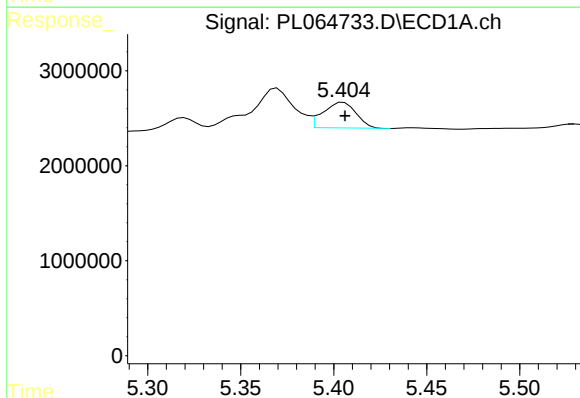


#11 alpha-Chlordane

R.T.: 5.405 min
Delta R.T.: 0.000 min
Response: 3331435
Conc: 0.96 ng/ml

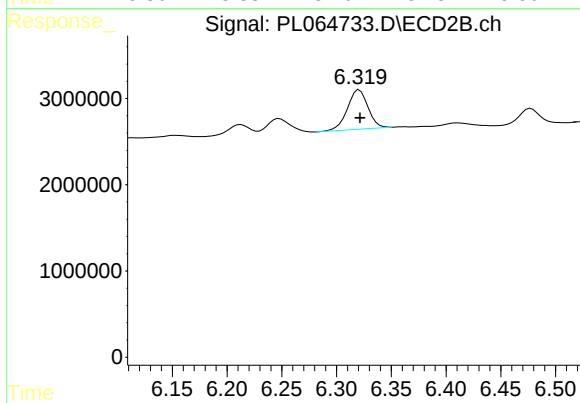

#11 alpha-Chlordane


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 5951806
Conc: 2.59 ng/ml

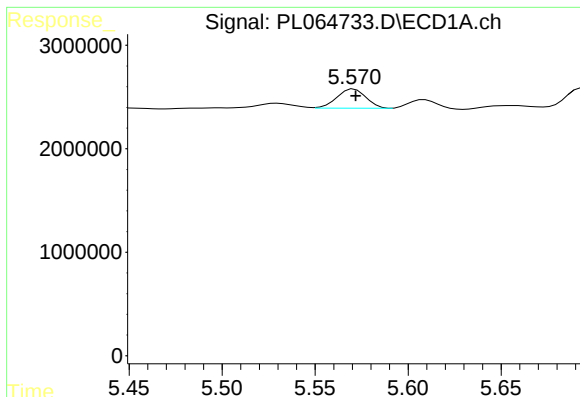

#12 4,4'-DDE


R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 2014032
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
26572

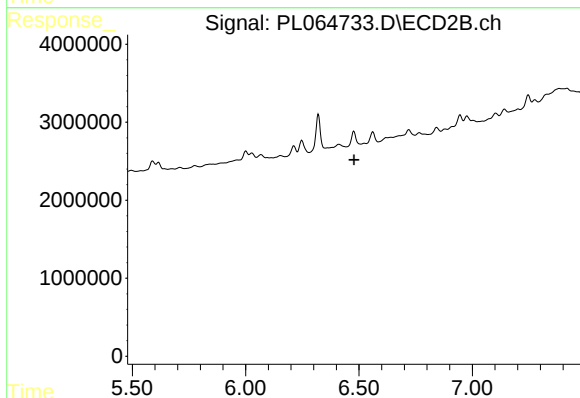


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.478 min
Response: 0
Conc: N.D.

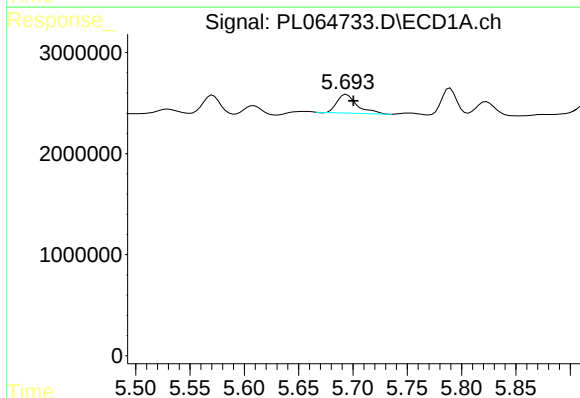


#13 Dieldrin

R.T.: 5.694 min
Delta R.T.: -0.006 min
Response: 2400820
Conc: 0.73 ng/ml

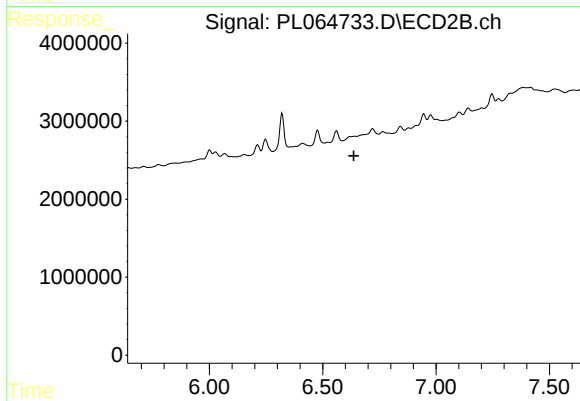

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

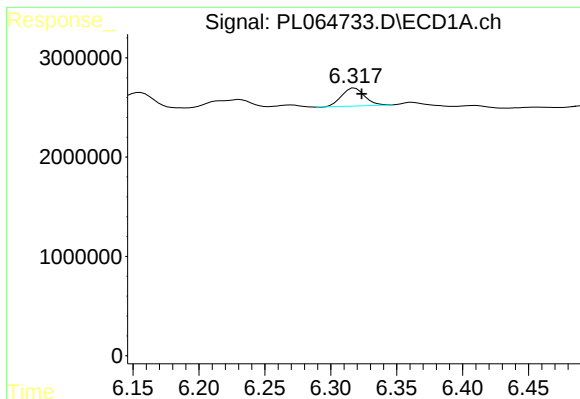

#17 4,4'-DDT


R.T.: 6.318 min
Delta R.T.: -0.005 min
Response: 2190071
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
26572

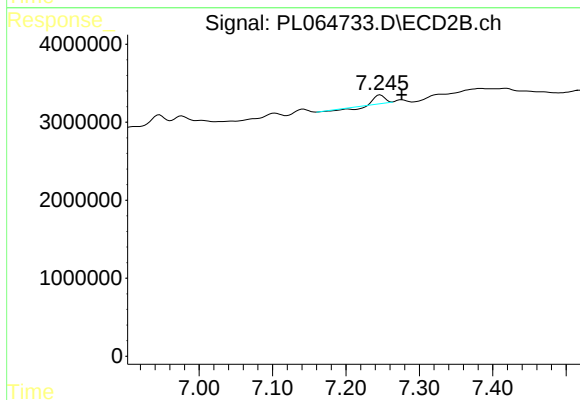


#17 4,4'-DDT

R.T.: 7.247 min
Delta R.T.: -0.029 min
Response: 532855
Conc: 0.35 ng/ml

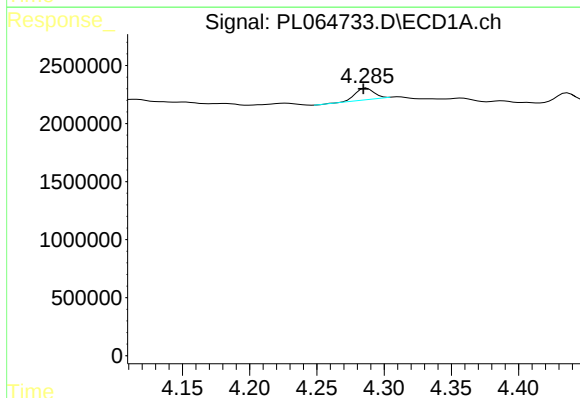


#23 Chlordane-1

R.T.: 4.287 min
Delta R.T.: 0.002 min
Response: 946405
Conc: 8.33 ng/ml

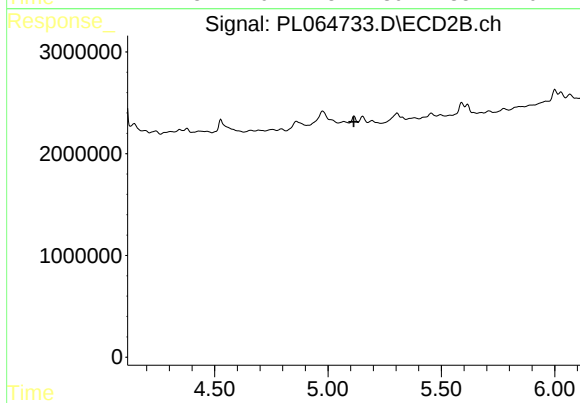

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.114 min
Response: 0
Conc: N.D.

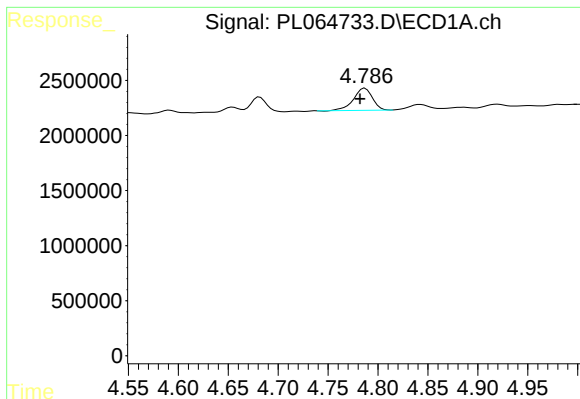

#24 Chlordane-2


R.T.: 4.787 min
Delta R.T.: 0.005 min
Response: 2635525
Conc: 21.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
26572

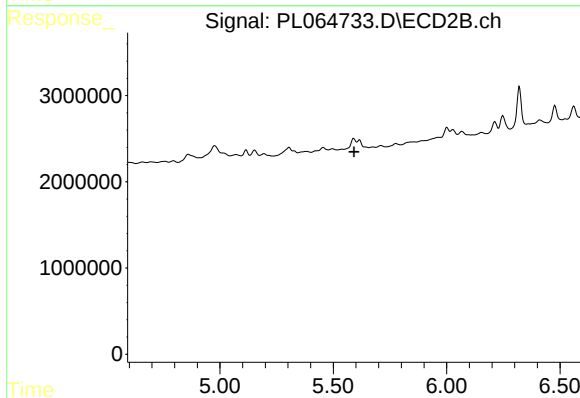


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.592 min
Response: 0
Conc: N.D.

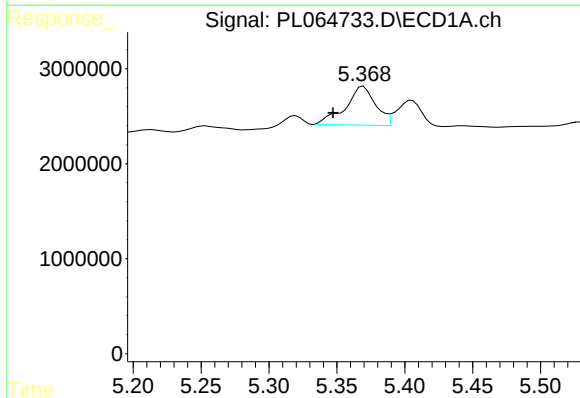


#25 Chlordane-3

R.T.: 5.370 min
Delta R.T.: 0.022 min
Response: 6322643
Conc: 19.24 ng/ml

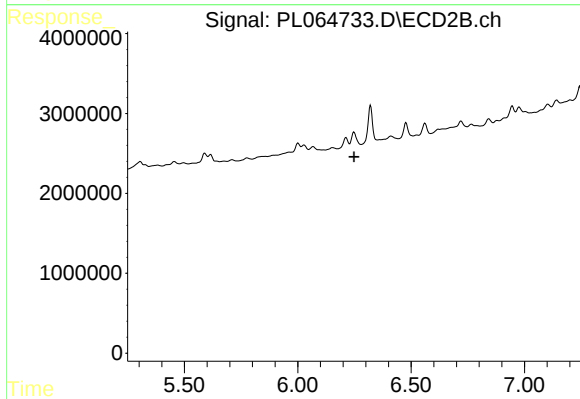

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

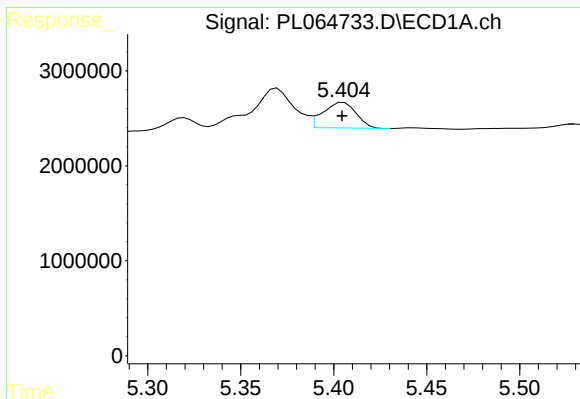

#26 Chlordane-4


R.T.: 5.405 min
Delta R.T.: 0.000 min
Response: 3331435
Conc: 12.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
26572

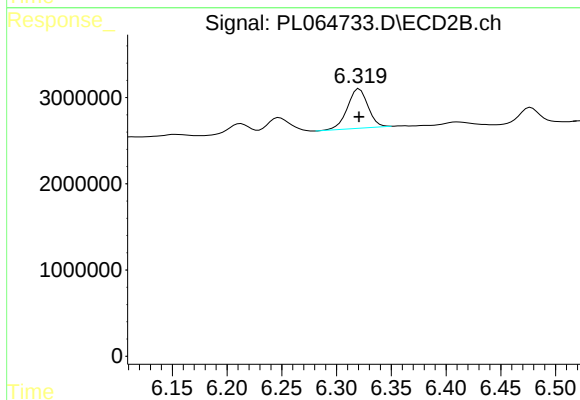


#26 Chlordane-4

R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 5951806
Conc: 16.07 ng/ml

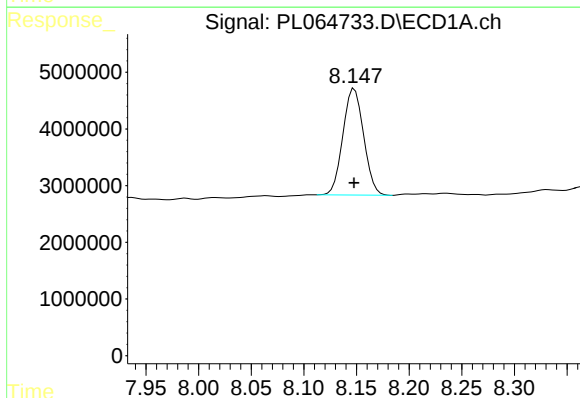

#28 Decachlorobiphenyl

R.T.: 8.148 min
Delta R.T.: 0.000 min
Response: 25846156
Conc: 11.49 ng/ml

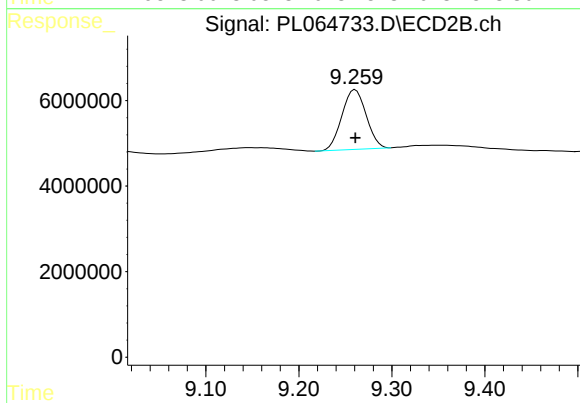

#28 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: 0.000 min
Response: 25283488
Conc: 13.31 ng/ml