

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
 Data File : PL064744.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2021 03:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 04:40:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.101	64052046	48520097	22.766	22.461
28)	SA Decachlor...	8.147	9.259	49162713	39254016	21.862	20.667
Target Compounds							
14)	MA Endrin	5.962	0.000	3004725	0	1.000	N.D. #
23)	Chlordane-1	4.311f	0.000	2809966	0	24.719	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
Data File : PL064744.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2021 03:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 04:40:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

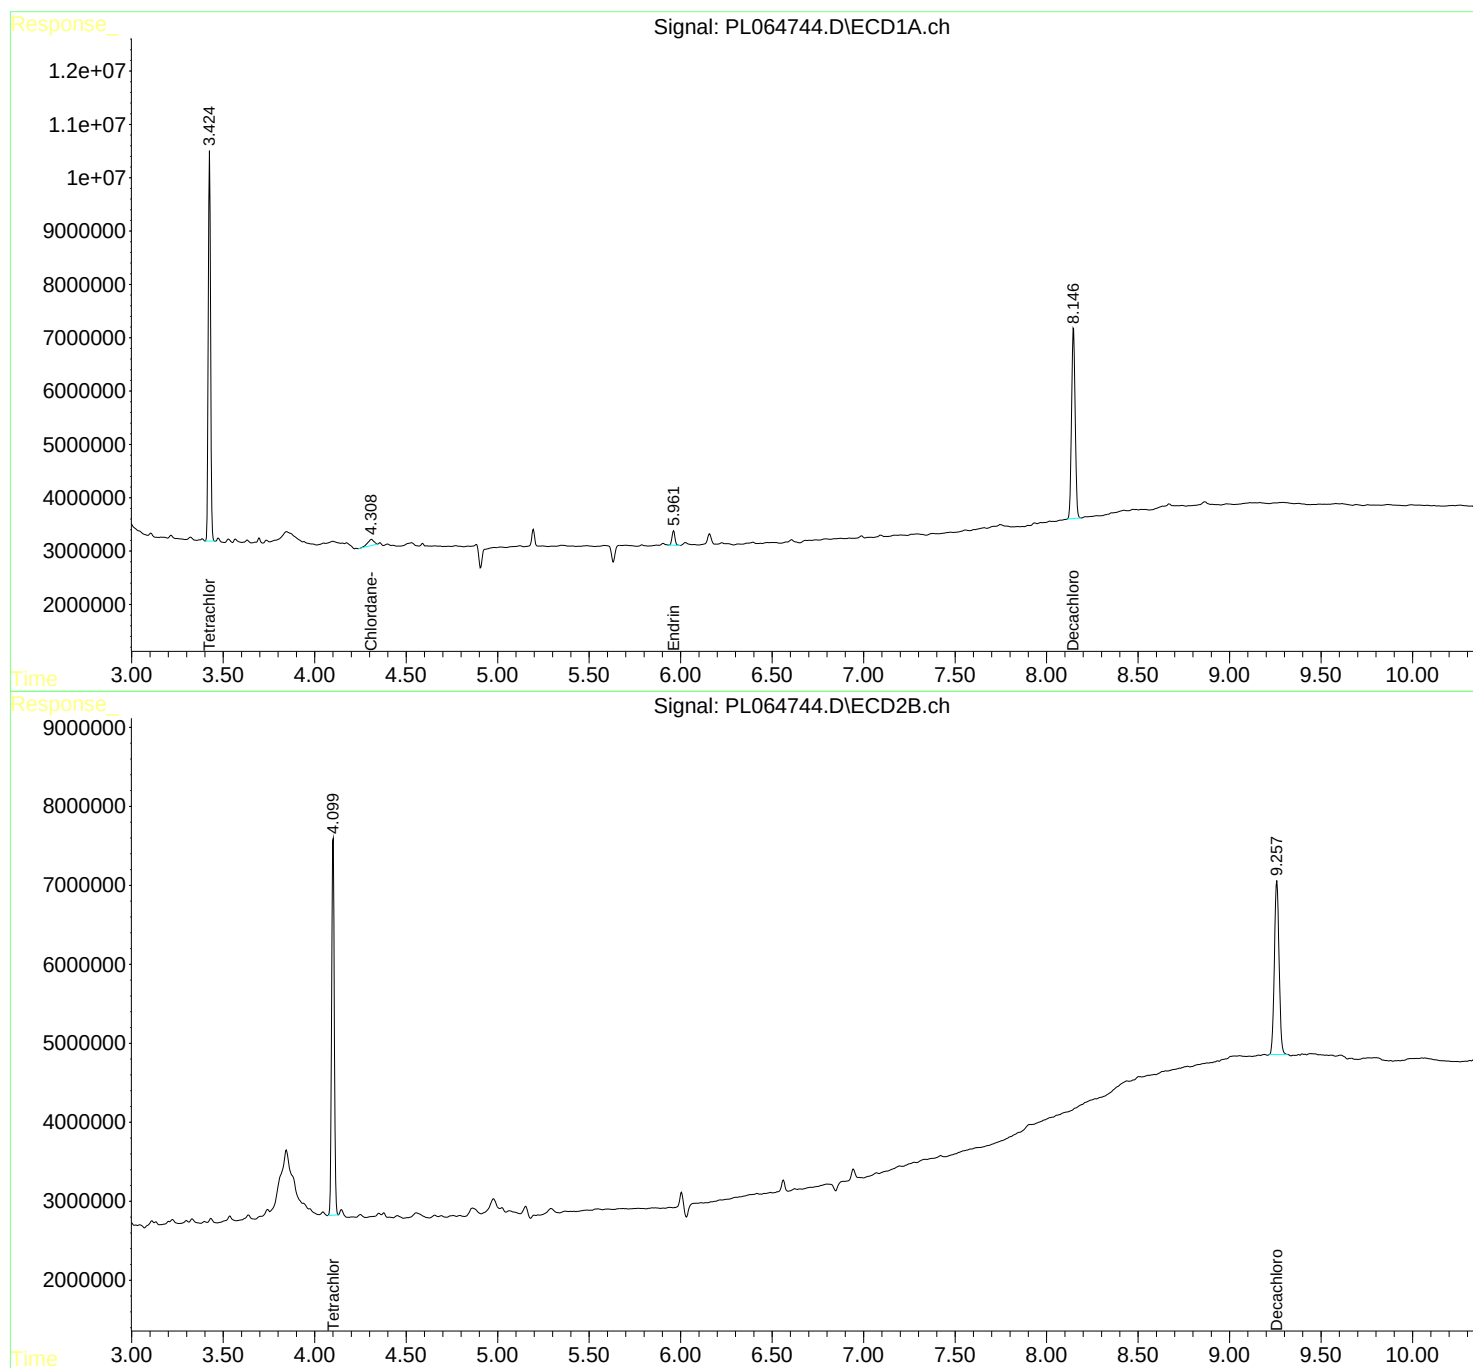


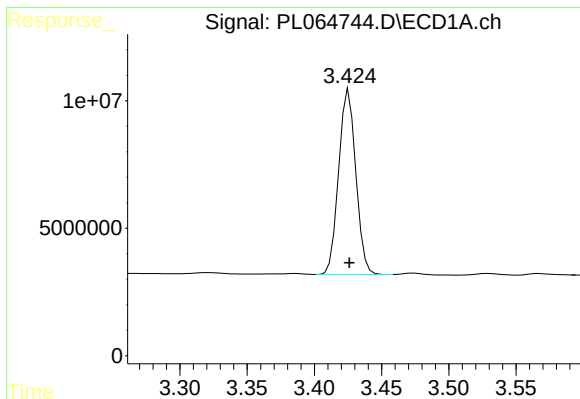

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 64052046
Conc: 22.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

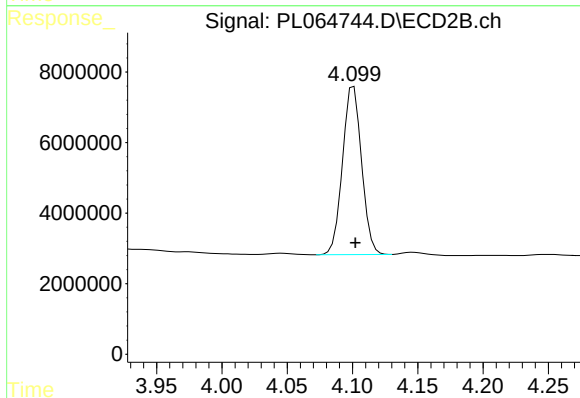


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.001 min
Response: 48520097
Conc: 22.46 ng/ml

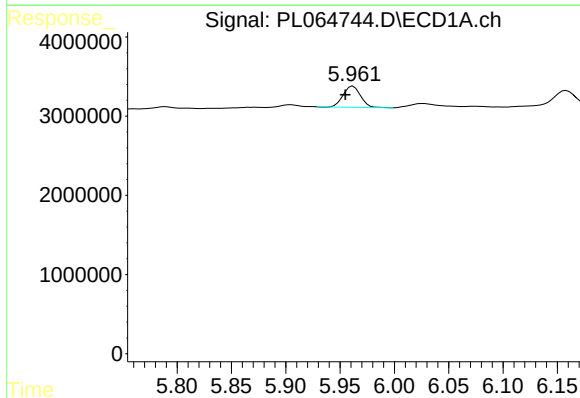


#14 Endrin

R.T.: 5.962 min
Delta R.T.: 0.007 min
Response: 3004725
Conc: 1.00 ng/ml

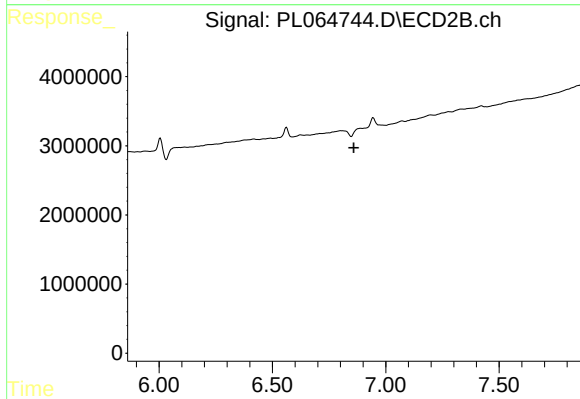

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.858 min
Response: 0
Conc: N.D.

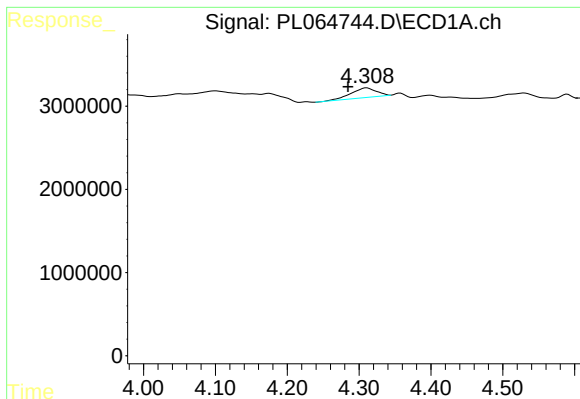

#23 Chlordane-1


R.T.: 4.311 min
Delta R.T.: 0.026 min
Response: 2809966
Conc: 24.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

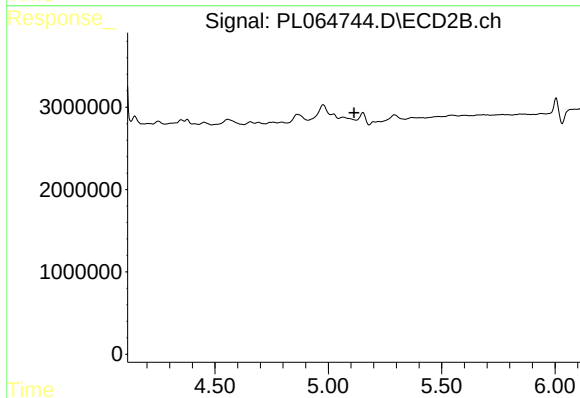


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.114 min
Response: 0
Conc: N.D.

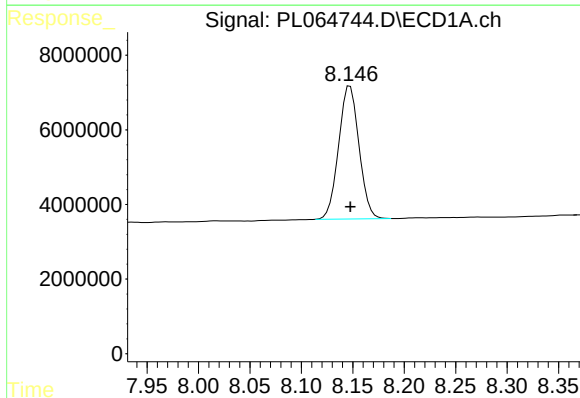

#28 Decachlorobiphenyl

R.T.: 8.147 min
Delta R.T.: 0.000 min
Response: 49162713
Conc: 21.86 ng/ml

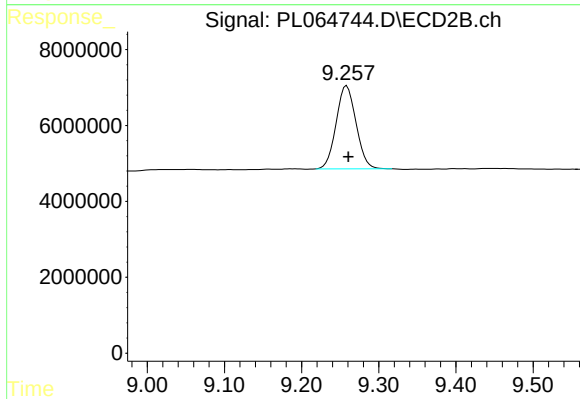

#28 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.002 min
Response: 39254016
Conc: 20.67 ng/ml