

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
 Data File : PL064708.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 17:46
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 02:15:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.102	155.3E6	116.3E6	55.190	53.840
28)	SA Decachlor...	8.148	9.260	120.0E6	92677122	53.374	48.793
Target Compounds							
23)	Chlordane-1	4.286	5.115	51183508	42623012	450.255	485.300
24)	Chlordane-2	4.784	5.591	56840460	45354509	459.389	520.155
25)	Chlordane-3	5.348	6.247	159.6E6	152.8E6	485.667	499.805
26)	Chlordane-4	5.405	6.320	132.2E6	184.8E6	480.498	498.717
27)	Chlordane-5	6.234	7.140	50872517	27239787	502.799	482.685



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
Data File : PL064708.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 17:46
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 02:15:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

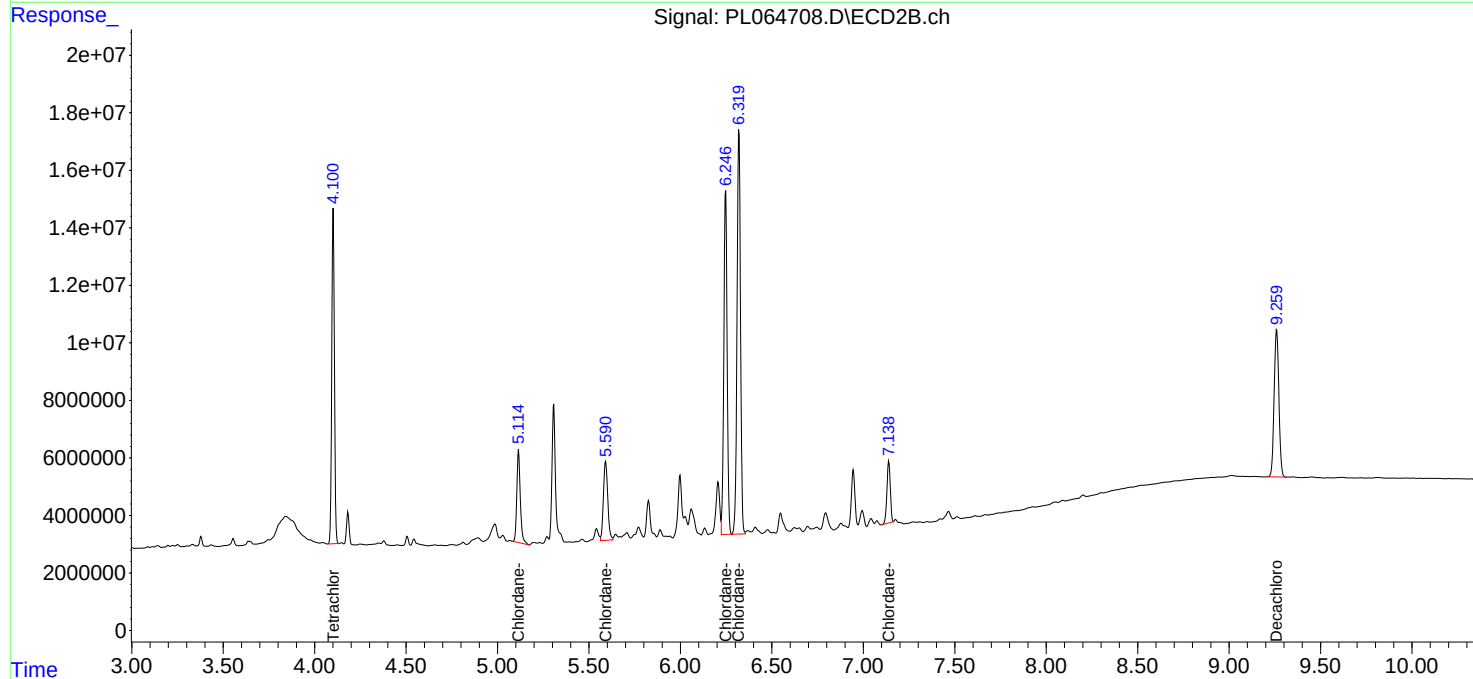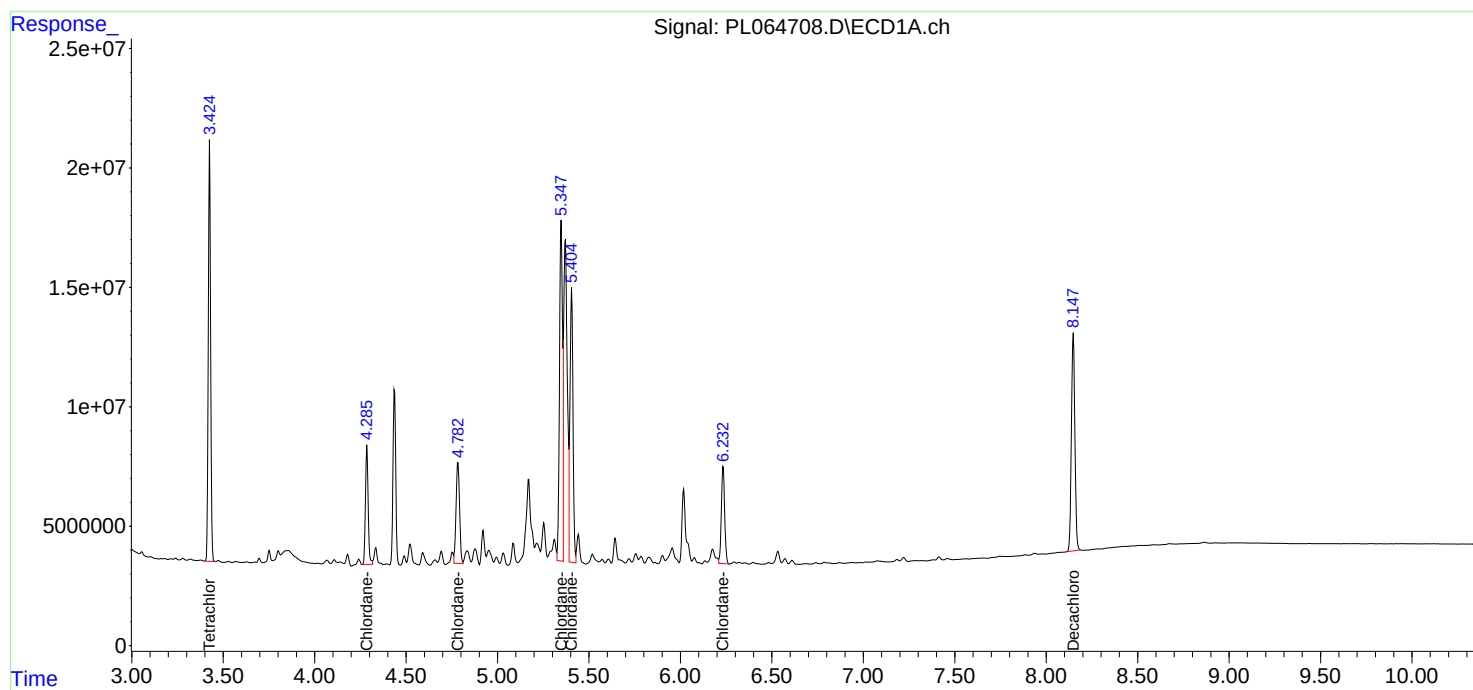


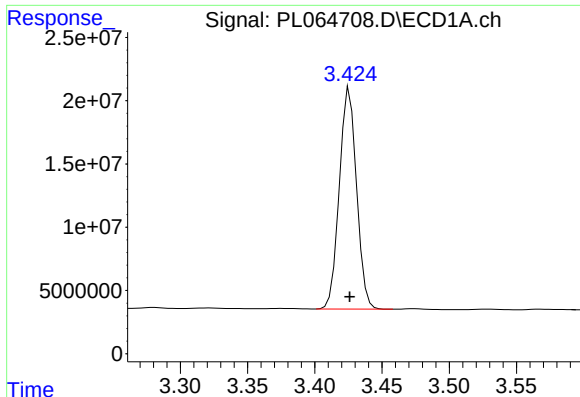

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 155276373
Conc: 55.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

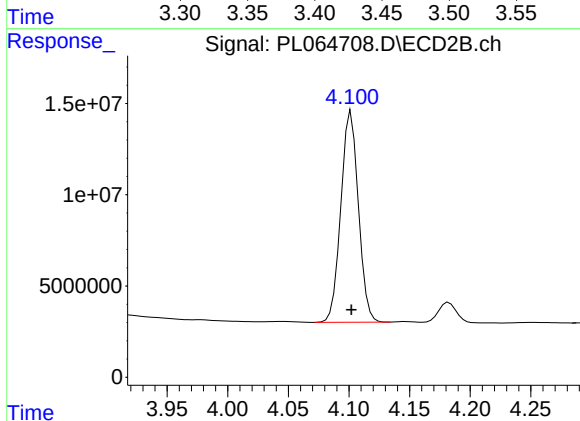


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 116304744
Conc: 53.84 ng/ml

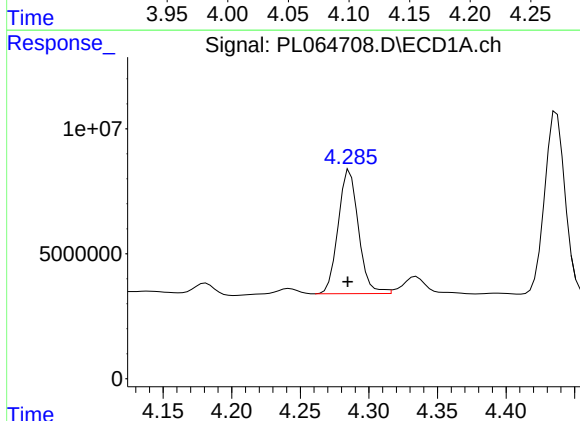


#23 Chlordane-1

R.T.: 4.286 min
Delta R.T.: 0.002 min
Response: 51183508
Conc: 450.25 ng/ml

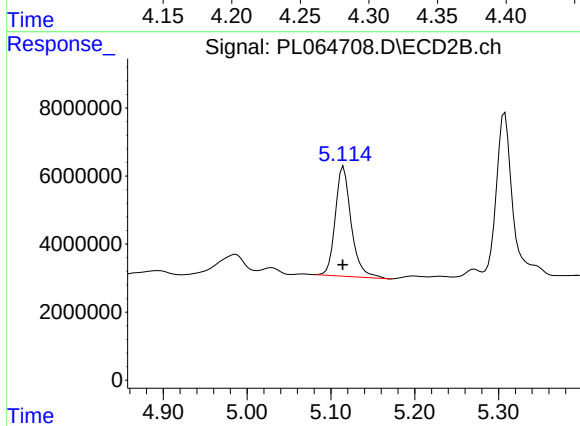

#23 Chlordane-1


R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 42623012
Conc: 485.30 ng/ml

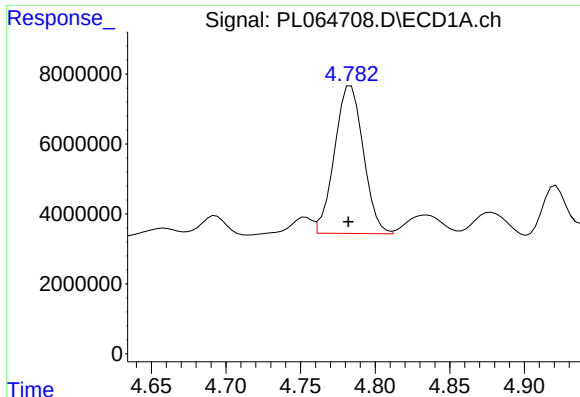

#24 Chlordane-2


R.T.: 4.784 min
Delta R.T.: 0.002 min
Response: 56840460
Conc: 459.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

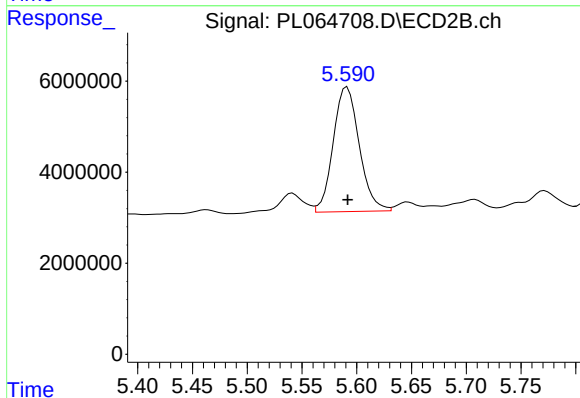


#24 Chlordane-2

R.T.: 5.591 min
Delta R.T.: 0.000 min
Response: 45354509
Conc: 520.15 ng/ml

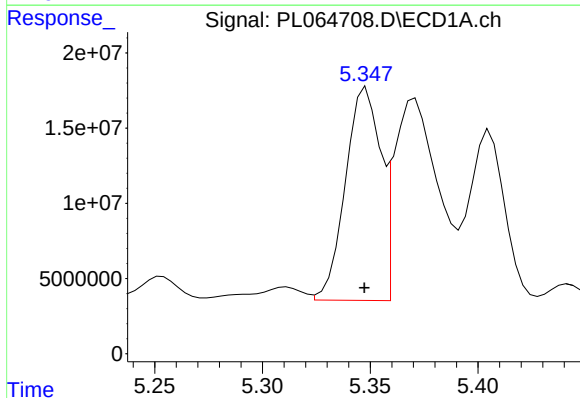


#25 Chlordane-3

R.T.: 5.348 min
Delta R.T.: 0.001 min
Response: 159597364
Conc: 485.67 ng/ml

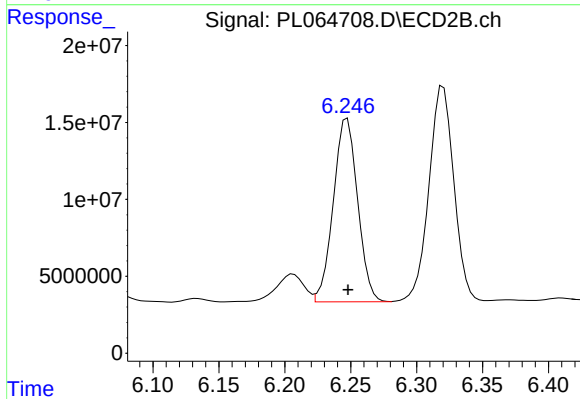

#25 Chlordane-3


R.T.: 6.247 min
Delta R.T.: 0.000 min
Response: 152819544
Conc: 499.81 ng/ml

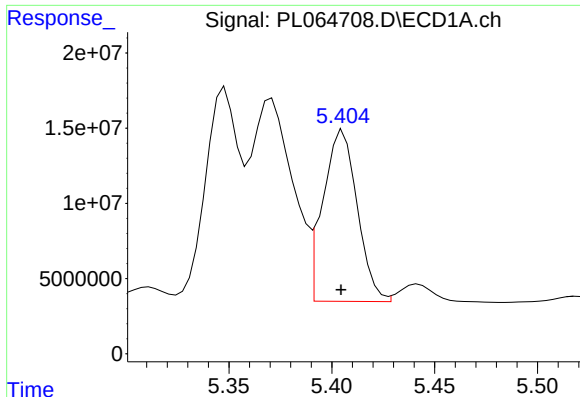

#26 Chlordane-4


R.T.: 5.405 min
Delta R.T.: 0.000 min
Response: 132206768
Conc: 480.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

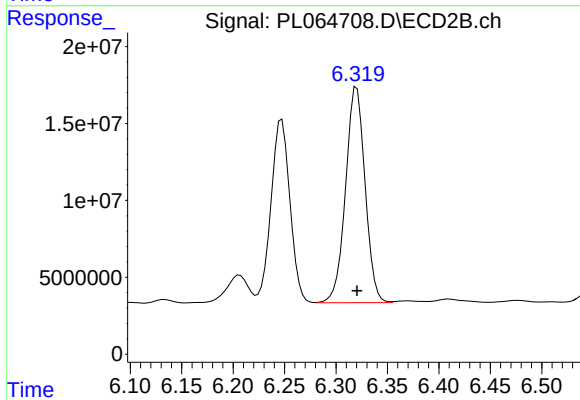


#26 Chlordane-4

R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 184763527
Conc: 498.72 ng/ml

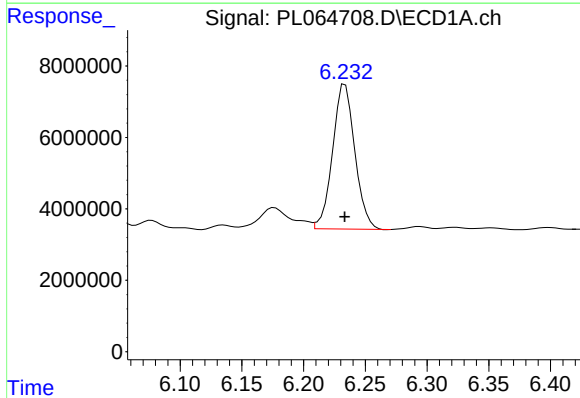


#27 Chlordane-5

R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 50872517
Conc: 502.80 ng/ml

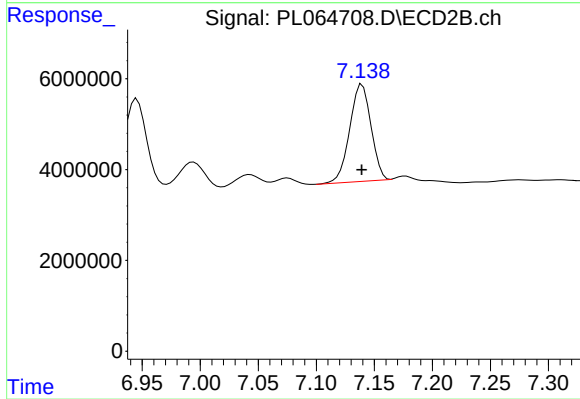

#27 Chlordane-5


R.T.: 7.140 min
Delta R.T.: 0.000 min
Response: 27239787
Conc: 482.69 ng/ml

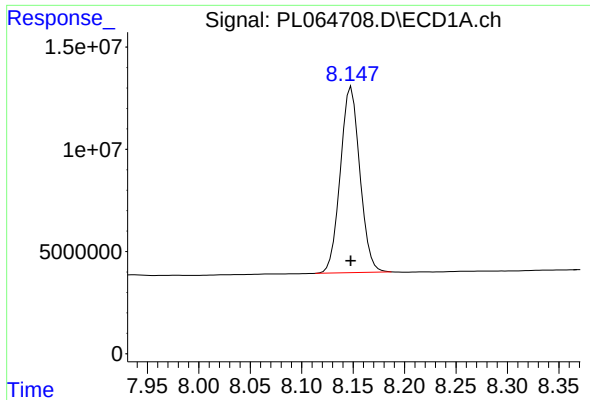

#28 Decachlorobiphenyl

R.T.: 8.148 min
Delta R.T.: 0.000 min
Response: 120028349
Conc: 53.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

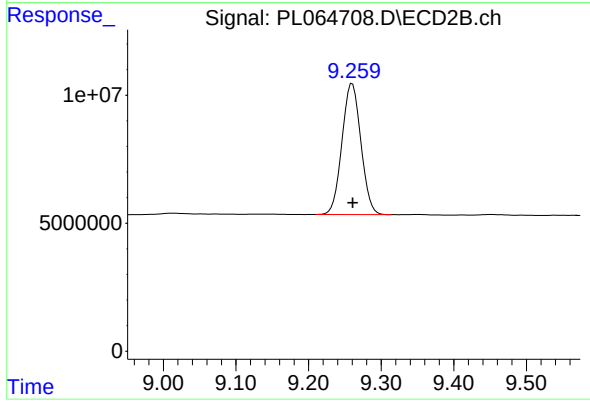

#28 Decachlorobiphenyl

R.T.: 9.260 min
Delta R.T.: 0.000 min
Response: 92677122
Conc: 48.79 ng/ml