

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
 Data File : PL064731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 23:30
 Operator : AR\AJ
 Sample : M1340-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-26586

Manual Integrations
 APPROVED

Ankita
 2/10/2021 1:59:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:16:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.101	63923076	40045737	22.720m	18.538m
28)	SA Decachlor...	8.154	9.265	17875172	25561695	7.949	13.458 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
Data File : PL064731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 23:30
Operator : AR\AJ
Sample : M1340-01
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT-26586


Manual Integrations
APPROVED

Ankita
2/10/2021 1:59:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:16:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

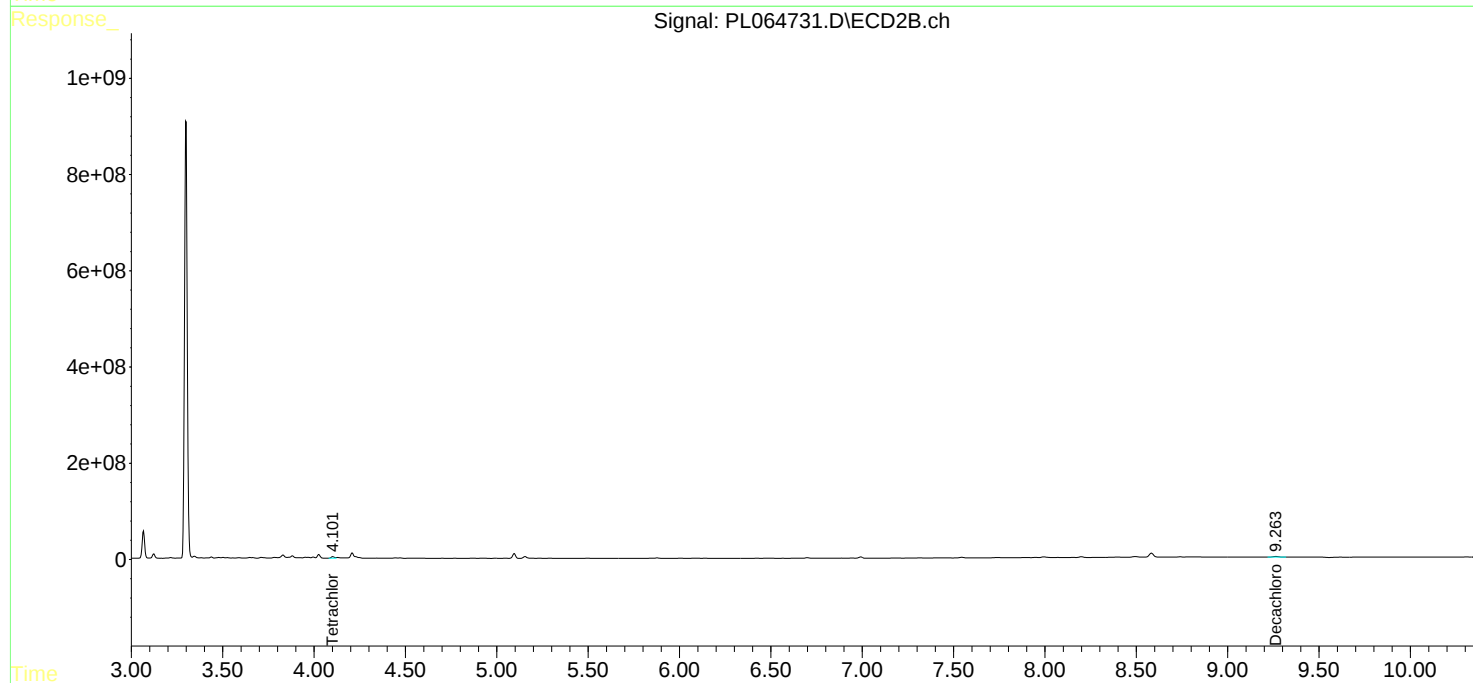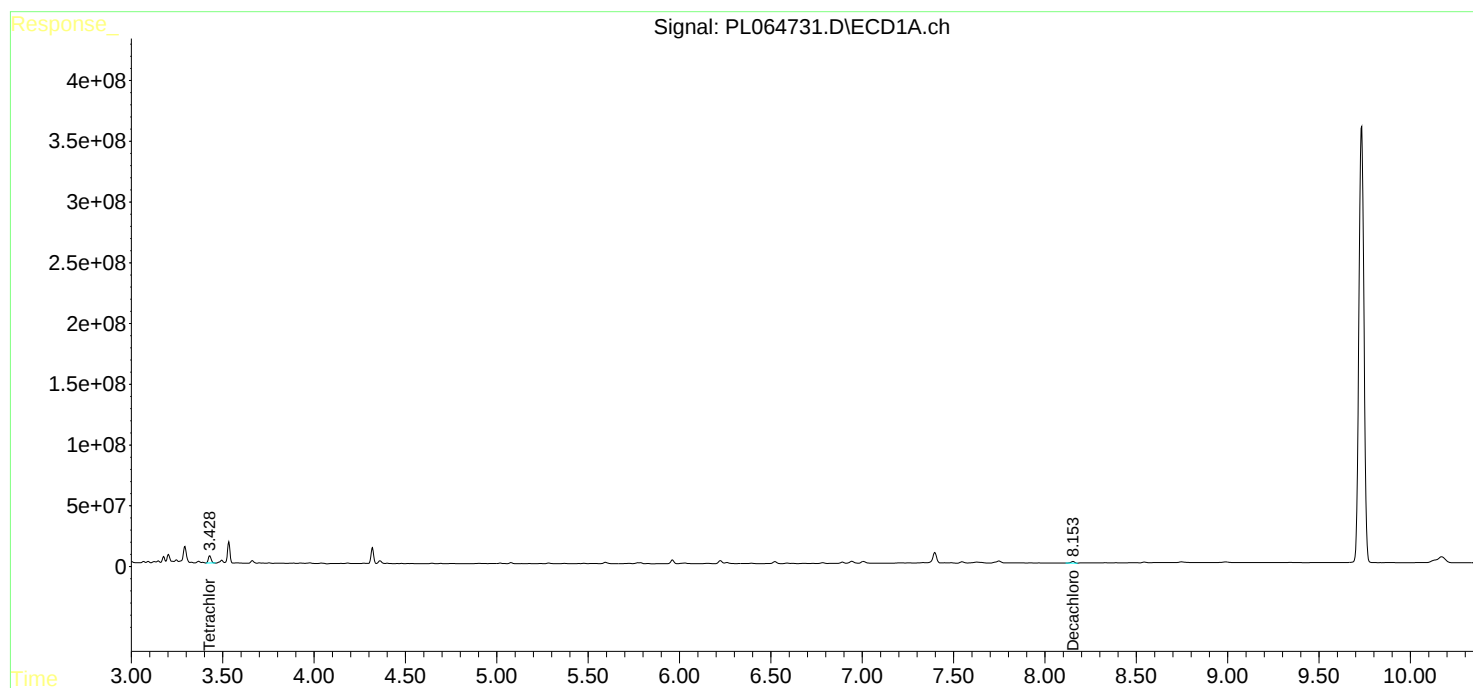

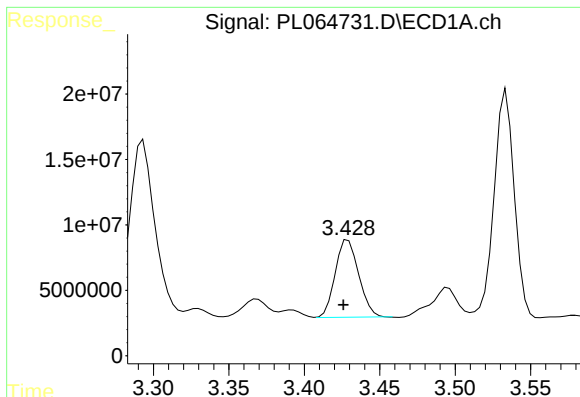


#1 Tetrachloro-m-xylene

R.T.: 3.428 min
Delta R.T.: 0.002 min
Response: 63923076
Conc: 22.72 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CHRT-26586


Manual Integrations
APPROVED

Ankita
2/10/2021 1:59:06 PM

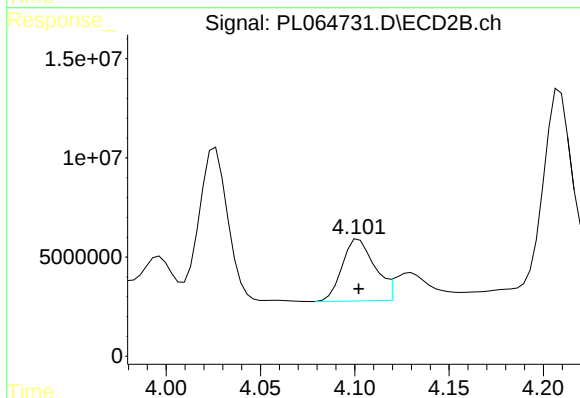


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.001 min
Response: 40045737
Conc: 18.54 ng/ml m

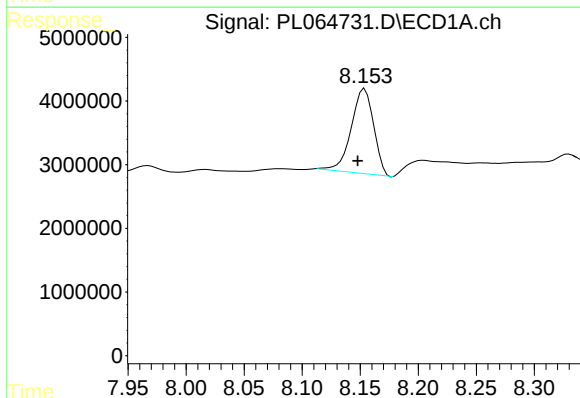

#28 Decachlorobiphenyl

R.T.: 8.154 min
Delta R.T.: 0.006 min
Response: 17875172
Conc: 7.95 ng/ml

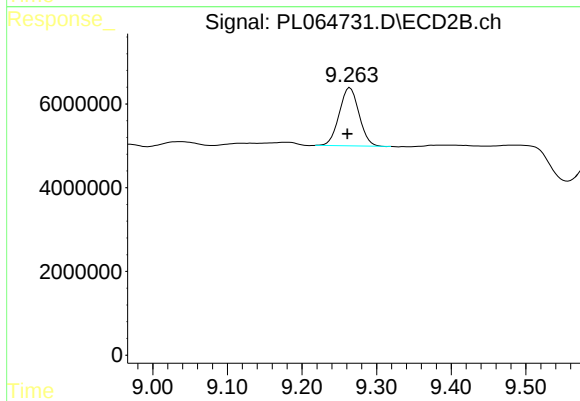

#28 Decachlorobiphenyl

R.T.: 9.265 min
Delta R.T.: 0.004 min
Response: 25561695
Conc: 13.46 ng/ml