

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
 Data File : PL064732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 23:44
 Operator : AR\AJ
 Sample : M1341-01
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20057

Manual Integrations
 APPROVED

Ankita
 2/10/2021 1:59:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:16:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.426	4.102	24134610	20465741	8.578	9.474
28) SA Decachlor...	8.148	9.260	19369248	23144406	8.613	12.185 #
Target Compounds						
10) B gamma-Chl...	5.353	6.247	844057	2230508	0.241m	0.965m#
11) B alpha-Chl...	5.405	6.321	2807717	5196425	0.811	2.257 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
Data File : PL064732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 23:44
Operator : AR\AJ
Sample : M1341-01
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20057


Manual Integrations
APPROVED

Ankita
2/10/2021 1:59:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:16:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

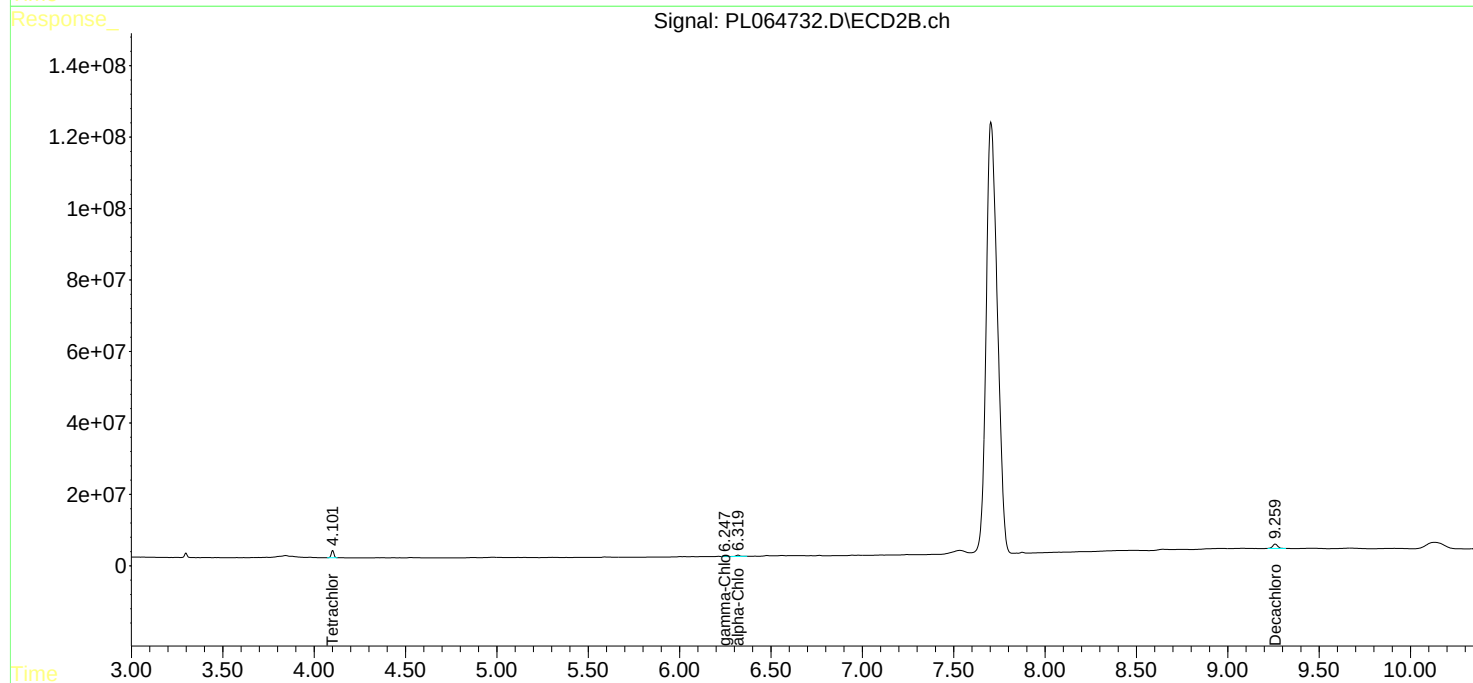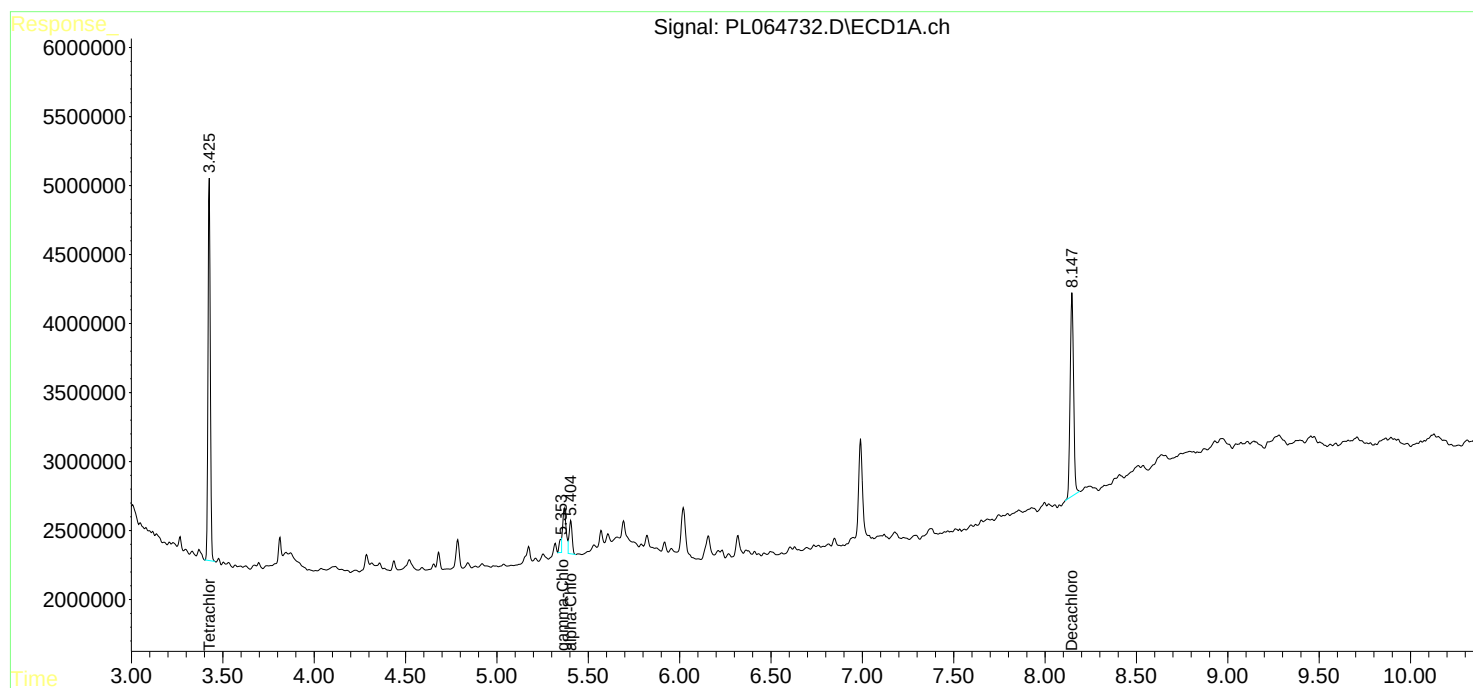

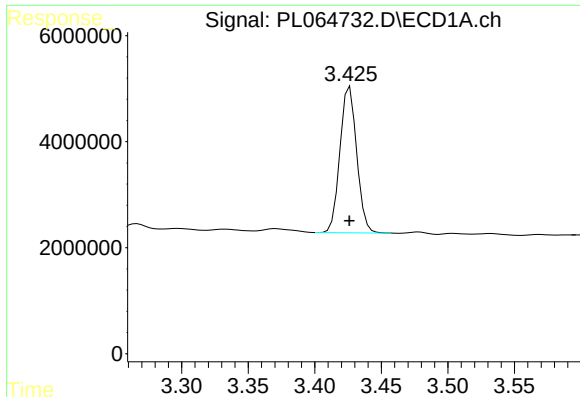


#1 Tetrachloro-m-xylene

R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 24134610
Conc: 8.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
20057


Manual Integrations
APPROVED

Ankita
2/10/2021 1:59:08 PM

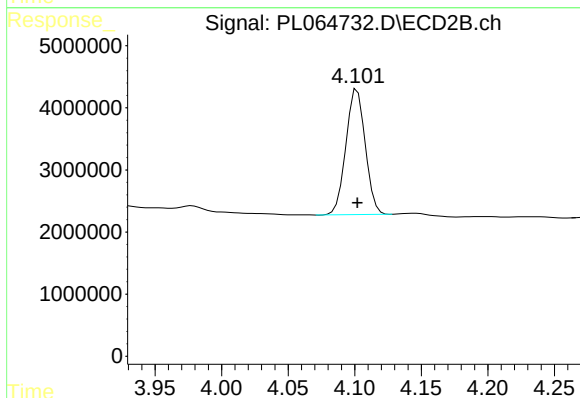


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 20465741
Conc: 9.47 ng/ml

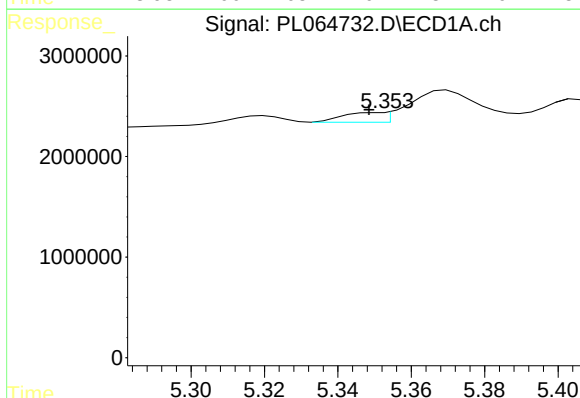


#10 gamma-Chlordane

R.T.: 5.353 min
Delta R.T.: 0.004 min
Response: 844057
Conc: 0.24 ng/ml m

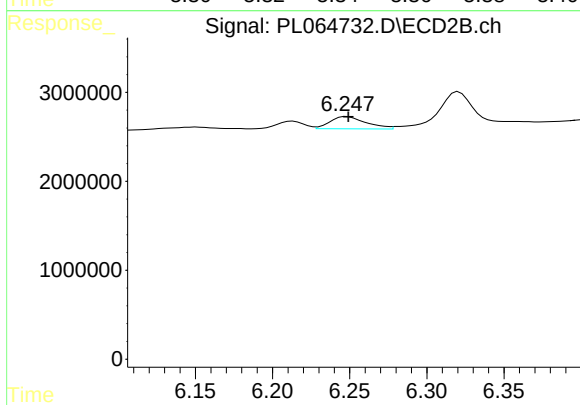

#10 gamma-Chlordane

R.T.: 6.247 min
Delta R.T.: -0.002 min
Response: 2230508
Conc: 0.97 ng/ml m

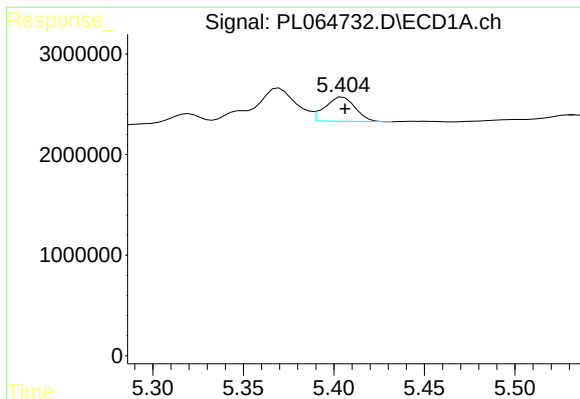


#11 alpha-Chlordane

R.T.: 5.405 min
Delta R.T.: -0.001 min
Response: 2807717
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
20057


Manual Integrations
APPROVED

Ankita
2/10/2021 1:59:08 PM

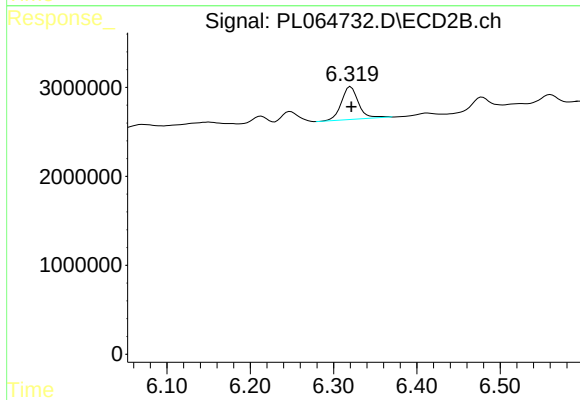


#11 alpha-Chlordane

R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 5196425
Conc: 2.26 ng/ml

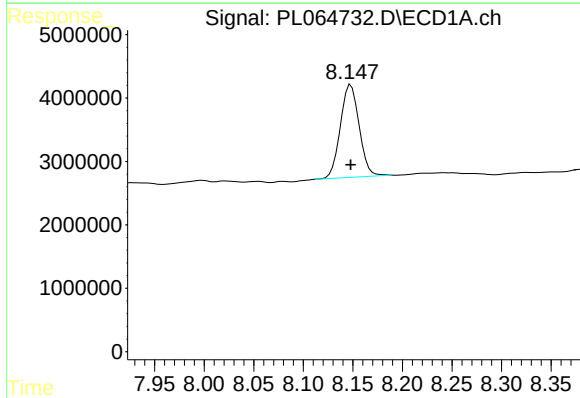

#28 Decachlorobiphenyl

R.T.: 8.148 min
Delta R.T.: 0.000 min
Response: 19369248
Conc: 8.61 ng/ml

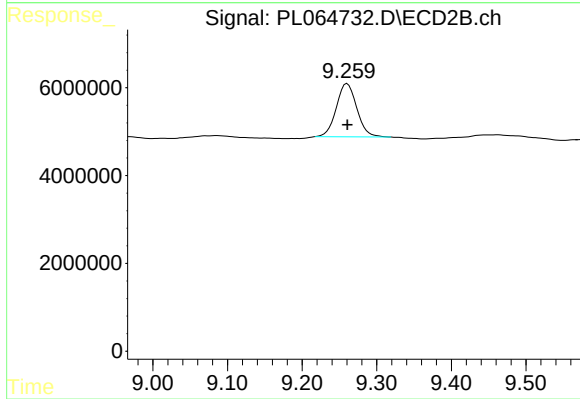

#28 Decachlorobiphenyl

R.T.: 9.260 min
Delta R.T.: 0.000 min
Response: 23144406
Conc: 12.19 ng/ml