

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
 Data File : PL064741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2021 02:20
 Operator : AR\AJ
 Sample : M1317-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 R-A

Manual Integrations
 APPROVED

Ankita
 2/11/2021 9:17:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 04:40:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.103	32875364	29745495	11.685	13.770
28)	SA Decachlor...	8.147	9.258	38105892	35176971	16.945	18.520
Target Compounds							
16)	A 4,4'-DDD	6.086	6.976	6118663	11644202	2.416m	6.717m#
17)	MA 4,4'-DDT	6.320	7.273	7677050	4500432	3.404	2.952m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
Data File : PL064741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2021 02:20
Operator : AR\AJ
Sample : M1317-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
R-A


Manual Integrations
APPROVED

Ankita
2/11/2021 9:17:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 04:40:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

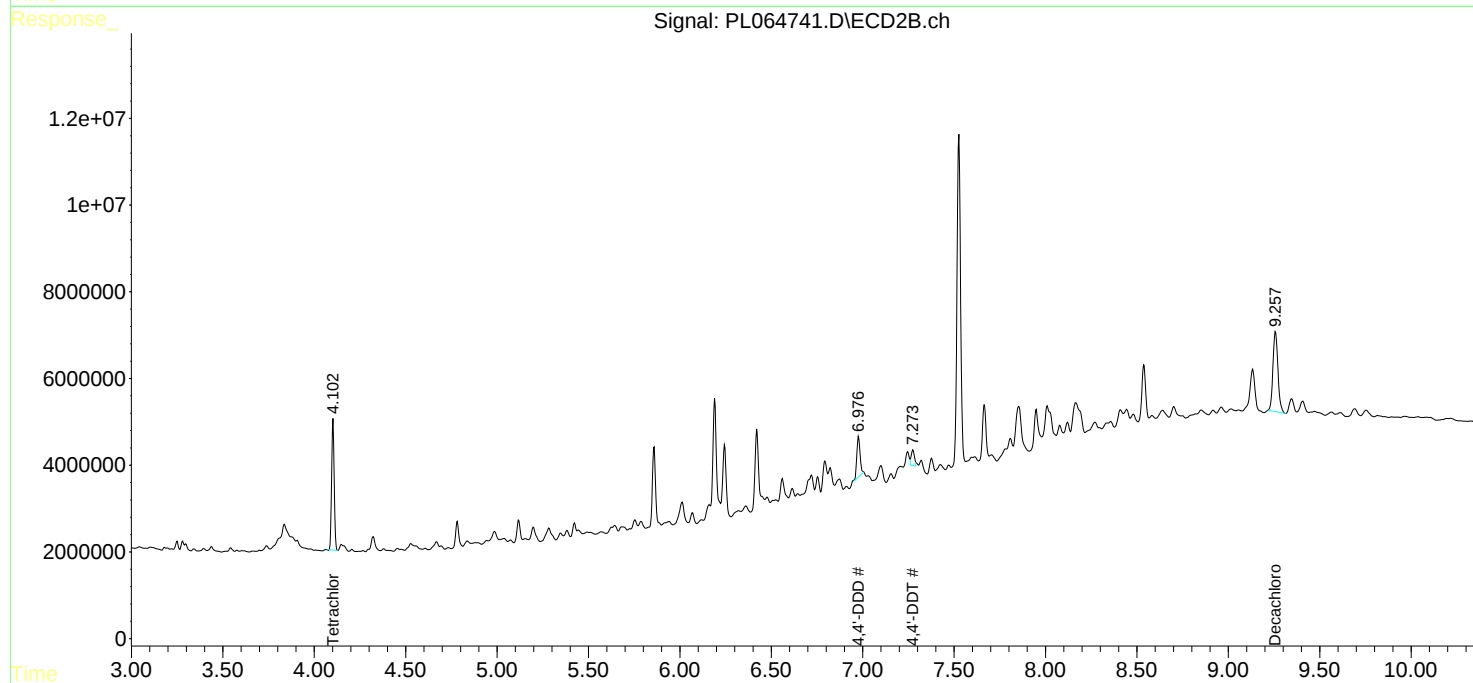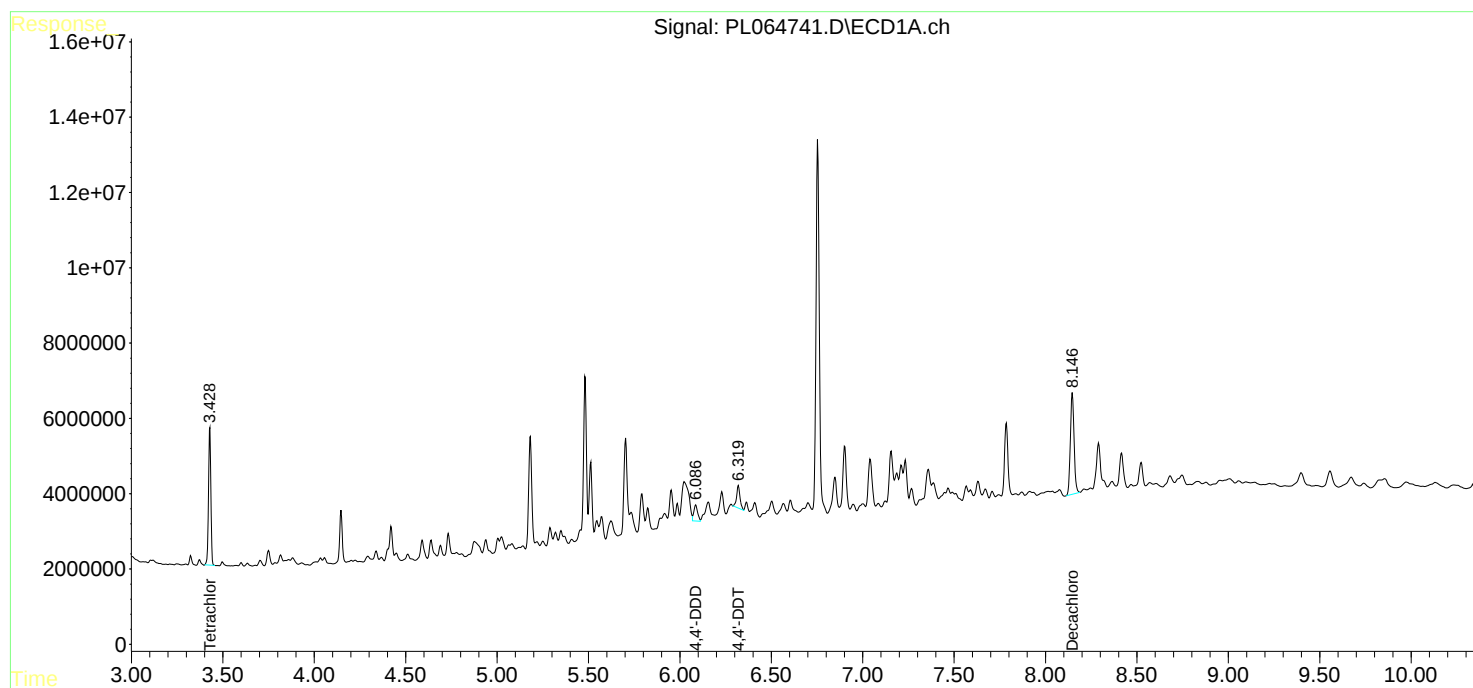

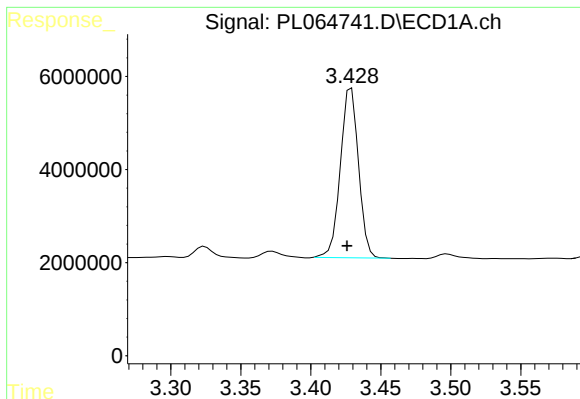


#1 Tetrachloro-m-xylene

R.T.: 3.429 min
Delta R.T.: 0.003 min
Response: 32875364
Conc: 11.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
R-A


Manual Integrations
APPROVED

Ankita
2/11/2021 9:17:00 AM

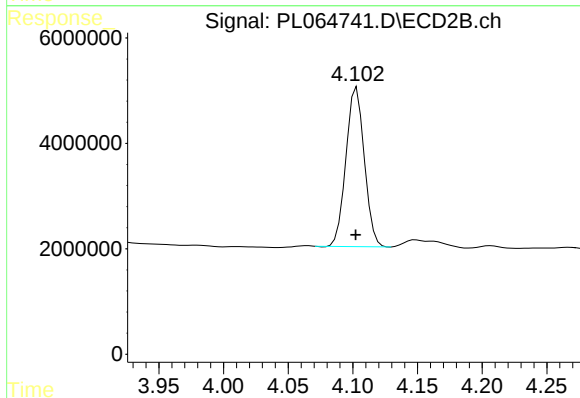


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 29745495
Conc: 13.77 ng/ml

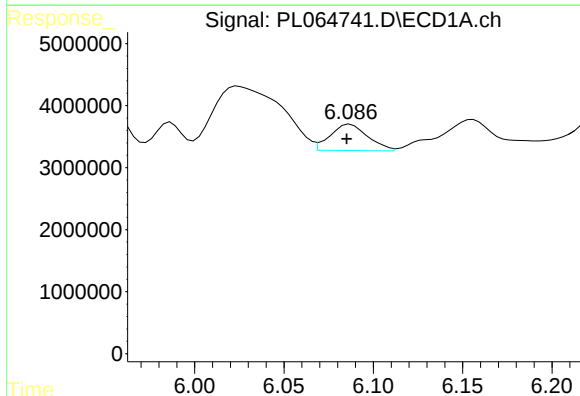


#16 4,4'-DDD

R.T.: 6.086 min
Delta R.T.: 0.000 min
Response: 6118663
Conc: 2.42 ng/ml m

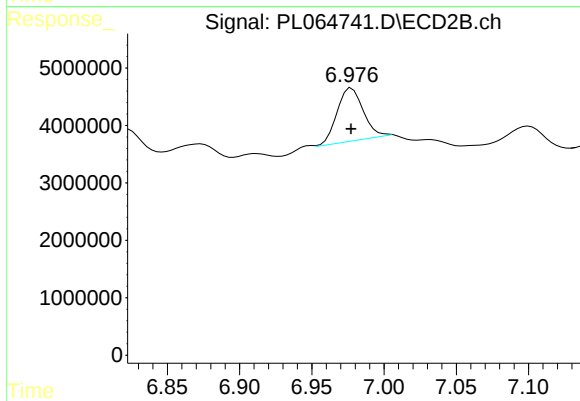

#16 4,4'-DDD

R.T.: 6.976 min
Delta R.T.: -0.001 min
Response: 11644202
Conc: 6.72 ng/ml m

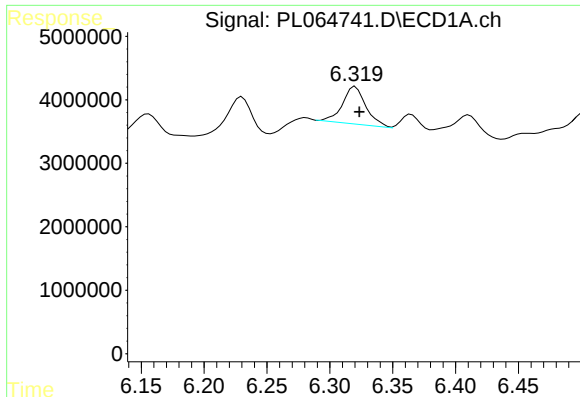


#17 4,4'-DDT

R.T.: 6.320 min
Delta R.T.: -0.003 min
Response: 7677050
Conc: 3.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
R-A


Manual Integrations
APPROVED

Ankita
2/11/2021 9:17:00 AM

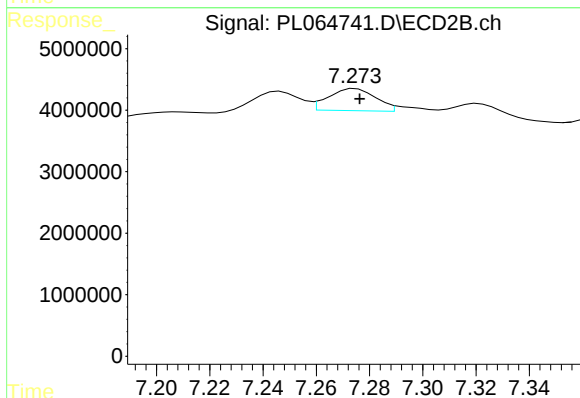


#17 4,4'-DDT

R.T.: 7.273 min
Delta R.T.: -0.003 min
Response: 4500432
Conc: 2.95 ng/ml m

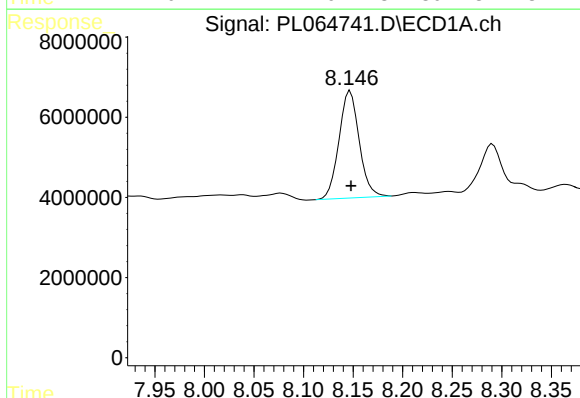

#28 Decachlorobiphenyl

R.T.: 8.147 min
Delta R.T.: 0.000 min
Response: 38105892
Conc: 16.94 ng/ml

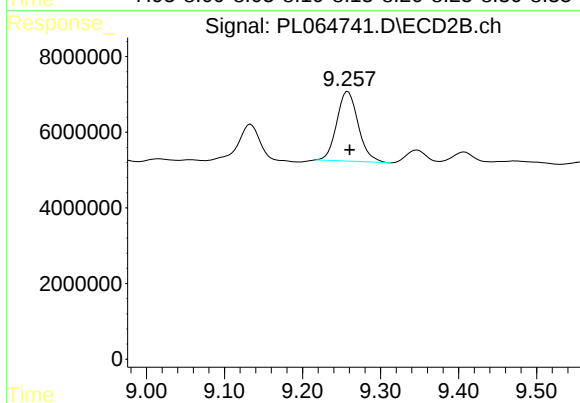

#28 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.002 min
Response: 35176971
Conc: 18.52 ng/ml