

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021020\
 Data File : PL056439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2020 15:10
 Operator : AJ\MA
 Sample : L1446-04DL 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-640-XDL

Manual Integrations
 APPROVED

mohammad
 2/11/2020 3:21:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 15:33:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.499	4.016	48531005	7050445	4.634	2.411 #
28)	SA Decachlor...	8.252	9.090	11696861	3705686	1.111	1.638m#
Target Compounds							
15)	B Endosulfa...	6.332	6.948	1385.5E6	180.2E6	105.935m	66.940m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021020\
Data File : PL056439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2020 15:10
Operator : AJ\MA
Sample : L1446-04DL 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-640-XDL


Manual Integrations
APPROVED

mohammad
2/11/2020 3:21:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 15:33:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

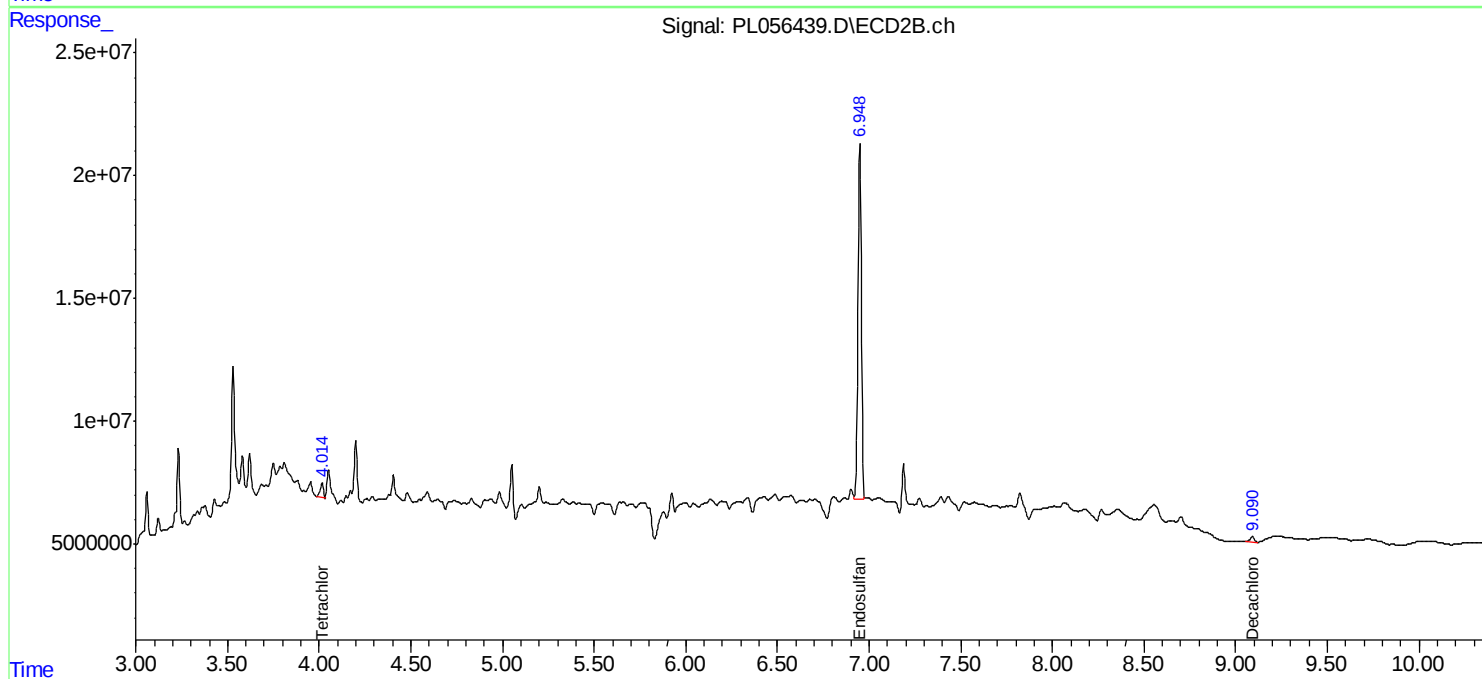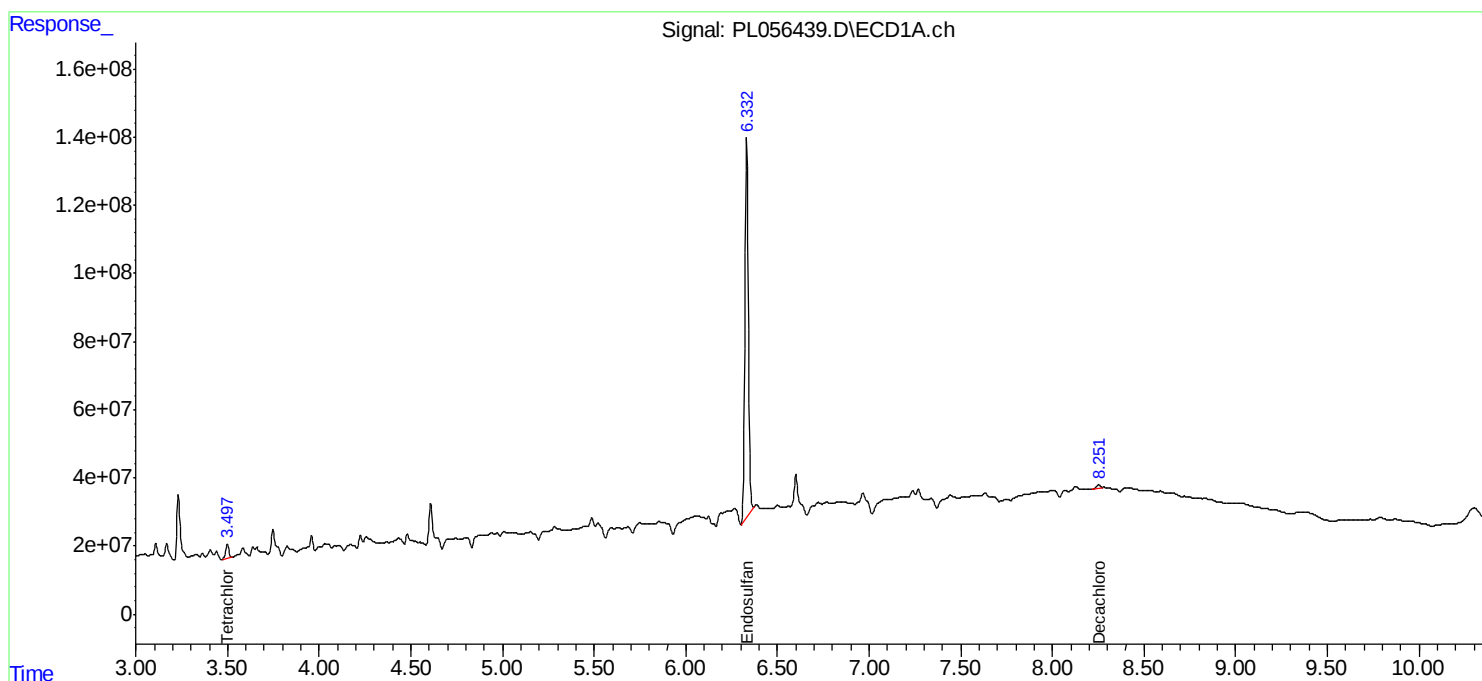

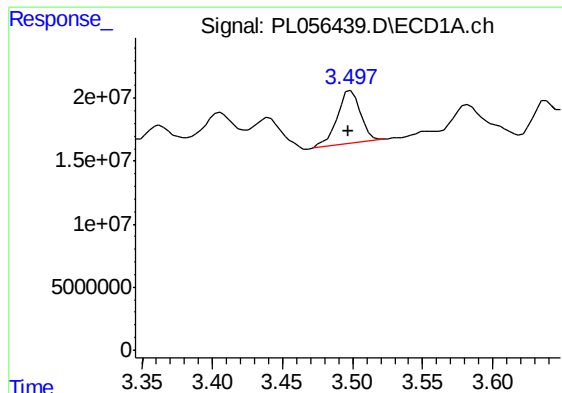


#1 Tetrachloro-m-xylene

R.T.: 3.499 min
Delta R.T.: 0.002 min
Response: 48531005
Conc: 4.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-640-XDL


Manual Integrations
APPROVED

mohammad
2/11/2020 3:21:45 PM

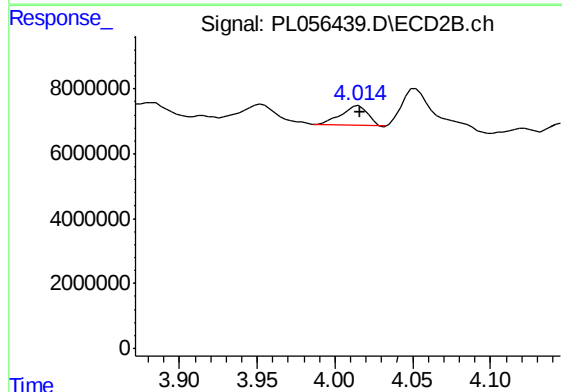


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 7050445
Conc: 2.41 ng/ml

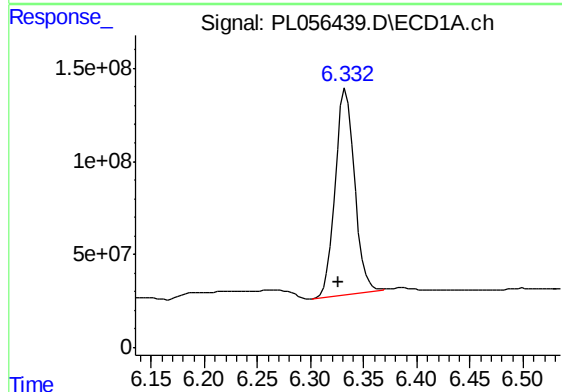


#15 Endosulfan II

R.T.: 6.332 min
Delta R.T.: 0.005 min
Response: 1385459787
Conc: 105.93 ng/ml m

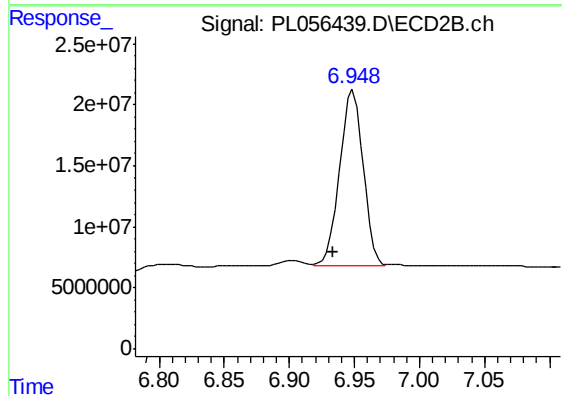

#15 Endosulfan II

R.T.: 6.948 min
Delta R.T.: 0.014 min
Response: 180209312
Conc: 66.94 ng/ml m

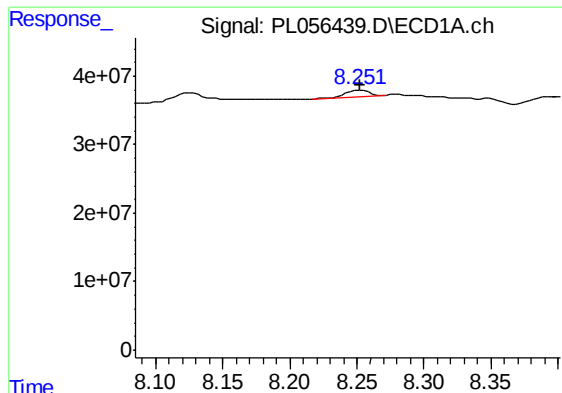


#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 11696861
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-640-XDL

Manual Integrations
APPROVED

mohammad
2/11/2020 3:21:45 PM

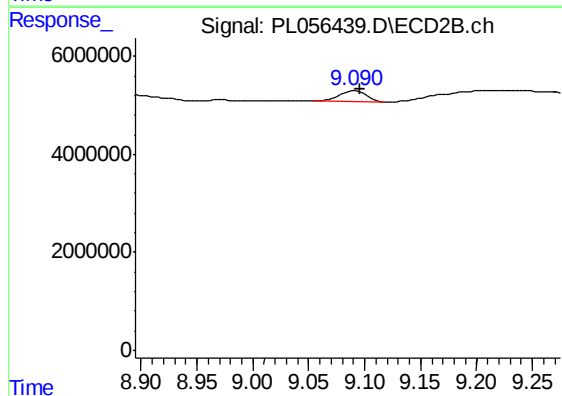

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: -0.006 min
Response: 3705686
Conc: 1.64 ng/ml m