

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021021\
 Data File : PL064758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2021 15:23
 Operator : AR\AJ
 Sample : M1348-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 05:54:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.425	4.100	61171055	49449632	21.742	22.891
28)	SA Decachlor...	8.146	9.257	52569982	42269696	23.377	22.254
Target Compounds							
6)	B beta-BHC	4.393	4.966	4715556	6898105	2.759	1.653 #
12)	B 4,4'-DDE	5.594f	0.000	1939431	0	0.620	N.D. #
13)	MA Dieldrin	5.719f	0.000	5556001	0	1.694	N.D. #
19)	B Endosulfa...	6.622	0.000	3994054	0	1.408	N.D. #
23)	Chlordane-1	4.313f	0.000	5544719	0	48.776	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021021\
Data File : PL064758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2021 15:23
Operator : AR\AJ
Sample : M1348-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 05:54:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

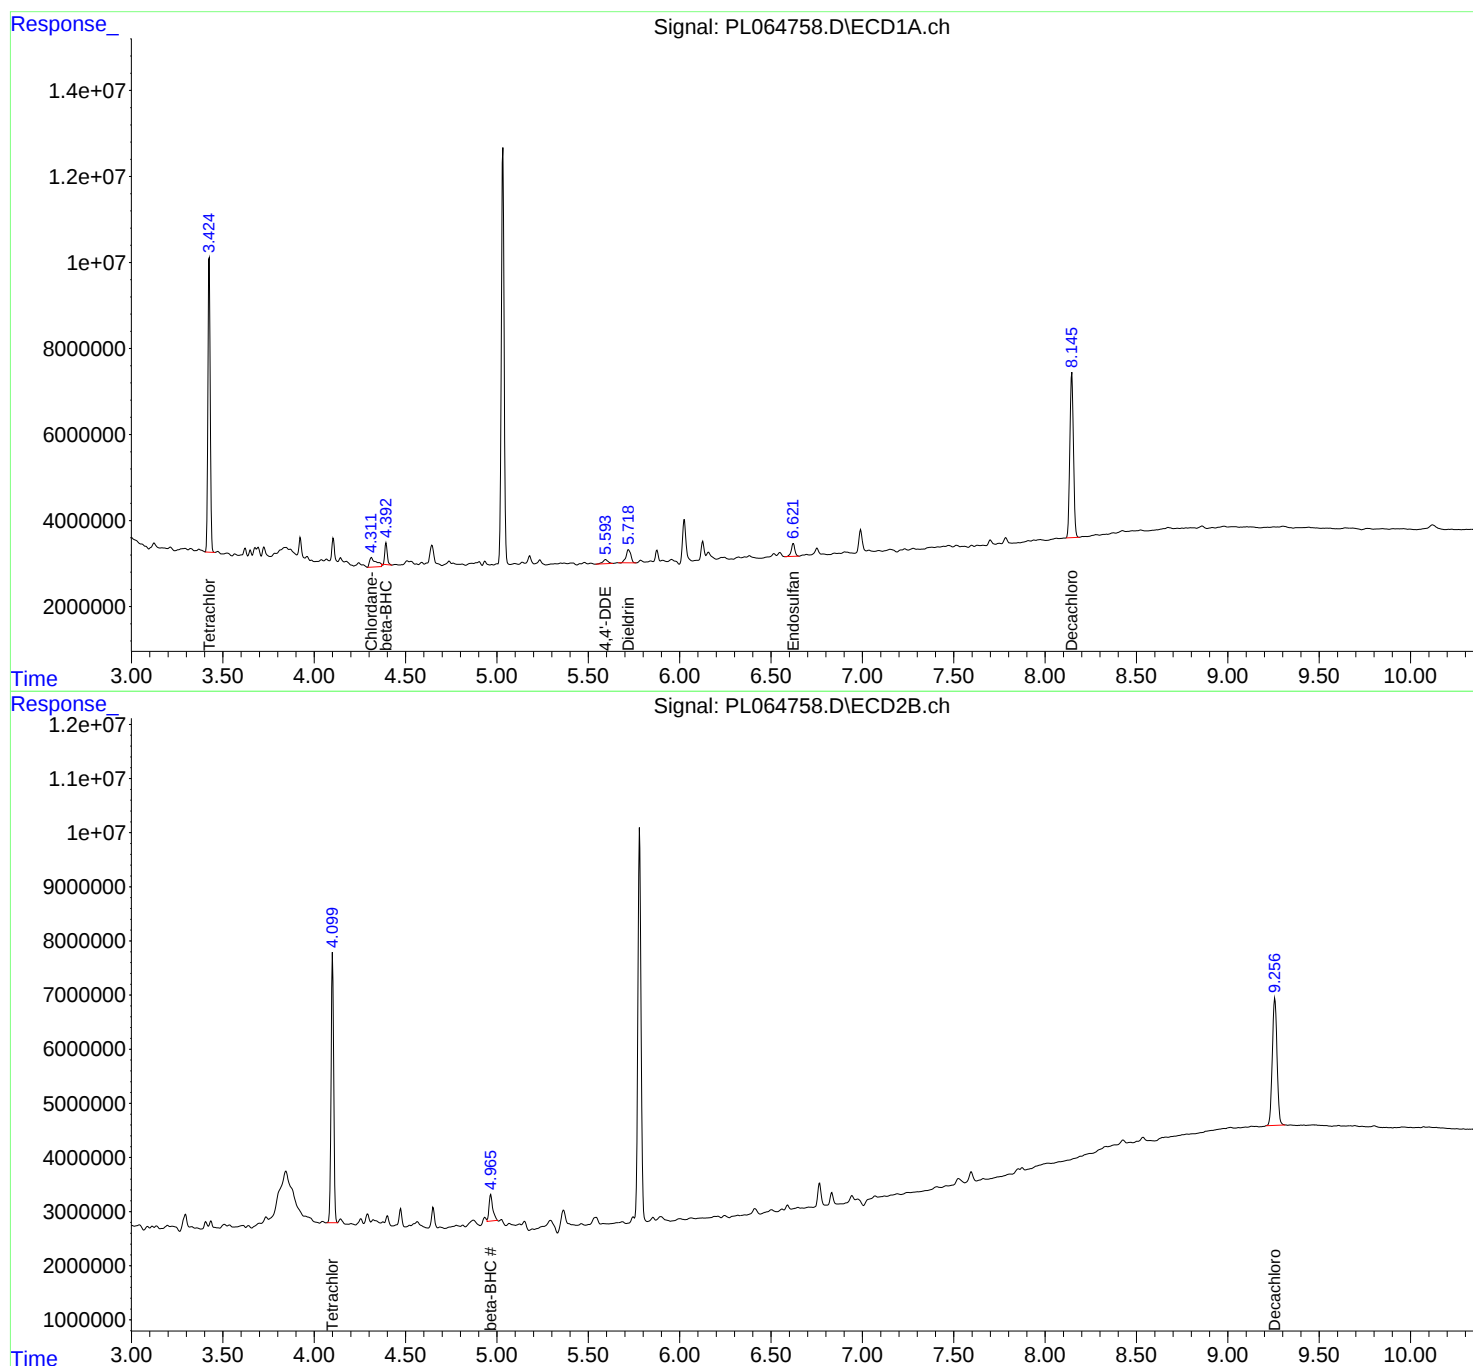


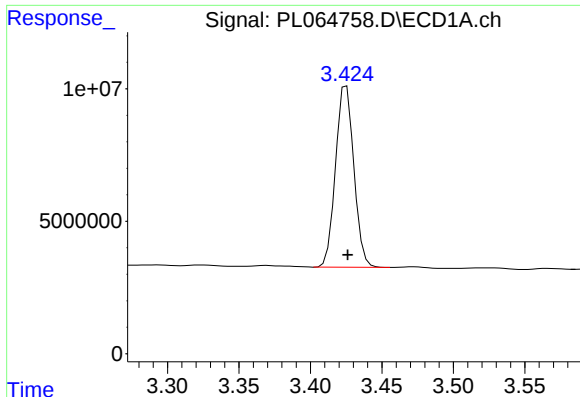

#1 Tetrachloro-m-xylene


R.T.: 3.425 min
Delta R.T.: 0.000 min
Response: 61171055
Conc: 21.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

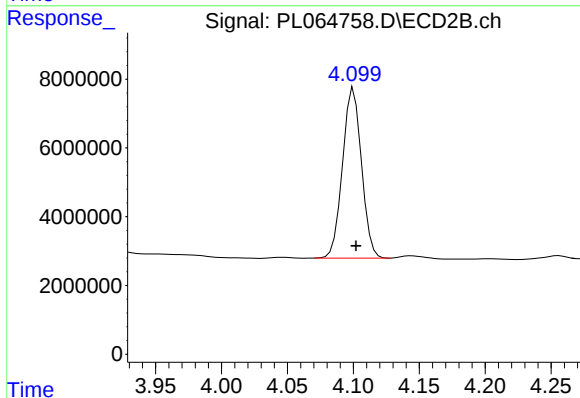


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.002 min
Response: 49449632
Conc: 22.89 ng/ml

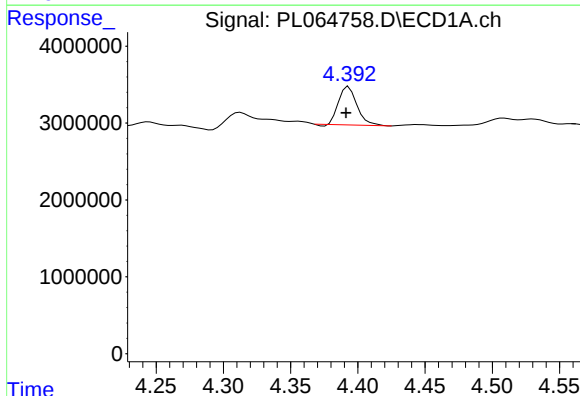


#6 beta-BHC

R.T.: 4.393 min
Delta R.T.: 0.002 min
Response: 4715556
Conc: 2.76 ng/ml

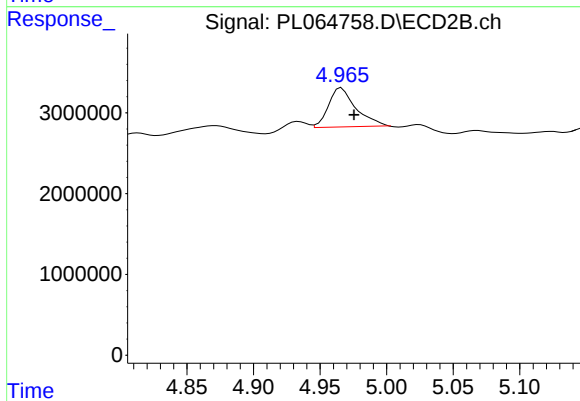

#6 beta-BHC


R.T.: 4.966 min
Delta R.T.: -0.009 min
Response: 6898105
Conc: 1.65 ng/ml

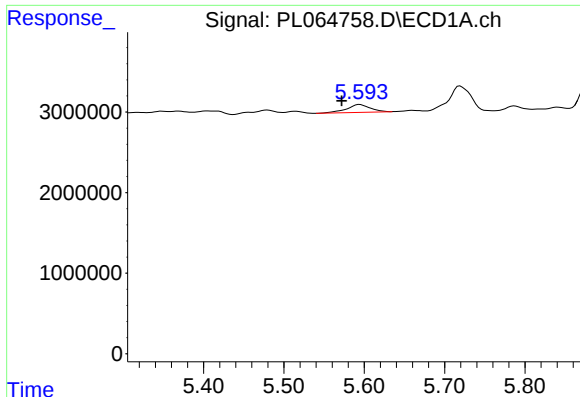

#12 4,4'-DDE


R.T.: 5.594 min
Delta R.T.: 0.022 min
Response: 1939431
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

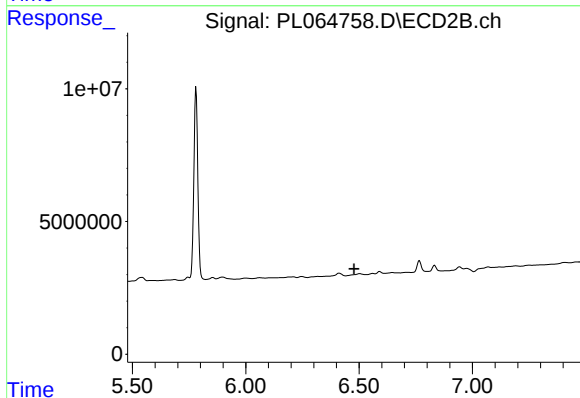


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.478 min
Response: 0
Conc: N.D.

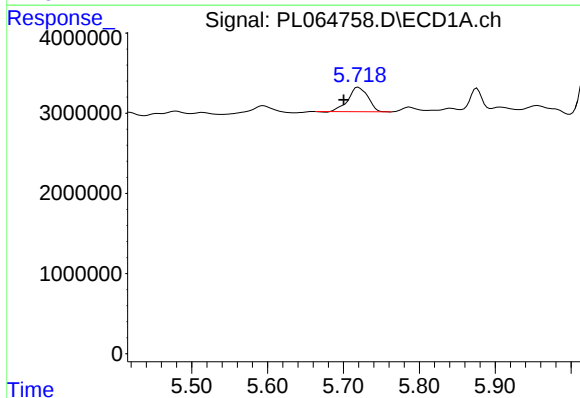


#13 Dieldrin

R.T.: 5.719 min
Delta R.T.: 0.019 min
Response: 5556001
Conc: 1.69 ng/ml

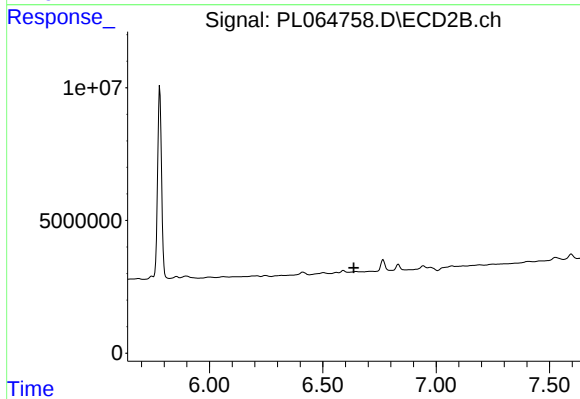

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

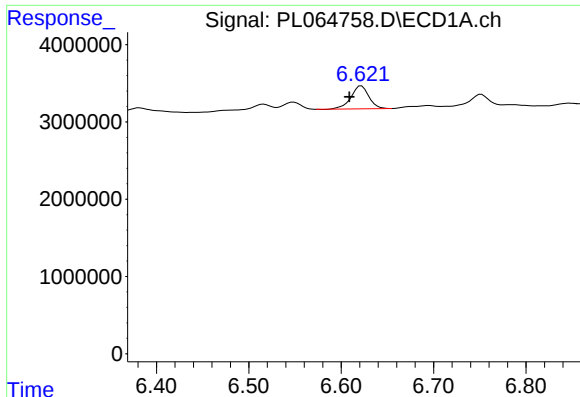

#19 Endosulfan Sulfate


R.T.: 6.622 min
Delta R.T.: 0.013 min
Response: 3994054
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

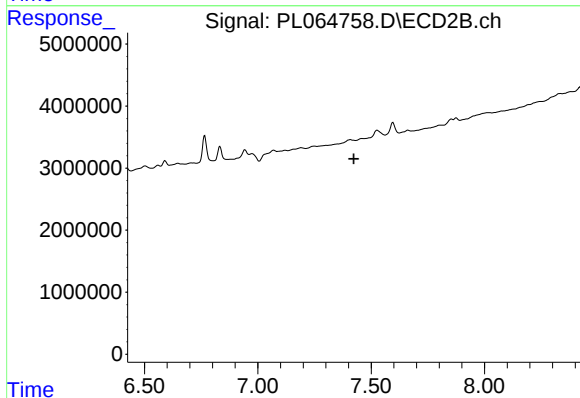


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.424 min
Response: 0
Conc: N.D.

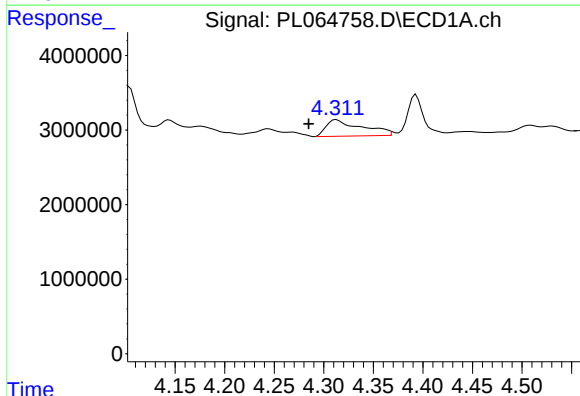


#23 Chlordane-1

R.T.: 4.313 min
Delta R.T.: 0.028 min
Response: 5544719
Conc: 48.78 ng/ml

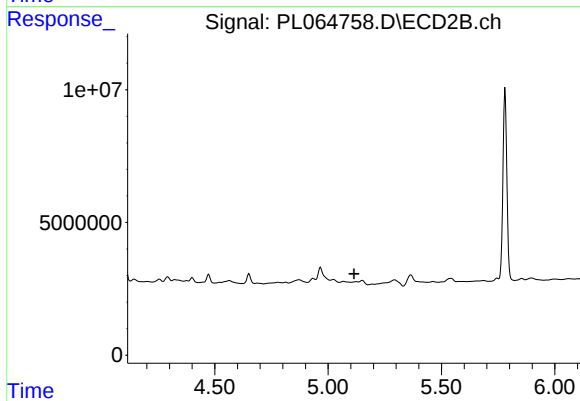

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

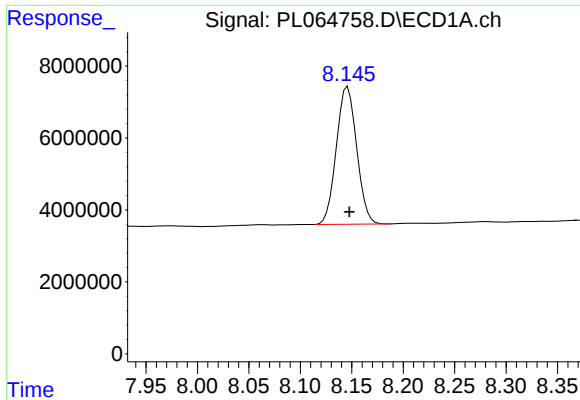

#28 Decachlorobiphenyl

R.T.: 8.146 min
Delta R.T.: -0.002 min
Response: 52569982
Conc: 23.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

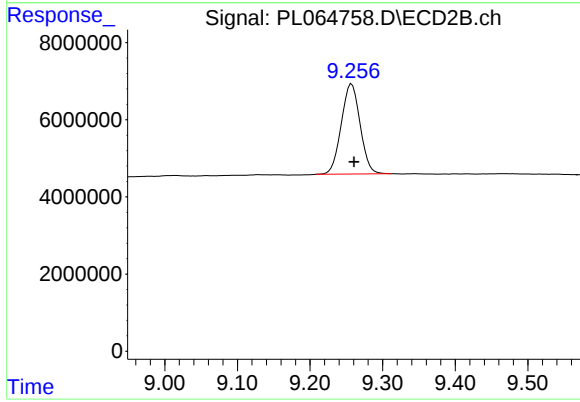

#28 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.003 min
Response: 42269696
Conc: 22.25 ng/ml