

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021023\
 Data File : PL080837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2023 11:28
 Operator : AR\AJ
 Sample : PB150752BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB150752BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/13/2023
 Supervised By : Ankita Jodhani 02/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 21:31:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.687	36823145	35866288	17.168	16.329
2)	SA Decachlor...	8.787	7.833	24625641	29914188	14.066m	12.556

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021023\
Data File : PL080837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2023 11:28
Operator : AR\AJ
Sample : PB150752BL
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB150752BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/13/2023
Supervised By : Ankita Jodhani 02/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 21:31:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

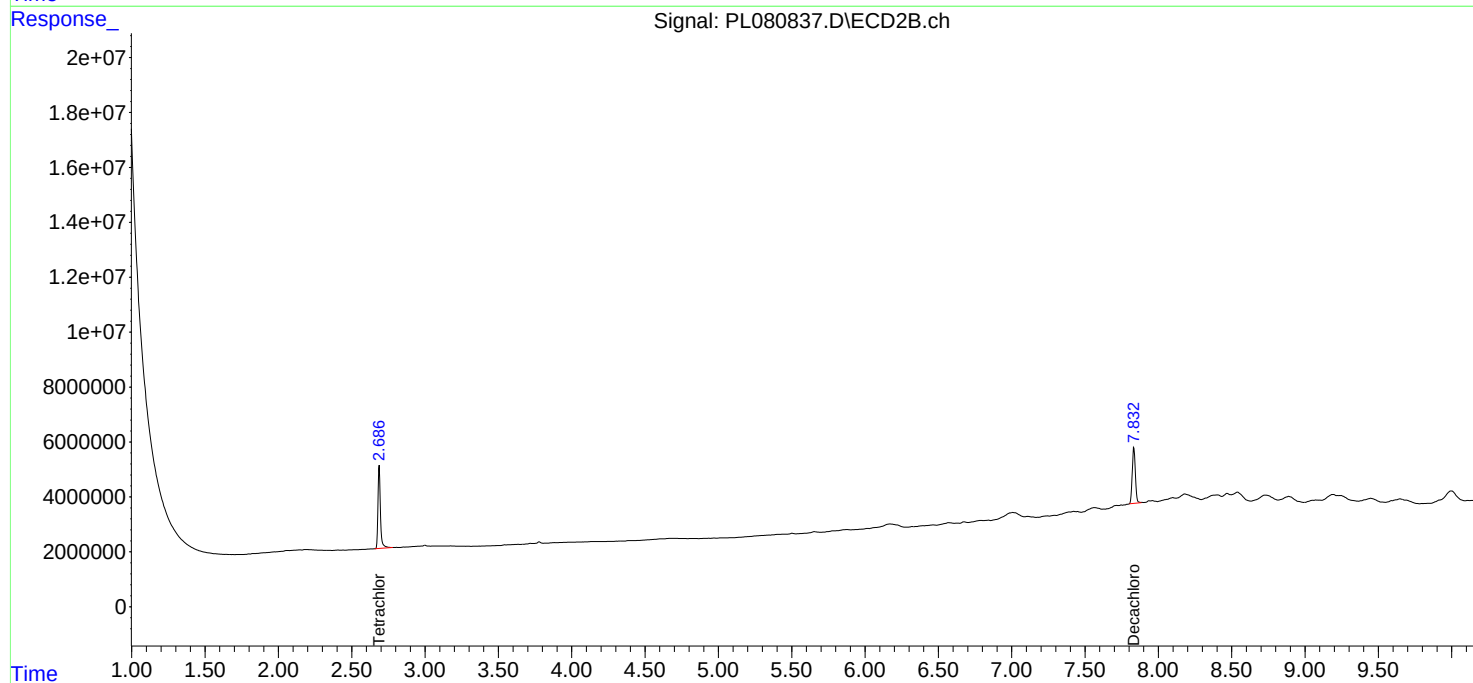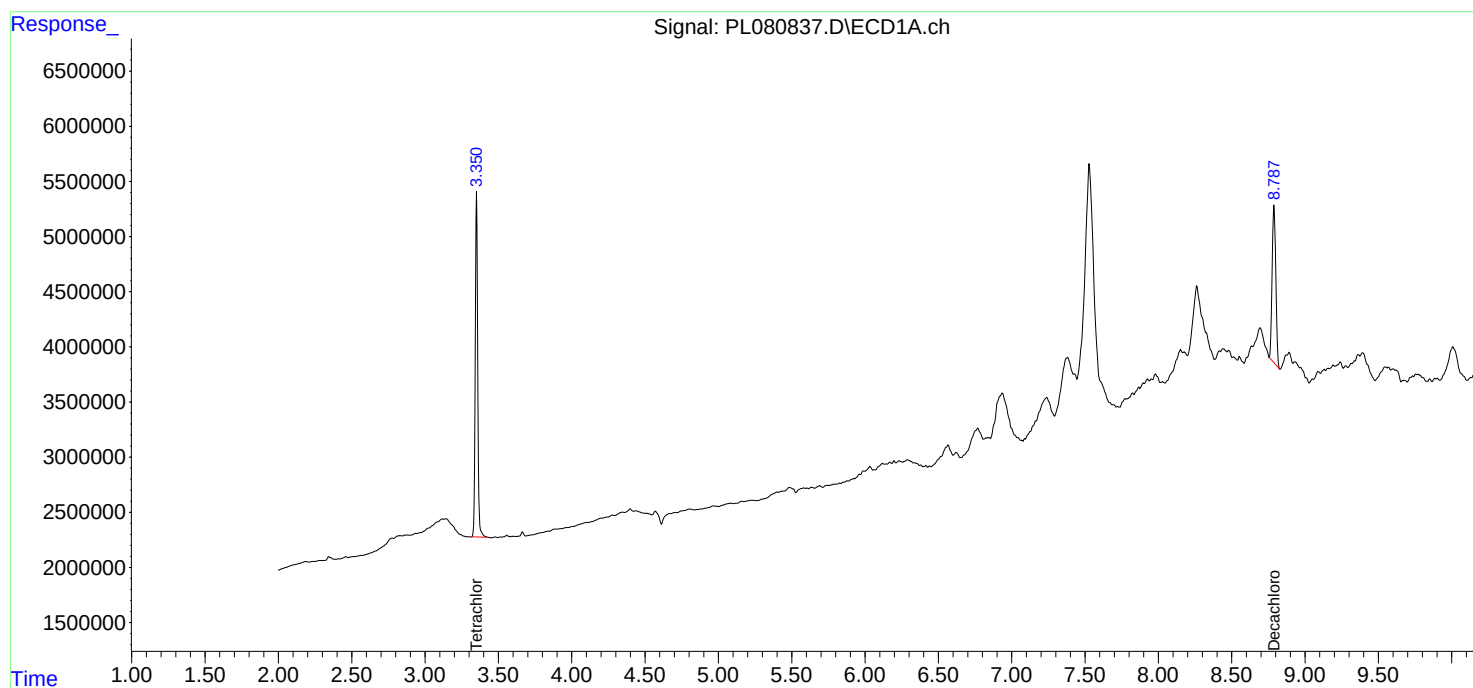

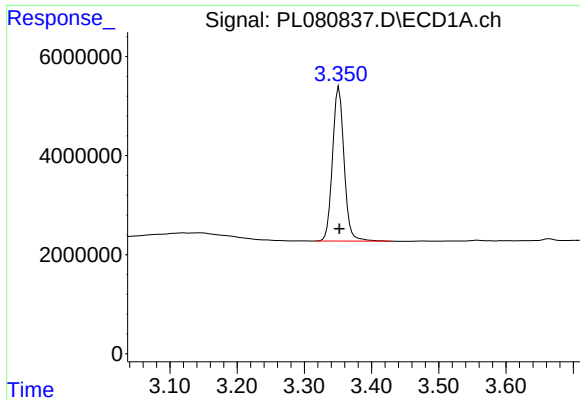


#1 Tetrachloro-m-xylene

R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 36823145
Conc: 17.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB150752BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/13/2023
Supervised By :Ankita Jodhani 02/13/2023

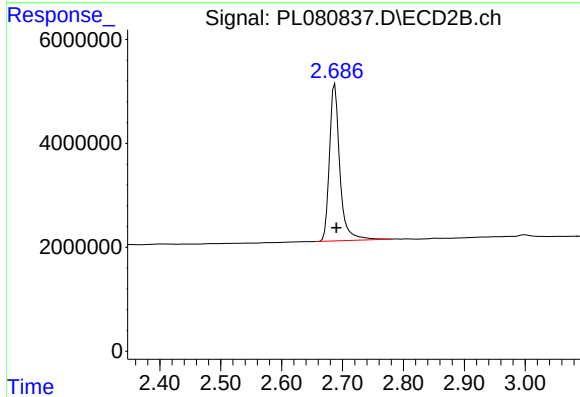


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: -0.002 min
Response: 35866288
Conc: 16.33 ng/ml

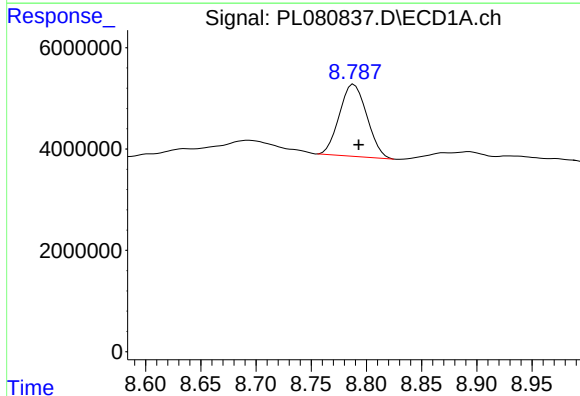

#28 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: -0.006 min
Response: 24625641
Conc: 14.07 ng/ml m

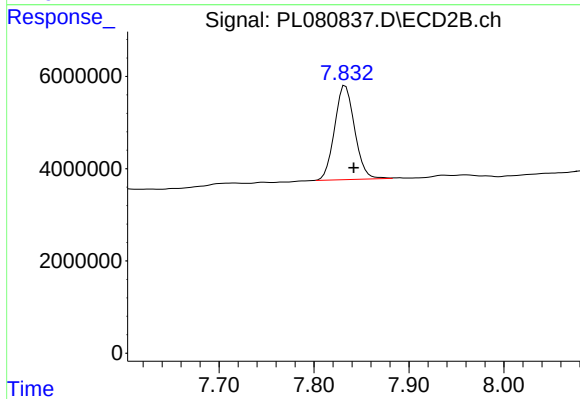

#28 Decachlorobiphenyl

R.T.: 7.833 min
Delta R.T.: -0.009 min
Response: 29914188
Conc: 12.56 ng/ml