

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021023\
 Data File : PL080842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2023 12:37
 Operator : AR\AJ
 Sample : 01508-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RS-2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/13/2023
 Supervised By : Ankita Jodhani 02/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 21:43:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.350	2.688	36954990	37626639	17.230m	17.131
28) SA Decachlor...	8.788	7.833	27189971	28555954	15.530	11.986

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021023\
Data File : PL080842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2023 12:37
Operator : AR\AJ
Sample : 01508-06
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RS-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/13/2023
Supervised By : Ankita Jodhani 02/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 21:43:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

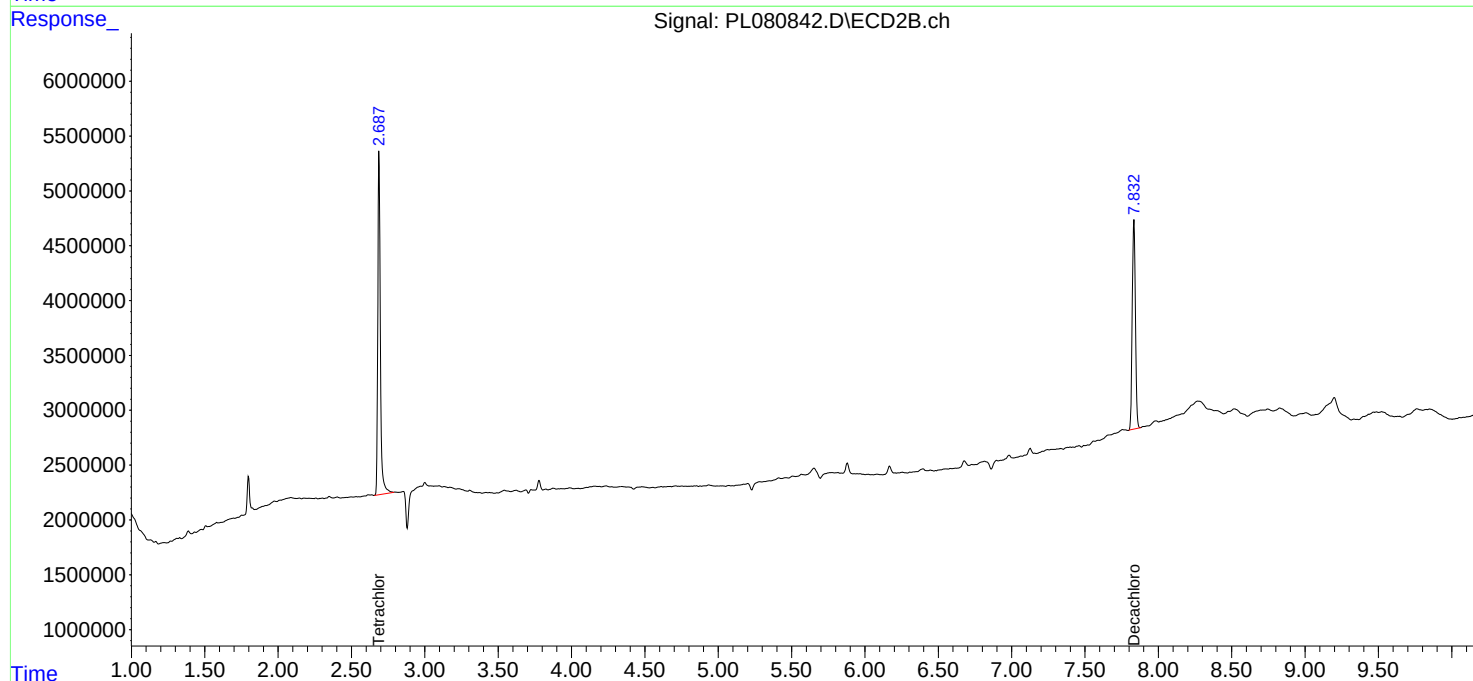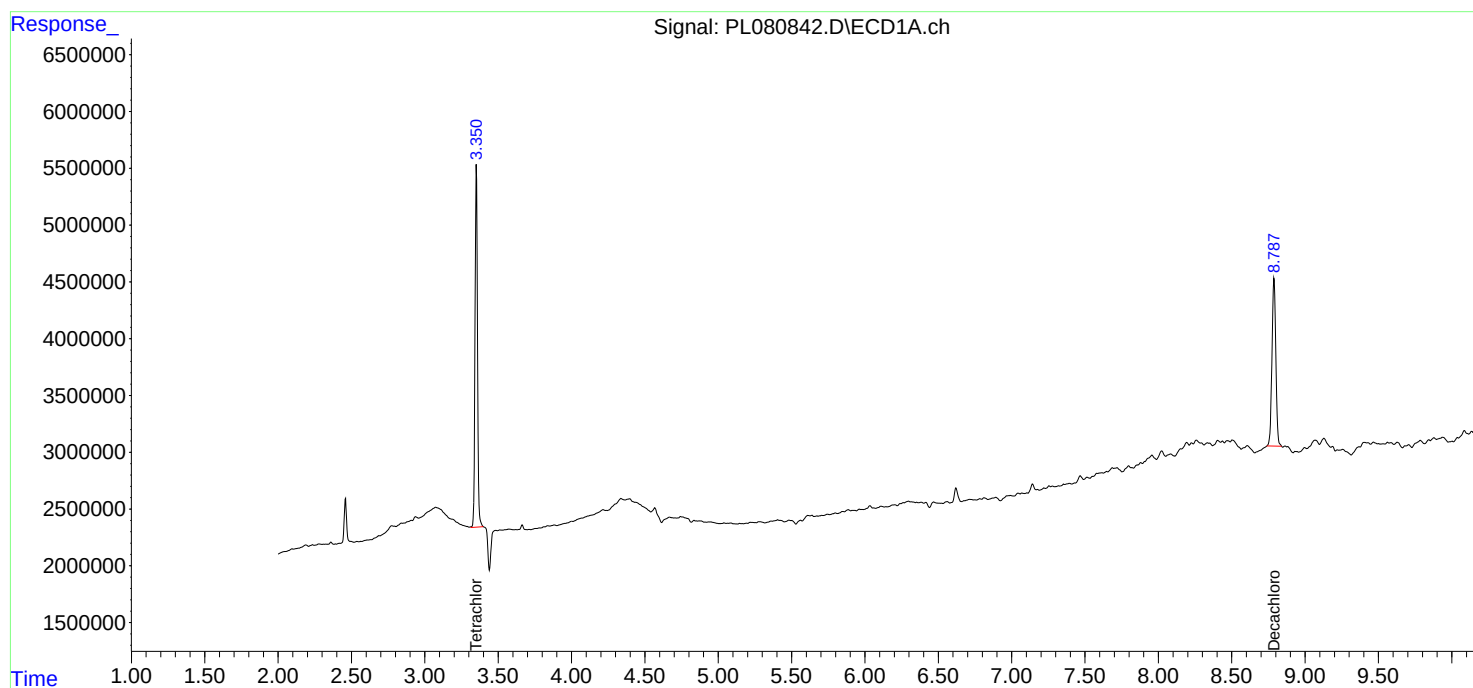

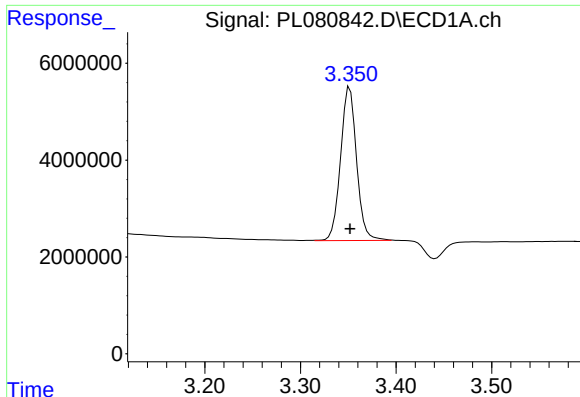


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.002 min
Response: 36954990
Conc: 17.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
RS-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/13/2023
Supervised By :Ankita Jodhani 02/13/2023

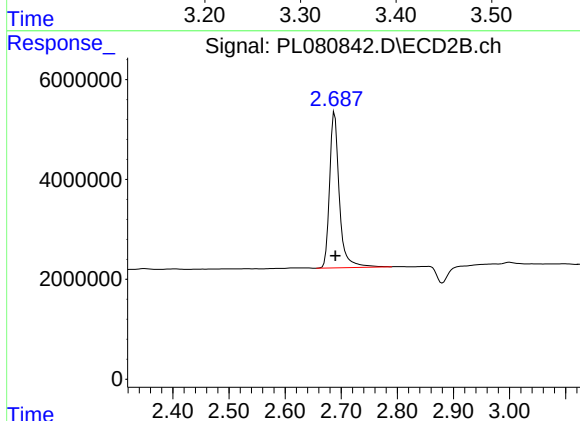


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: -0.001 min
Response: 37626639
Conc: 17.13 ng/ml

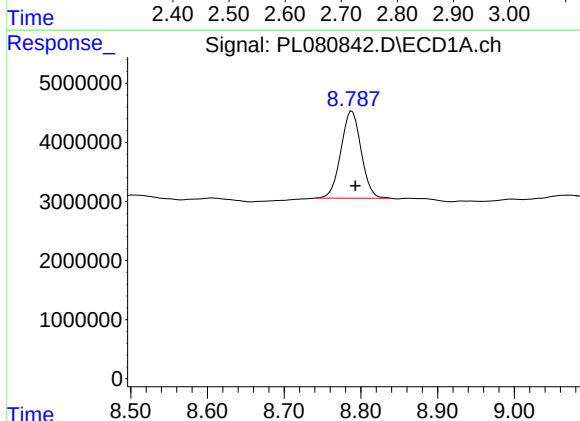

#28 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: -0.005 min
Response: 27189971
Conc: 15.53 ng/ml

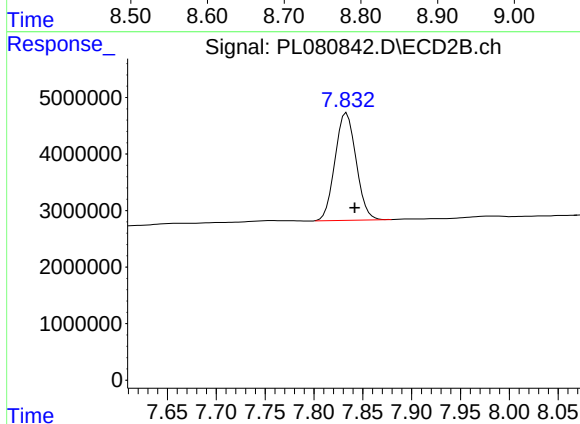

#28 Decachlorobiphenyl

R.T.: 7.833 min
Delta R.T.: -0.008 min
Response: 28555954
Conc: 11.99 ng/ml