

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021119\
 Data File : PL044628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2019 17:48
 Operator : AJ\SJ
 Sample : K1453-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 M-8-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 22:00:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.365	3.984	122.7E6	39415837	17.240	16.778
28) SA Decachlor...	8.048	9.042	108.7E6	39822303	14.910	17.980
Target Compounds						
15) B Endosulfa...	0.000	6.904	0	2415771	N.D.	1.049 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021119\
Data File : PL044628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2019 17:48
Operator : AJ\SJ
Sample : K1453-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
M-8-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 22:00:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

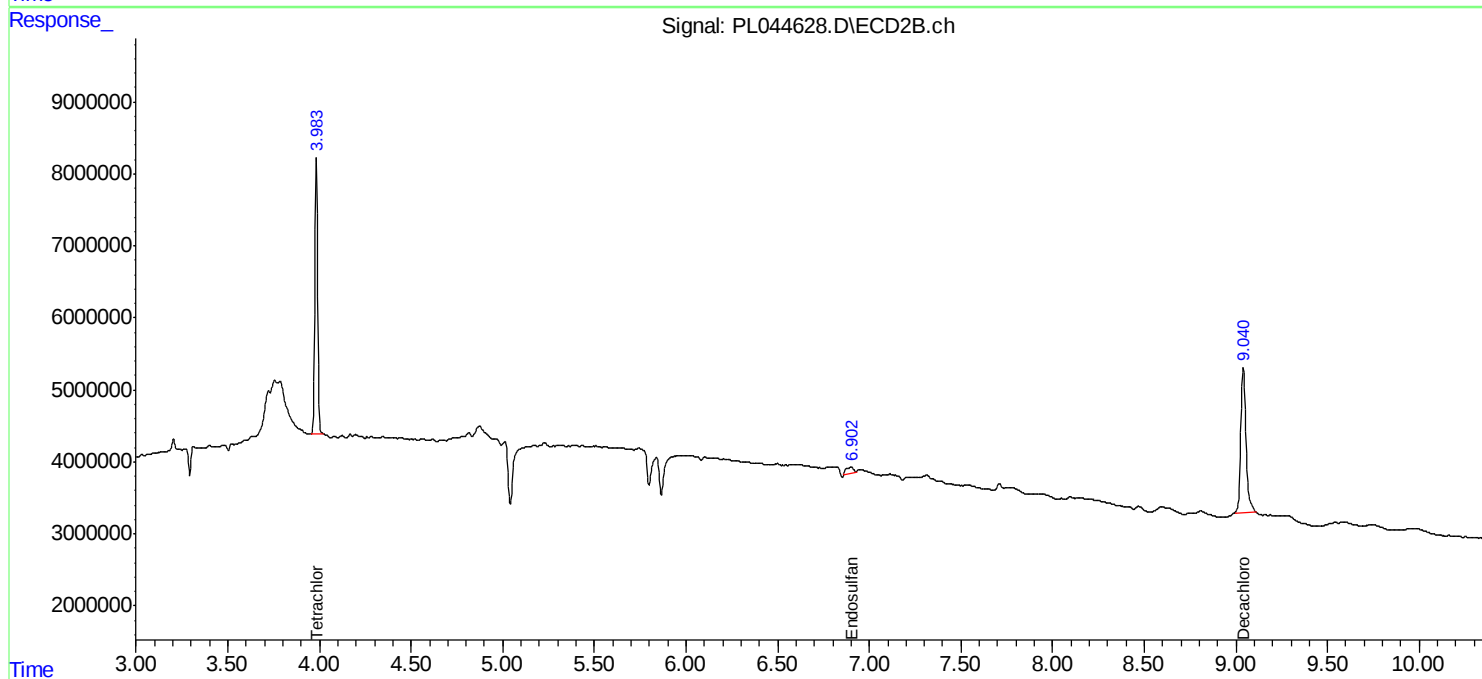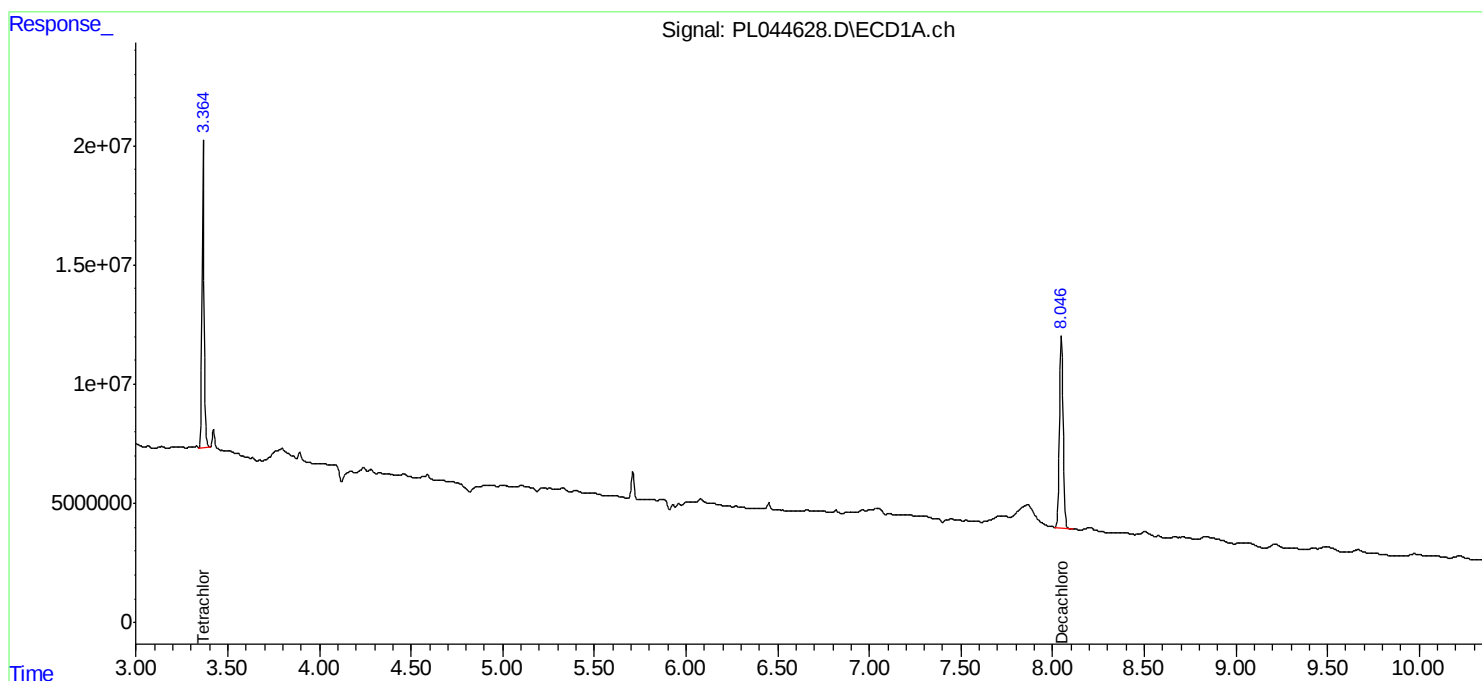


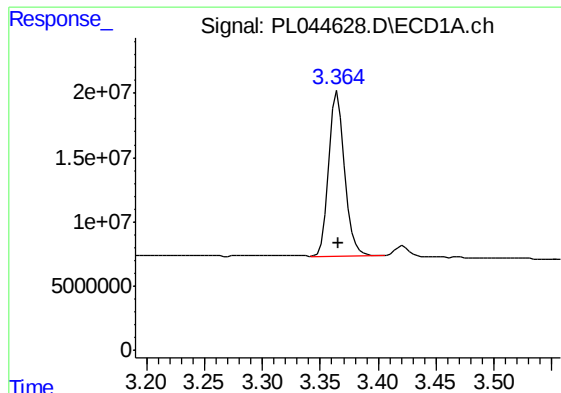

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 122675763
Conc: 17.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-8-S

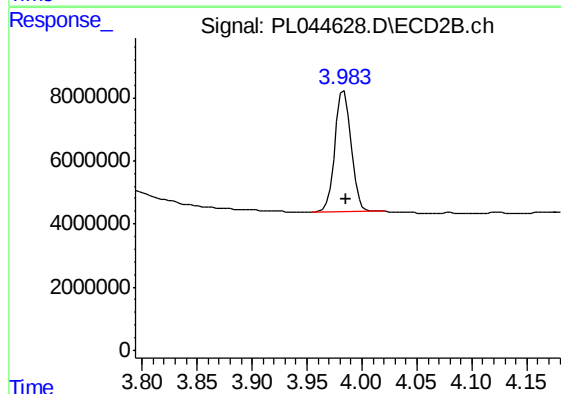


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 39415837
Conc: 16.78 ng/ml

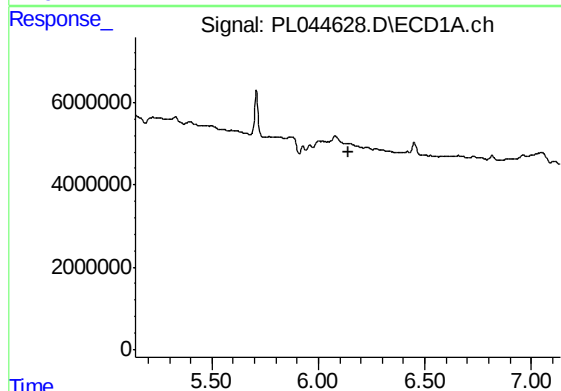


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.139 min
Response: 0
Conc: N.D.

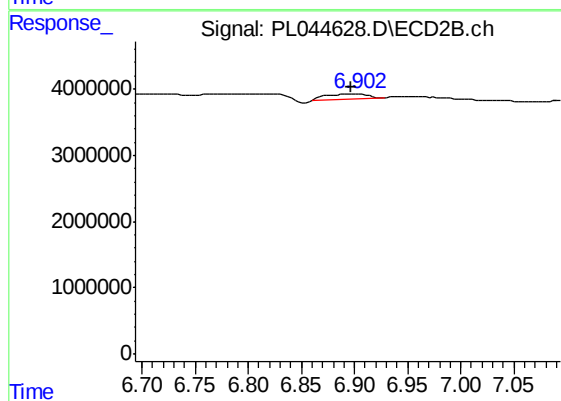

#15 Endosulfan II


R.T.: 6.904 min
Delta R.T.: 0.007 min
Response: 2415771
Conc: 1.05 ng/ml

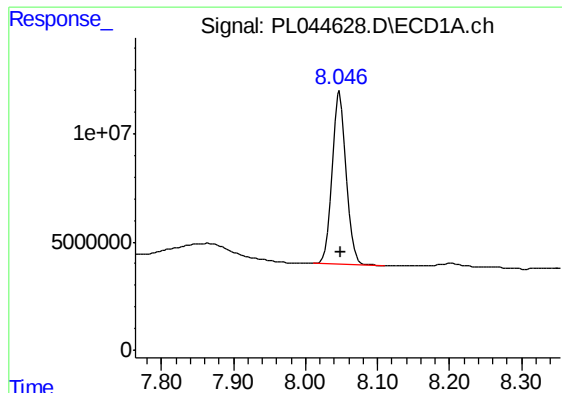

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: -0.001 min
Response: 108749175
Conc: 14.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-8-S

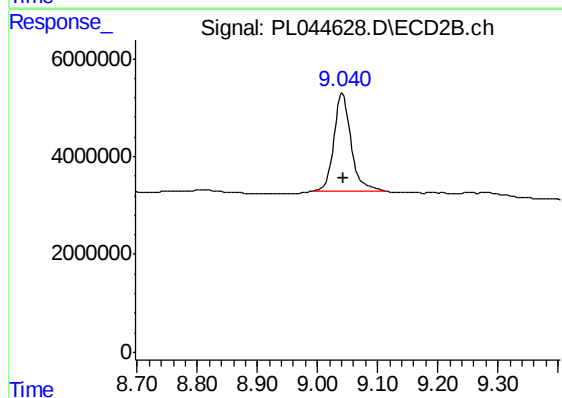

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: -0.001 min
Response: 39822303
Conc: 17.98 ng/ml