

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021119\
 Data File : PL044626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2019 17:20
 Operator : AJ\SJ
 Sample : K1450-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HOSPITAL-BOX-CULVERT-TP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 21:59:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.984	138.9E6	41283299	19.525	17.573
28)	SA Decachlor...	8.048	9.041	144.1E6	42399287	19.761	19.143

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021119\
Data File : PL044626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2019 17:20
Operator : AJ\SJ
Sample : K1450-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HOSPITAL-BOX-CULVERT-TP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 21:59:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

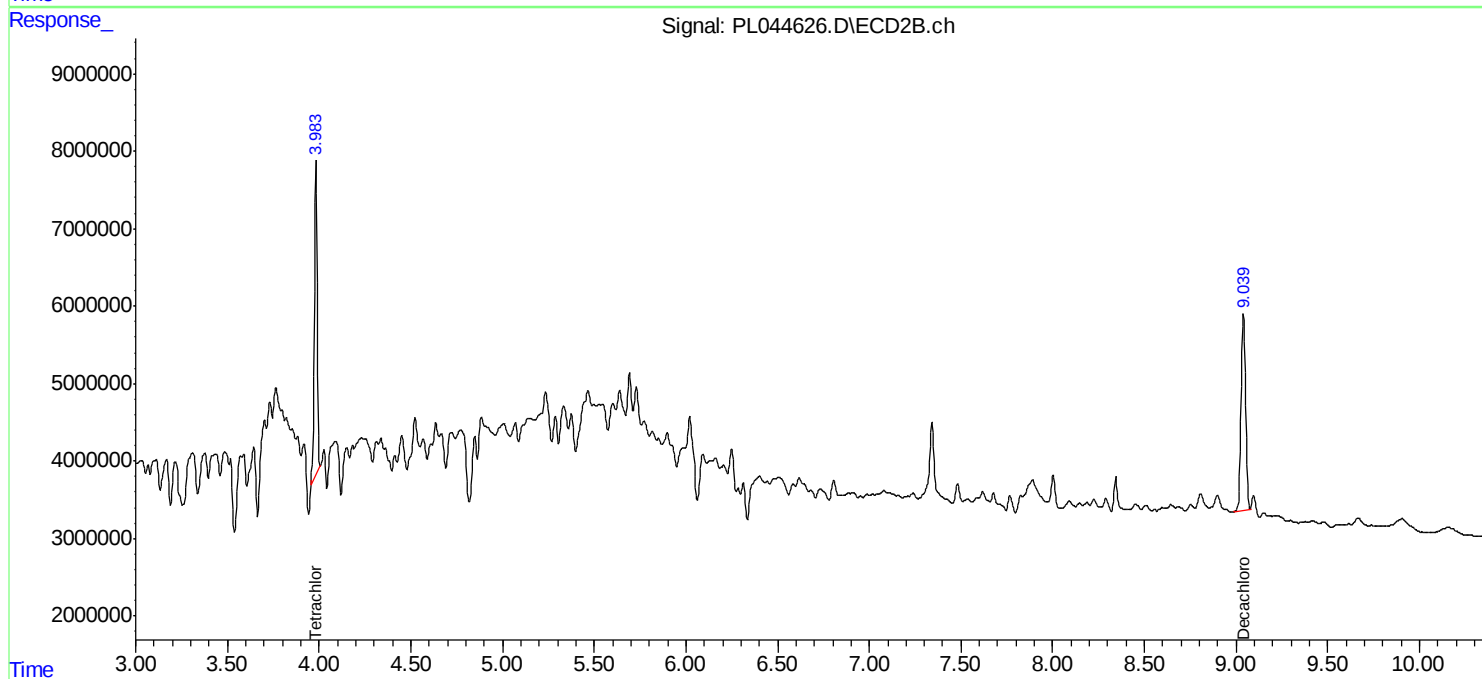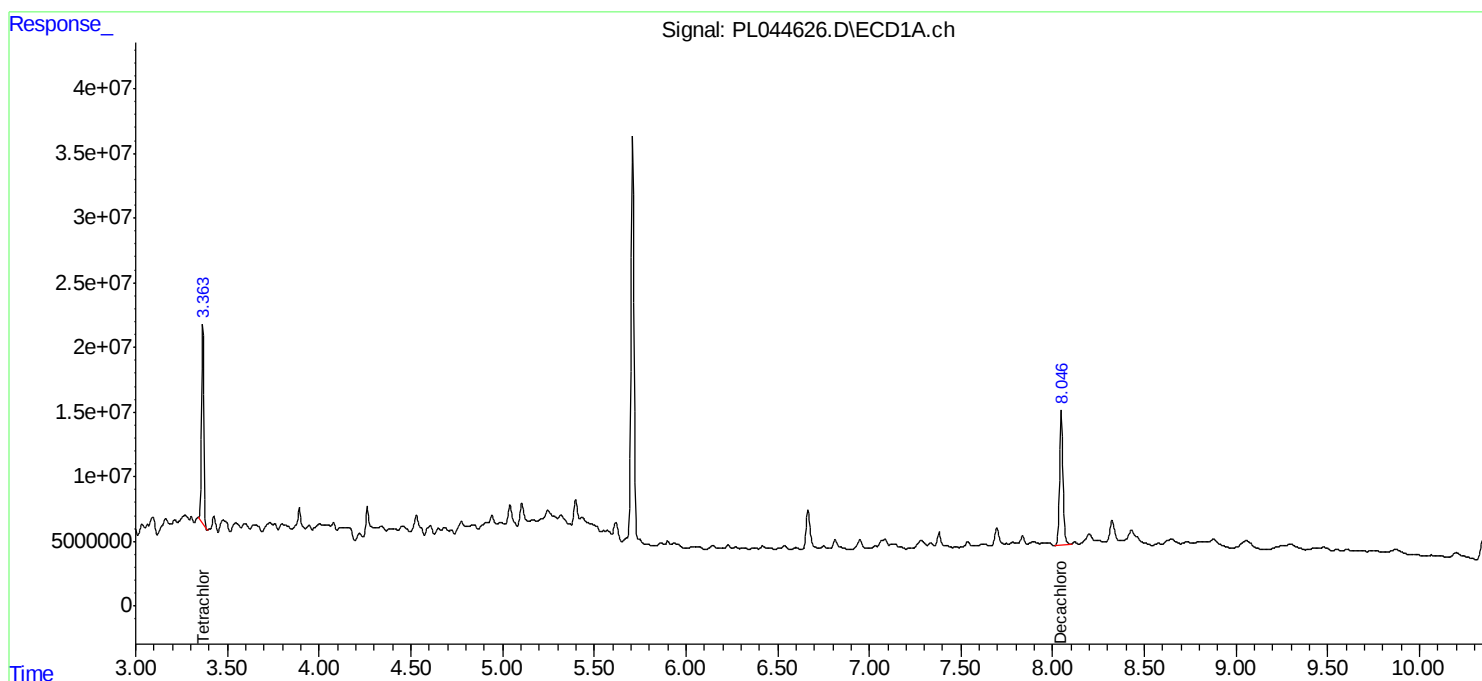


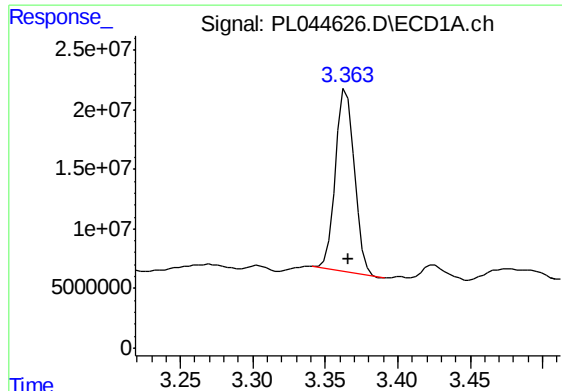

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 138938656
Conc: 19.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
HOSPITAL-BOX-CULVERT-TP

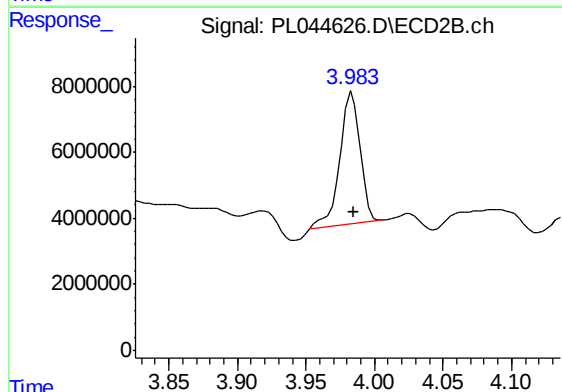


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 41283299
Conc: 17.57 ng/ml

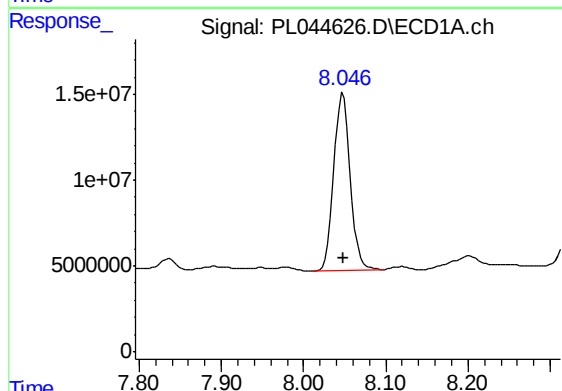

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: -0.001 min
Response: 144125338
Conc: 19.76 ng/ml

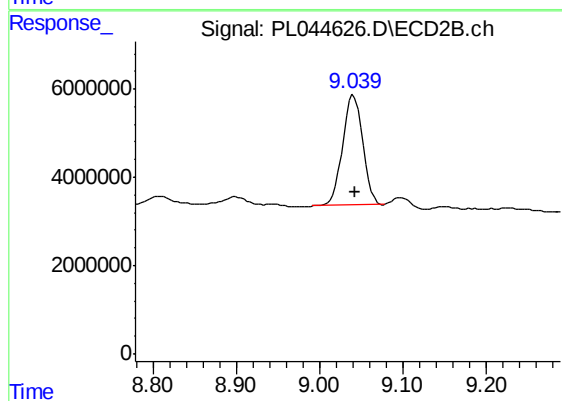

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: -0.002 min
Response: 42399287
Conc: 19.14 ng/ml