

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021119\
 Data File : PL044661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 01:34
 Operator : AJ\SJ
 Sample : K1450-04
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HOSPITAL-BOX-CULVERT-TP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 01:59:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.984	132.9E6	43995258	18.676	18.728
28)	SA Decachlor...	8.047	9.040	106.1E6	30709824	14.554	13.865

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021119\
Data File : PL044661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 01:34
Operator : AJ\SJ
Sample : K1450-04
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HOSPITAL-BOX-CULVERT-TP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 01:59:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

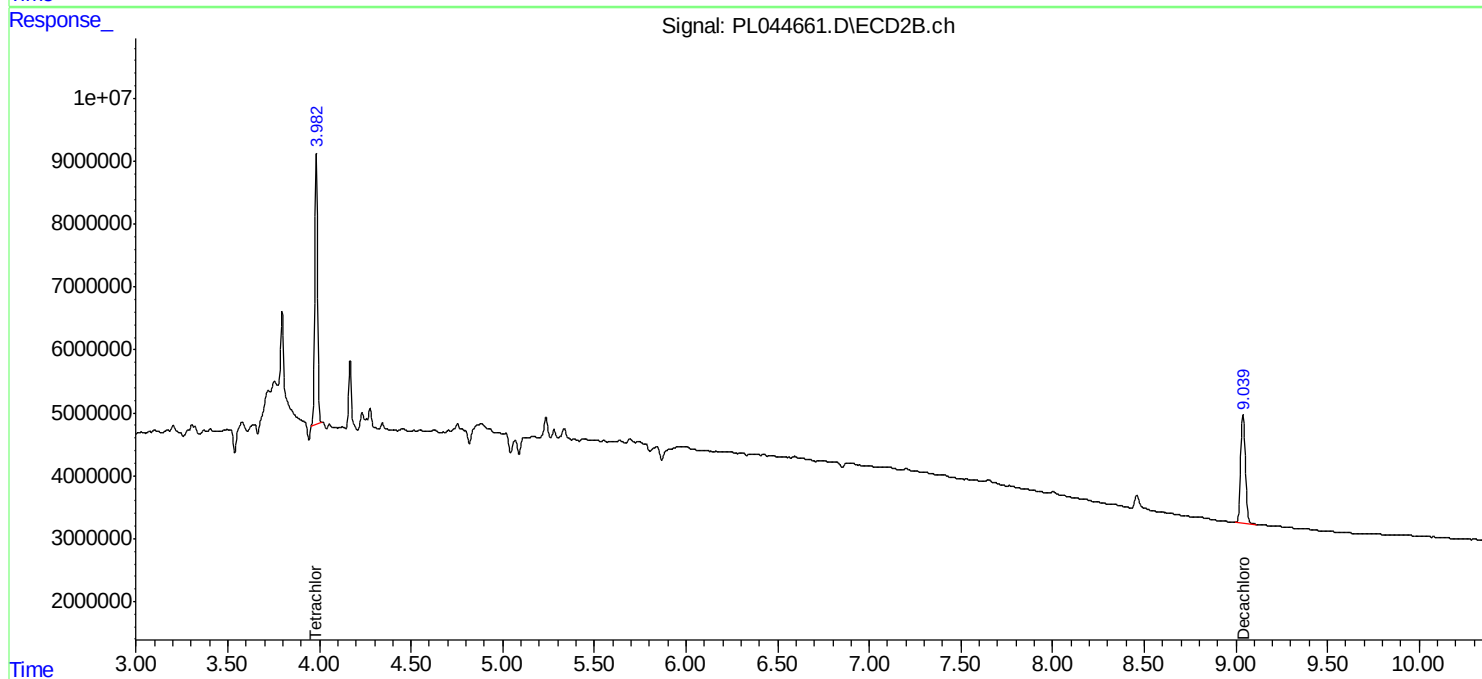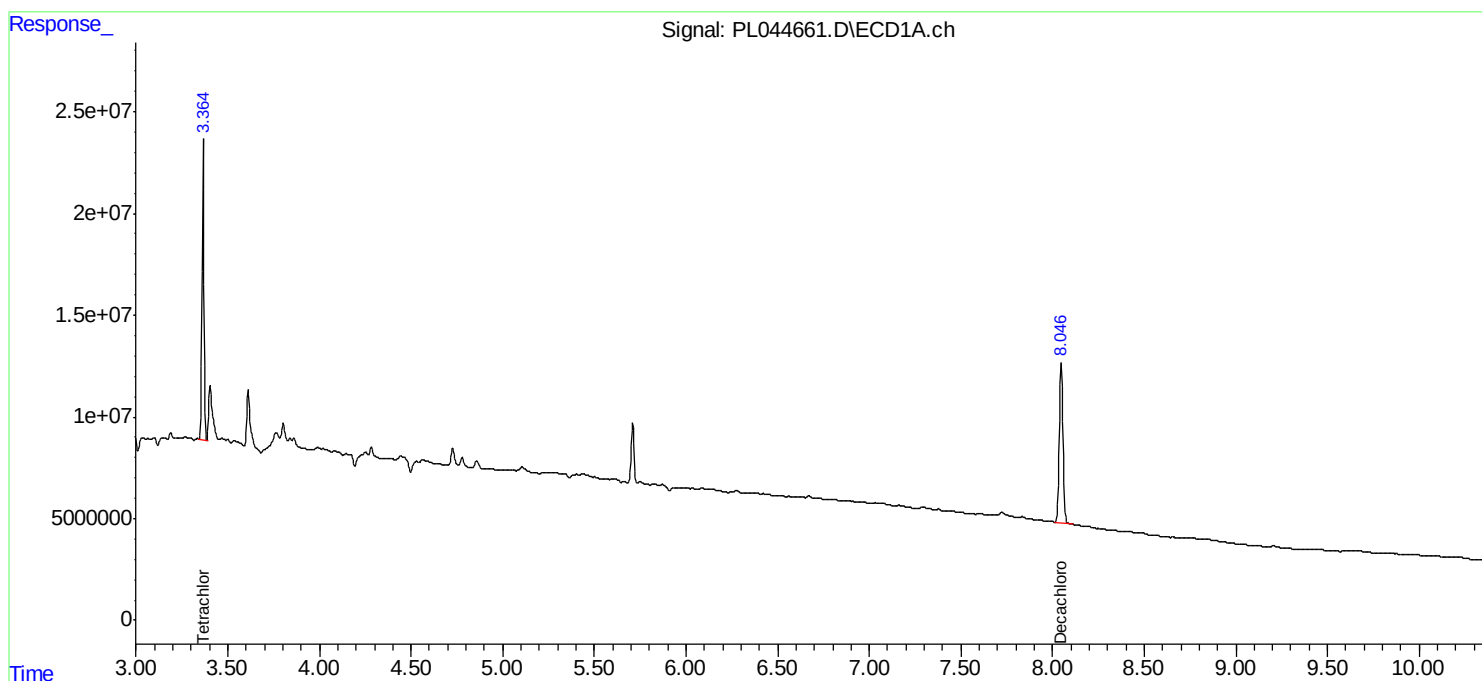


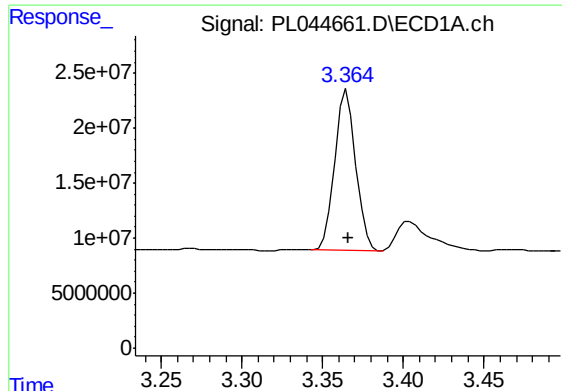

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 132893166
Conc: 18.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
HOSPITAL-BOX-CULVERT-TP

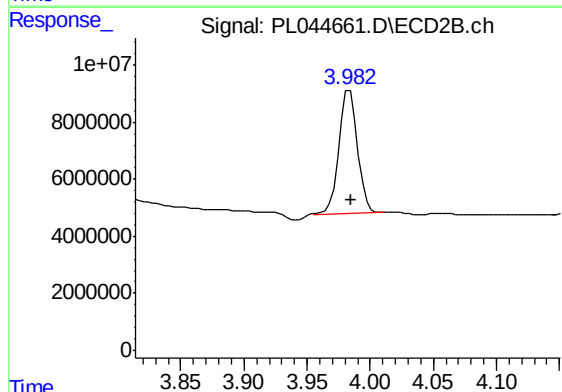


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 43995258
Conc: 18.73 ng/ml

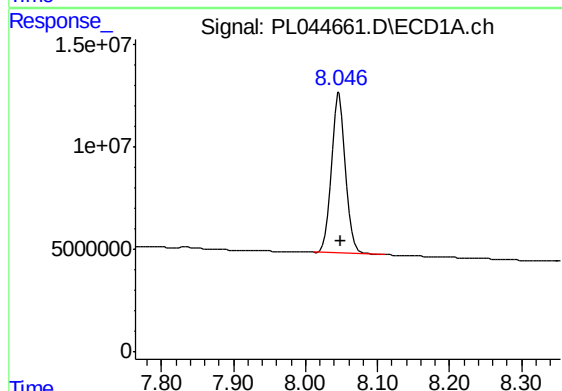

#28 Decachlorobiphenyl

R.T.: 8.047 min
Delta R.T.: -0.002 min
Response: 106149635
Conc: 14.55 ng/ml

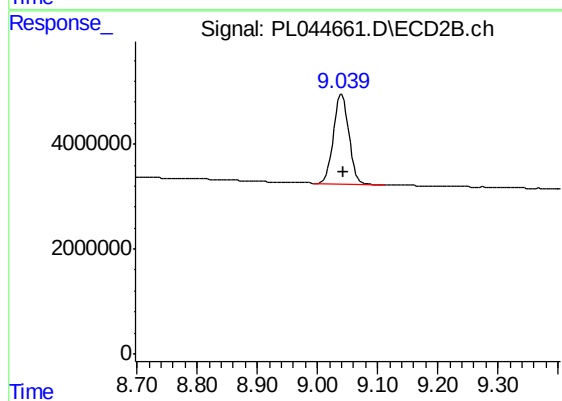

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: -0.003 min
Response: 30709824
Conc: 13.87 ng/ml