

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021120\
 Data File : PL056465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2020 15:27
 Operator : AJ\MA
 Sample : L1466-04DL 20X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 00:24:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	0.000	31216387	0	2.981	N.D. #
Target Compounds							
2)	A alpha-BHC	3.960f	0.000	29264328	0	1.642	N.D. #
4)	MA Heptachlor	4.510	0.000	8836110	0	0.550	N.D. #
5)	MB Aldrin	4.745f	0.000	12401826	0	0.762	N.D. #
6)	B beta-BHC	4.486f	0.000	4500136	0	0.683	N.D. #
7)	B delta-BHC	0.000	5.053f	0 14803394	N.D.	4.616	#
11)	B alpha-Chl...	5.489	0.000	42152523	0	2.740	N.D. #
12)	B 4,4'-DDE	5.679f	0.000	39292629	0	2.711	N.D. #
15)	B Endosulfa...	6.334	6.950f	927.2E6	105.2E6	70.895	39.066 #
17)	MA 4,4'-DDT	6.391f	0.000	62209037	0	5.692	N.D. #
24)	Chlordane-2	4.874	0.000	18494948	0	42.216	N.D. #
26)	Chlordane-4	5.489	0.000	42152523	0	38.957	N.D. #
27)	Chlordane-5	6.334	0.000	927.2E6	0 2235.108	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021120\
Data File : PL056465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2020 15:27
Operator : AJ\MA
Sample : L1466-04DL 20X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 00:24:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

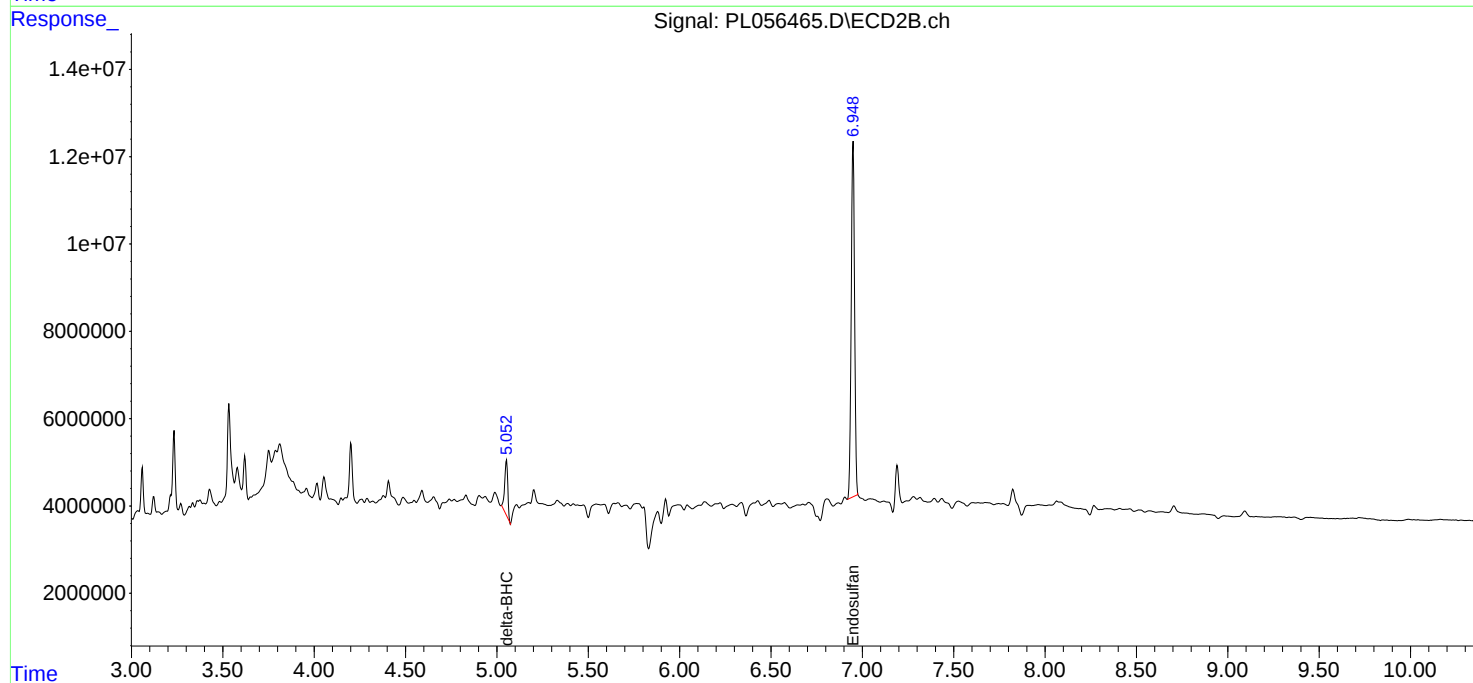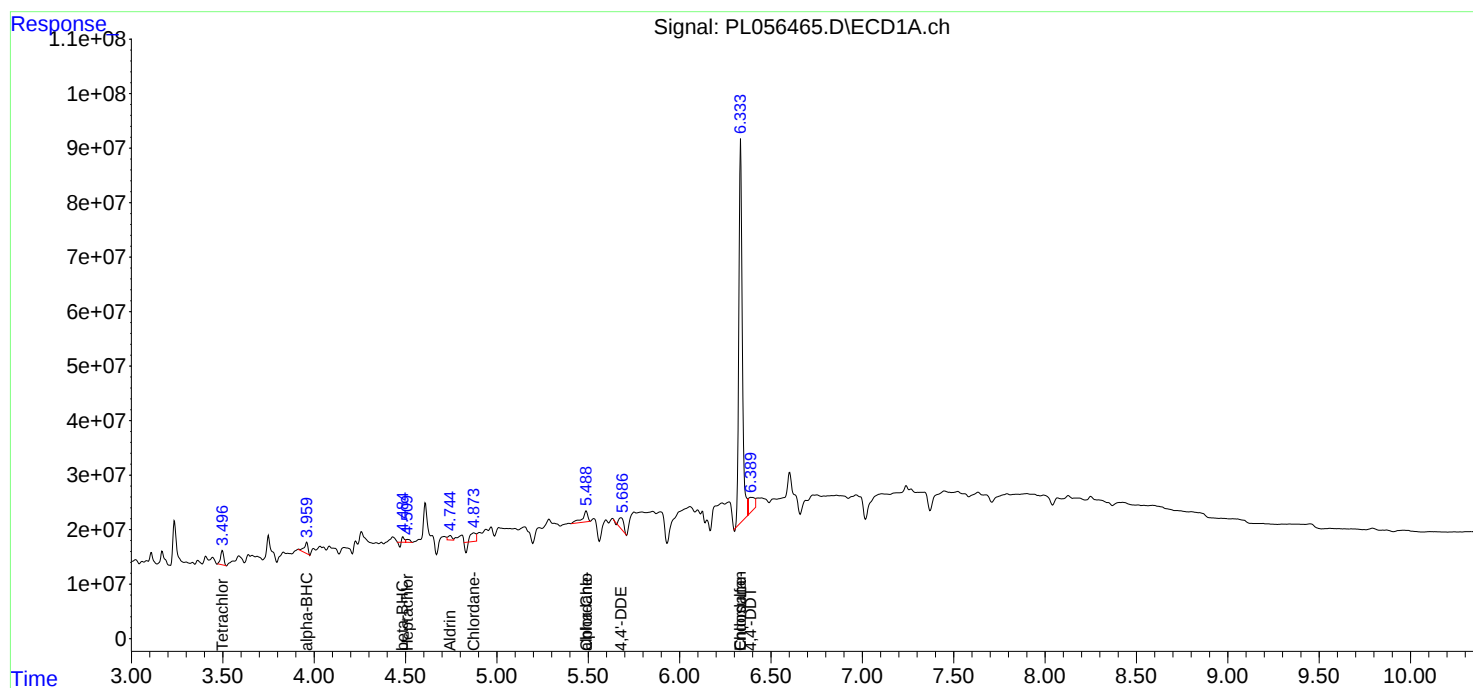


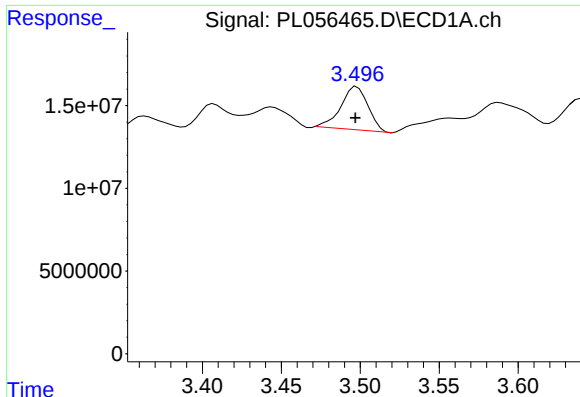

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 31216387
Conc: 2.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

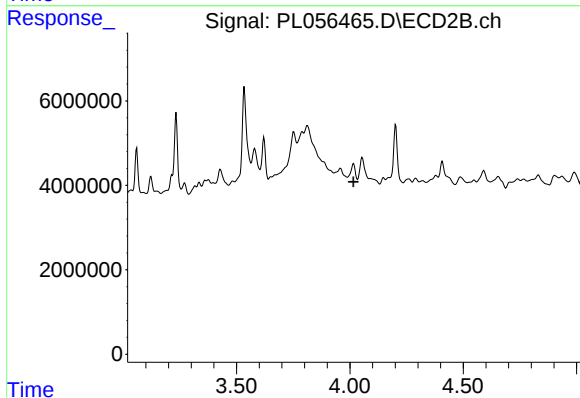


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.016 min
Response: 0
Conc: N.D.

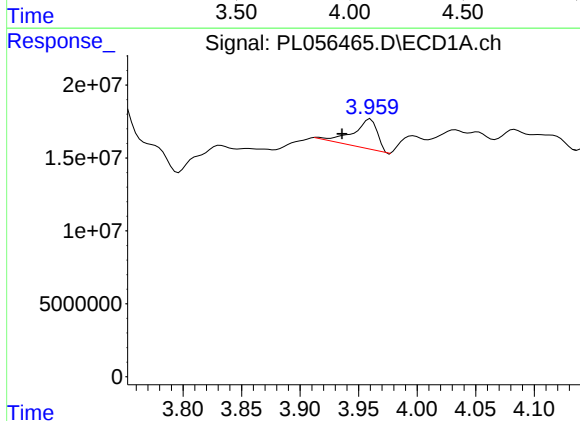


#2 alpha-BHC

R.T.: 3.960 min
Delta R.T.: 0.024 min
Response: 29264328
Conc: 1.64 ng/ml

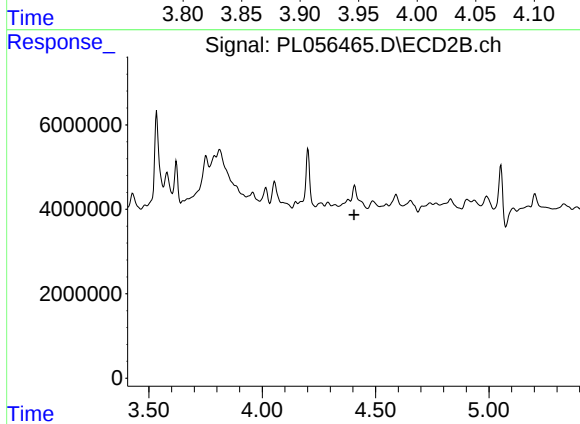

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.405 min
Response: 0
Conc: N.D.

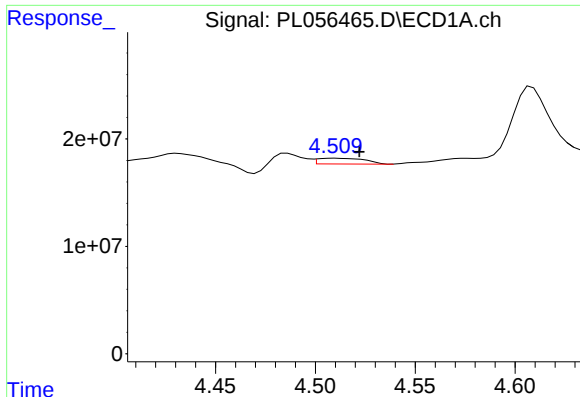

#4 Heptachlor


R.T.: 4.510 min
Delta R.T.: -0.012 min
Response: 8836110
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

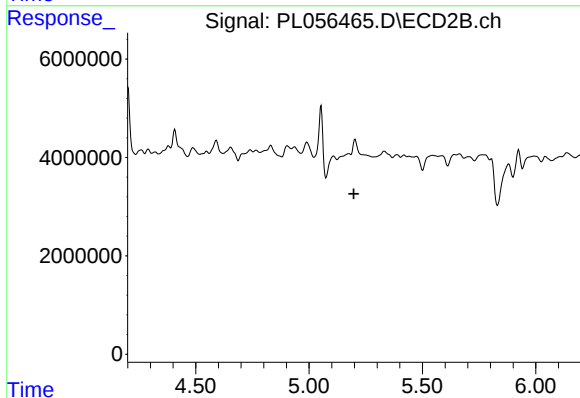


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.197 min
Response: 0
Conc: N.D.

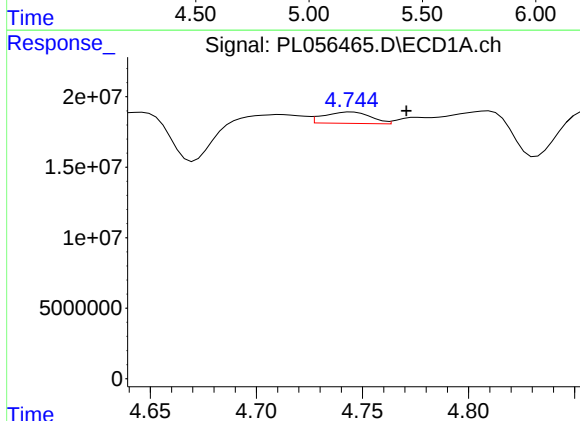


#5 Aldrin

R.T.: 4.745 min
Delta R.T.: -0.026 min
Response: 12401826
Conc: 0.76 ng/ml

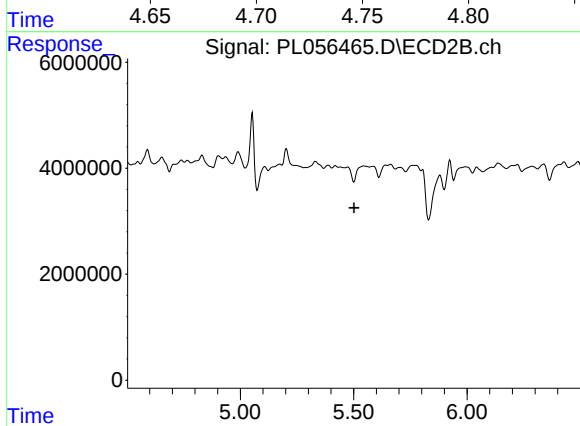

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

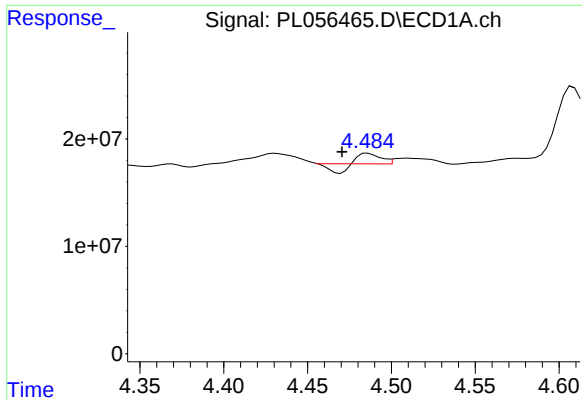

#6 beta-BHC


R.T.: 4.486 min
Delta R.T.: 0.015 min
Response: 4500136
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

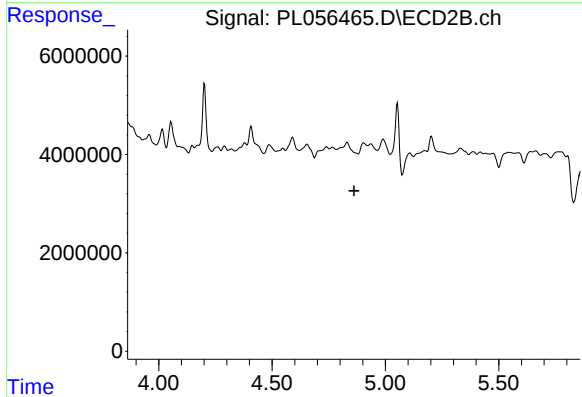


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.862 min
Response: 0
Conc: N.D.

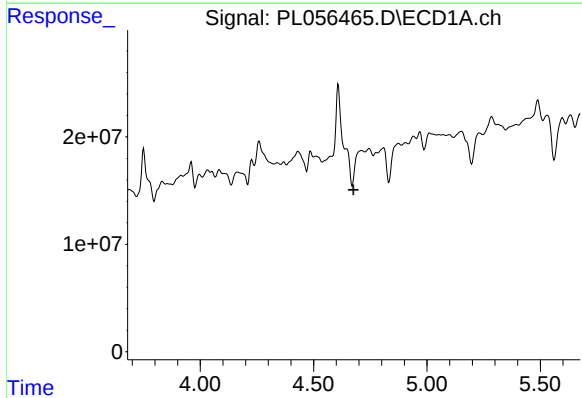


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.676 min
Response: 0
Conc: N.D.

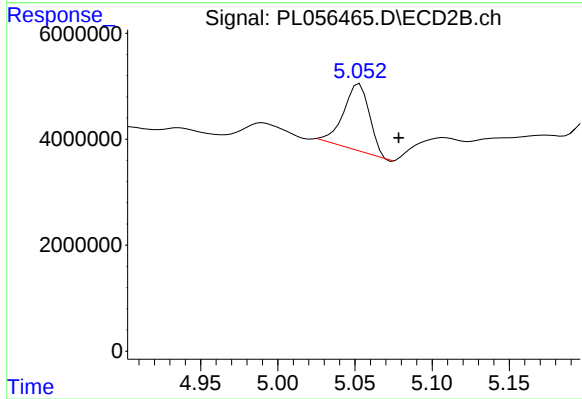

#7 delta-BHC


R.T.: 5.053 min
Delta R.T.: -0.025 min
Response: 14803394
Conc: 4.62 ng/ml

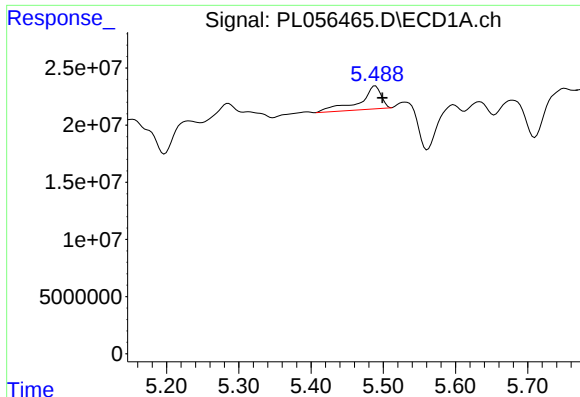

#11 alpha-Chlordane


R.T.: 5.489 min
Delta R.T.: -0.010 min
Response: 42152523
Conc: 2.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

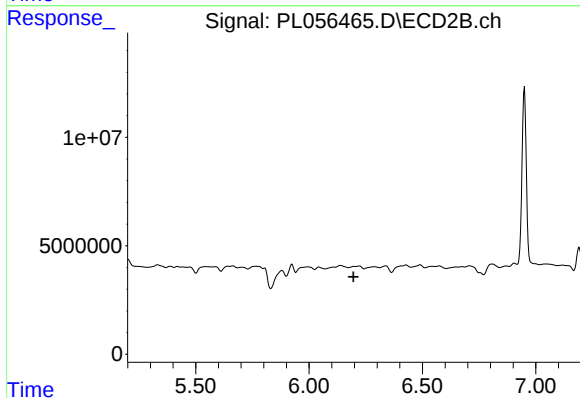


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.196 min
Response: 0
Conc: N.D.

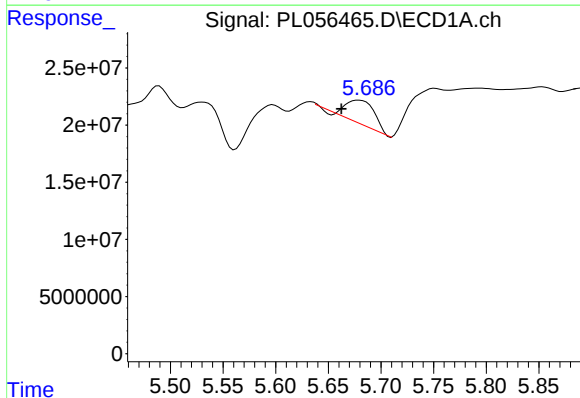


#12 4,4'-DDE

R.T.: 5.679 min
Delta R.T.: 0.017 min
Response: 39292629
Conc: 2.71 ng/ml

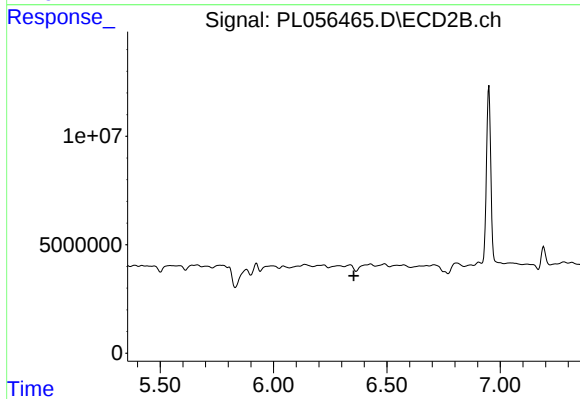

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

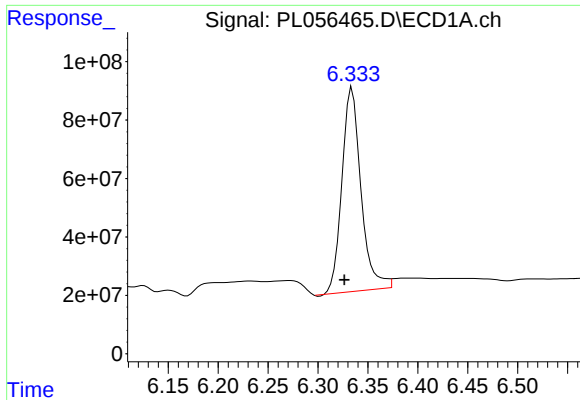

#15 Endosulfan II


R.T.: 6.334 min
Delta R.T.: 0.008 min
Response: 927194156
Conc: 70.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

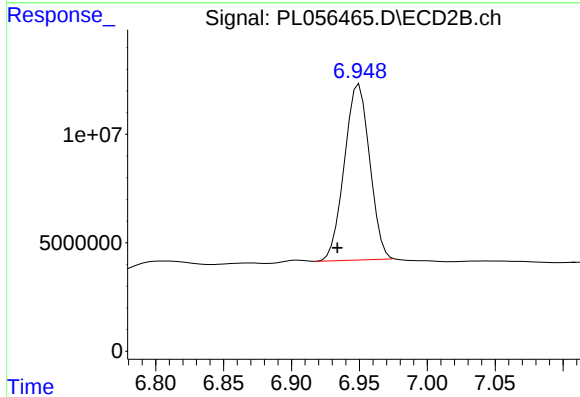


#15 Endosulfan II

R.T.: 6.950 min
Delta R.T.: 0.016 min
Response: 105169066
Conc: 39.07 ng/ml

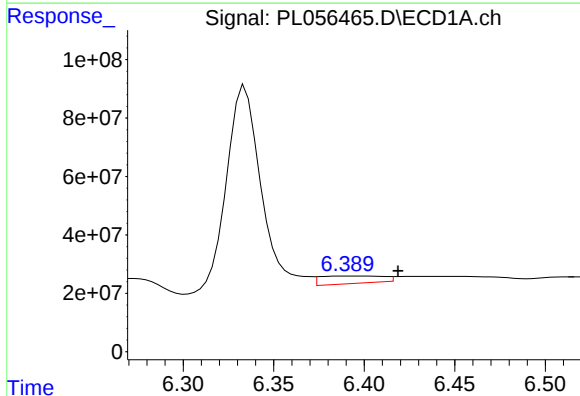


#17 4,4'-DDT

R.T.: 6.391 min
Delta R.T.: -0.027 min
Response: 62209037
Conc: 5.69 ng/ml

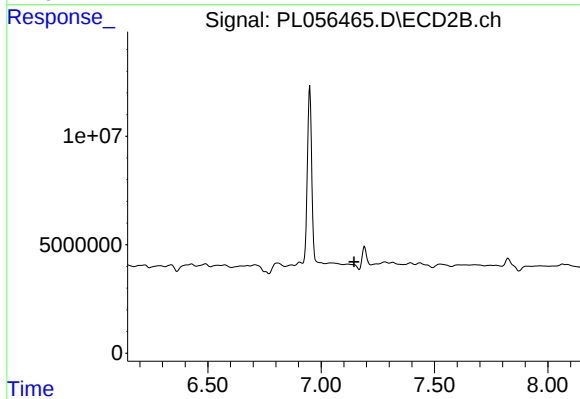

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.146 min
Response: 0
Conc: N.D.

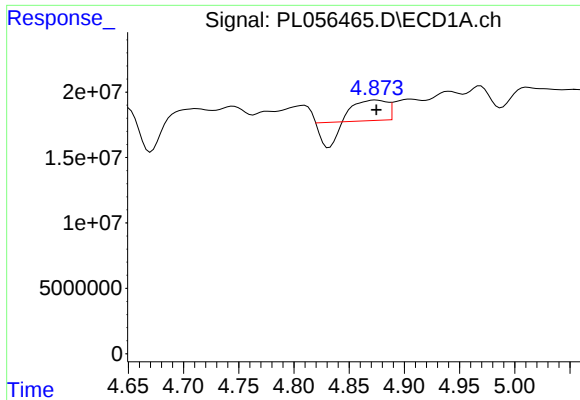

#24 Chlordane-2


R.T.: 4.874 min
Delta R.T.: 0.000 min
Response: 18494948
Conc: 42.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

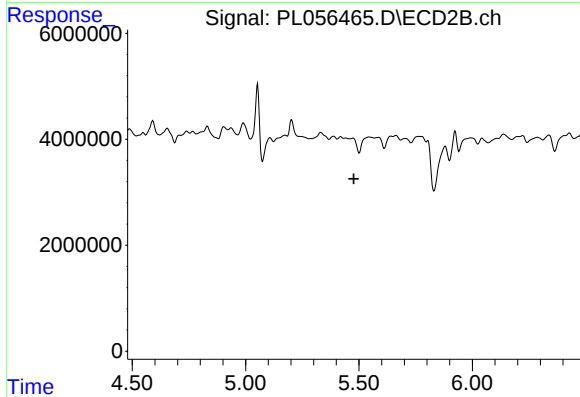


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.477 min
Response: 0
Conc: N.D.

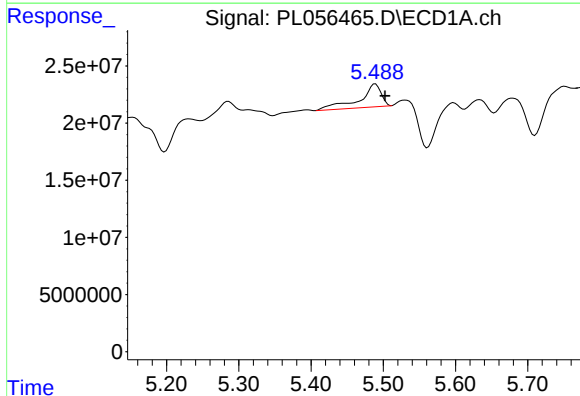


#26 Chlordane-4

R.T.: 5.489 min
Delta R.T.: -0.013 min
Response: 42152523
Conc: 38.96 ng/ml

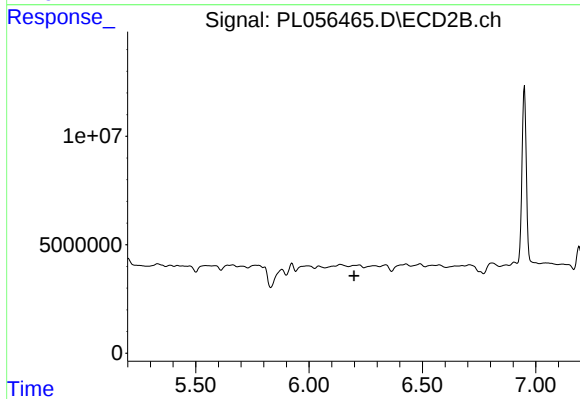

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.199 min
Response: 0
Conc: N.D.

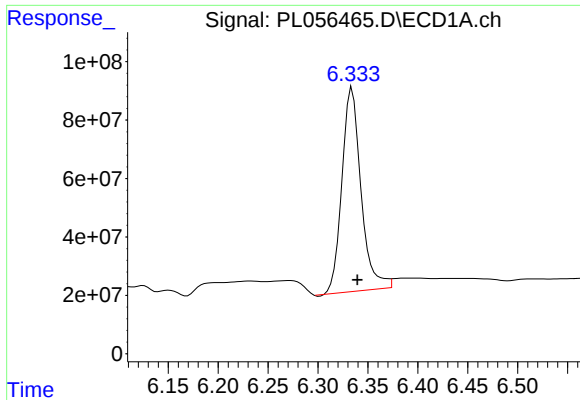

#27 Chlordane-5


R.T.: 6.334 min
Delta R.T.: -0.005 min
Response: 927194156
Conc: 2235.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

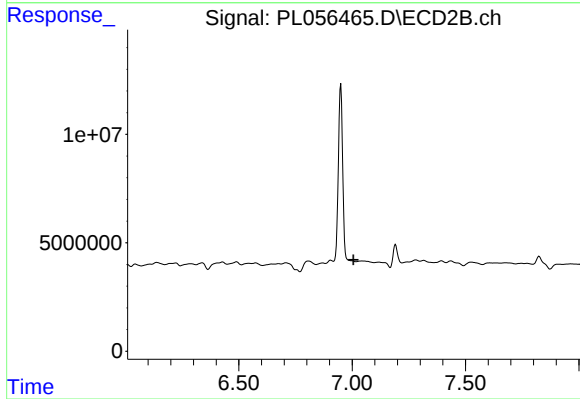


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

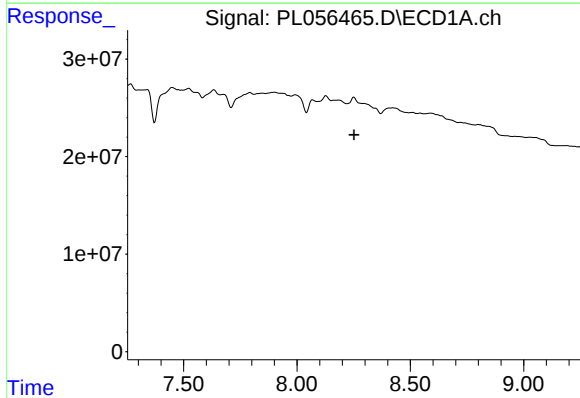

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.252 min
Response: 0
Conc: N.D.

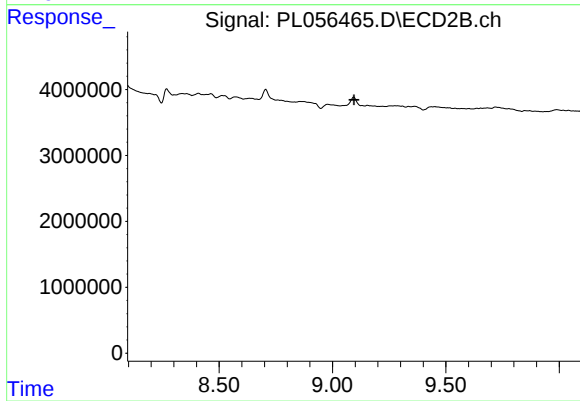

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.