

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021120\
 Data File : PL056485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2020 20:08
 Operator : AJ\MA
 Sample : L1372-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 00:28:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.016	141.3E6	39957960	13.492	13.665
28)	SA Decachlor...	8.251	9.093	101.6E6	17630698	9.652	7.794
Target Compounds							
10)	B gamma-Chl...	5.439	6.127	12549963	12289065	0.800	3.864 #
11)	B alpha-Chl...	5.498	6.200	13185618	18227236	0.857	5.750 #
12)	B 4,4'-DDE	5.660	6.355	21979196	9021962	1.516	3.012 #
17)	MA 4,4'-DDT	6.417	7.153	7595335	15441910	0.695	6.726 #
23)	Chlordane-1	4.370	0.000	26219474	0	69.264	N.D. #
24)	Chlordane-2	4.870	0.000	7155391	0	16.332	N.D. #
25)	Chlordane-3	5.439	6.127	12549963	12289065	9.940	32.698 #
26)	Chlordane-4	5.498	6.200	13185618	18227236	12.186	41.486 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021120\
Data File : PL056485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2020 20:08
Operator : AJ\MA
Sample : L1372-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 00:28:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

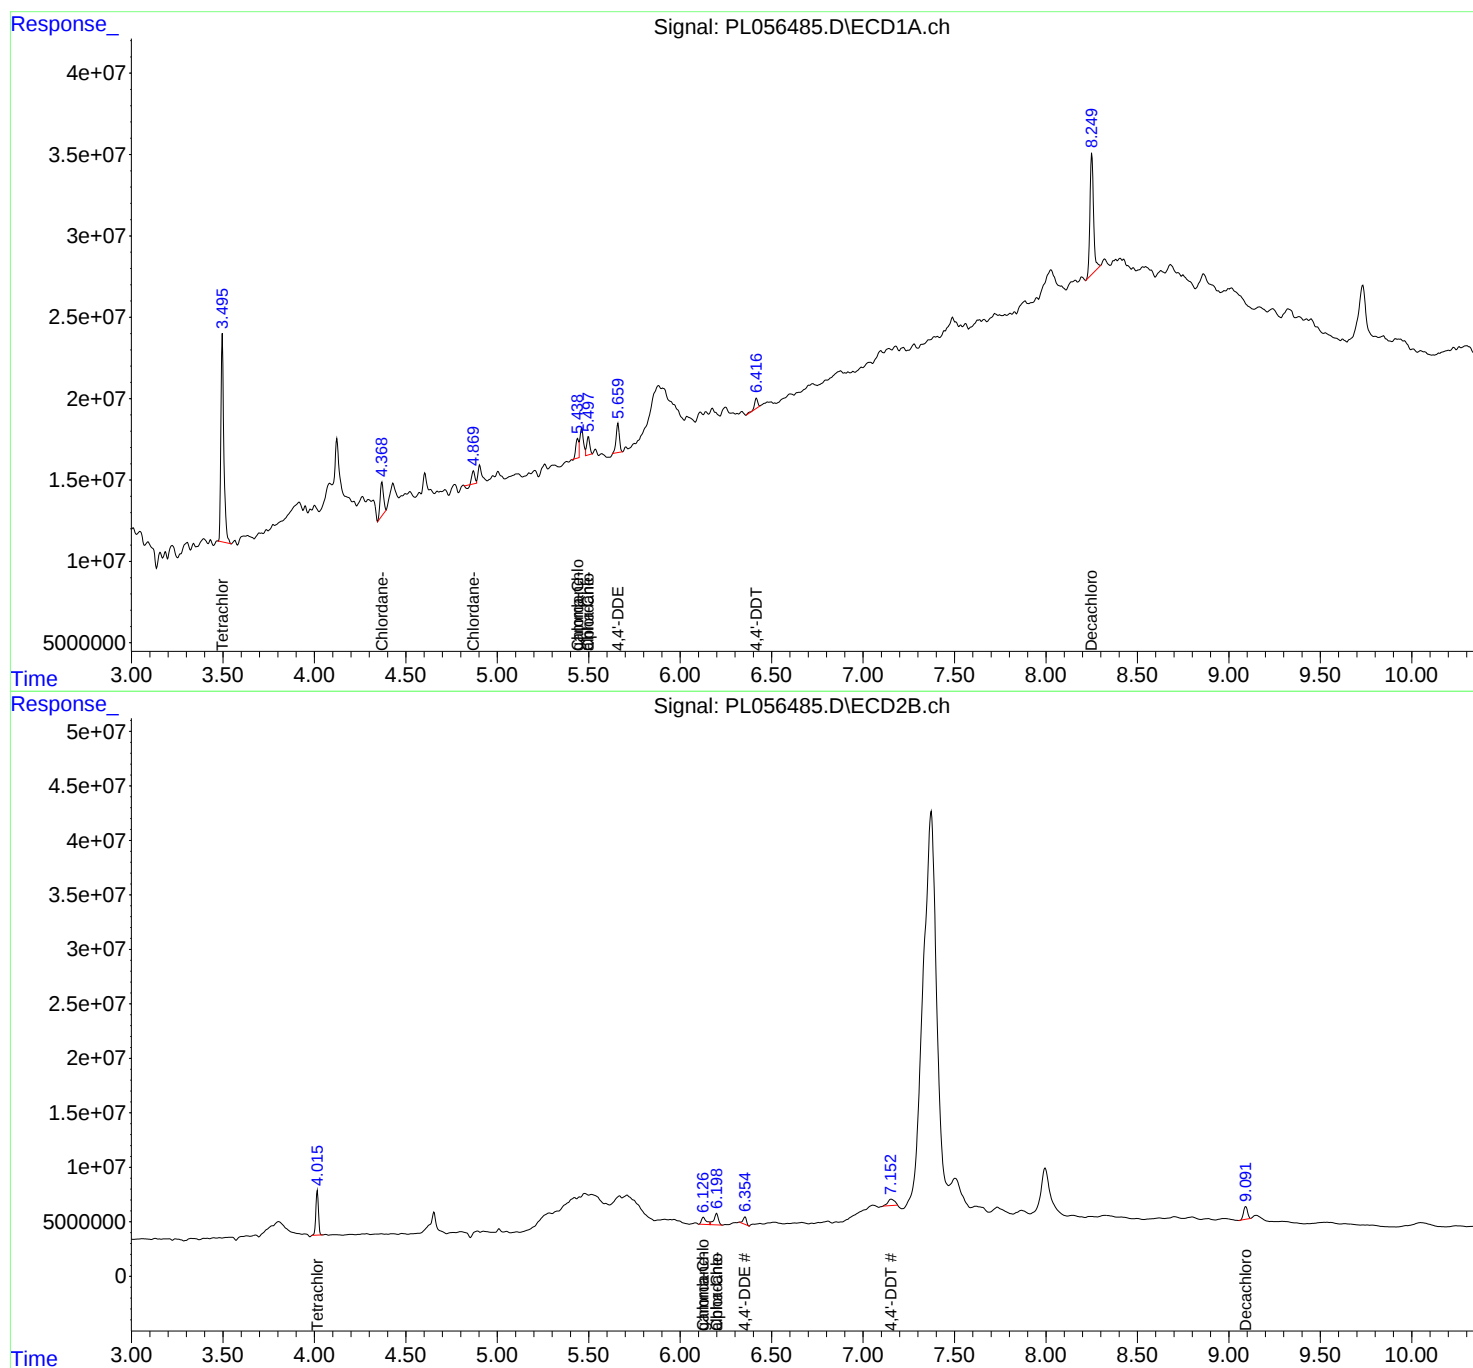


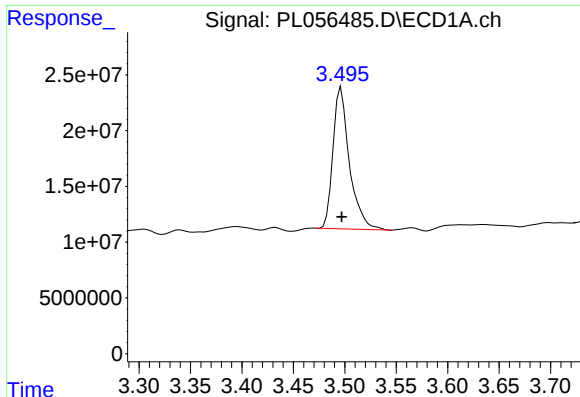

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 141302566
Conc: 13.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

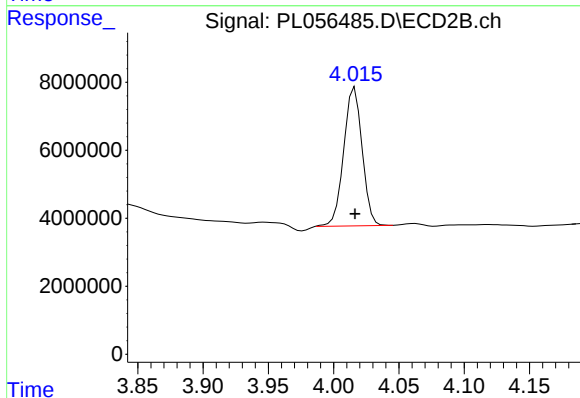


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 39957960
Conc: 13.67 ng/ml

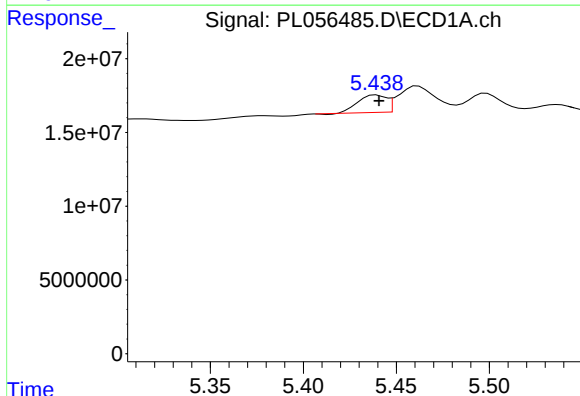


#10 gamma-Chlordane

R.T.: 5.439 min
Delta R.T.: -0.001 min
Response: 12549963
Conc: 0.80 ng/ml

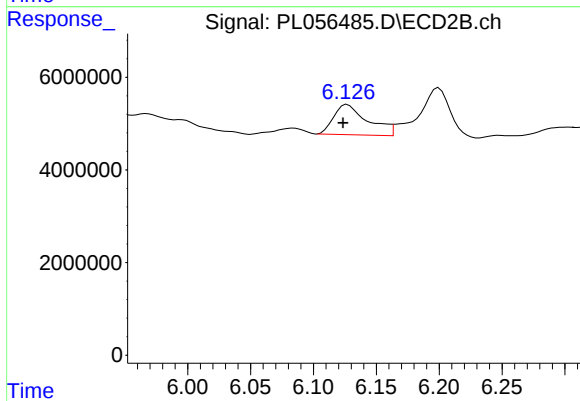

#10 gamma-Chlordane


R.T.: 6.127 min
Delta R.T.: 0.003 min
Response: 12289065
Conc: 3.86 ng/ml

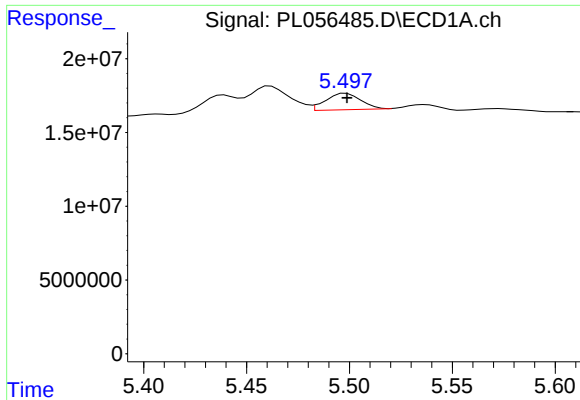

#11 alpha-Chlordane


R.T.: 5.498 min
Delta R.T.: 0.000 min
Response: 13185618
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

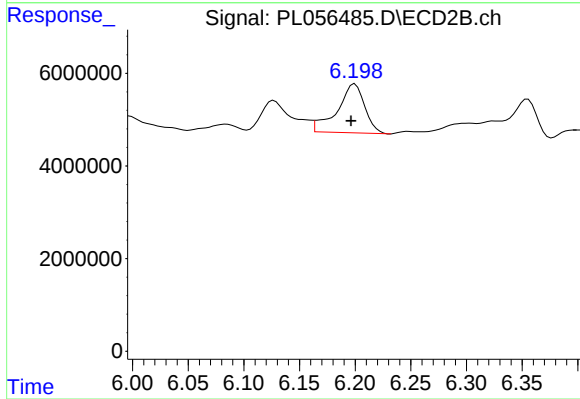


#11 alpha-Chlordane

R.T.: 6.200 min
Delta R.T.: 0.003 min
Response: 18227236
Conc: 5.75 ng/ml

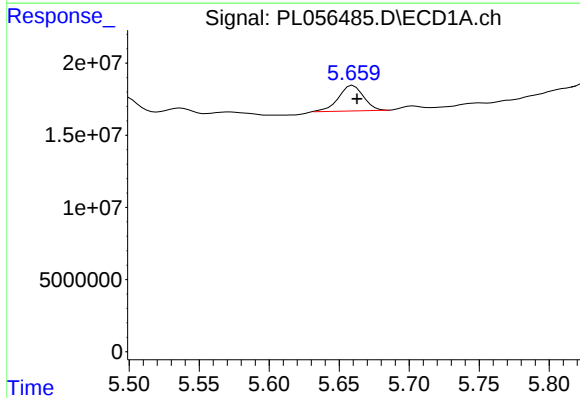


#12 4,4'-DDE

R.T.: 5.660 min
Delta R.T.: -0.003 min
Response: 21979196
Conc: 1.52 ng/ml

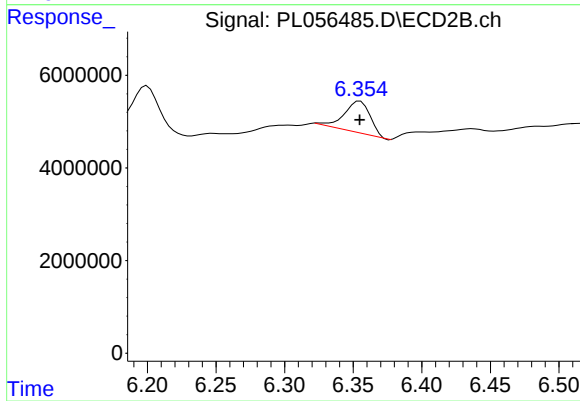

#12 4,4'-DDE


R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 9021962
Conc: 3.01 ng/ml

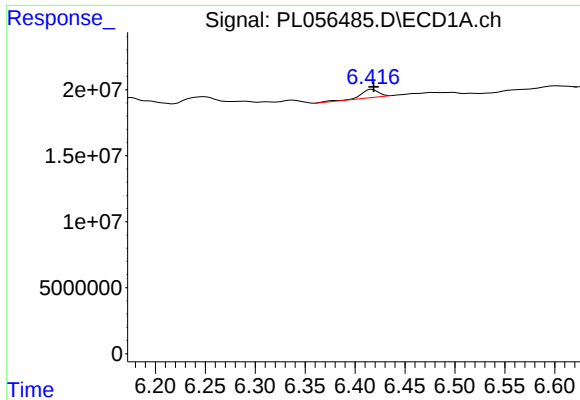

#17 4,4'-DDT


R.T.: 6.417 min
Delta R.T.: -0.002 min
Response: 7595335
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

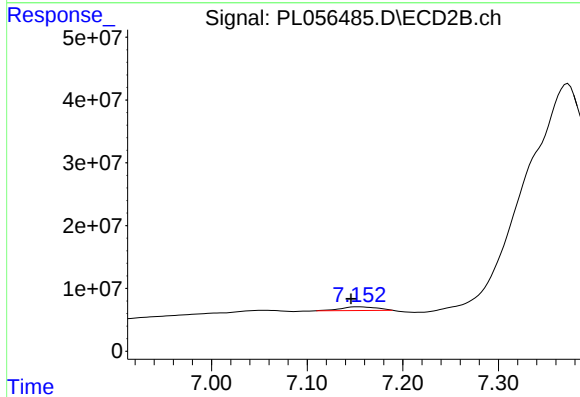


#17 4,4'-DDT

R.T.: 7.153 min
Delta R.T.: 0.007 min
Response: 15441910
Conc: 6.73 ng/ml

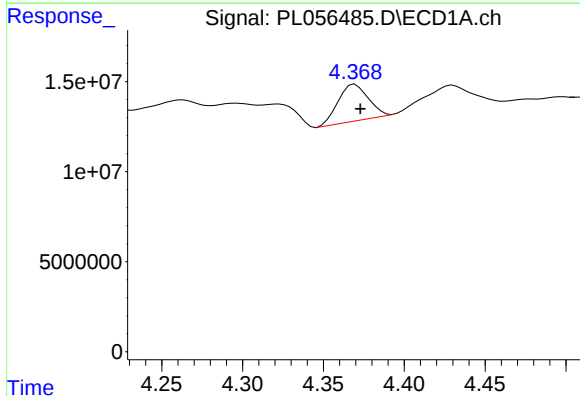


#23 Chlordane-1

R.T.: 4.370 min
Delta R.T.: -0.003 min
Response: 26219474
Conc: 69.26 ng/ml

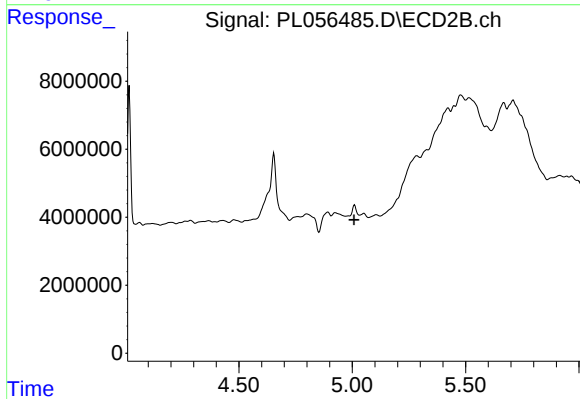

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.008 min
Response: 0
Conc: N.D.

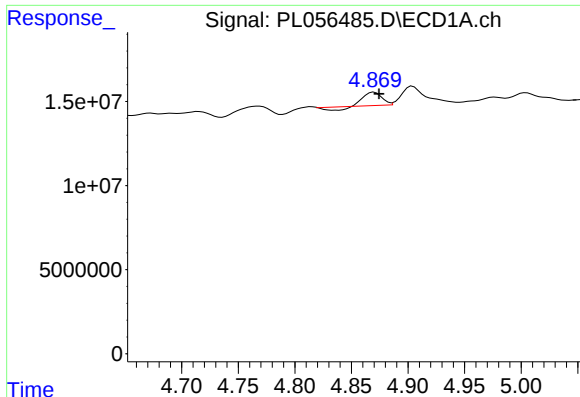

#24 Chlordane-2


R.T.: 4.870 min
Delta R.T.: -0.005 min
Response: 7155391
Conc: 16.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

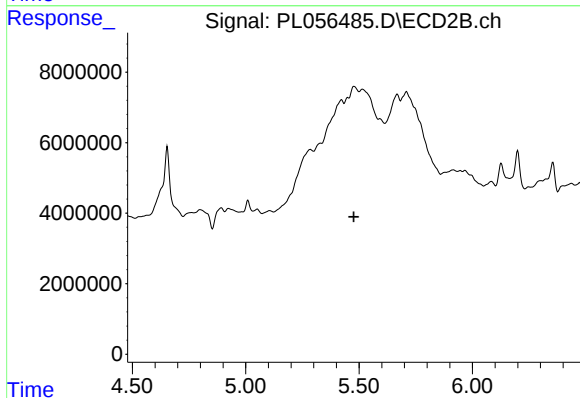


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.477 min
Response: 0
Conc: N.D.

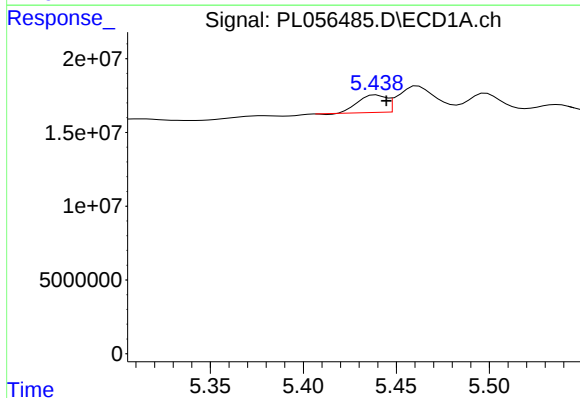


#25 Chlordane-3

R.T.: 5.439 min
Delta R.T.: -0.005 min
Response: 12549963
Conc: 9.94 ng/ml

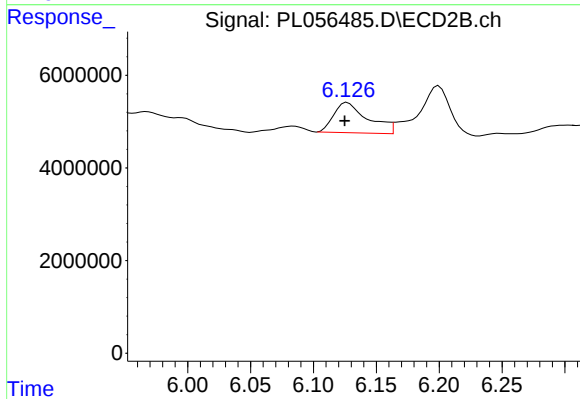

#25 Chlordane-3


R.T.: 6.127 min
Delta R.T.: 0.002 min
Response: 12289065
Conc: 32.70 ng/ml

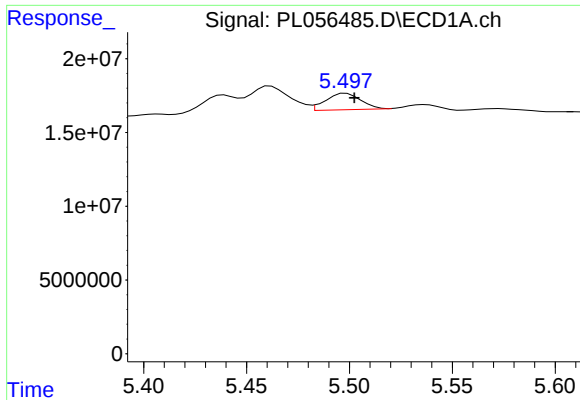

#26 Chlordane-4


R.T.: 5.498 min
Delta R.T.: -0.004 min
Response: 13185618
Conc: 12.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

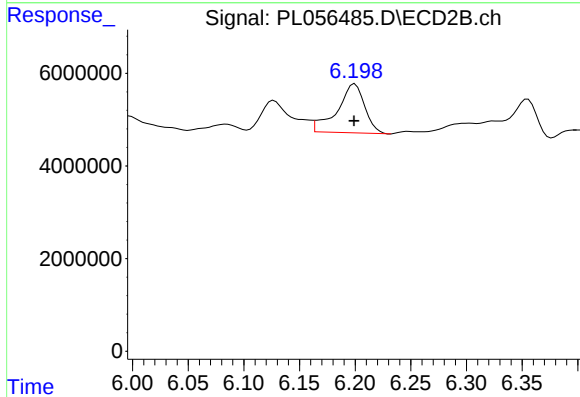


#26 Chlordane-4

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 18227236
Conc: 41.49 ng/ml

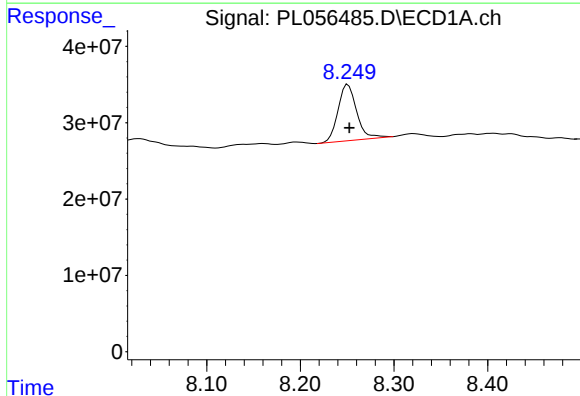

#28 Decachlorobiphenyl

R.T.: 8.251 min
Delta R.T.: -0.001 min
Response: 101615073
Conc: 9.65 ng/ml

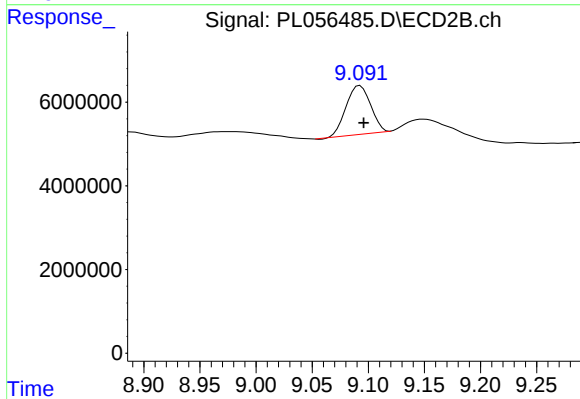

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.003 min
Response: 17630698
Conc: 7.79 ng/ml