

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021120\
 Data File : PL056491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2020 21:33
 Operator : AJ\MA
 Sample : L1438-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 00:29:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.017	199.5E6	62971715	19.050	21.536
28)	SA Decachlor...	8.251	9.092	170.6E6	41726104	16.204	18.447
Target Compounds							
4)	MA Heptachlor	4.528	0.000	946552	0	0.059	N.D. #
23)	Chlordane-1	4.391f	0.000	7598810	0	20.074	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021120\
Data File : PL056491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2020 21:33
Operator : AJ\MA
Sample : L1438-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 00:29:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

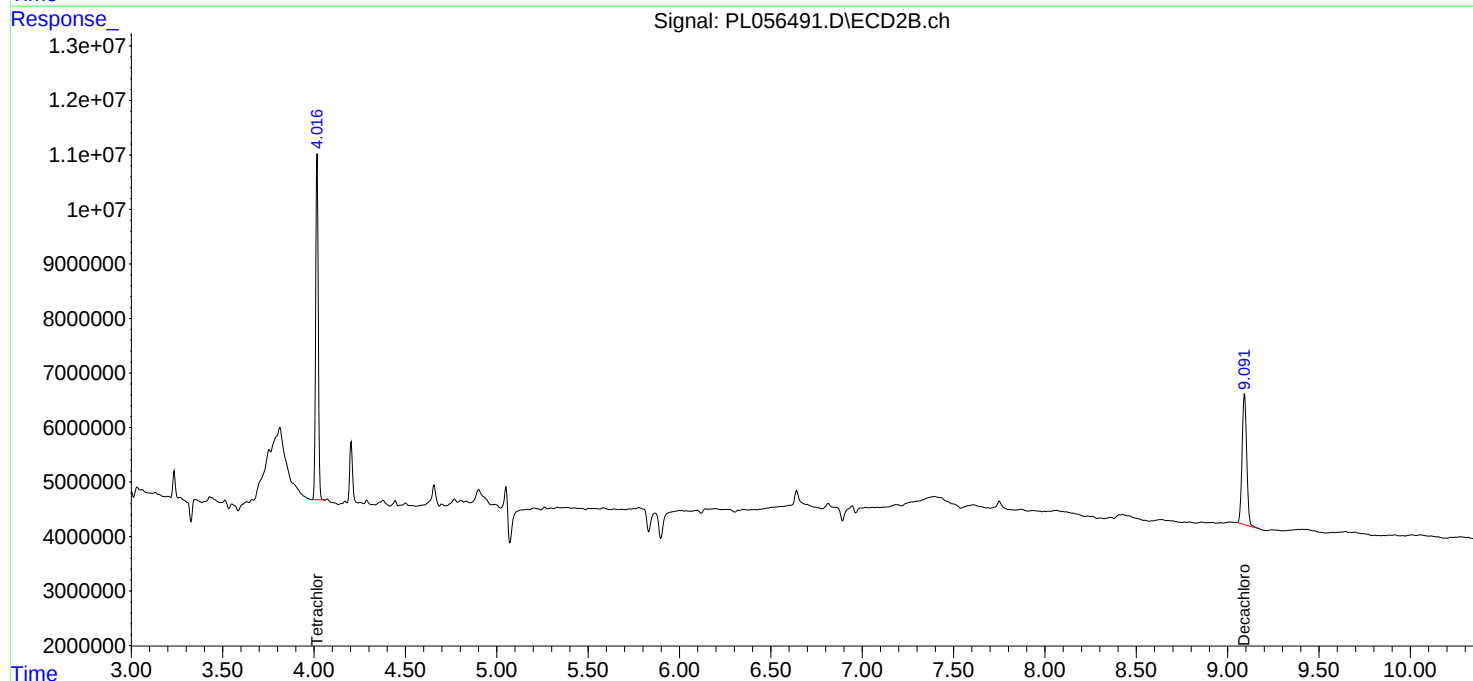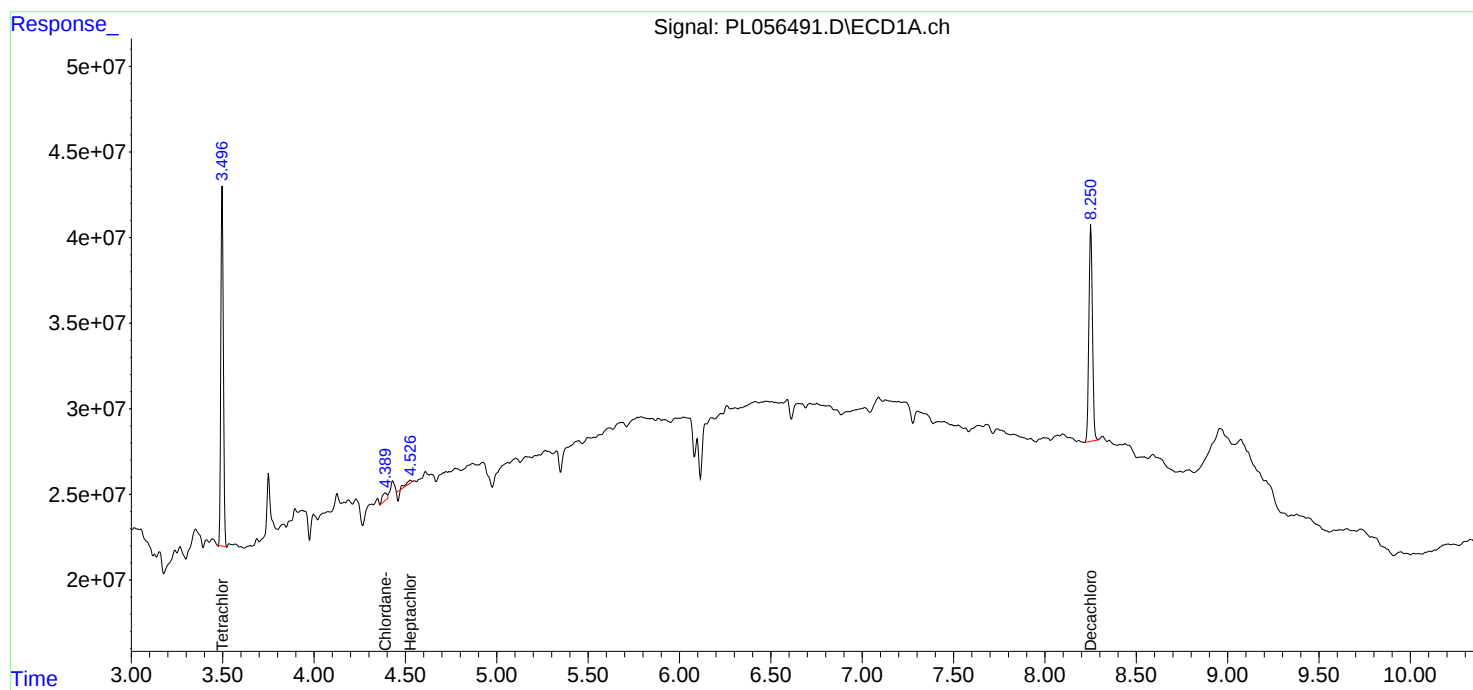


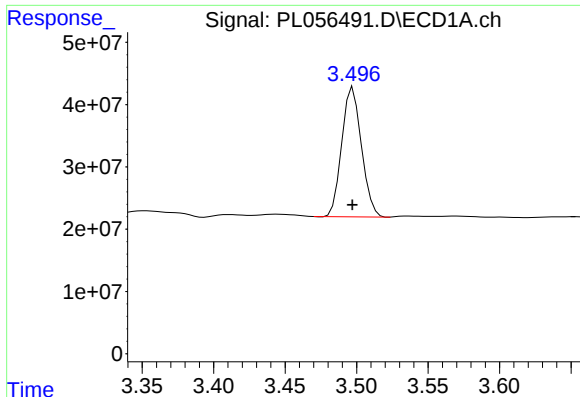

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 199506006
Conc: 19.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

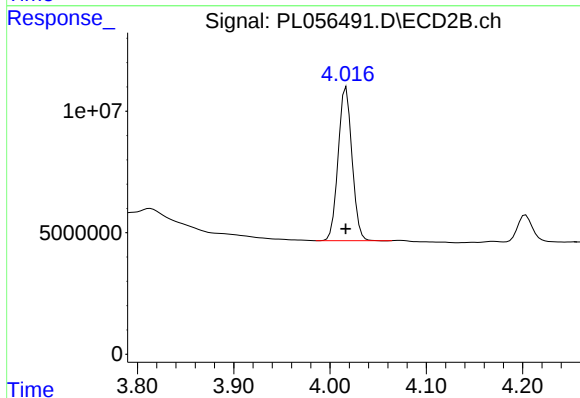


#1 Tetrachloro-m-xylene

R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 62971715
Conc: 21.54 ng/ml

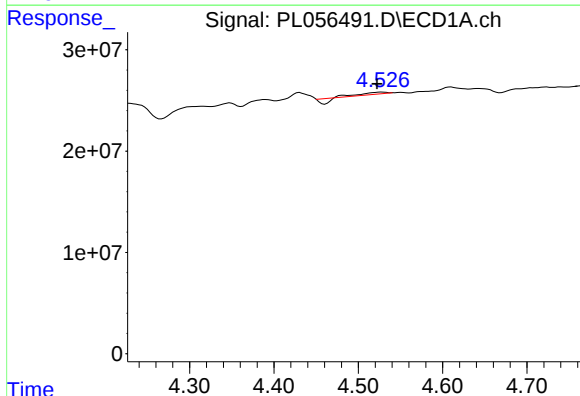


#4 Heptachlor

R.T.: 4.528 min
Delta R.T.: 0.005 min
Response: 946552
Conc: 0.06 ng/ml

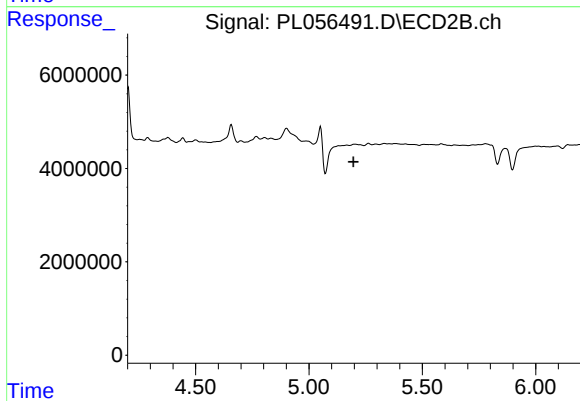

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.197 min
Response: 0
Conc: N.D.

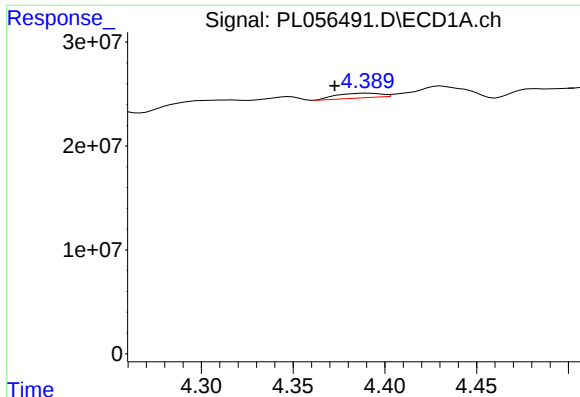

#23 Chlordane-1


R.T.: 4.391 min
Delta R.T.: 0.018 min
Response: 7598810
Conc: 20.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

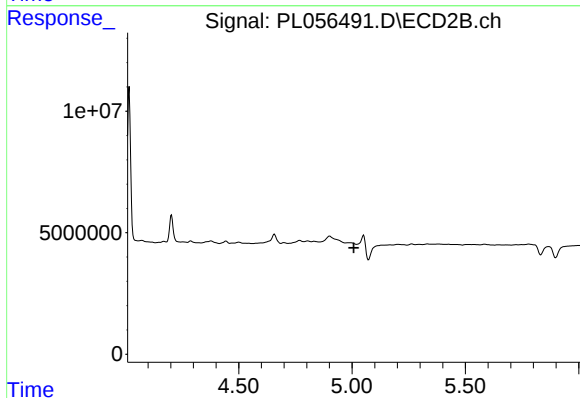


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

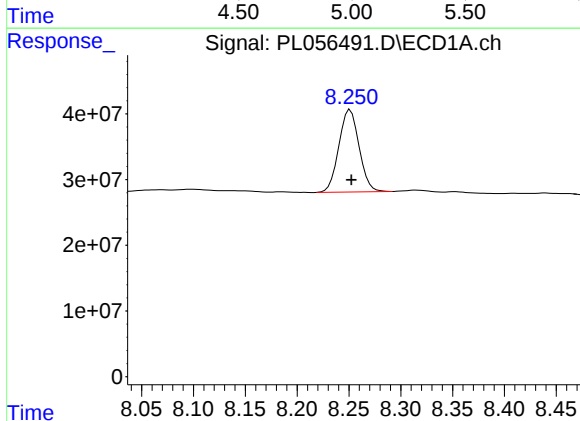

#28 Decachlorobiphenyl

R.T.: 8.251 min
Delta R.T.: 0.000 min
Response: 170594353
Conc: 16.20 ng/ml

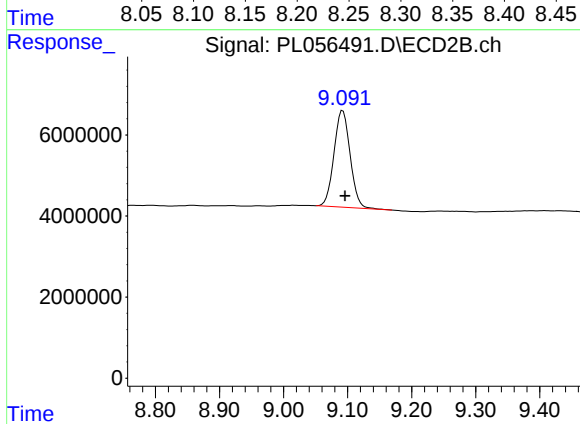

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: -0.003 min
Response: 41726104
Conc: 18.45 ng/ml