

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021120\
 Data File : PL056465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2020 15:27
 Operator : AJ\MA
 Sample : L1446-04DL 20X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-640-XDL

Manual Integrations
 APPROVED

mohammad
 2/12/2020 12:33:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 00:24:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.015	31216387	4179899	2.981	1.429m#
28)	SA Decachlor...	8.249	9.092	9394889	2357270	0.892m	1.042m
Target Compounds							
15)	B Endosulfa...	6.333	6.948	961.7E6	107.1E6	73.533m	39.790m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021120\
Data File : PL056465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2020 15:27
Operator : AJ\MA
Sample : L1446-04DL 20X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-640-XDL


Manual Integrations
APPROVED

mohammad
2/12/2020 12:33:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 00:24:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

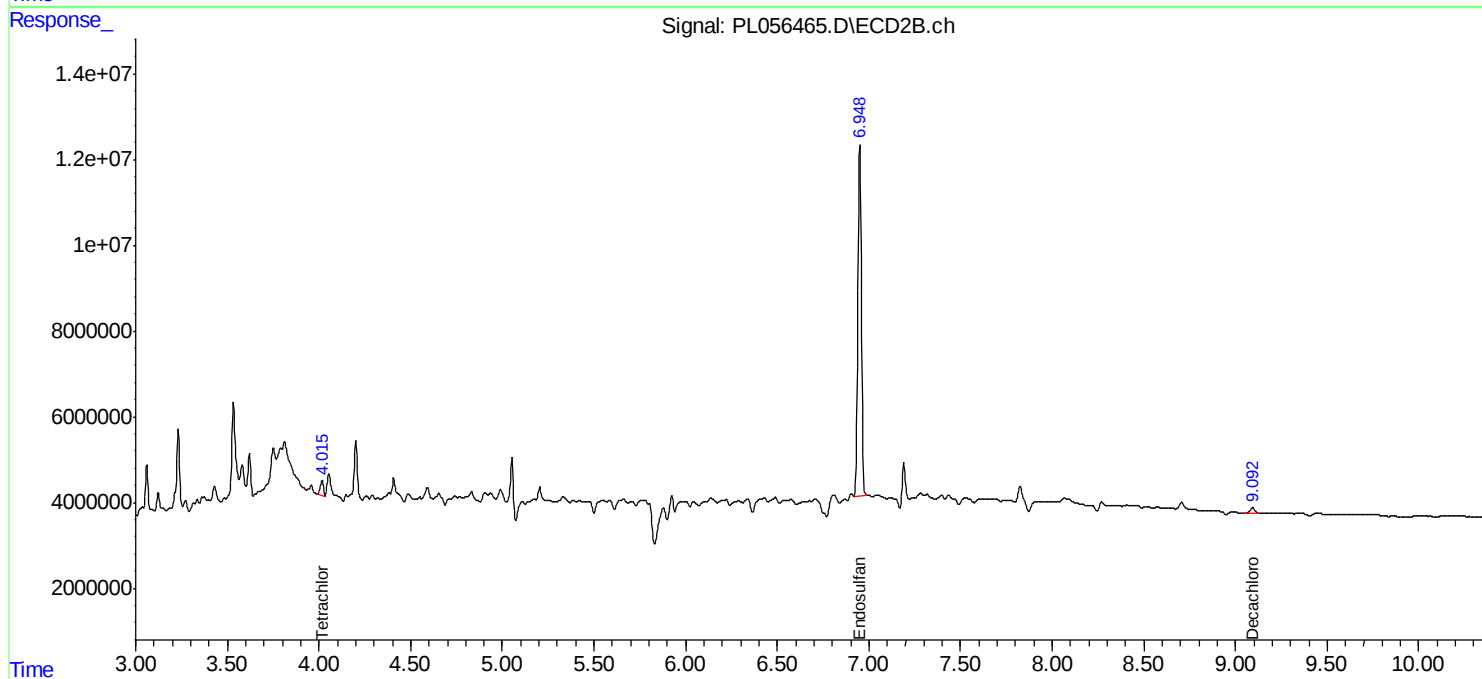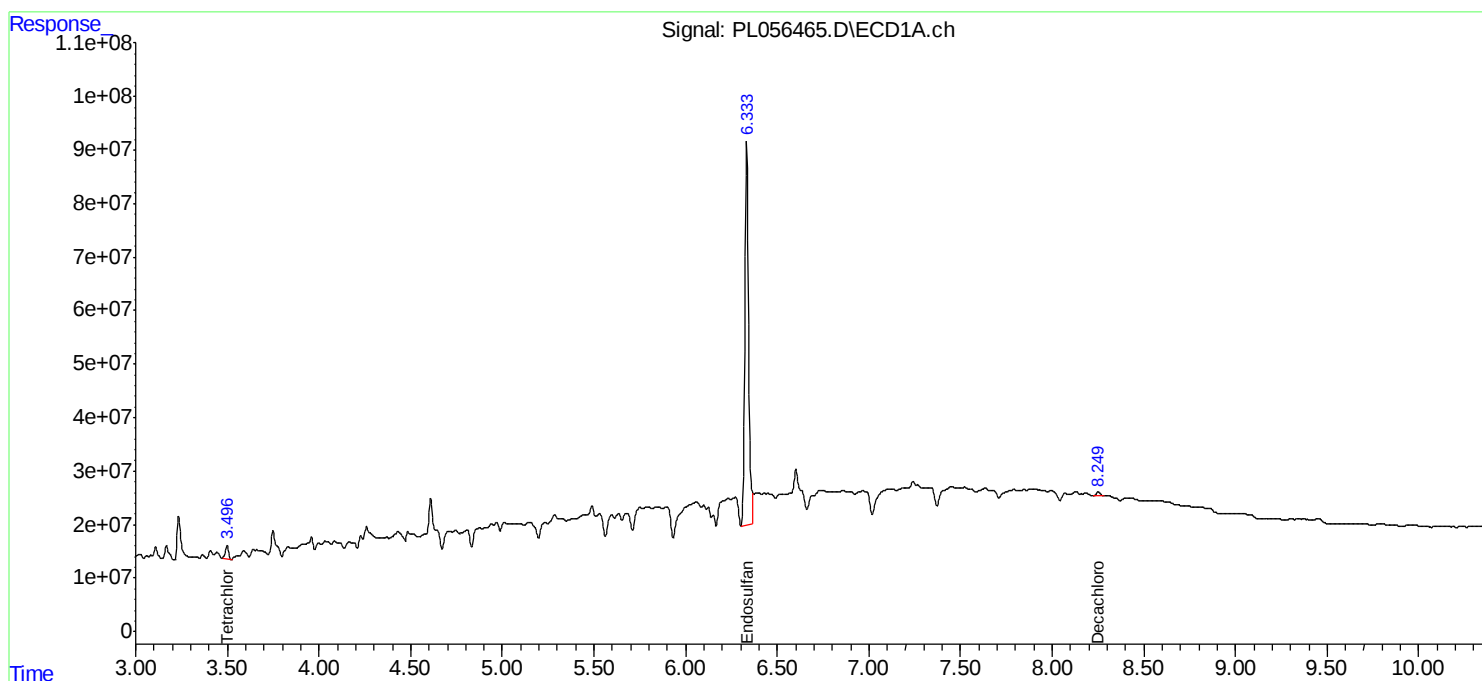

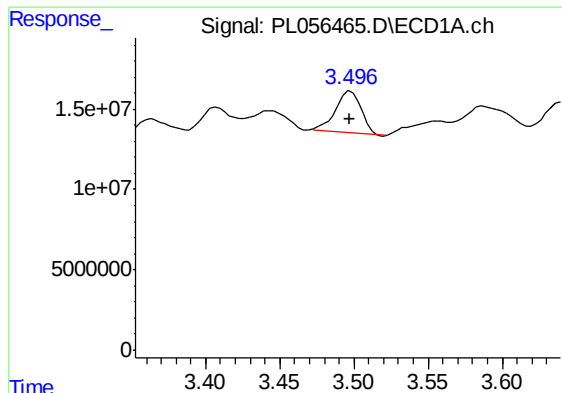


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 31216387
Conc: 2.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-640-XDL


Manual Integrations
APPROVED

mohammad
2/12/2020 12:33:20 PM

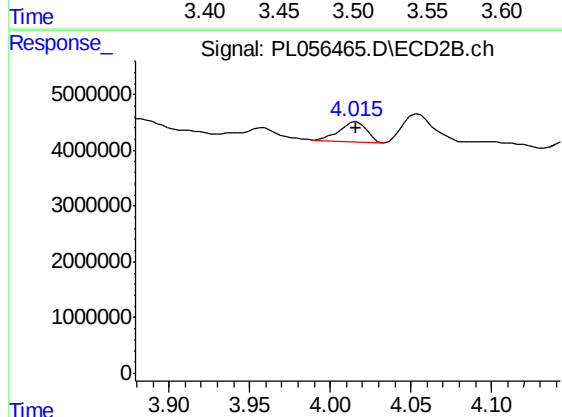


#1 Tetrachloro-m-xylene

R.T.: 4.015 min
Delta R.T.: -0.002 min
Response: 4179899
Conc: 1.43 ng/ml m

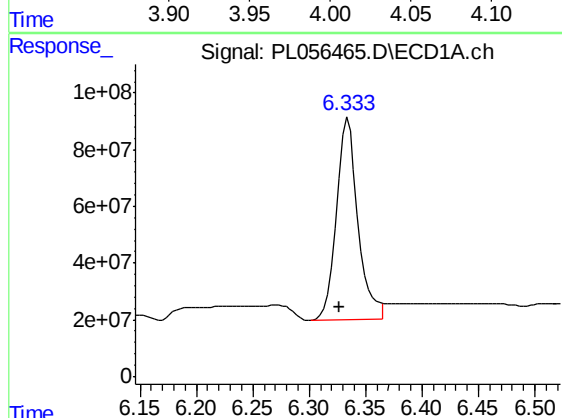


#15 Endosulfan II

R.T.: 6.333 min
Delta R.T.: 0.006 min
Response: 961691822
Conc: 73.53 ng/ml m

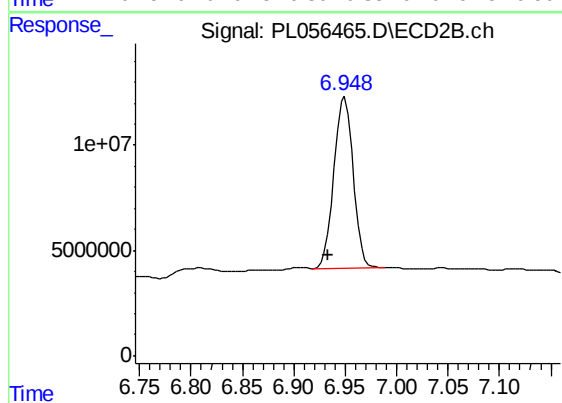

#15 Endosulfan II

R.T.: 6.948 min
Delta R.T.: 0.015 min
Response: 107118275
Conc: 39.79 ng/ml m

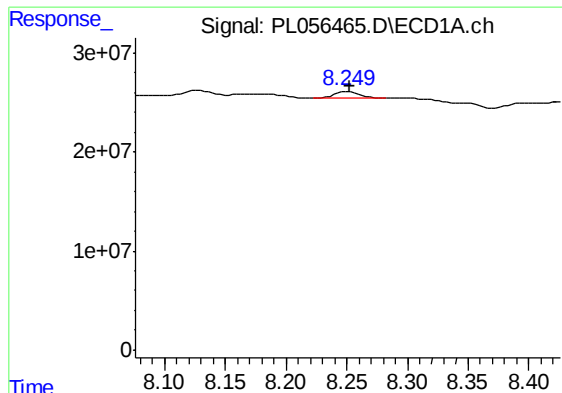


#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: -0.003 min
Response: 9394889
Conc: 0.89 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HP-640-XDL

Manual Integrations
APPROVED

mohammad
2/12/2020 12:33:20 PM

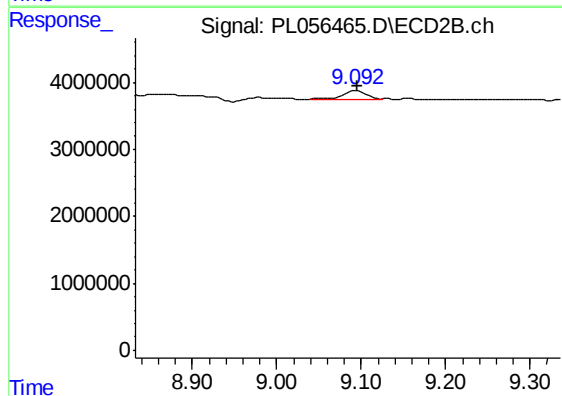

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: -0.004 min
Response: 2357270
Conc: 1.04 ng/ml m