

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021121\
 Data File : PL064772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2021 15:09
 Operator : AR\AJ
 Sample : M1333-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT27339-CHRT20101

Manual Integrations
 APPROVED

Ankita
 2/12/2021 8:30:31 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 16:00:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.099	57344370	40786155	20.382m	18.881
28)	SA Decachlor...	8.148	9.258	46105629	33972832	20.502	17.886

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021121\
Data File : PL064772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2021 15:09
Operator : AR\AJ
Sample : M1333-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT27339-CHRT20101


Manual Integrations
APPROVED

Ankita
2/12/2021 8:30:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 16:00:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

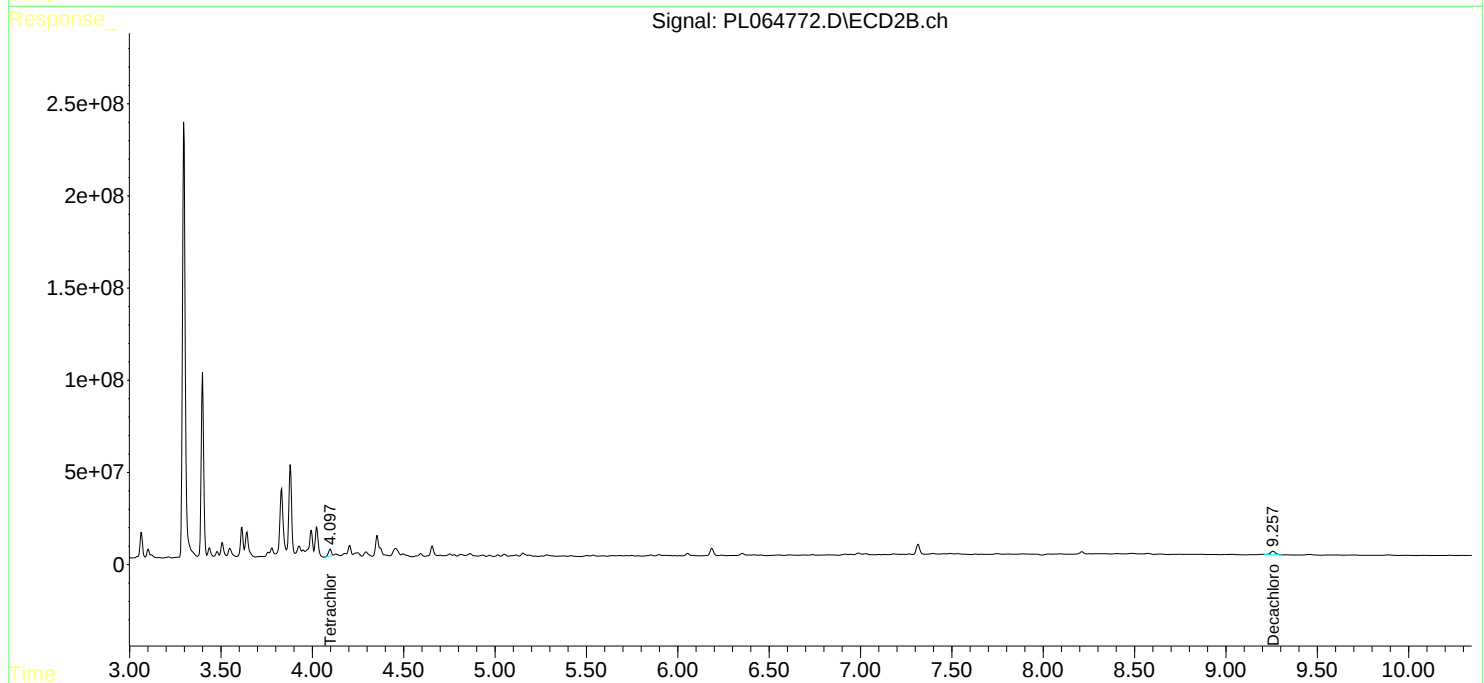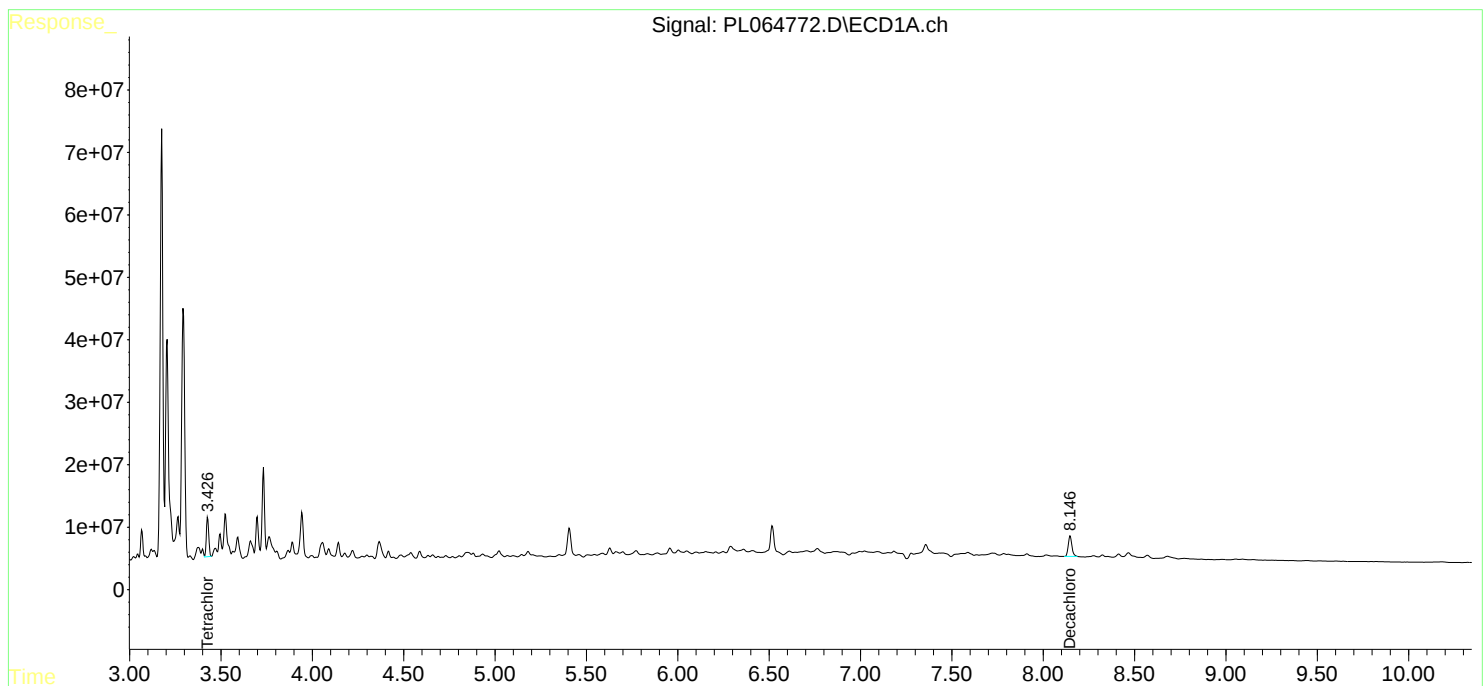

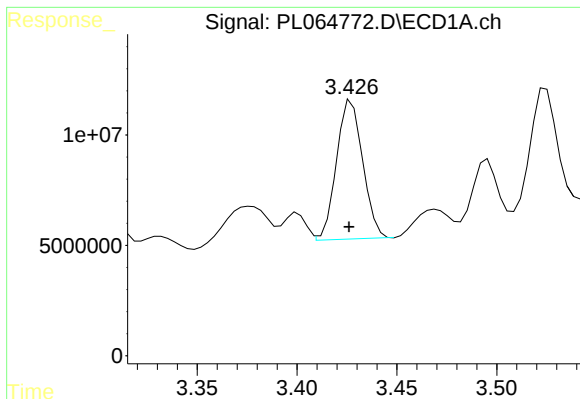


#1 Tetrachloro-m-xylene

R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 57344370
Conc: 20.38 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CHRT27339-CHRT20101


Manual Integrations
APPROVED

Ankita
2/12/2021 8:30:31 AM

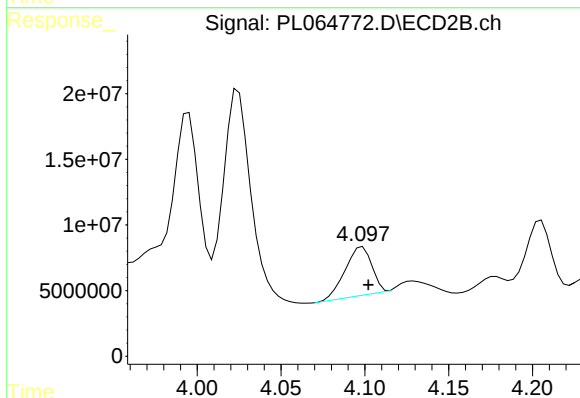


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: -0.003 min
Response: 40786155
Conc: 18.88 ng/ml

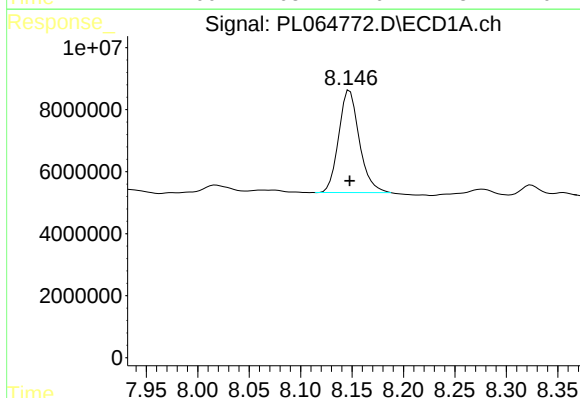

#28 Decachlorobiphenyl

R.T.: 8.148 min
Delta R.T.: 0.000 min
Response: 46105629
Conc: 20.50 ng/ml

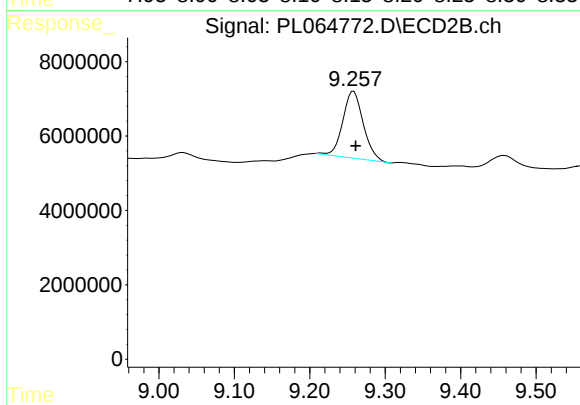

#28 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.003 min
Response: 33972832
Conc: 17.89 ng/ml