

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021122\
 Data File : PL072634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2022 22:48
 Operator : AR\AJ
 Sample : N1449-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20220038-FIELD-BLANK

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/14/2022
 Supervised By :Ankita Jodhani 02/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 04:17:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 05:14:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.576f	5.491	9682547	33749441	20.109	19.538
2)	SA Decachlor...	10.335f	11.386	10728730	22404237	14.172m	14.128

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021122\
Data File : PL072634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2022 22:48
Operator : AR\AJ
Sample : N1449-04
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20220038-FIELD-BLANK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/14/2022
Supervised By : Ankita Jodhani 02/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 04:17:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 05:14:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

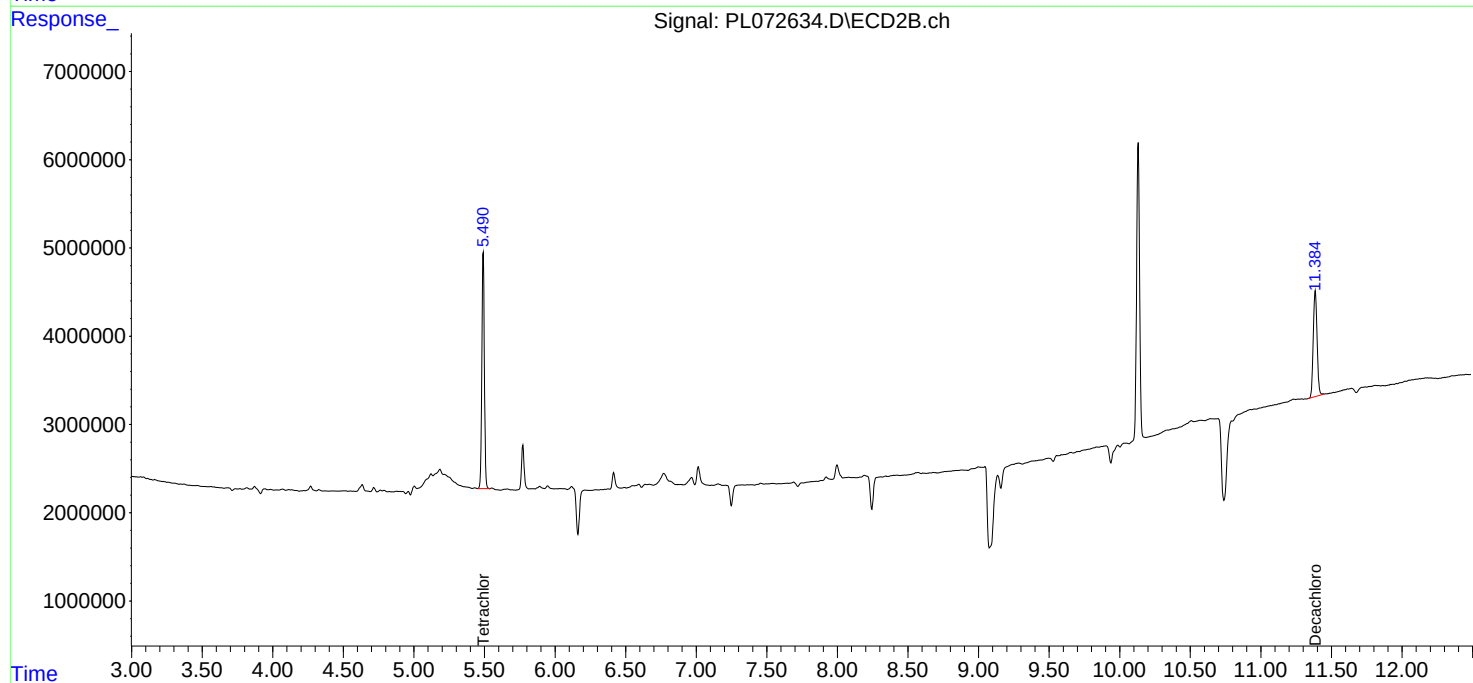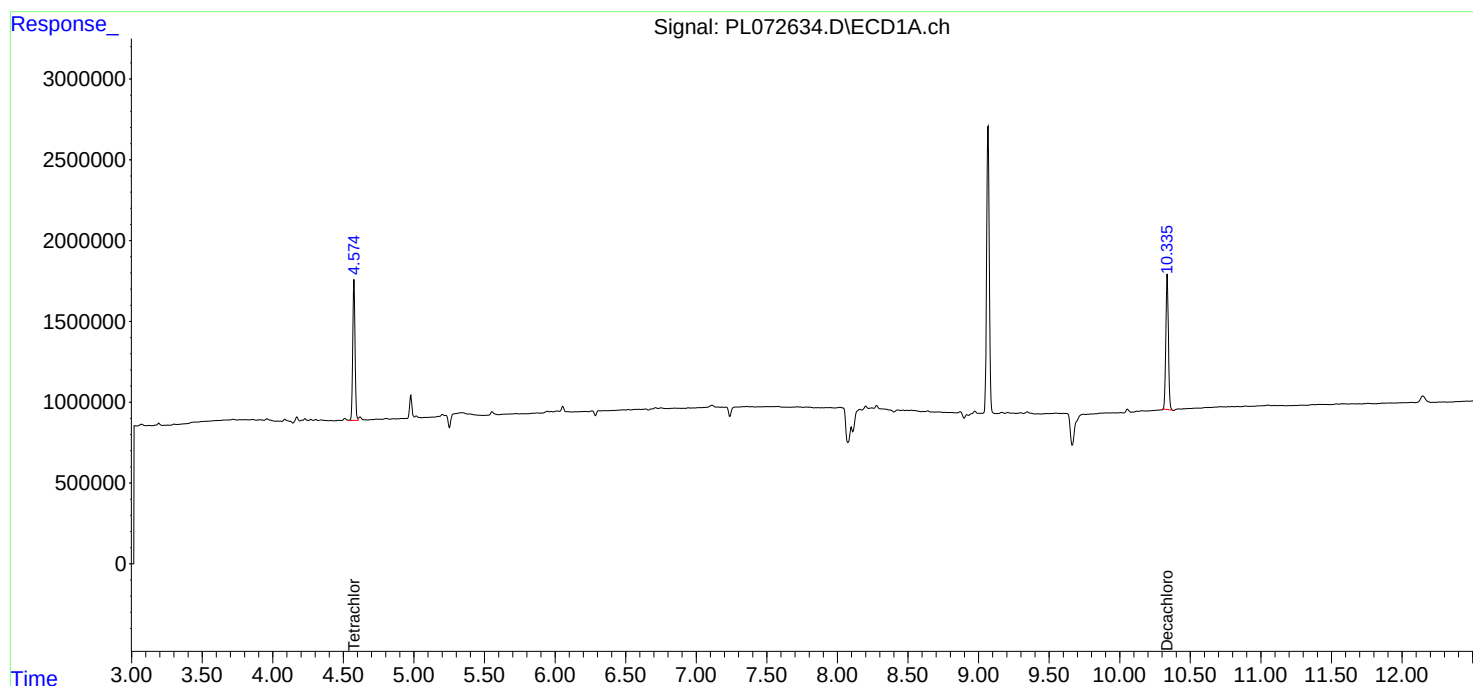

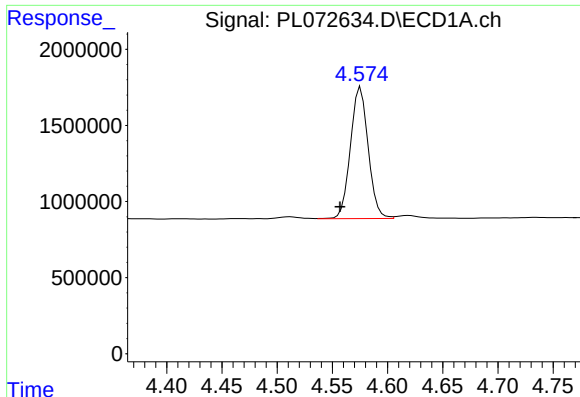


#1 Tetrachloro-m-xylene

R.T.: 4.576 min
Delta R.T.: 0.019 min
Response: 9682547
Conc: 20.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
20220038-FIELD-BLANK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/14/2022
Supervised By :Ankita Jodhani 02/14/2022

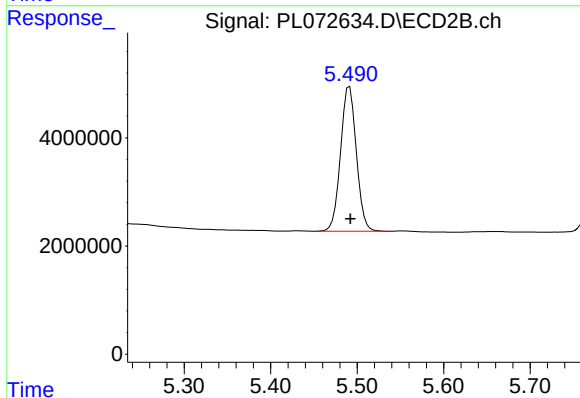


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.001 min
Response: 33749441
Conc: 19.54 ng/ml

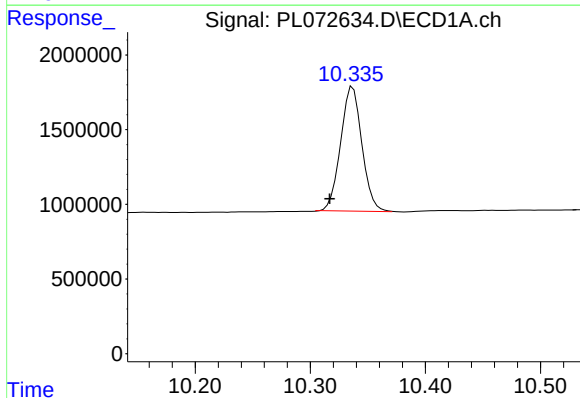

#28 Decachlorobiphenyl

R.T.: 10.335 min
Delta R.T.: 0.018 min
Response: 10728730
Conc: 14.17 ng/ml m

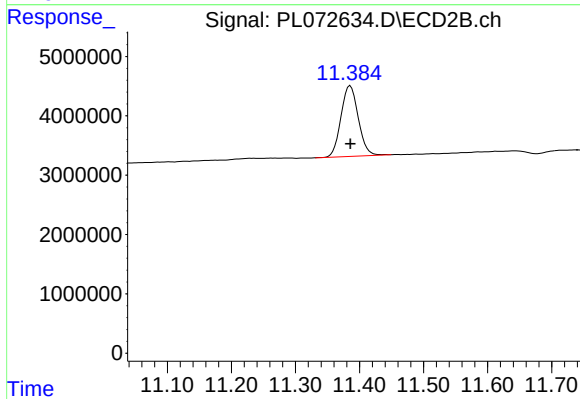

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: 0.000 min
Response: 22404237
Conc: 14.13 ng/ml