

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021122\
 Data File : PL072637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2022 23:39
 Operator : AR\AJ
 Sample : N1477-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20220073-105-21-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 04:18:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 05:14:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.491	9852047	34212428	20.461	19.806
28)	SA Decachlor...	10.317	11.385	15135438	31628789	19.993	19.945

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021122\
Data File : PL072637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2022 23:39
Operator : AR\AJ
Sample : N1477-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20220073-105-21-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 04:18:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 05:14:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

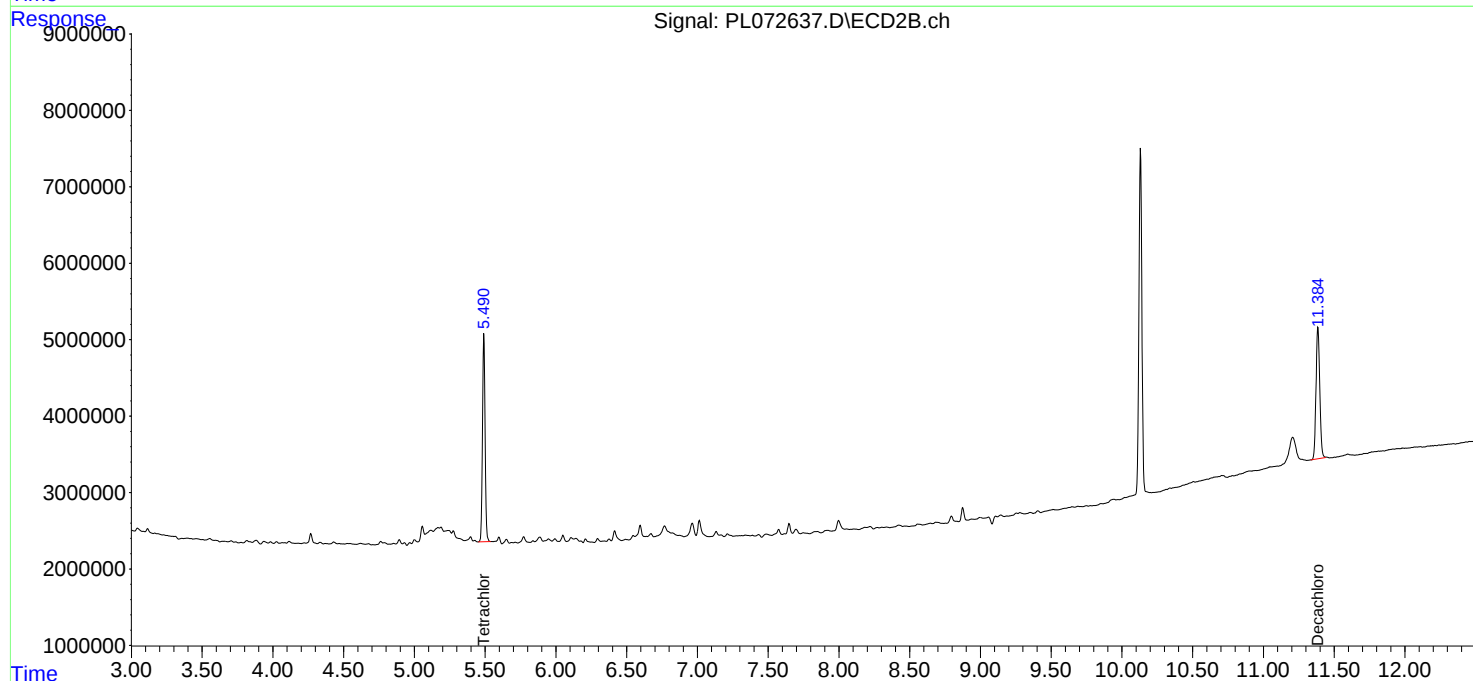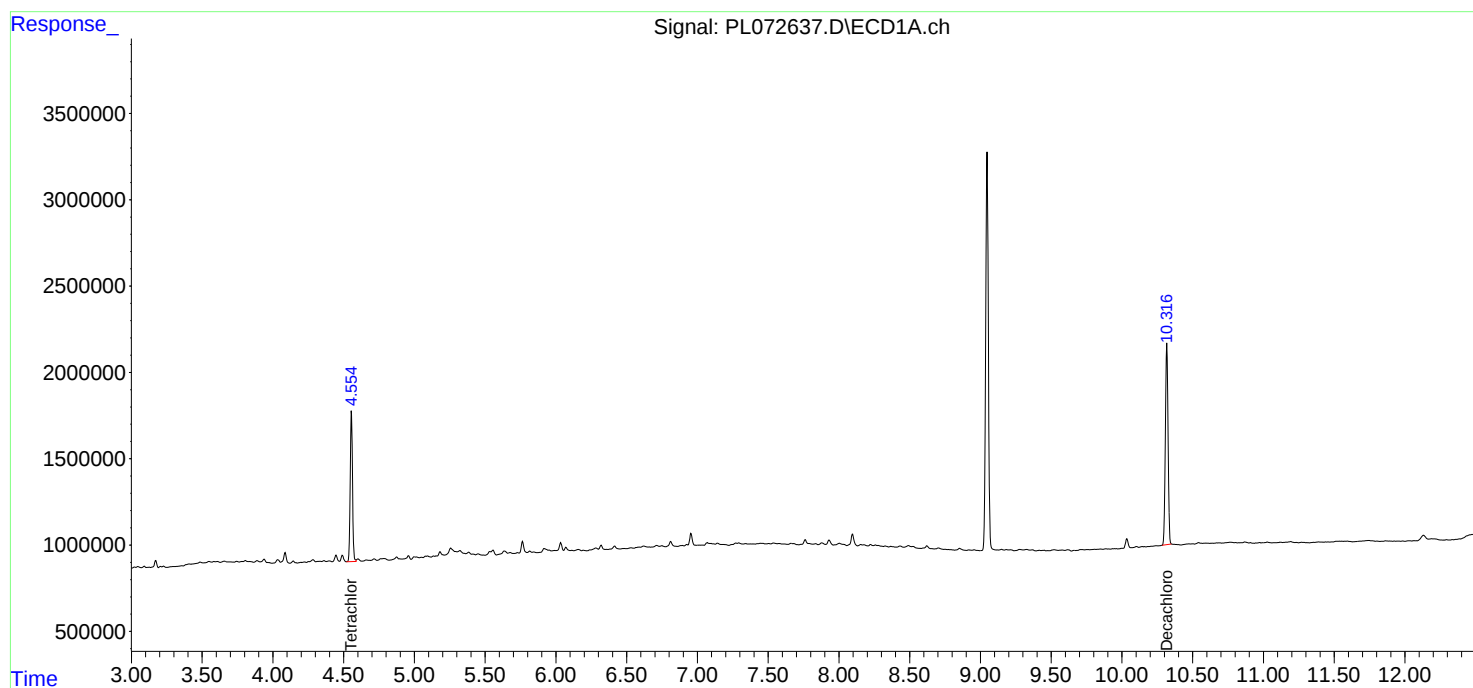


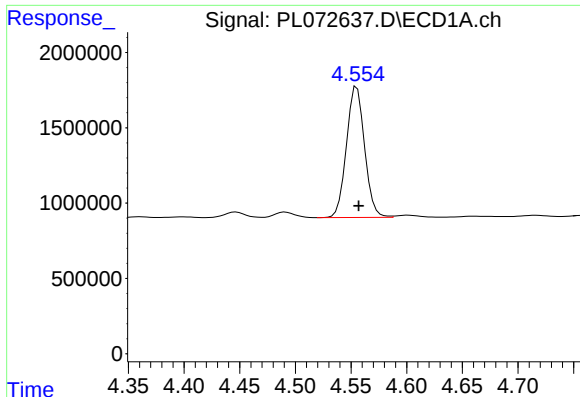

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.002 min
Response: 9852047
Conc: 20.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
20220073-105-21-SITE-WATER

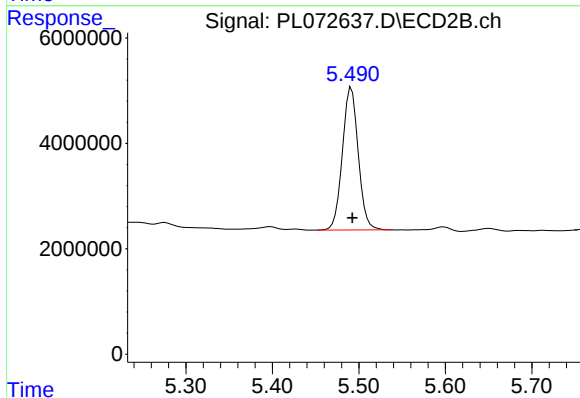


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.001 min
Response: 34212428
Conc: 19.81 ng/ml

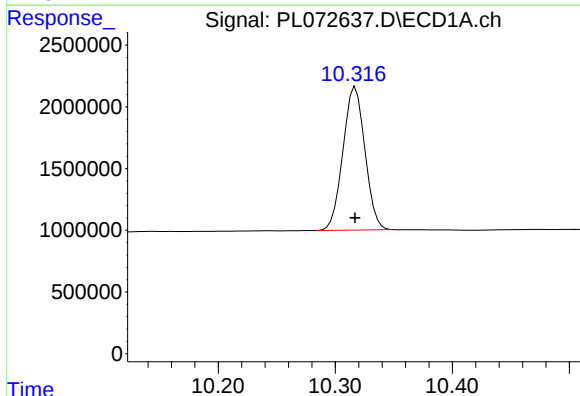

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: 0.000 min
Response: 15135438
Conc: 19.99 ng/ml

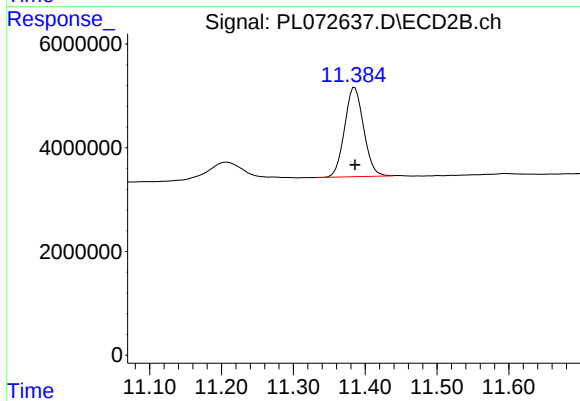

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: 0.000 min
Response: 31628789
Conc: 19.95 ng/ml