

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021219\
 Data File : PL044682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 14:27
 Operator : AJ\SJ
 Sample : K1458-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 00:04:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.984	57089877	19143749	8.023	8.149
28)	SA Decachlor...	8.049	9.043	76639154	24774643	10.508	11.186
Target Compounds							
4)	MA Heptachlor	0.000	5.188f	0	1749777	N.D.	0.574 #
8)	B Heptachlo...	0.000	5.847	0	1352589	N.D.	0.541 #
10)	B gamma-Chl...	5.282f	0.000	8937197	0	0.926	N.D. #
11)	B alpha-Chl...	0.000	6.165	0	5352788	N.D.	1.932 #
12)	B 4,4'-DDE	5.486	6.321	25445776	10497383	2.934	4.397 #
16)	A 4,4'-DDD	0.000	6.814	0	4001266	N.D.	2.084 #
17)	MA 4,4'-DDT	6.231	7.109	17608030	3133305	2.455	1.597 #
20)	A Methoxychlor	6.756f	0.000	5063790	0	1.262	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021219\
Data File : PL044682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 14:27
Operator : AJ\SJ
Sample : K1458-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 00:04:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

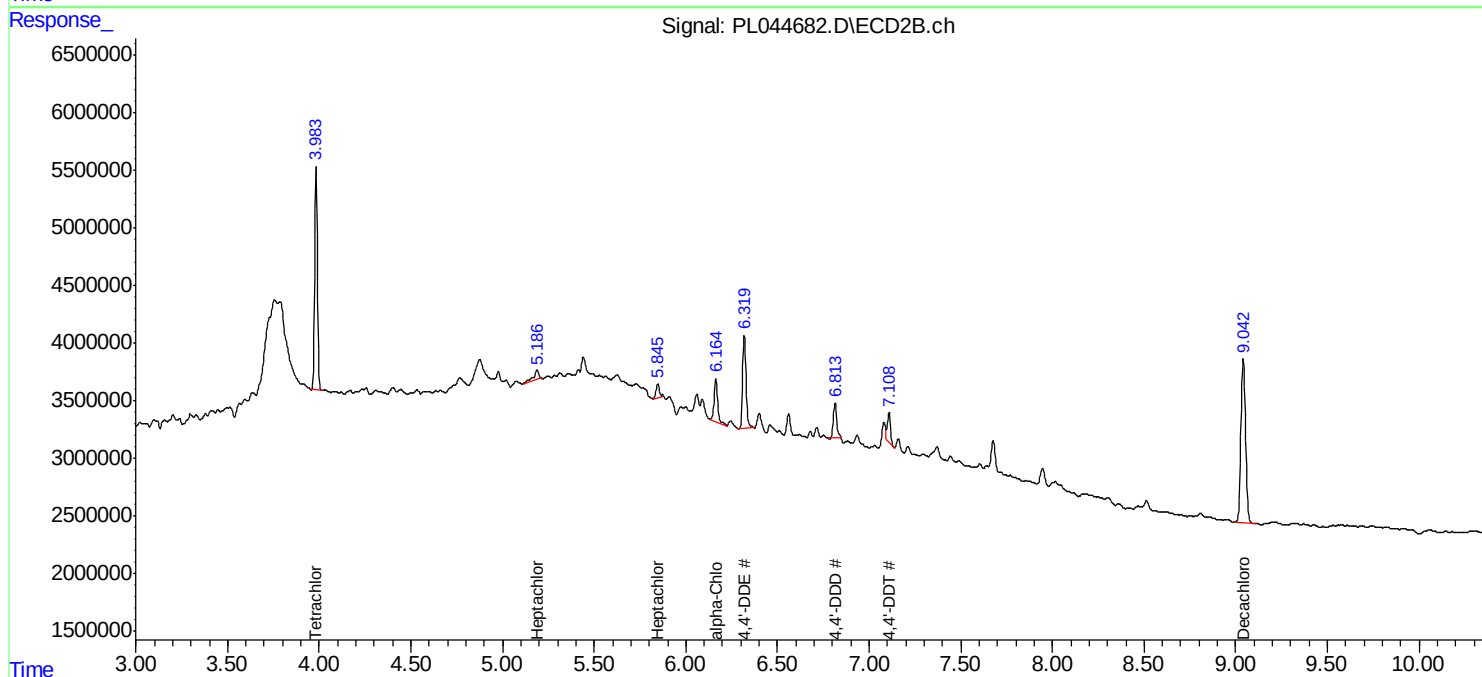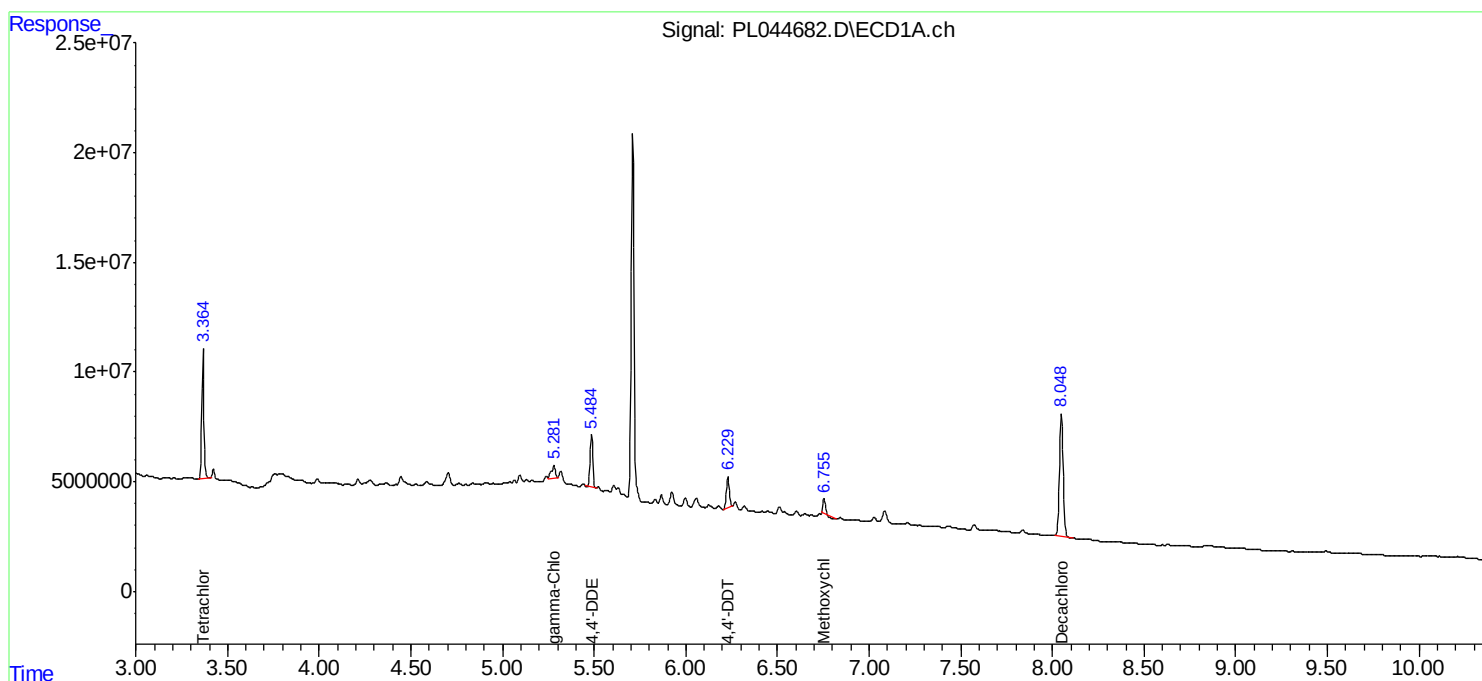


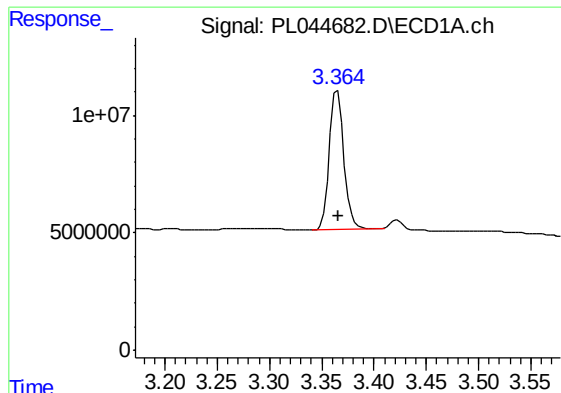

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 57089877
Conc: 8.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-1

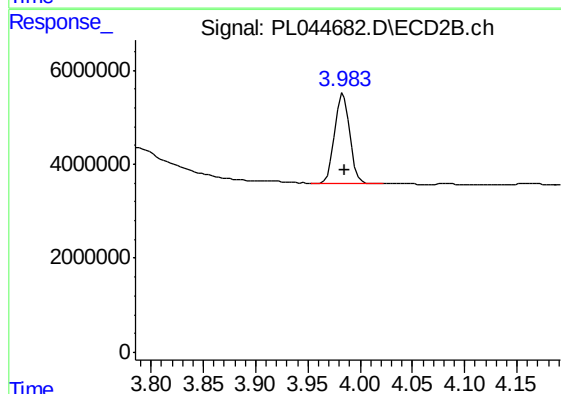


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 19143749
Conc: 8.15 ng/ml

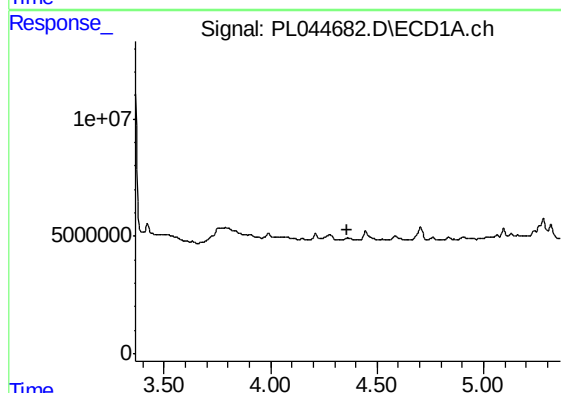


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.362 min
Response: 0
Conc: N.D.

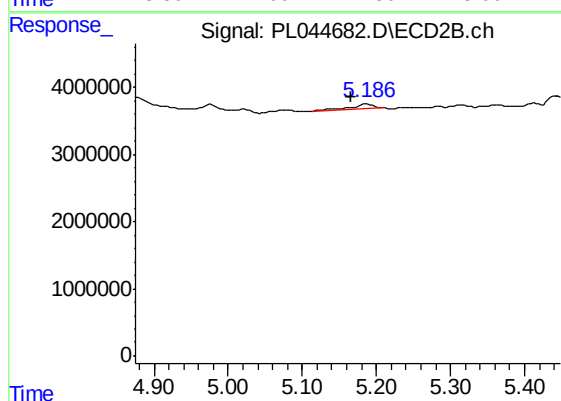

#4 Heptachlor


R.T.: 5.188 min
Delta R.T.: 0.022 min
Response: 1749777
Conc: 0.57 ng/ml

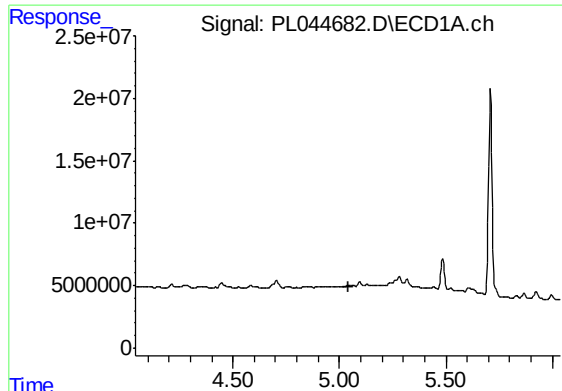

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-1

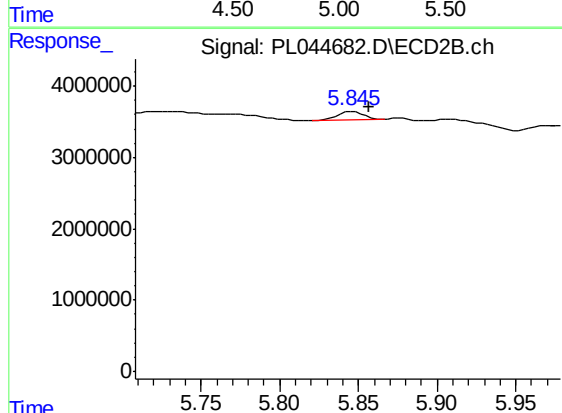


#8 Heptachlor epoxide

R.T.: 5.847 min
Delta R.T.: -0.010 min
Response: 1352589
Conc: 0.54 ng/ml

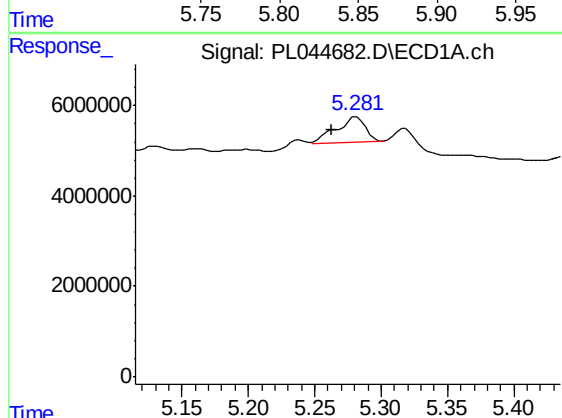


#10 gamma-Chlordane

R.T.: 5.282 min
Delta R.T.: 0.019 min
Response: 8937197
Conc: 0.93 ng/ml

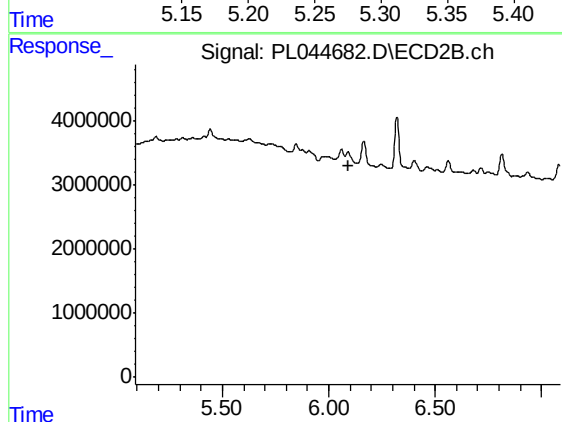

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.091 min
Response: 0
Conc: N.D.

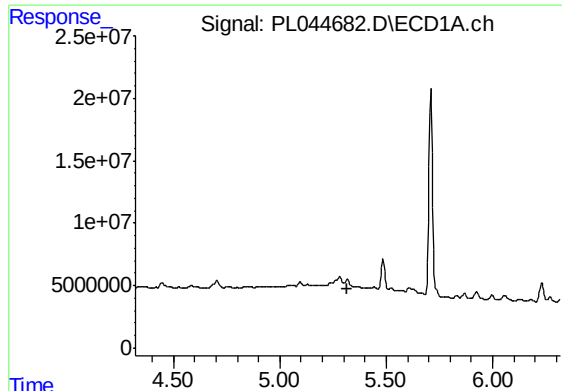

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-1

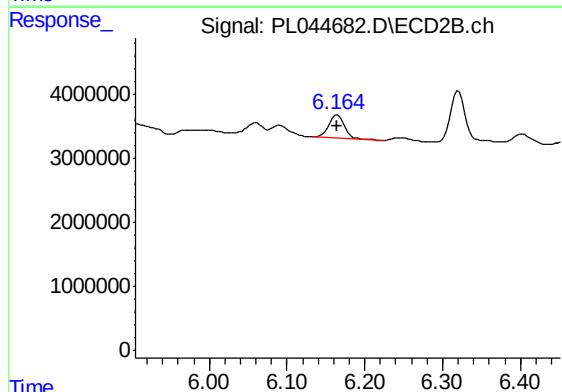


#11 alpha-Chlordane

R.T.: 6.165 min
Delta R.T.: 0.000 min
Response: 5352788
Conc: 1.93 ng/ml

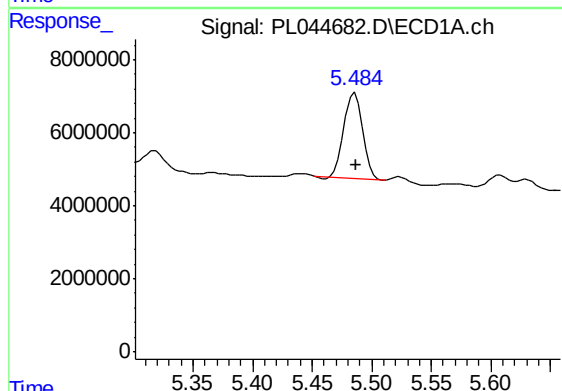


#12 4,4'-DDE

R.T.: 5.486 min
Delta R.T.: -0.001 min
Response: 25445776
Conc: 2.93 ng/ml

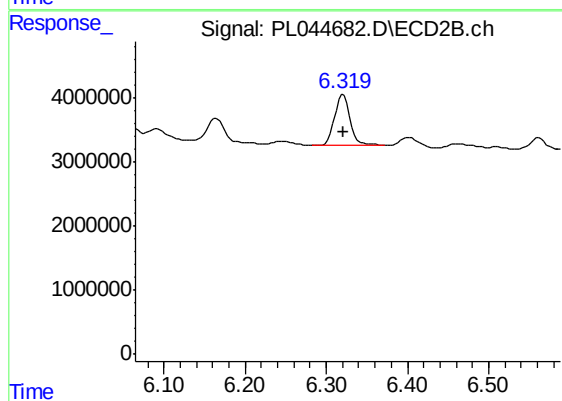

#12 4,4'-DDE


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 10497383
Conc: 4.40 ng/ml

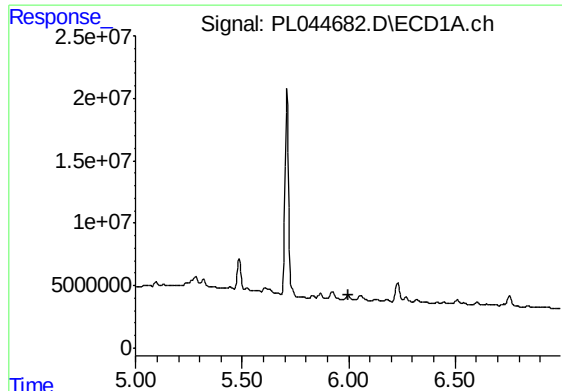

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-1

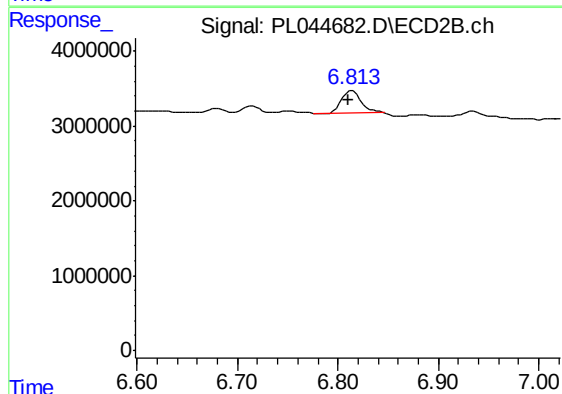


#16 4,4'-DDD

R.T.: 6.814 min
Delta R.T.: 0.003 min
Response: 4001266
Conc: 2.08 ng/ml

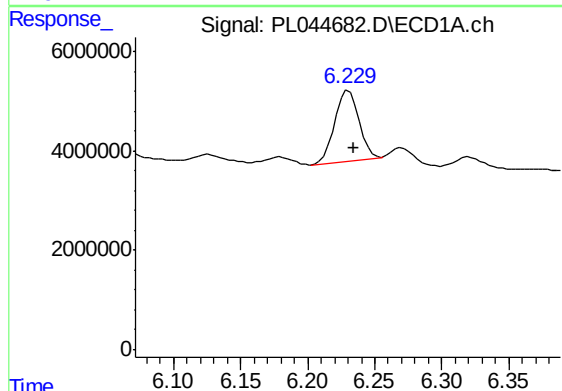


#17 4,4'-DDT

R.T.: 6.231 min
Delta R.T.: -0.003 min
Response: 17608030
Conc: 2.46 ng/ml

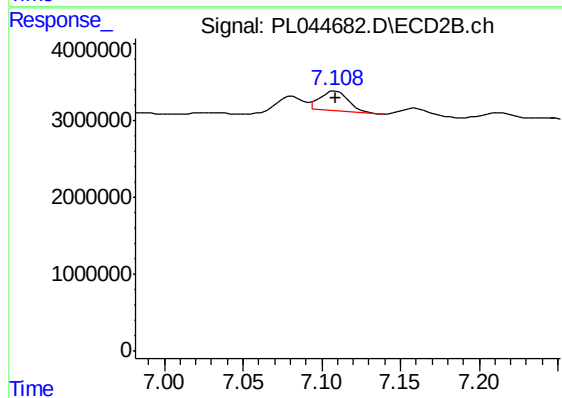

#17 4,4'-DDT


R.T.: 7.109 min
Delta R.T.: 0.000 min
Response: 3133305
Conc: 1.60 ng/ml

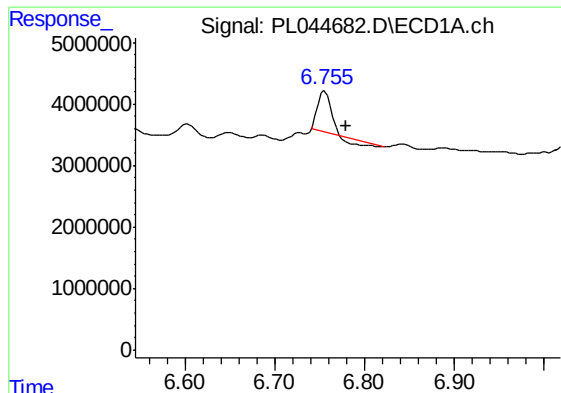

#20 Methoxychlor


R.T.: 6.756 min
Delta R.T.: -0.023 min
Response: 5063790
Conc: 1.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-1

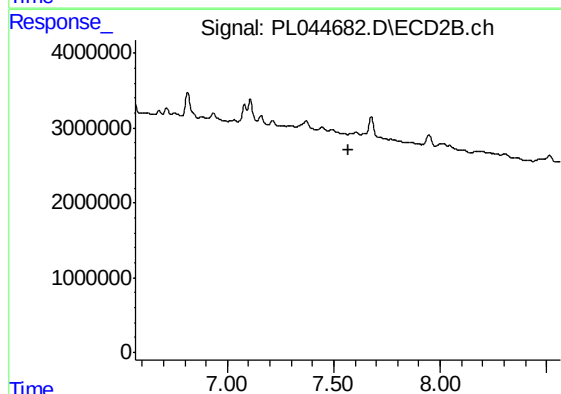


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.567 min
Response: 0
Conc: N.D.

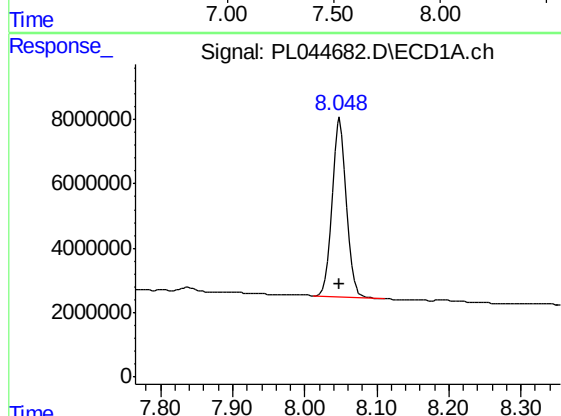

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.000 min
Response: 76639154
Conc: 10.51 ng/ml

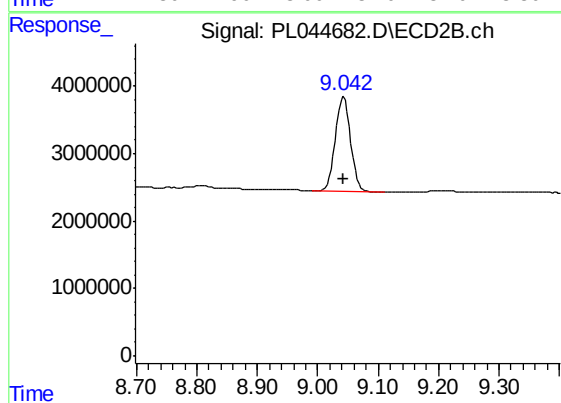

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 24774643
Conc: 11.19 ng/ml