

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021219\
 Data File : PL044691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 17:04
 Operator : AJ\SJ
 Sample : K1459-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 M-10-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 00:06:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.365	3.985	65337277	22191616	9.182	9.447
28) SA Decachlor...	8.050	9.044	86346066	26840094	11.839	12.118
Target Compounds						
11) B alpha-Chl...	0.000	6.166	0	1858872	N.D.	0.671 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021219\
Data File : PL044691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 17:04
Operator : AJ\SJ
Sample : K1459-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
M-10-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 00:06:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

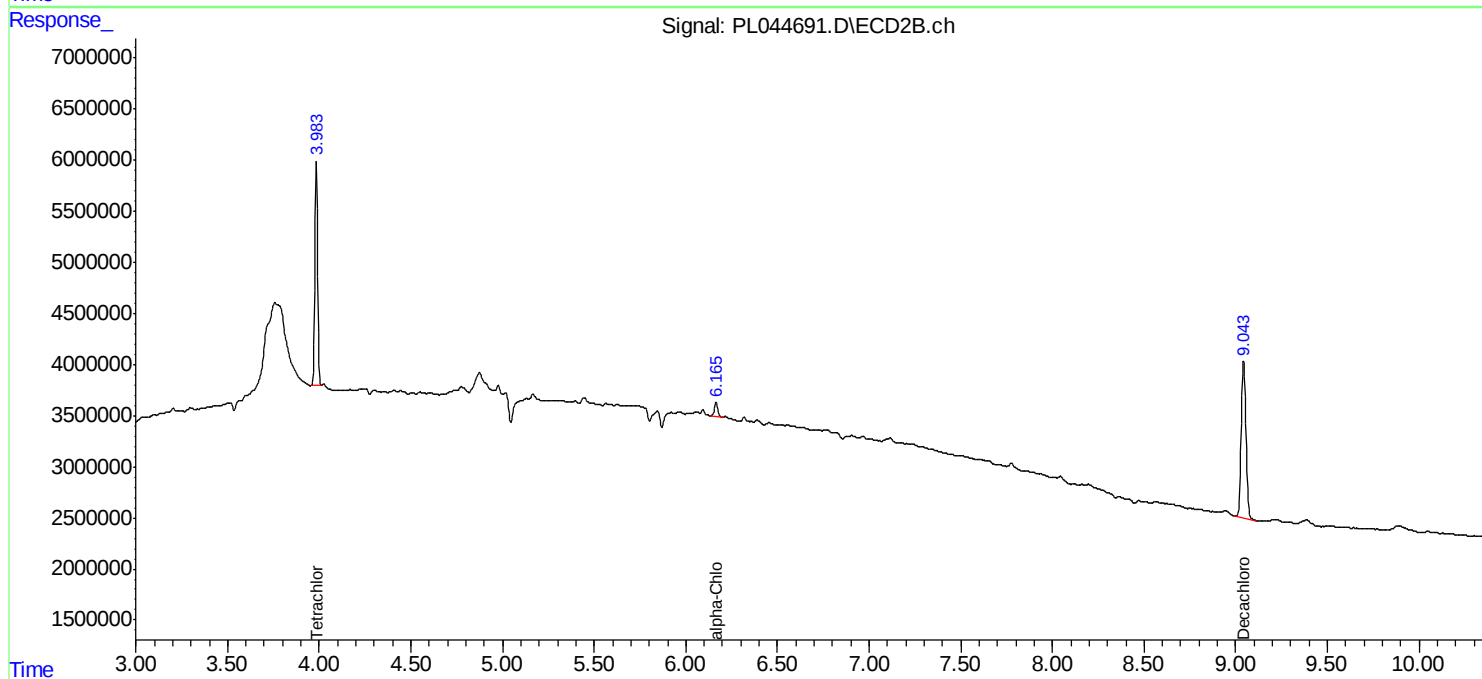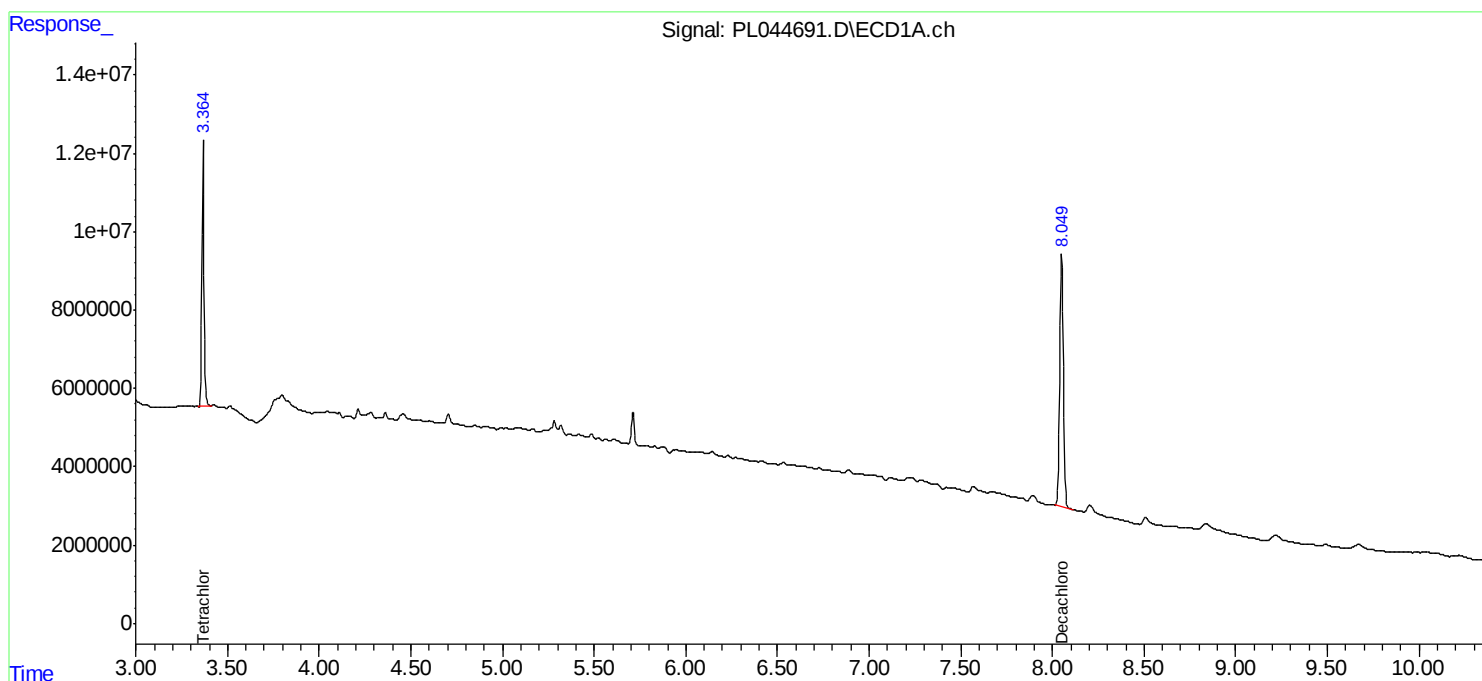


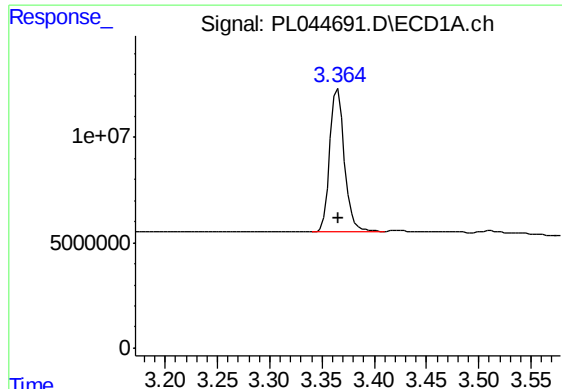

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 65337277
Conc: 9.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-10-S

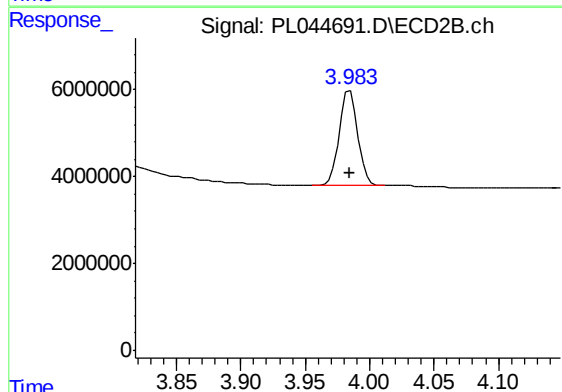


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 22191616
Conc: 9.45 ng/ml

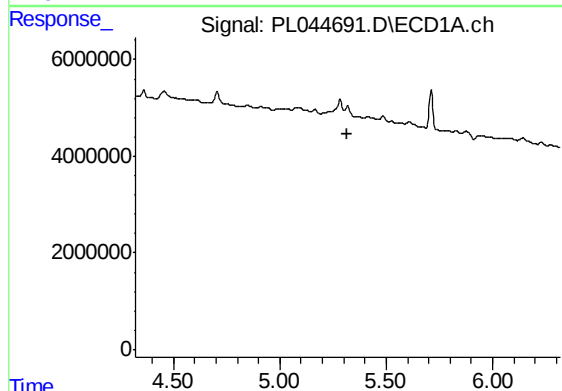


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.319 min
Response: 0
Conc: N.D.

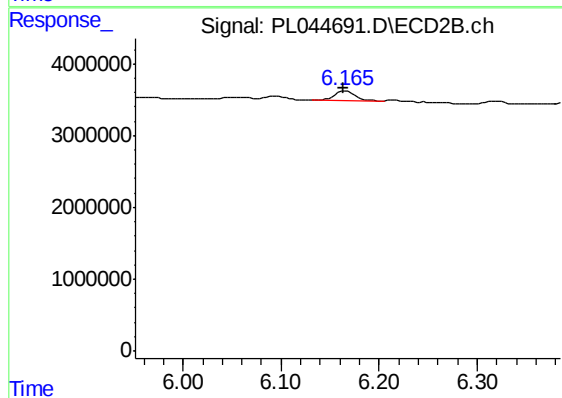

#11 alpha-Chlordane


R.T.: 6.166 min
Delta R.T.: 0.002 min
Response: 1858872
Conc: 0.67 ng/ml

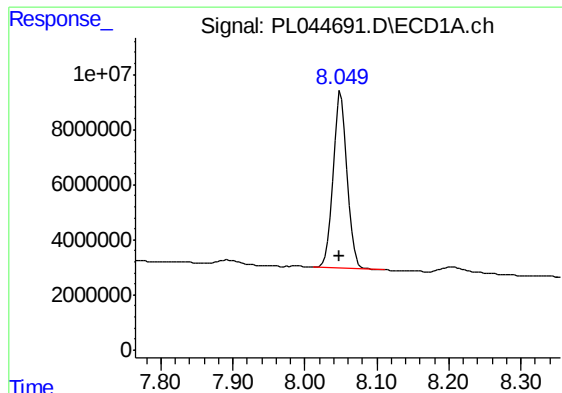

#28 Decachlorobiphenyl

R.T.: 8.050 min
Delta R.T.: 0.000 min
Response: 86346066
Conc: 11.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-10-S

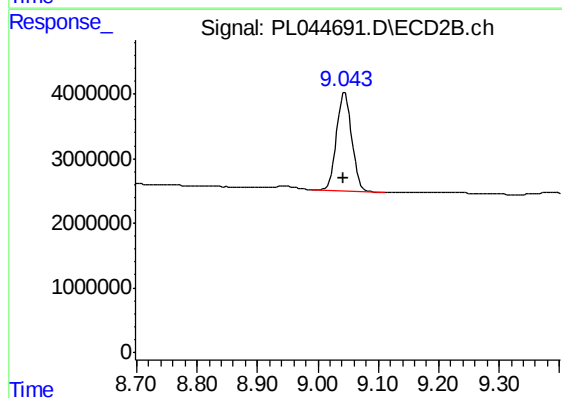

#28 Decachlorobiphenyl

R.T.: 9.044 min
Delta R.T.: 0.001 min
Response: 26840094
Conc: 12.12 ng/ml