

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021219\
 Data File : PL044694.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 17:46
 Operator : AJ\SJ
 Sample : K1461-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-PIT-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 00:06:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.365	3.984	52137205	17609683	7.327	7.496
28) SA Decachlor...	8.050	9.045	68357618	20258907	9.372	9.147
Target Compounds						
12) B 4,4'-DDE	5.485	6.321	8034168	2704974	0.926	1.133



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021219\
Data File : PL044694.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 17:46
Operator : AJ\SJ
Sample : K1461-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 00:06:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

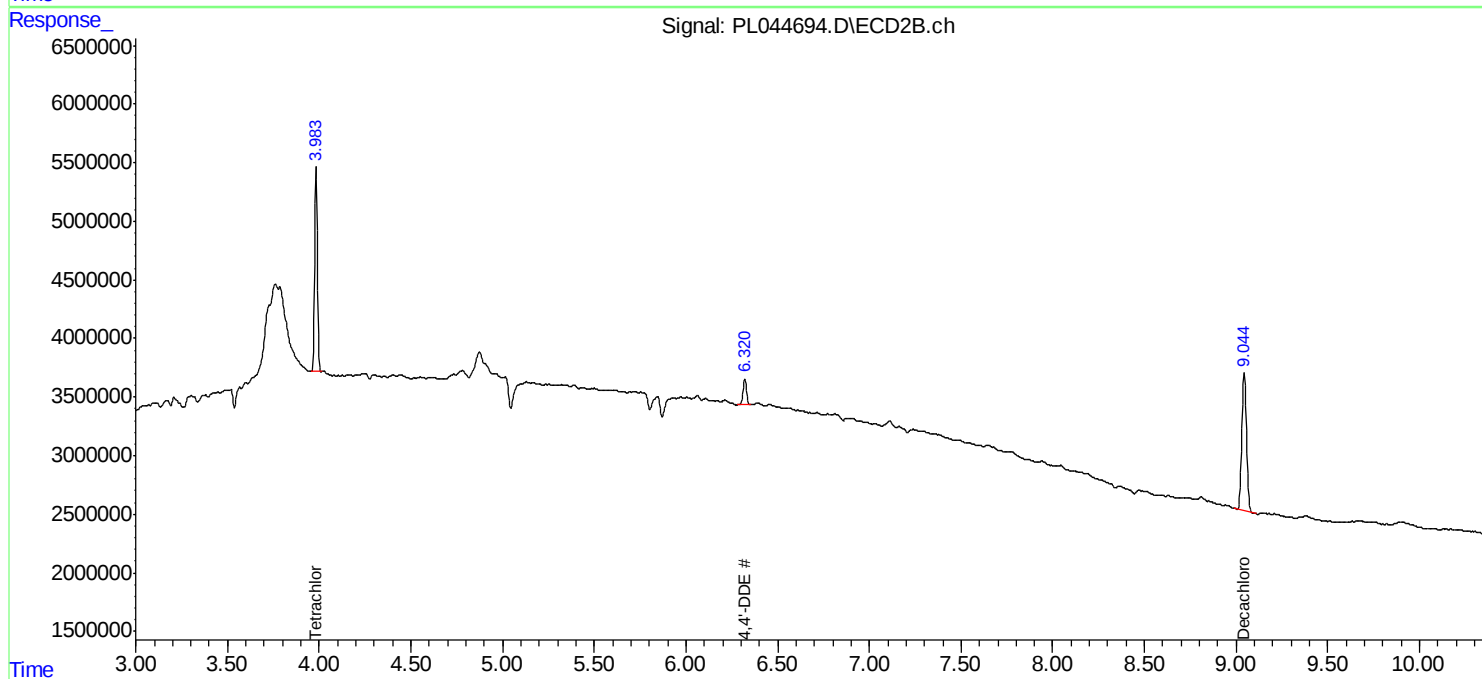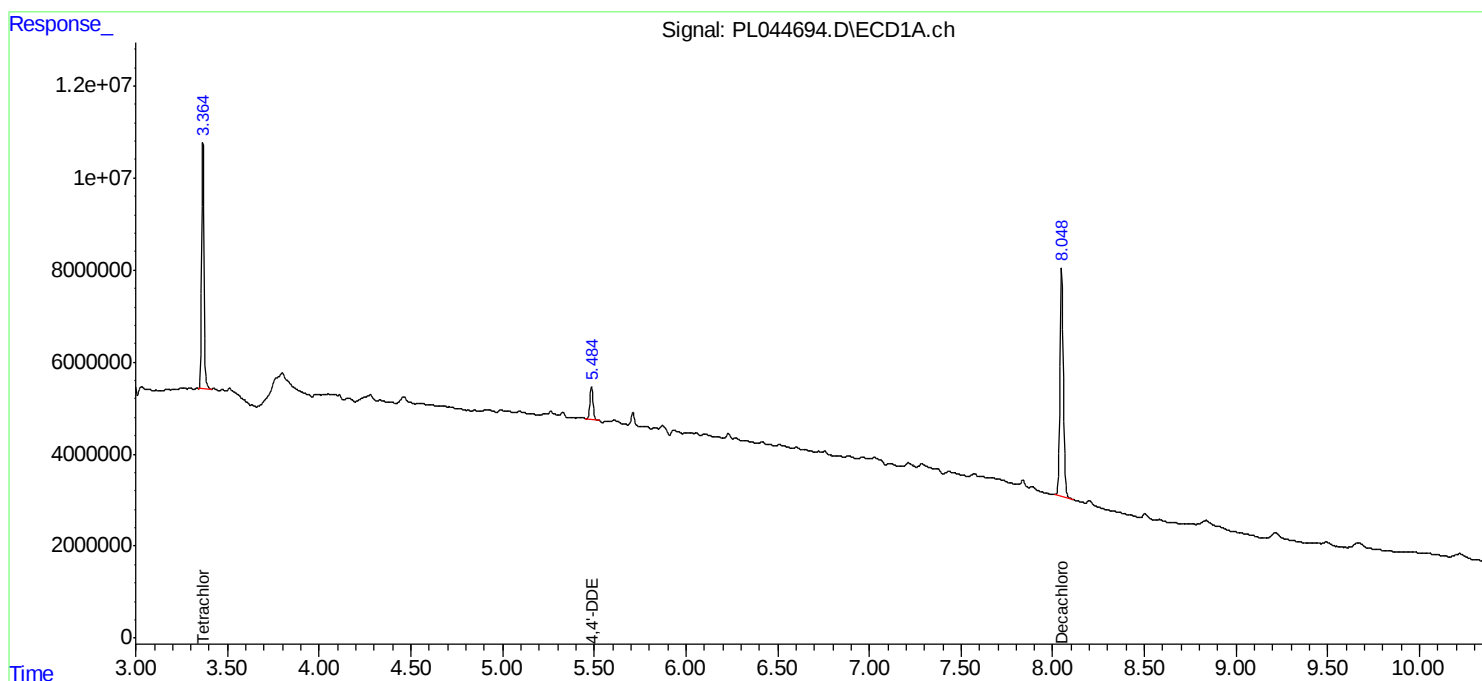


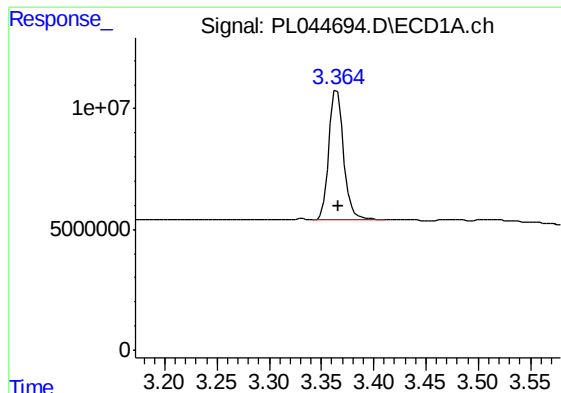

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 52137205
Conc: 7.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-3

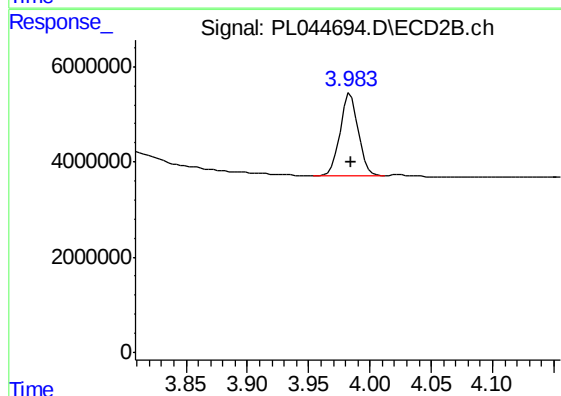


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 17609683
Conc: 7.50 ng/ml

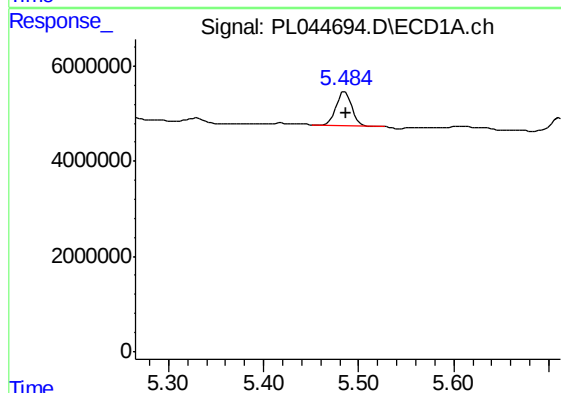


#12 4,4'-DDE

R.T.: 5.485 min
Delta R.T.: -0.002 min
Response: 8034168
Conc: 0.93 ng/ml

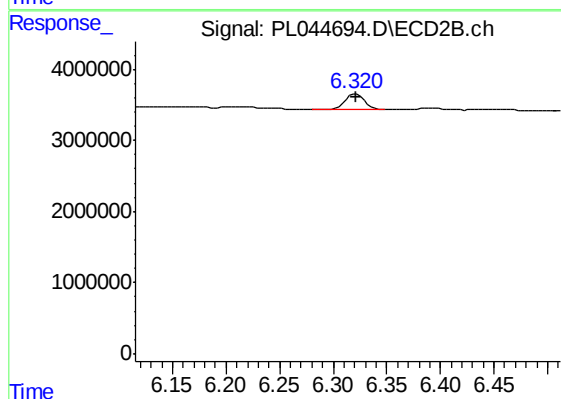

#12 4,4'-DDE


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 2704974
Conc: 1.13 ng/ml

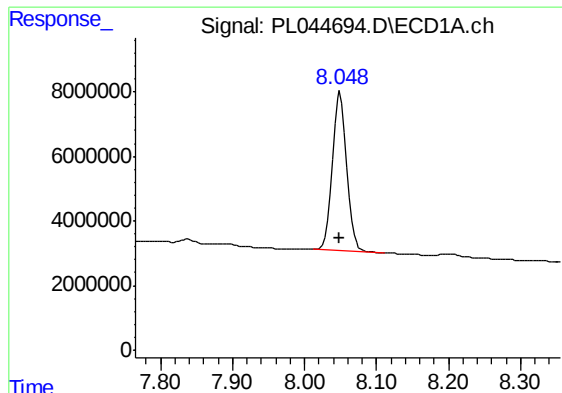

#28 Decachlorobiphenyl

R.T.: 8.050 min
Delta R.T.: 0.000 min
Response: 68357618
Conc: 9.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-3

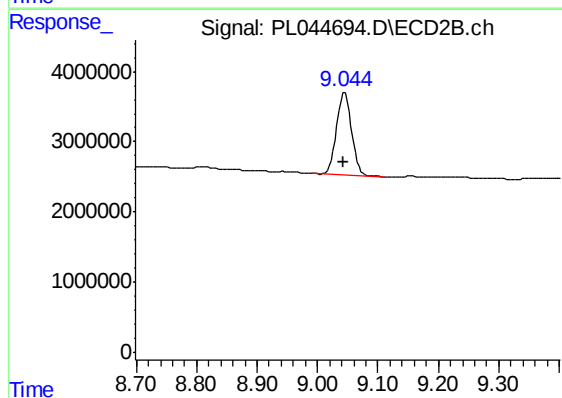

#28 Decachlorobiphenyl

R.T.: 9.045 min
Delta R.T.: 0.002 min
Response: 20258907
Conc: 9.15 ng/ml