

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021219\
 Data File : PL044687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2019 15:37
 Operator : AJ\SJ
 Sample : K1458-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-6

Manual Integrations
 APPROVED

Sohil
 2/13/2019 2:39:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 00:05:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.365	3.984	49548531	16842000	6.963	7.169
28) SA Decachlor...	8.049	9.043	66472366	19764776	9.114	8.924
Target Compounds						
12) B 4,4'-DDE	5.485	6.321	116.7E6	40296049	13.453m	16.877 #
17) MA 4,4'-DDT	6.232	7.108	205.3E6	48966340	28.629	24.960m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021219\
Data File : PL044687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2019 15:37
Operator : AJ\SJ
Sample : K1458-09
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-6


Manual Integrations
APPROVED

Sohil
2/13/2019 2:39:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 00:05:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

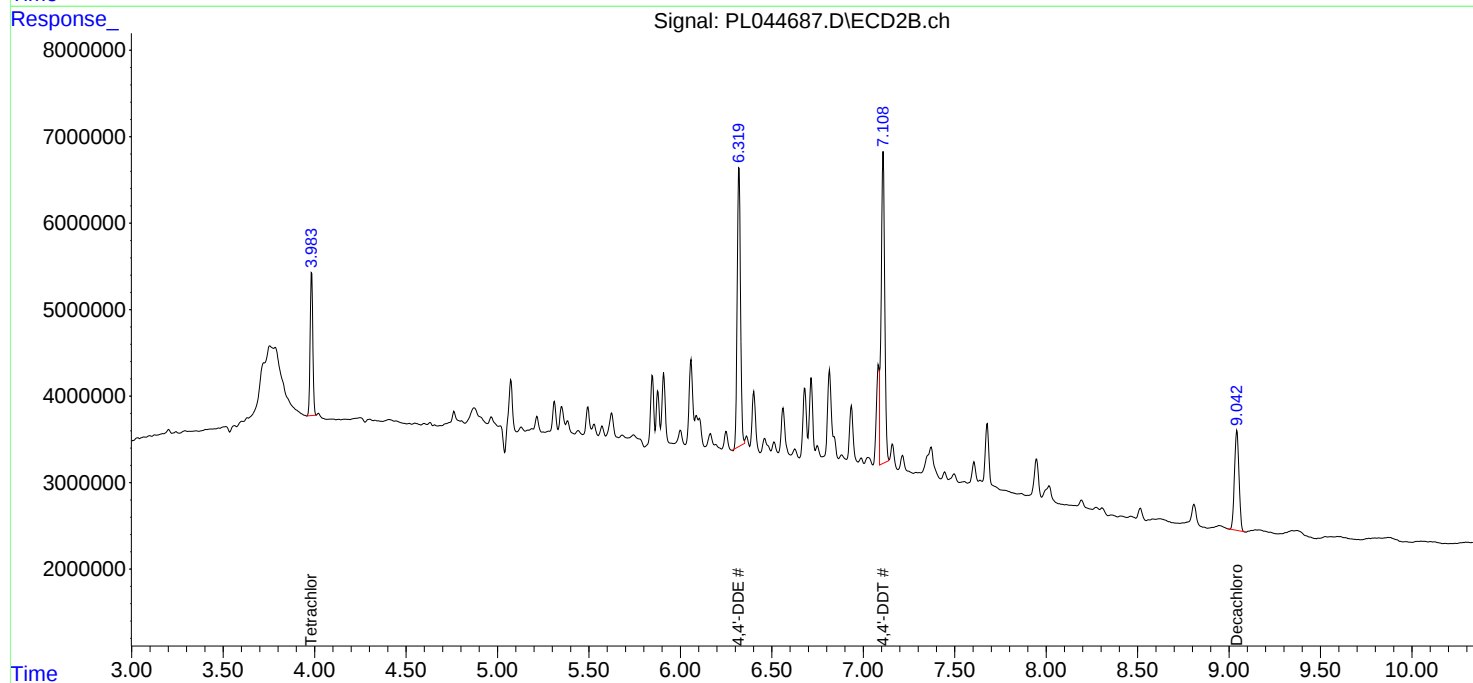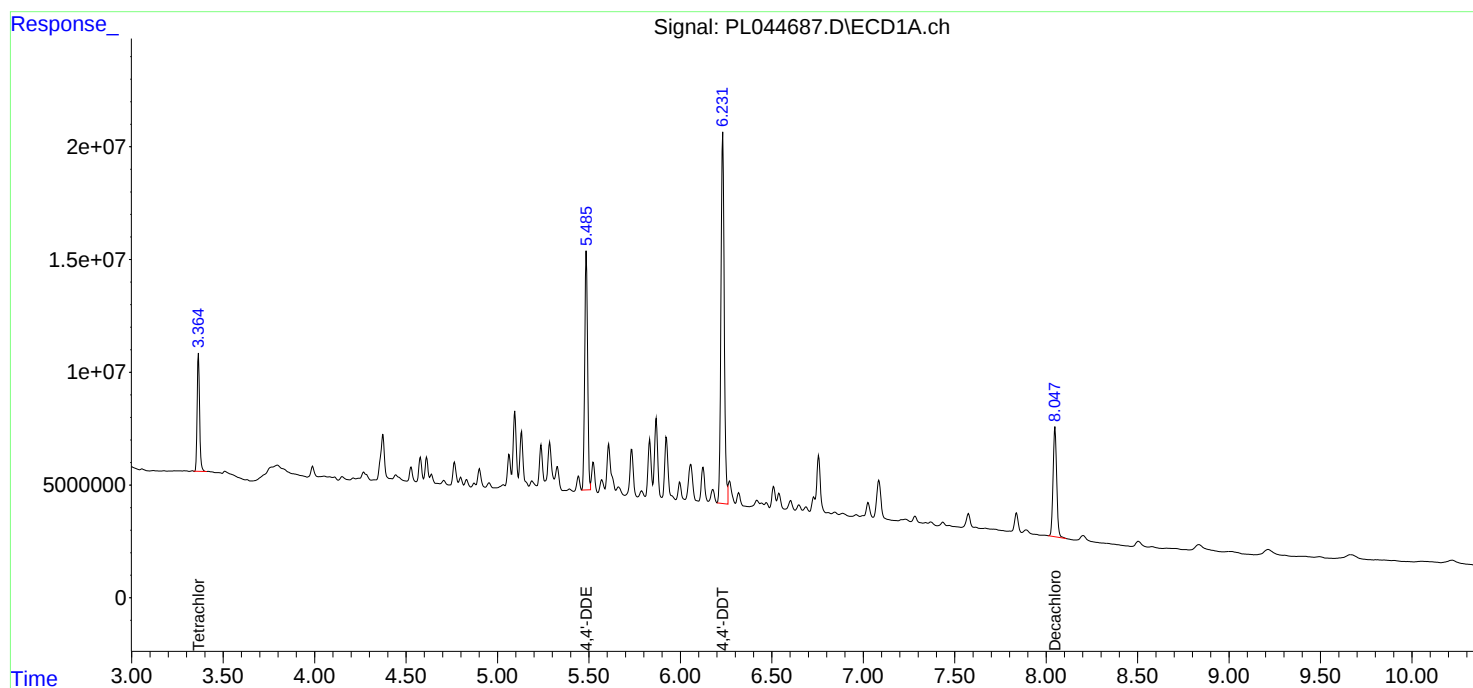

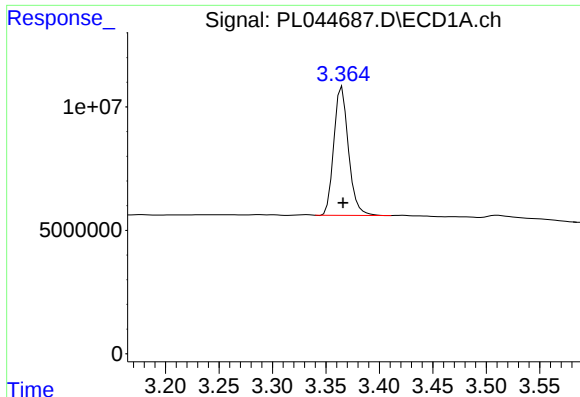


#1 Tetrachloro-m-xylene

R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 49548531
Conc: 6.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6


Manual Integrations
APPROVED

Sohil
2/13/2019 2:39:26 PM

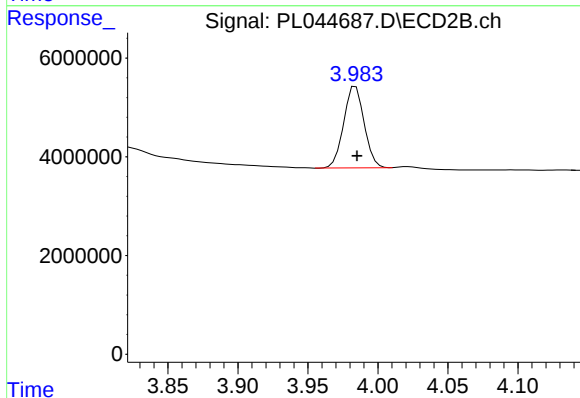


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 16842000
Conc: 7.17 ng/ml

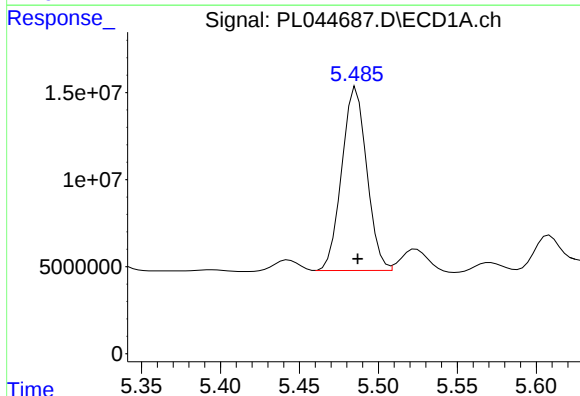


#12 4,4'-DDE

R.T.: 5.485 min
Delta R.T.: -0.002 min
Response: 116665897
Conc: 13.45 ng/ml m

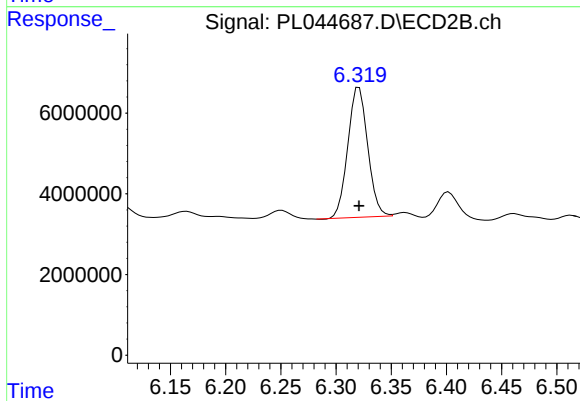

#12 4,4'-DDE

R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 40296049
Conc: 16.88 ng/ml

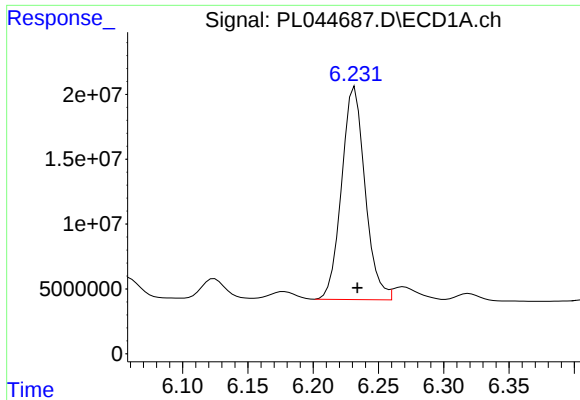


#17 4,4'-DDT

R.T.: 6.232 min
Delta R.T.: -0.002 min
Response: 205305742
Conc: 28.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6


Manual Integrations
APPROVED

Sohil
2/13/2019 2:39:26 PM

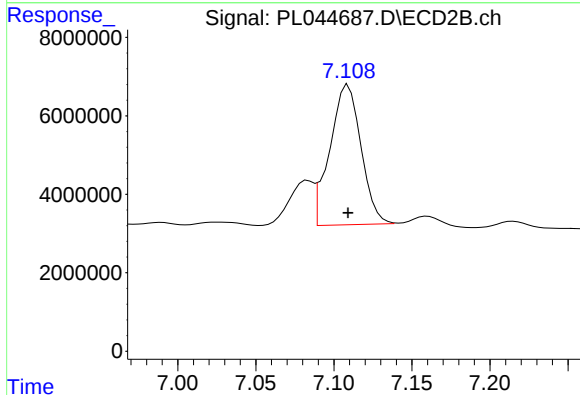


#17 4,4'-DDT

R.T.: 7.108 min
Delta R.T.: -0.001 min
Response: 48966340
Conc: 24.96 ng/ml m

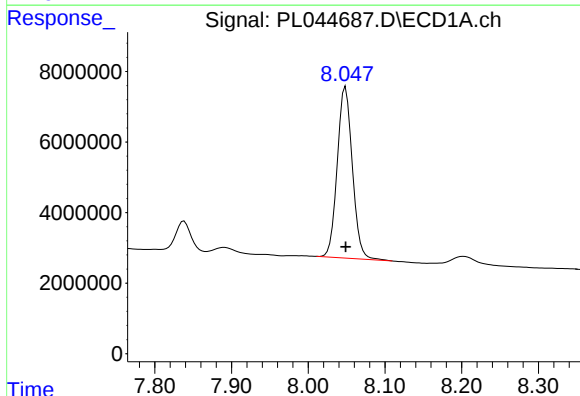

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.000 min
Response: 66472366
Conc: 9.11 ng/ml

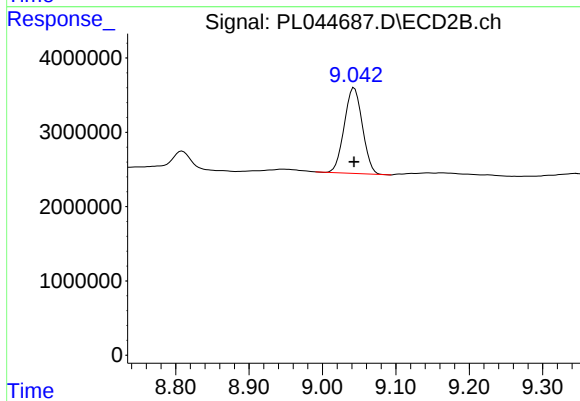

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 19764776
Conc: 8.92 ng/ml