

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021220\
 Data File : PL056499.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2020 15:10
 Operator : AJ\MA
 Sample : RESCHEK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHEK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 05:40:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 13 05:32:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.019	186.2E6	57570889	21.099	21.162
28)	SA Decachlor...	8.249	9.090	215.6E6	44250325	22.509	21.694
Target Compounds							
9)	A Endosulfan I	5.550	6.249	132.4E6	28163963	10.548	10.129
10)	B gamma-Chl...	5.438	6.126	124.0E6	28595149	9.018	9.776
12)	B 4,4'-DDE	5.659	6.356	253.4E6	55517665	19.931	19.813
13)	MA Dieldrin	5.794	6.506	262.4E6	59127679	19.672	20.316
14)	MA Endrin	6.056	0.000	147.5E6	0	12.595	N.D. #
18)	B Endrin al...	6.487	0.000	81948733	0	8.540	N.D. #
19)	B Endosulfa...	6.707	7.283	161.8E6	46543362	15.200	19.640 #
20)	A Methoxychlor	6.960	7.606	542.7E6	117.2E6	110.278	102.031
21)	B Endrin ke...	7.197	7.754	231.7E6	50282292	19.379	20.011
25)	Chlordane-3	5.438	6.126	124.0E6	28595149	94.479	73.790



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021220\
Data File : PL056499.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2020 15:10
Operator : AJ\MA
Sample : RESCHEK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RESCHEK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 05:40:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
Quant Title : GC Extractables
QLast Update : Thu Feb 13 05:32:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

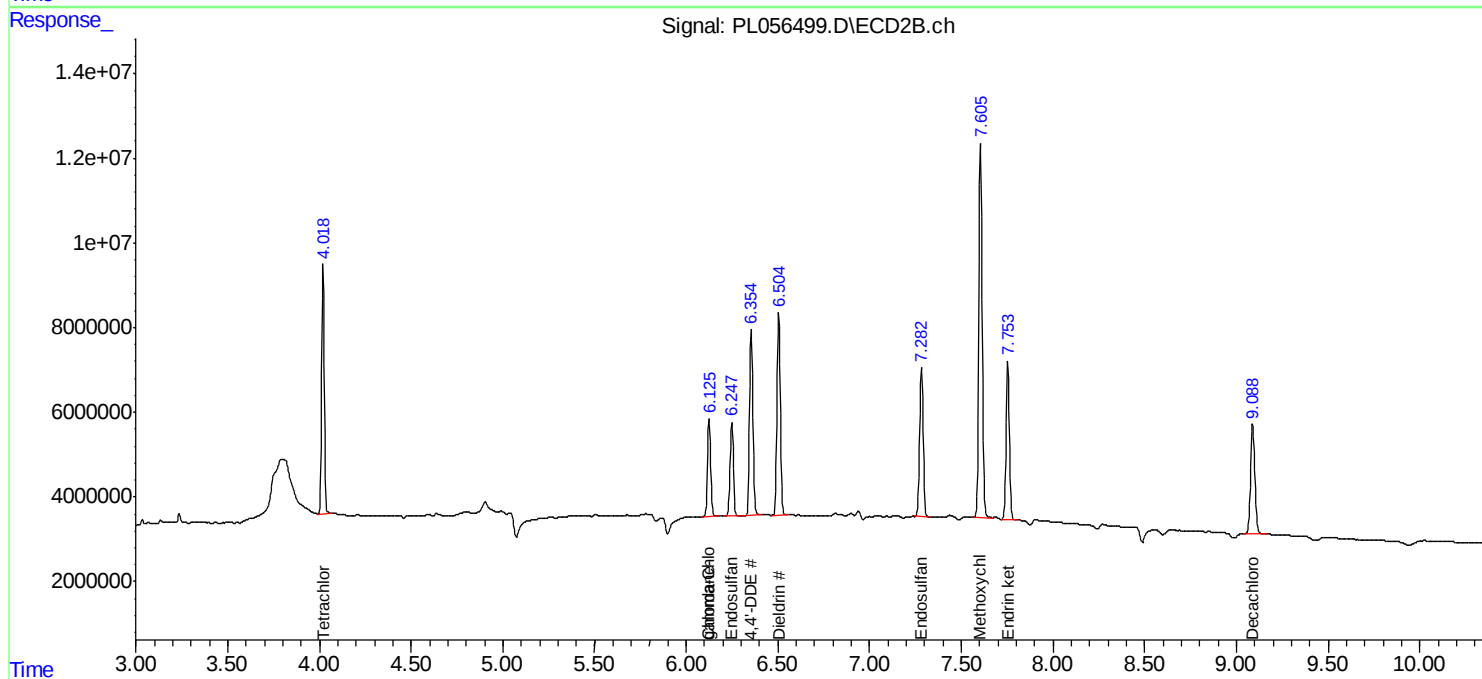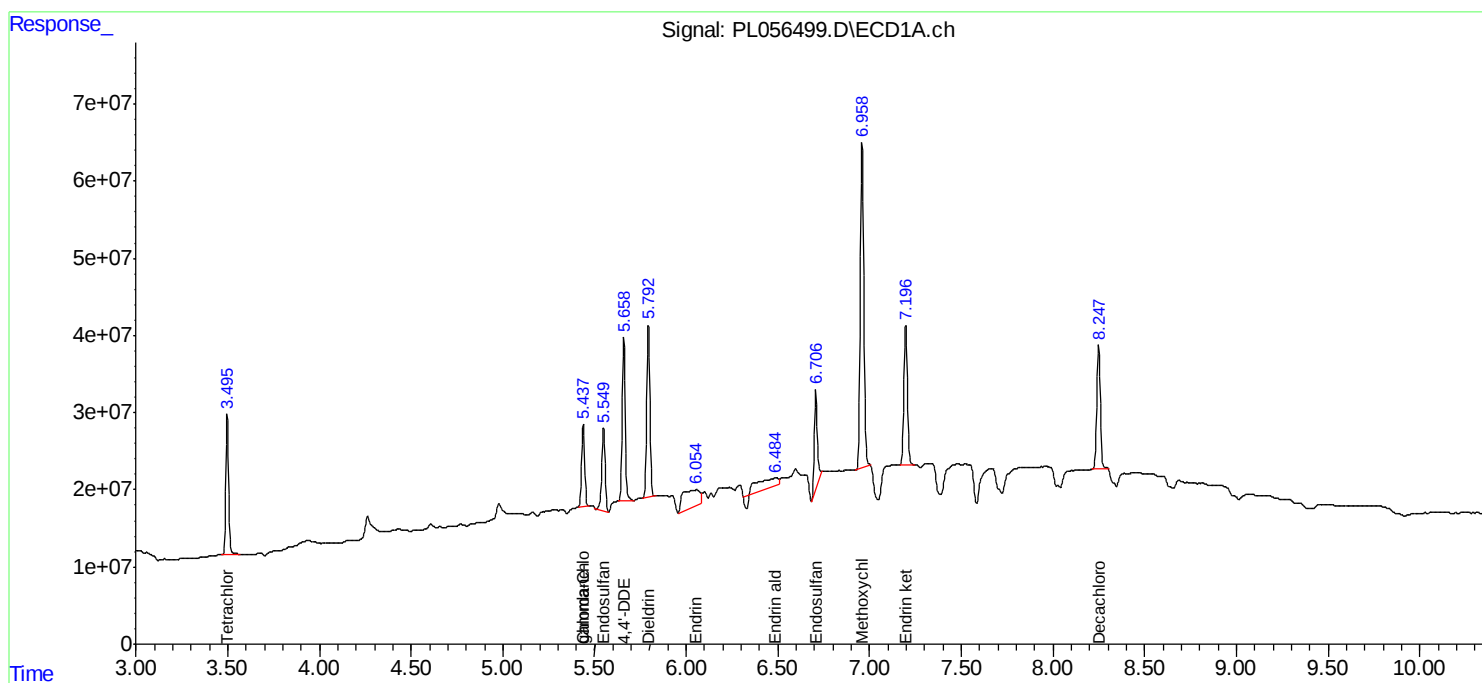


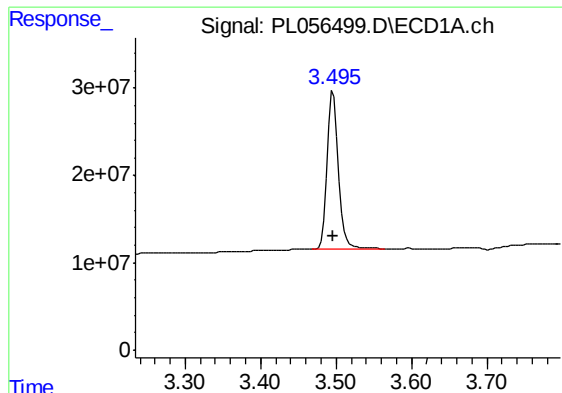

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 186170756
Conc: 21.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHEK

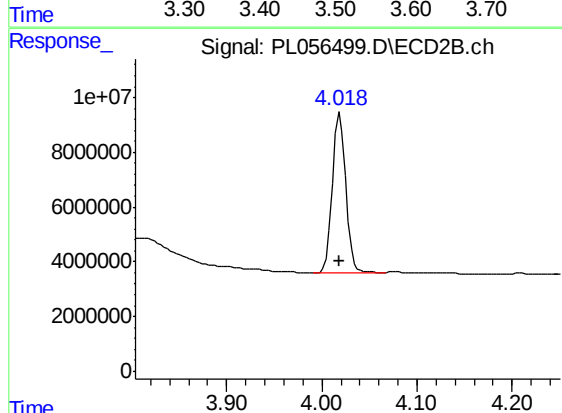


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 57570889
Conc: 21.16 ng/ml

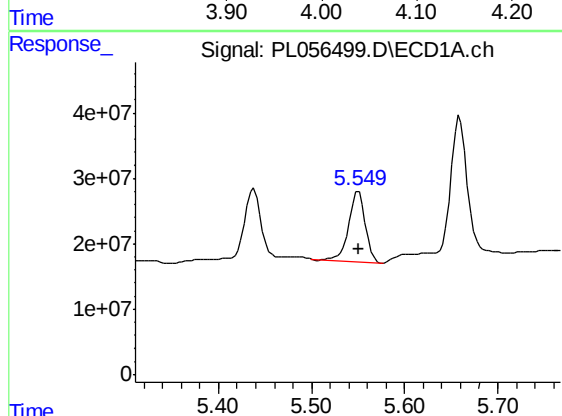


#9 Endosulfan I

R.T.: 5.550 min
Delta R.T.: 0.000 min
Response: 132355594
Conc: 10.55 ng/ml

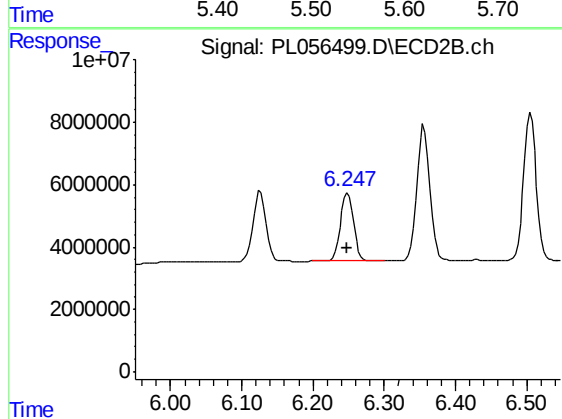

#9 Endosulfan I


R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 28163963
Conc: 10.13 ng/ml

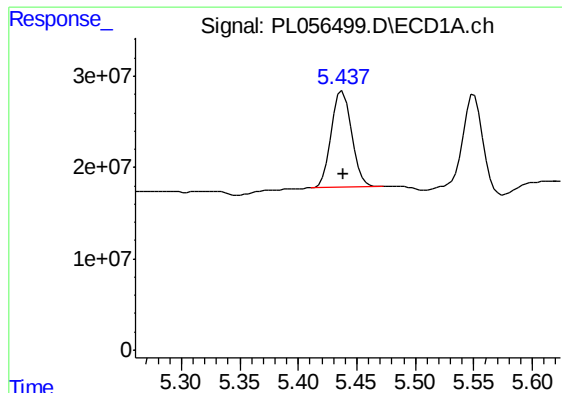

#10 gamma-Chlordane


R.T.: 5.438 min
Delta R.T.: 0.000 min
Response: 124047528
Conc: 9.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHEK

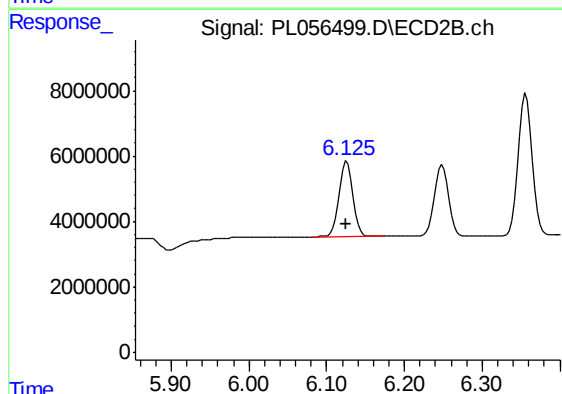


#10 gamma-Chlordane

R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 28595149
Conc: 9.78 ng/ml

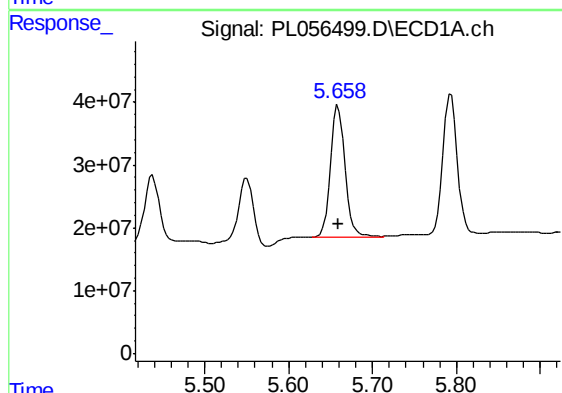


#12 4,4'-DDE

R.T.: 5.659 min
Delta R.T.: 0.000 min
Response: 253427410
Conc: 19.93 ng/ml

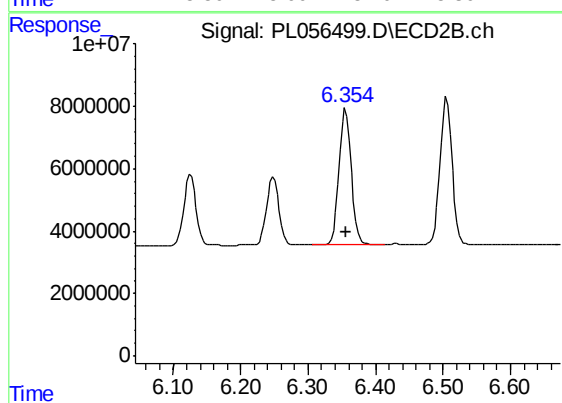

#12 4,4'-DDE


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 55517665
Conc: 19.81 ng/ml

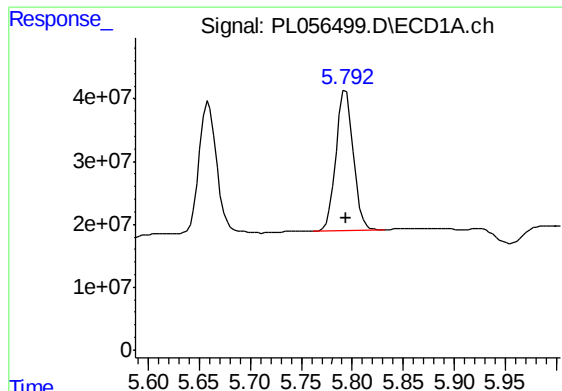

#13 Dieldrin


R.T.: 5.794 min
Delta R.T.: 0.000 min
Response: 262417754
Conc: 19.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

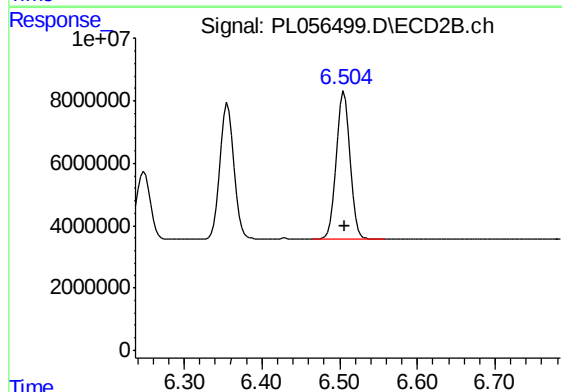


#13 Dieldrin

R.T.: 6.506 min
Delta R.T.: 0.000 min
Response: 59127679
Conc: 20.32 ng/ml

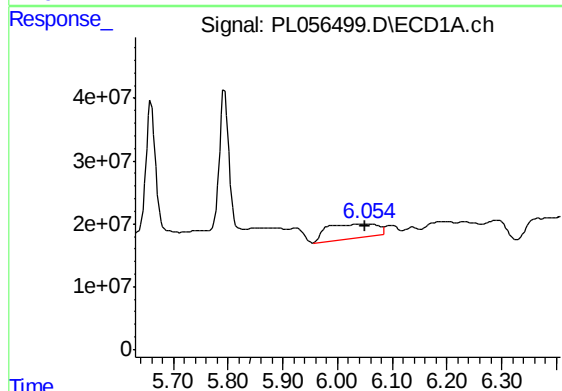


#14 Endrin

R.T.: 6.056 min
Delta R.T.: 0.005 min
Response: 147525586
Conc: 12.60 ng/ml

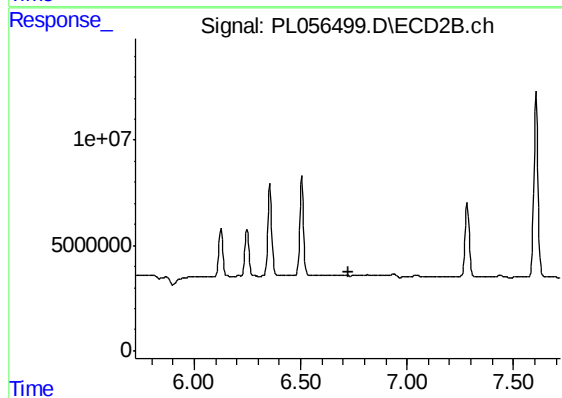

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.724 min
Response: 0
Conc: N.D.

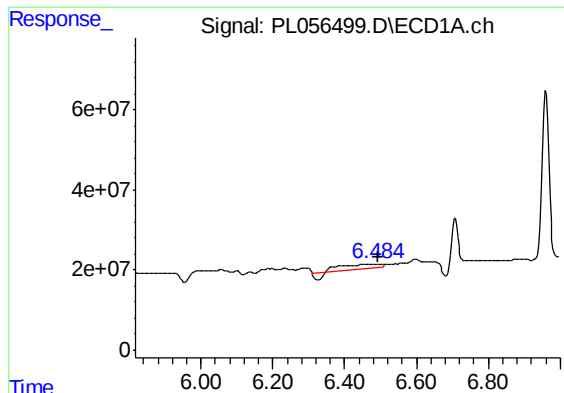

#18 Endrin aldehyde


R.T.: 6.487 min
Delta R.T.: -0.004 min
Response: 81948733
Conc: 8.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHEK

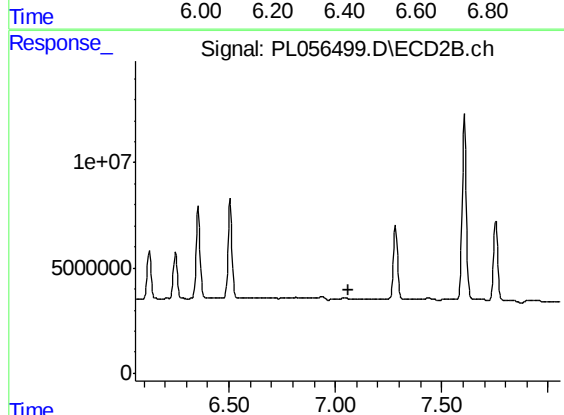


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.059 min
Response: 0
Conc: N.D.

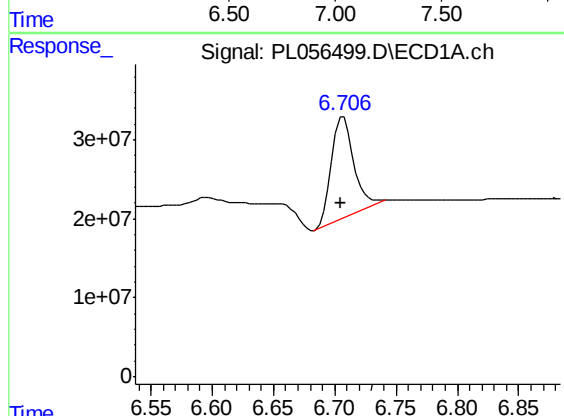


#19 Endosulfan Sulfate

R.T.: 6.707 min
Delta R.T.: 0.002 min
Response: 161812257
Conc: 15.20 ng/ml

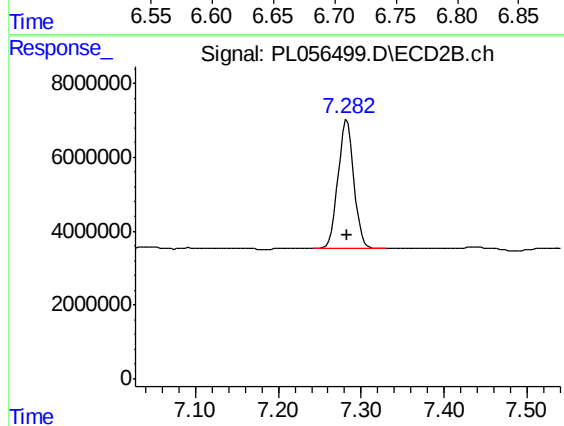

#19 Endosulfan Sulfate


R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 46543362
Conc: 19.64 ng/ml

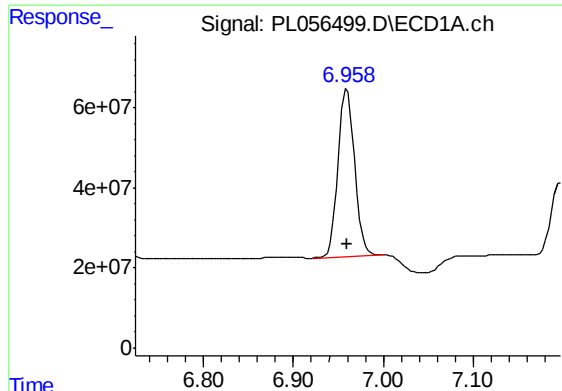

#20 Methoxychlor


R.T.: 6.960 min
Delta R.T.: 0.000 min
Response: 542650739
Conc: 110.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHEK

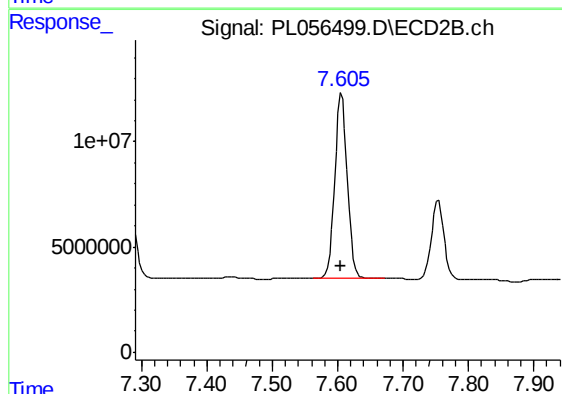


#20 Methoxychlor

R.T.: 7.606 min
Delta R.T.: 0.000 min
Response: 117194396
Conc: 102.03 ng/ml

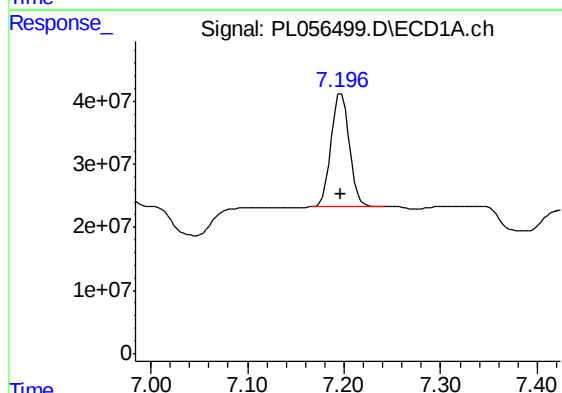


#21 Endrin ketone

R.T.: 7.197 min
Delta R.T.: 0.000 min
Response: 231731293
Conc: 19.38 ng/ml

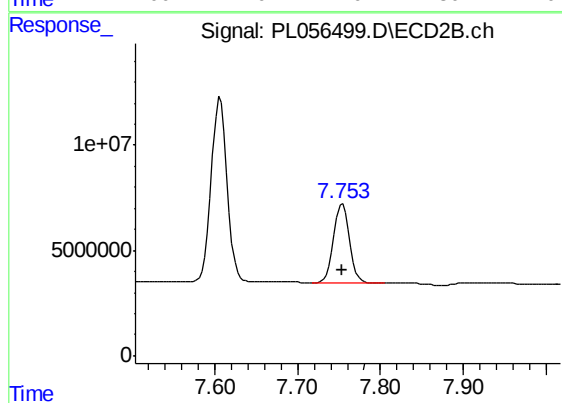

#21 Endrin ketone


R.T.: 7.754 min
Delta R.T.: 0.000 min
Response: 50282292
Conc: 20.01 ng/ml

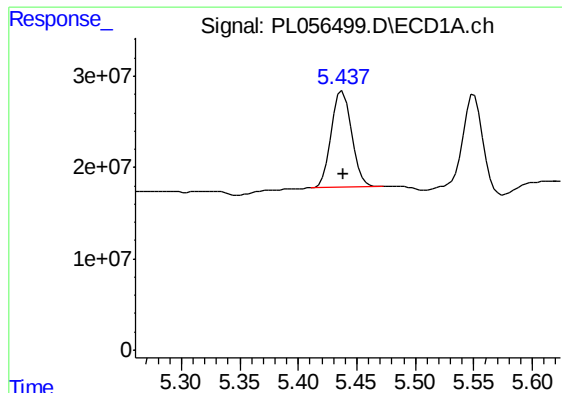

#25 Chlordane-3


R.T.: 5.438 min
Delta R.T.: 0.000 min
Response: 124047528
Conc: 94.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHEK

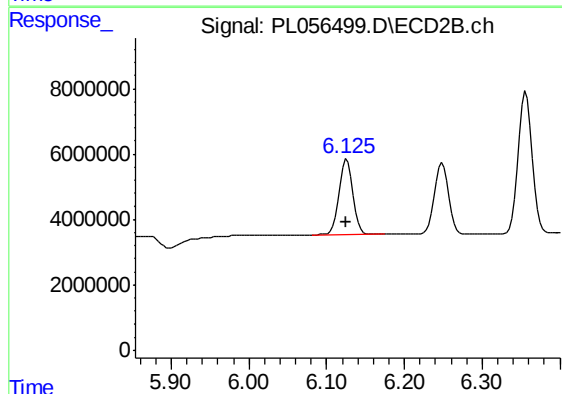


#25 Chlordane-3

R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 28595149
Conc: 73.79 ng/ml

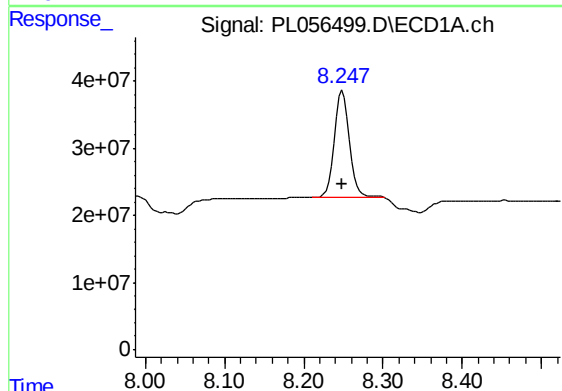

#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: 0.000 min
Response: 215618771
Conc: 22.51 ng/ml

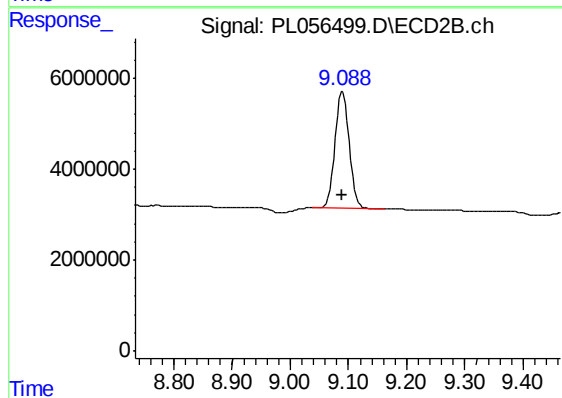

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 44250325
Conc: 21.69 ng/ml