

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021320\
 Data File : PL056528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2020 18:04
 Operator : AJ\MA
 Sample : L1511-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:19:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 13 05:32:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.020	99420587	32849967	11.268	12.075
28)	SA Decachlor...	8.251	9.095	130.4E6	28089968	13.609	13.771
Target Compounds							
11)	B alpha-Chl...	0.000	6.202	0	5552302	N.D.	1.890 #
26)	Chlordane-4	0.000	6.202	0	5552302	N.D.	12.200 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021320\
Data File : PL056528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2020 18:04
Operator : AJ\MA
Sample : L1511-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:19:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
Quant Title : GC Extractables
QLast Update : Thu Feb 13 05:32:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

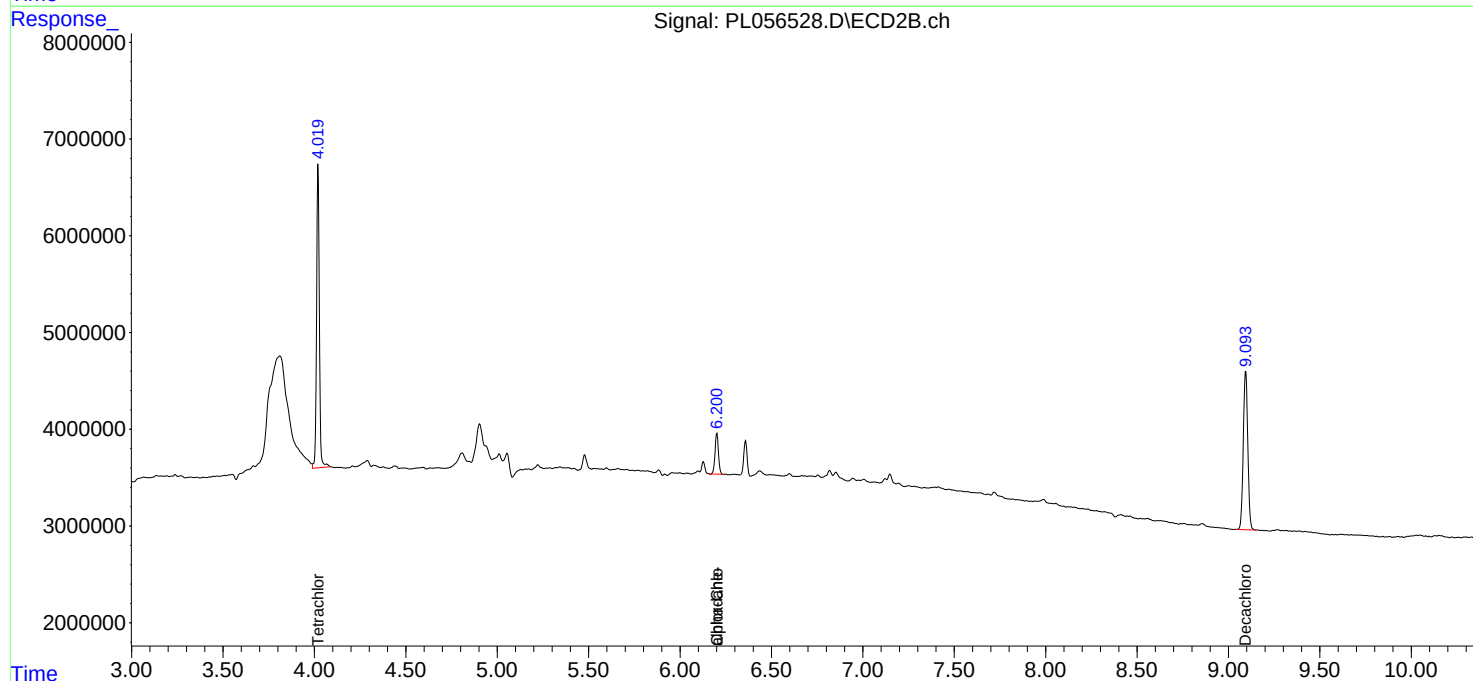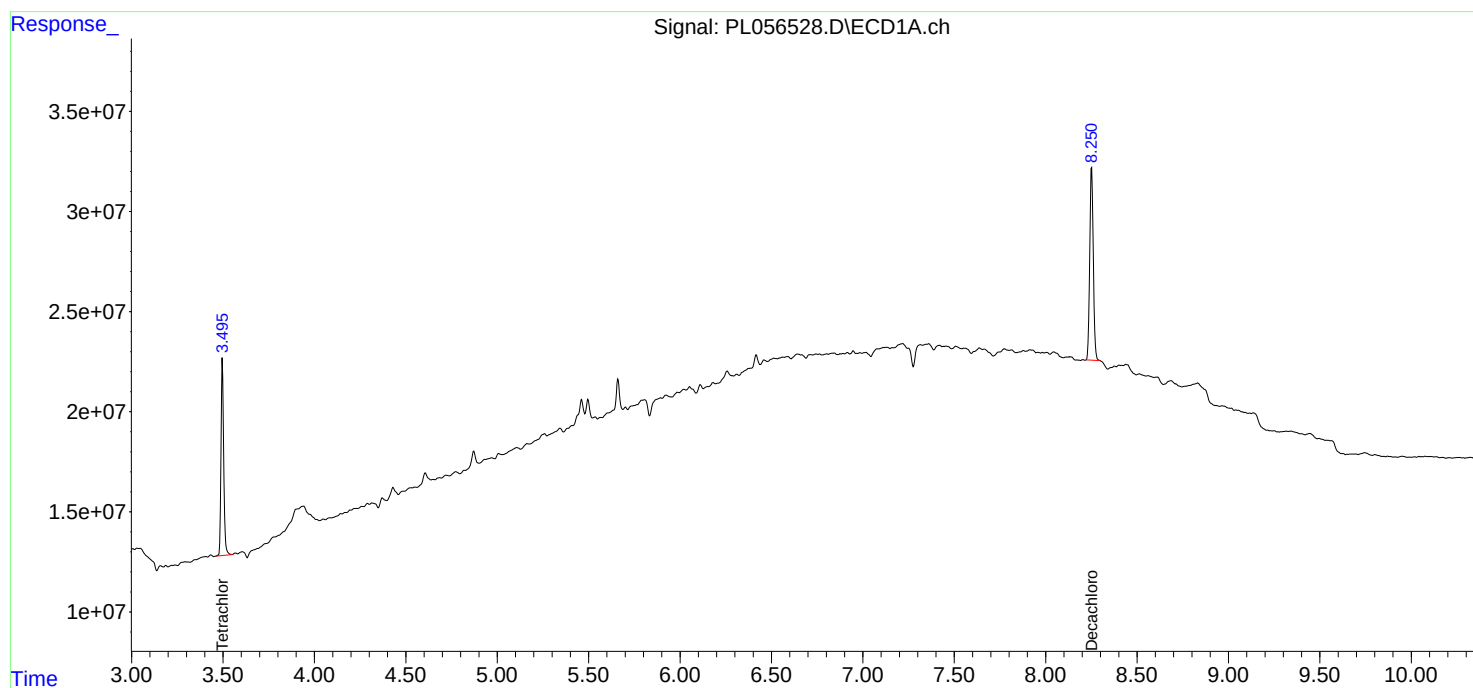


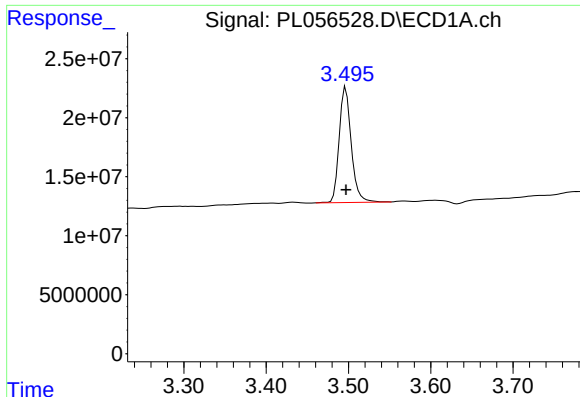

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 99420587
Conc: 11.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

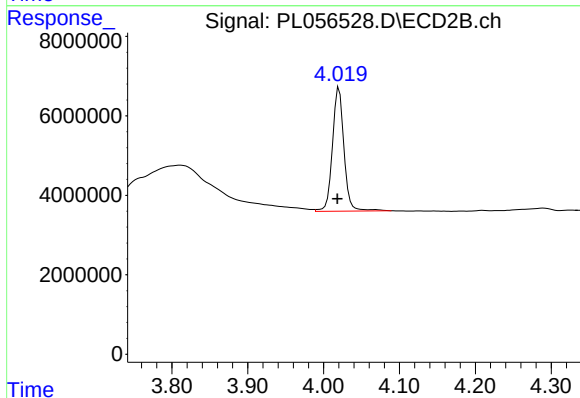


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.002 min
Response: 32849967
Conc: 12.08 ng/ml

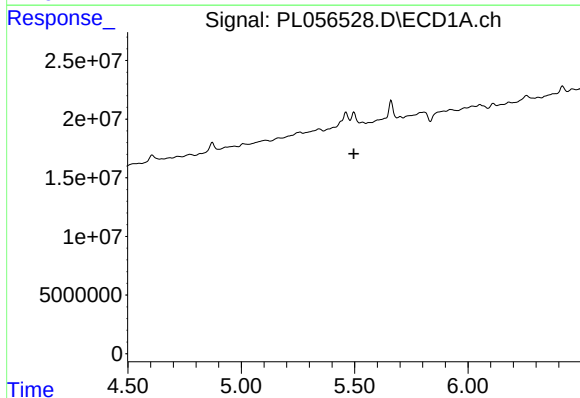


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

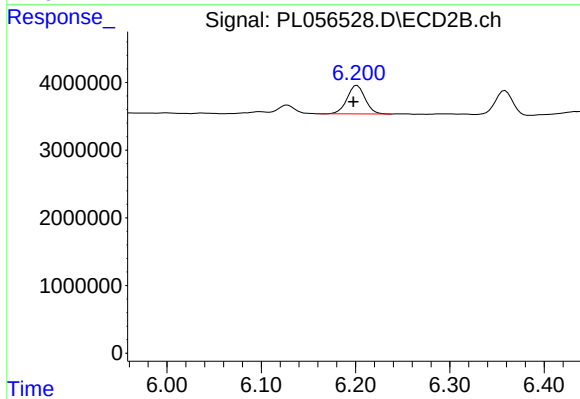

#11 alpha-Chlordane


R.T.: 6.202 min
Delta R.T.: 0.004 min
Response: 5552302
Conc: 1.89 ng/ml

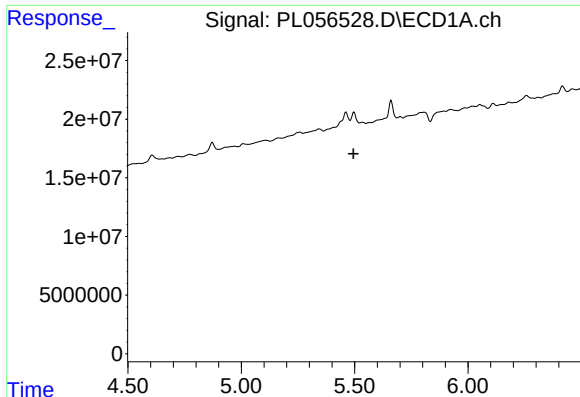

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

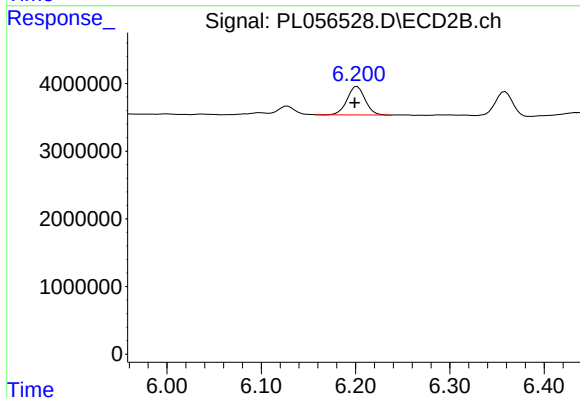


#26 Chlordane-4

R.T.: 6.202 min
Delta R.T.: 0.003 min
Response: 5552302
Conc: 12.20 ng/ml

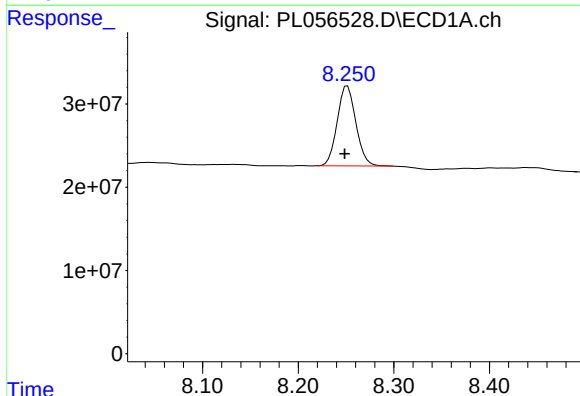

#28 Decachlorobiphenyl

R.T.: 8.251 min
Delta R.T.: 0.003 min
Response: 130364056
Conc: 13.61 ng/ml

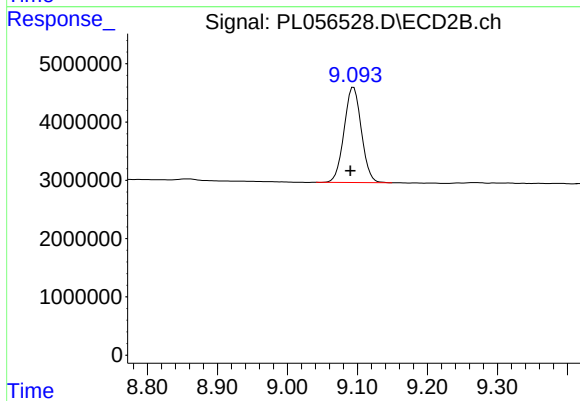

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.005 min
Response: 28089968
Conc: 13.77 ng/ml