

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021320\
 Data File : PL056530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2020 18:32
 Operator : AJ\MA
 Sample : L1514-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:19:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 13 05:32:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.020	263.3E6	81196481	29.845	29.847
28)	SA Decachlor...	8.251	9.095	234.6E6	48404441	24.489	23.730
Target Compounds							
12)	B 4,4'-DDE	5.660	6.358	1543.0E6	345.8E6	121.354	123.417
13)	MA Dieldrin	5.796	6.508	53453880	6861730	4.007	2.358 #
14)	MA Endrin	6.051	0.000	253.6E6	0	21.655	N.D. #
16)	A 4,4'-DDD	6.178	6.850	53975597	10651786	5.704	4.710
17)	MA 4,4'-DDT	6.418	7.149	935.3E6	215.3E6	98.691	101.923
18)	B Endrin al...	6.472f	0.000	61871469	0	6.447	N.D. #
23)	Chlordane-1	4.390f	0.000	16116870	0	42.843	N.D. #
27)	Chlordane-5	0.000	6.996	0	13469315	N.D.	167.476 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021320\
Data File : PL056530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2020 18:32
Operator : AJ\MA
Sample : L1514-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:19:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
Quant Title : GC Extractables
QLast Update : Thu Feb 13 05:32:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

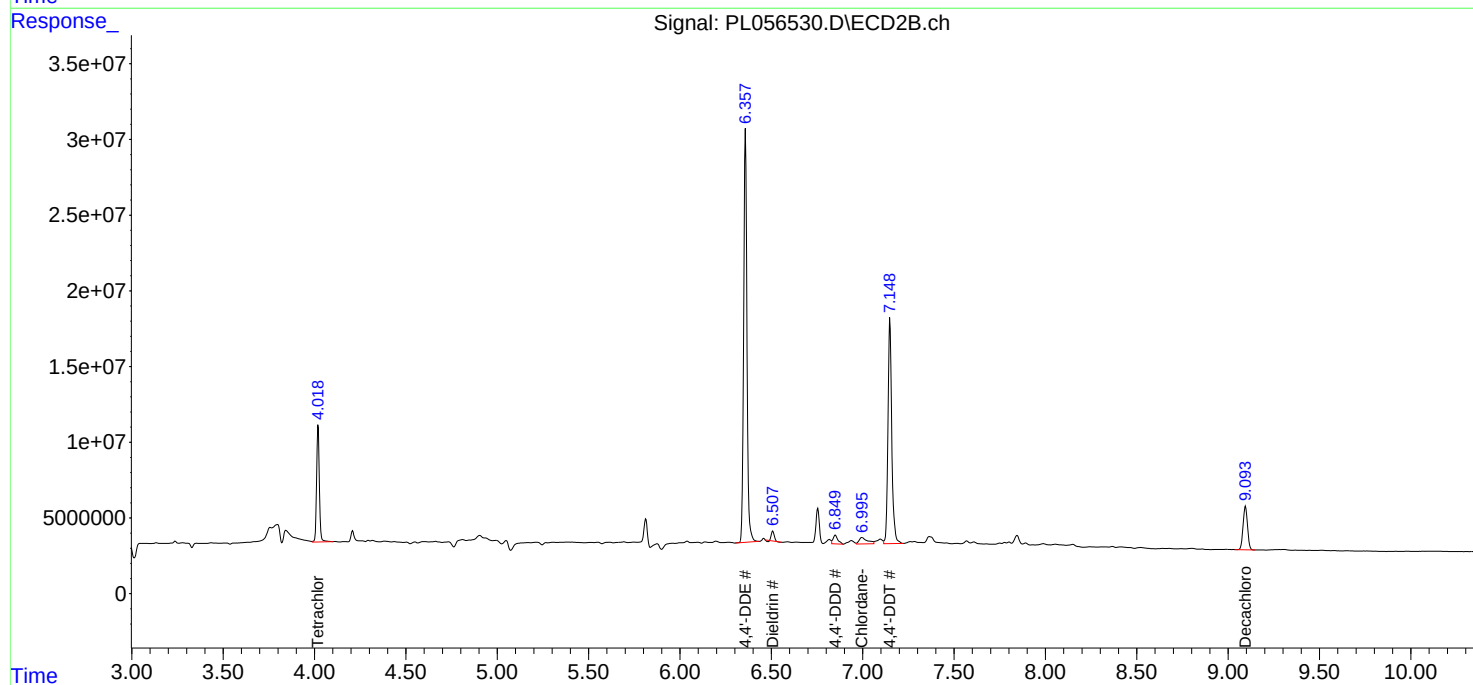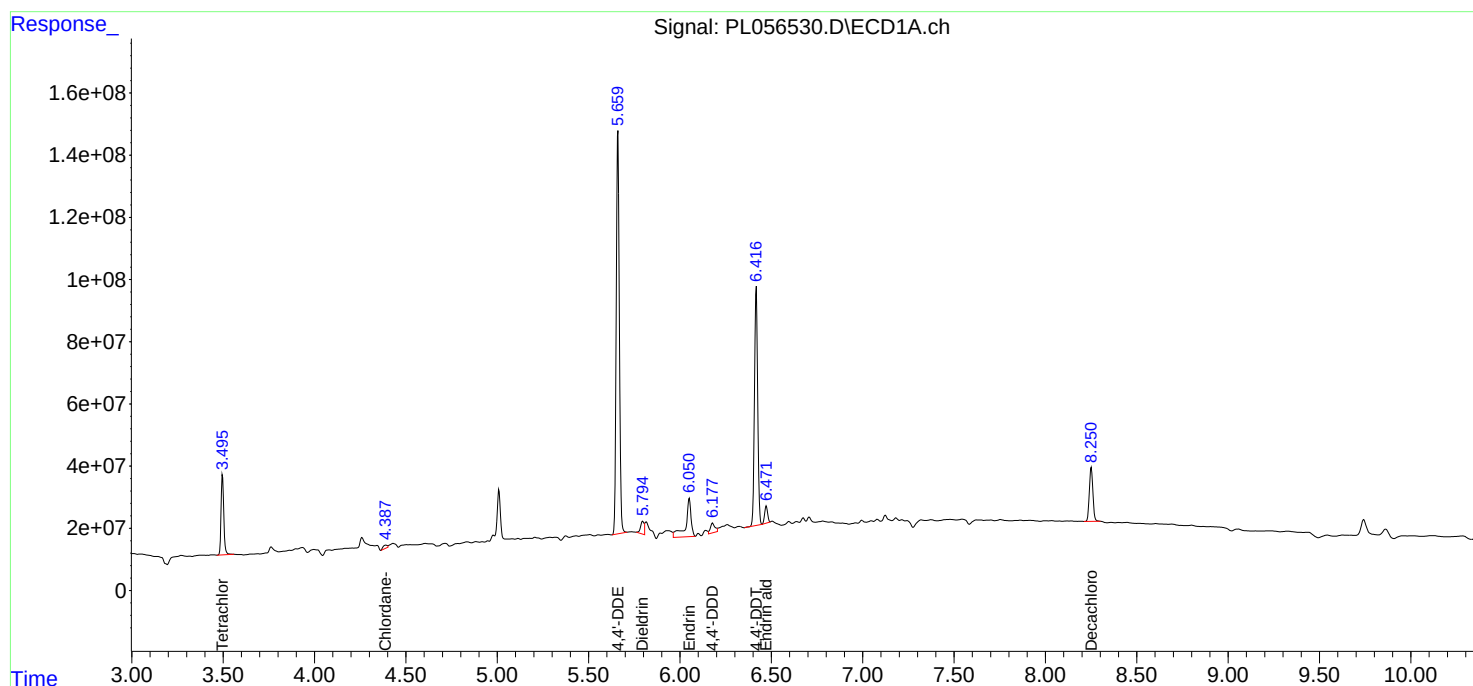


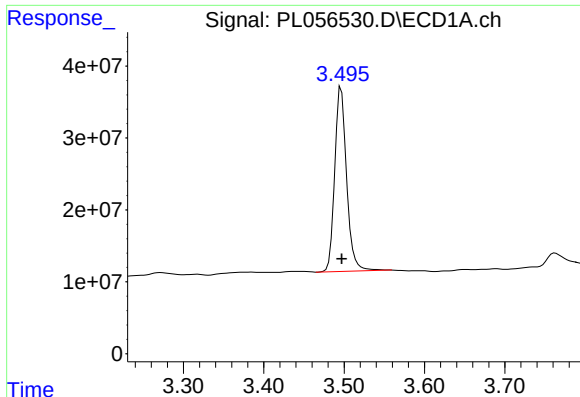

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 263336115
Conc: 29.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

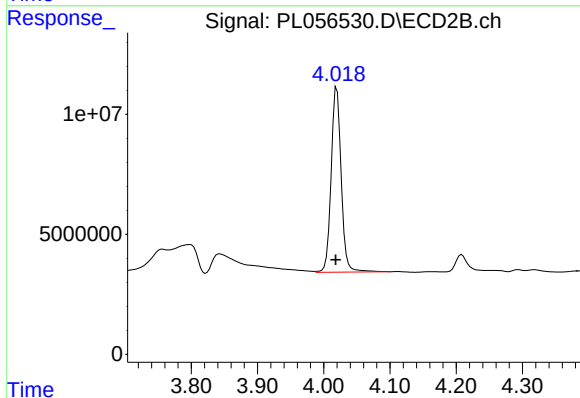


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.002 min
Response: 81196481
Conc: 29.85 ng/ml

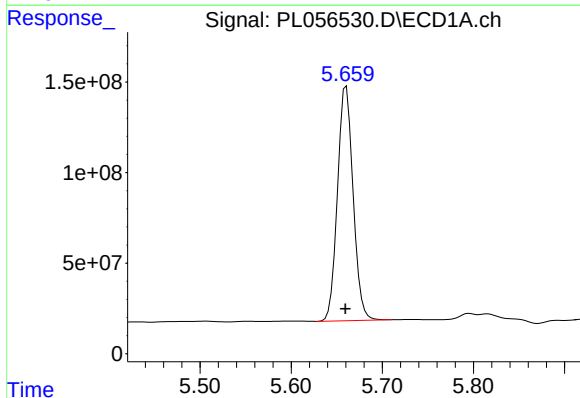


#12 4,4'-DDE

R.T.: 5.660 min
Delta R.T.: 0.000 min
Response: 1543044000
Conc: 121.35 ng/ml

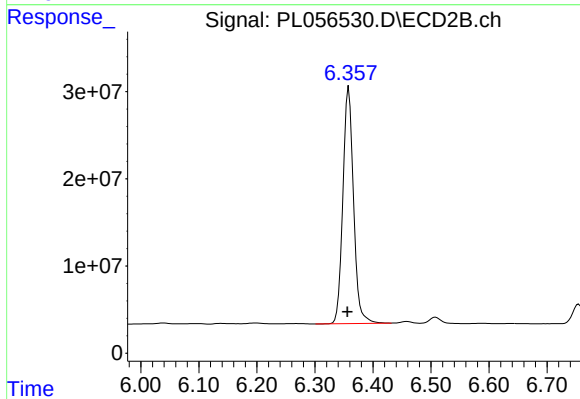

#12 4,4'-DDE


R.T.: 6.358 min
Delta R.T.: 0.002 min
Response: 345826386
Conc: 123.42 ng/ml

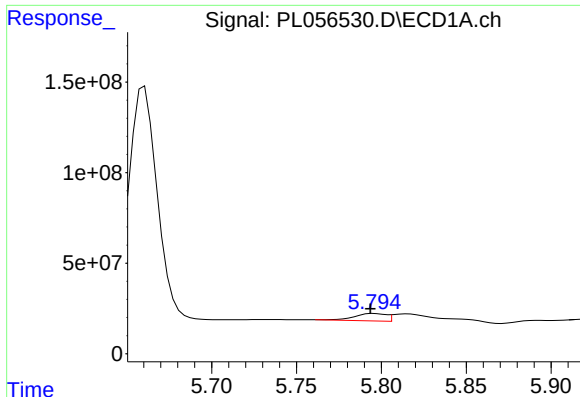

#13 Dieldrin


R.T.: 5.796 min
Delta R.T.: 0.002 min
Response: 53453880
Conc: 4.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

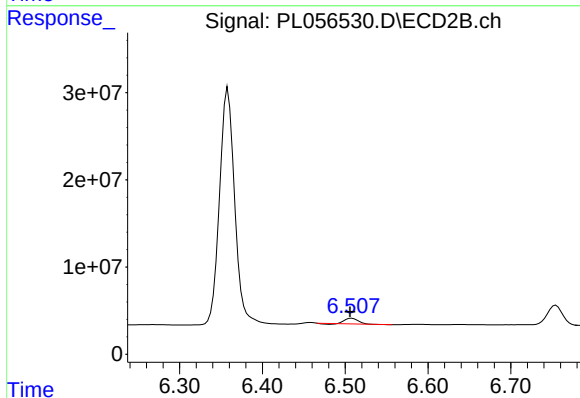


#13 Dieldrin

R.T.: 6.508 min
Delta R.T.: 0.002 min
Response: 6861730
Conc: 2.36 ng/ml

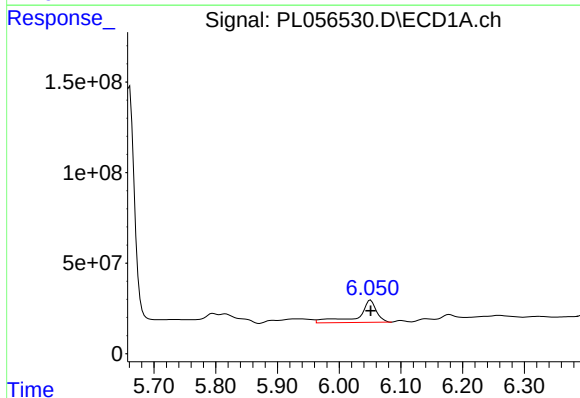


#14 Endrin

R.T.: 6.051 min
Delta R.T.: 0.000 min
Response: 253644507
Conc: 21.66 ng/ml

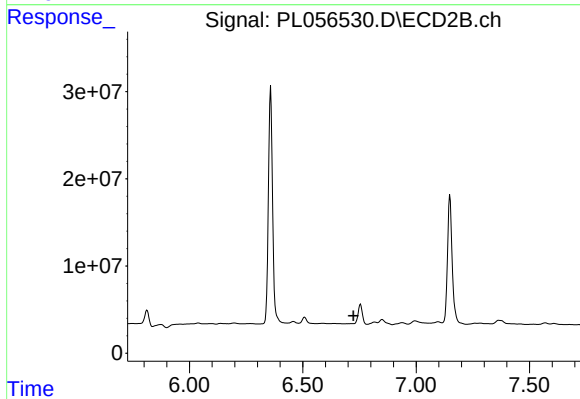

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.724 min
Response: 0
Conc: N.D.

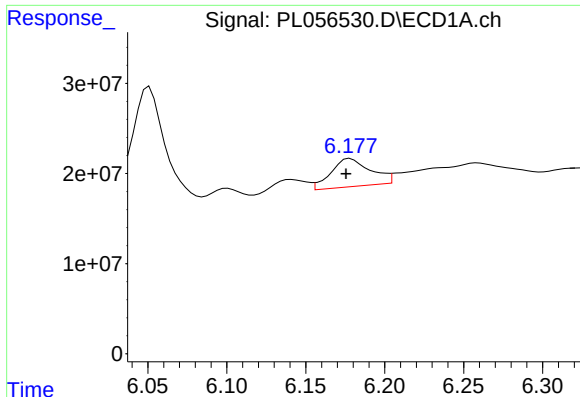

#16 4,4'-DDD


R.T.: 6.178 min
Delta R.T.: 0.003 min
Response: 53975597
Conc: 5.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

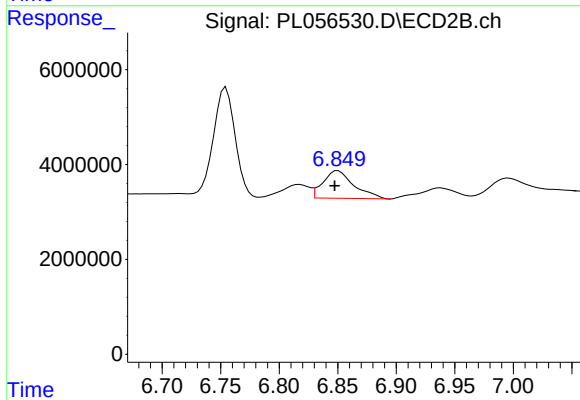


#16 4,4'-DDD

R.T.: 6.850 min
Delta R.T.: 0.003 min
Response: 10651786
Conc: 4.71 ng/ml

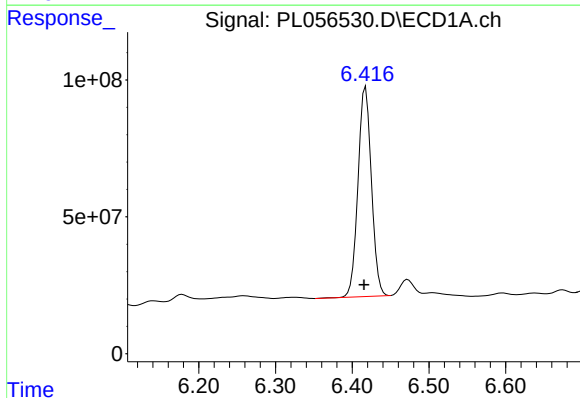


#17 4,4'-DDT

R.T.: 6.418 min
Delta R.T.: 0.002 min
Response: 935313876
Conc: 98.69 ng/ml

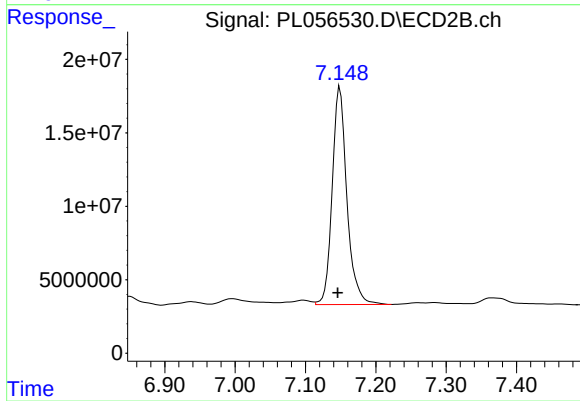

#17 4,4'-DDT


R.T.: 7.149 min
Delta R.T.: 0.003 min
Response: 215302625
Conc: 101.92 ng/ml

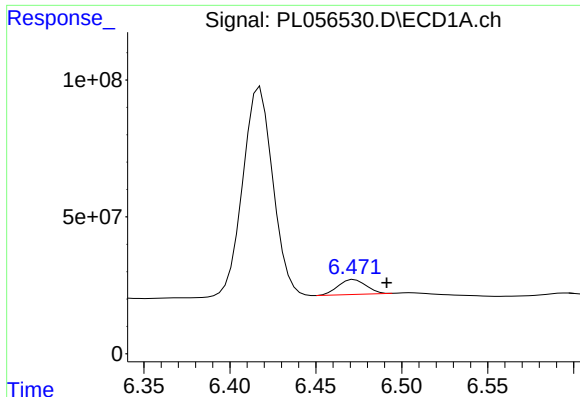

#18 Endrin aldehyde


R.T.: 6.472 min
Delta R.T.: -0.019 min
Response: 61871469
Conc: 6.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

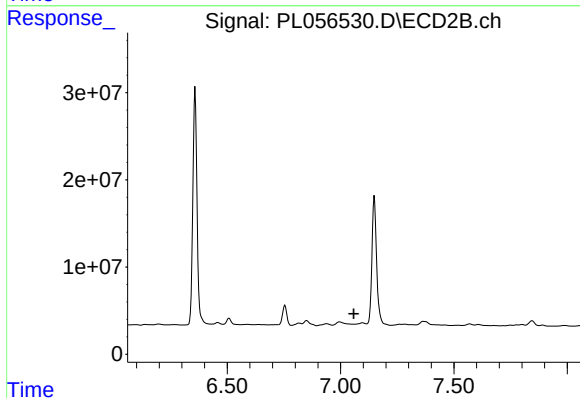


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.059 min
Response: 0
Conc: N.D.

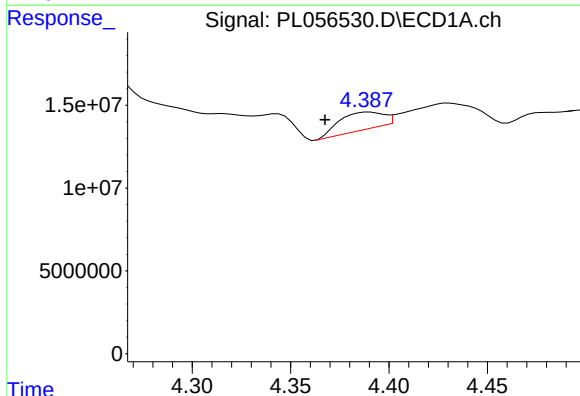


#23 Chlordane-1

R.T.: 4.390 min
Delta R.T.: 0.023 min
Response: 16116870
Conc: 42.84 ng/ml

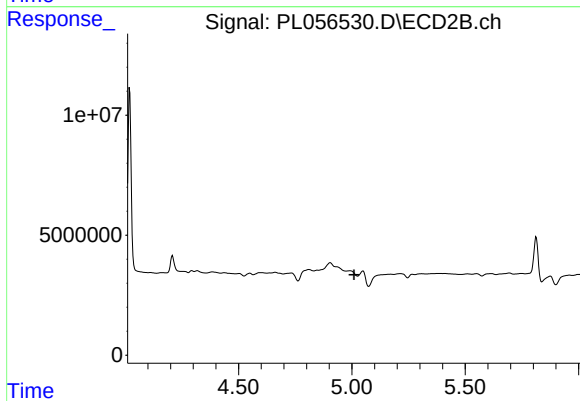

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.010 min
Response: 0
Conc: N.D.

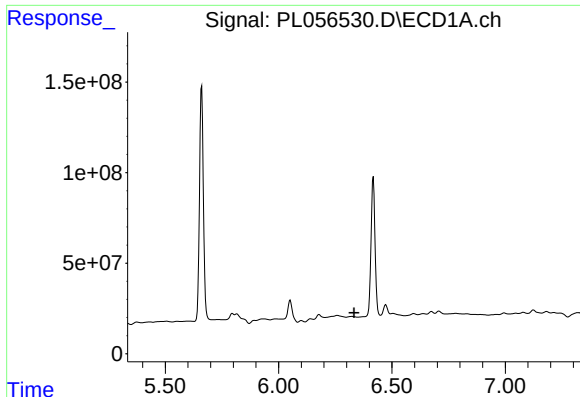

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

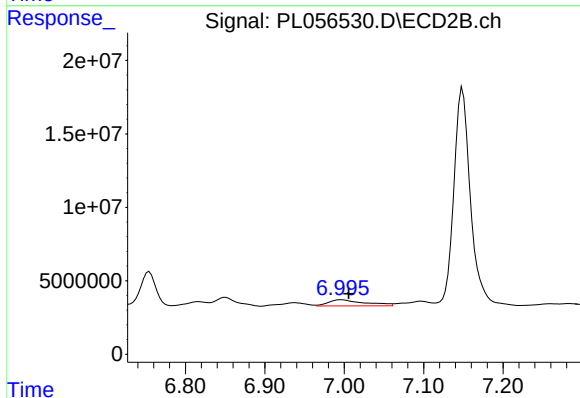


#27 Chlordane-5

R.T.: 6.996 min
Delta R.T.: -0.010 min
Response: 13469315
Conc: 167.48 ng/ml

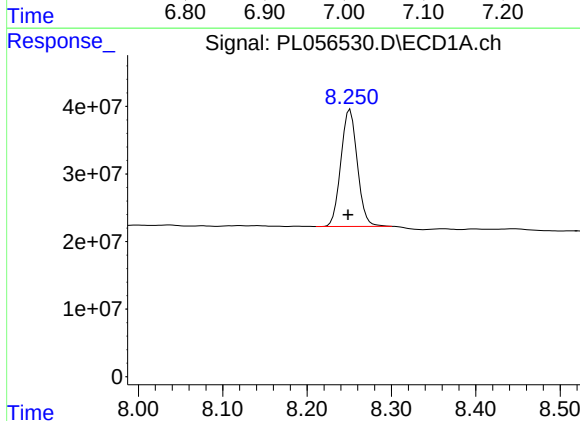

#28 Decachlorobiphenyl

R.T.: 8.251 min
Delta R.T.: 0.002 min
Response: 234587905
Conc: 24.49 ng/ml

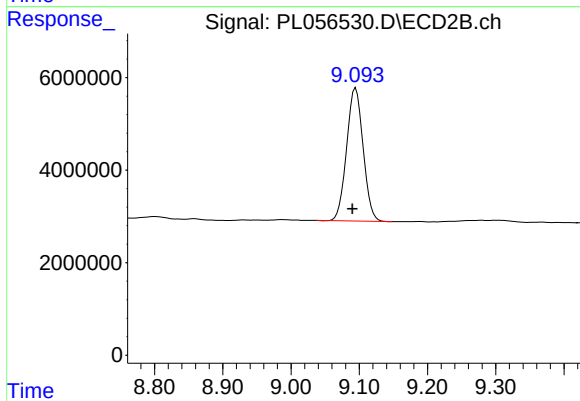

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.005 min
Response: 48404441
Conc: 23.73 ng/ml