

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021320\
 Data File : PL056532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2020 19:00
 Operator : AJ\MA
 Sample : L1515-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:20:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 13 05:32:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.020	164.4E6	52118535	18.635	19.158
28)	SA Decachlor...	8.251	9.094	138.0E6	28964217	14.408	14.200
Target Compounds							
2)	A alpha-BHC	0.000	4.436f	0	5317989	N.D.	1.306 #
10)	B gamma-Chl...	5.439	6.128	18057254	6380251	1.313	2.181 #
11)	B alpha-Chl...	5.497	6.202	31644887	14025340	2.323	4.775 #
12)	B 4,4'-DDE	5.661	6.359	49904021	10920026	3.925	3.897
14)	MA Endrin	6.053	0.000	123.5E6	0	10.547	N.D. #
16)	A 4,4'-DDD	6.178	0.000	10046362	0	1.062	N.D. #
25)	Chlordane-3	5.439	6.128	18057254	6380251	13.753	16.464
26)	Chlordane-4	5.497	6.202	31644887	14025340	29.125	30.818



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021320\
Data File : PL056532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2020 19:00
Operator : AJ\MA
Sample : L1515-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:20:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
Quant Title : GC Extractables
QLast Update : Thu Feb 13 05:32:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

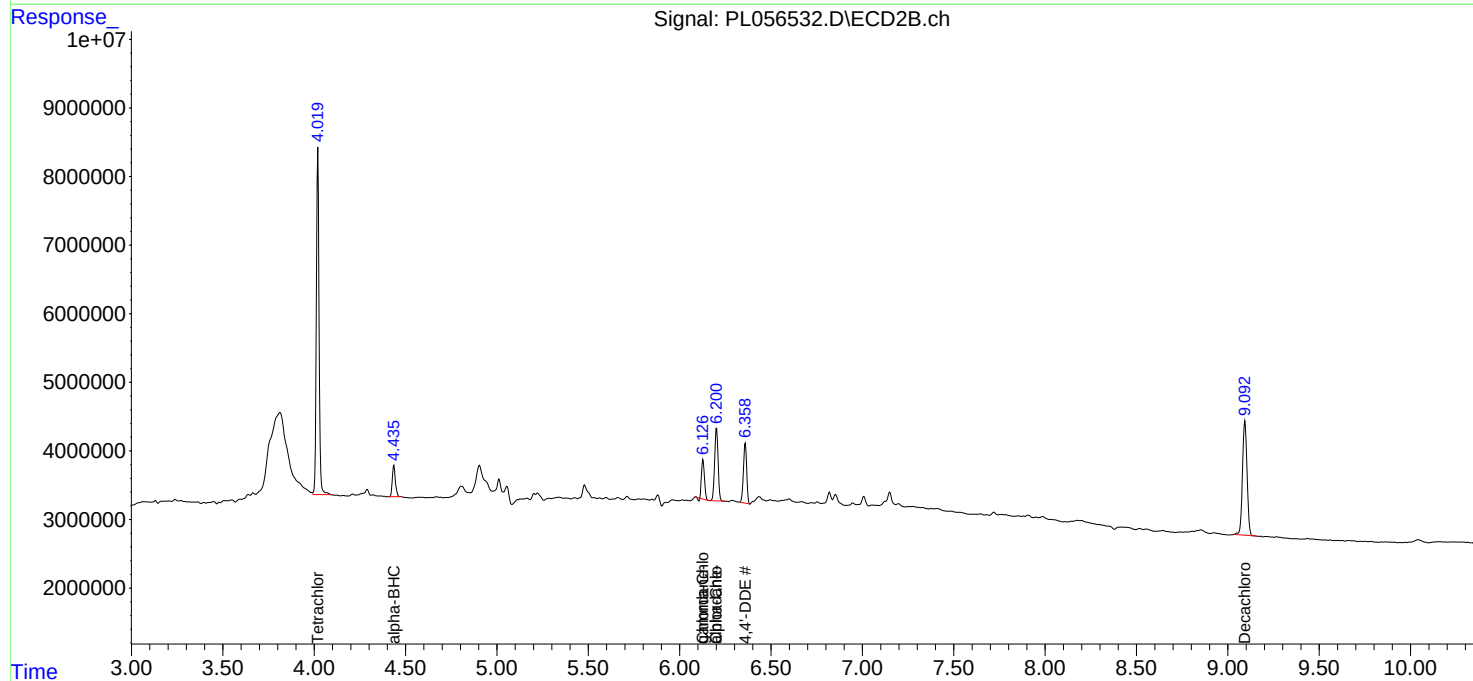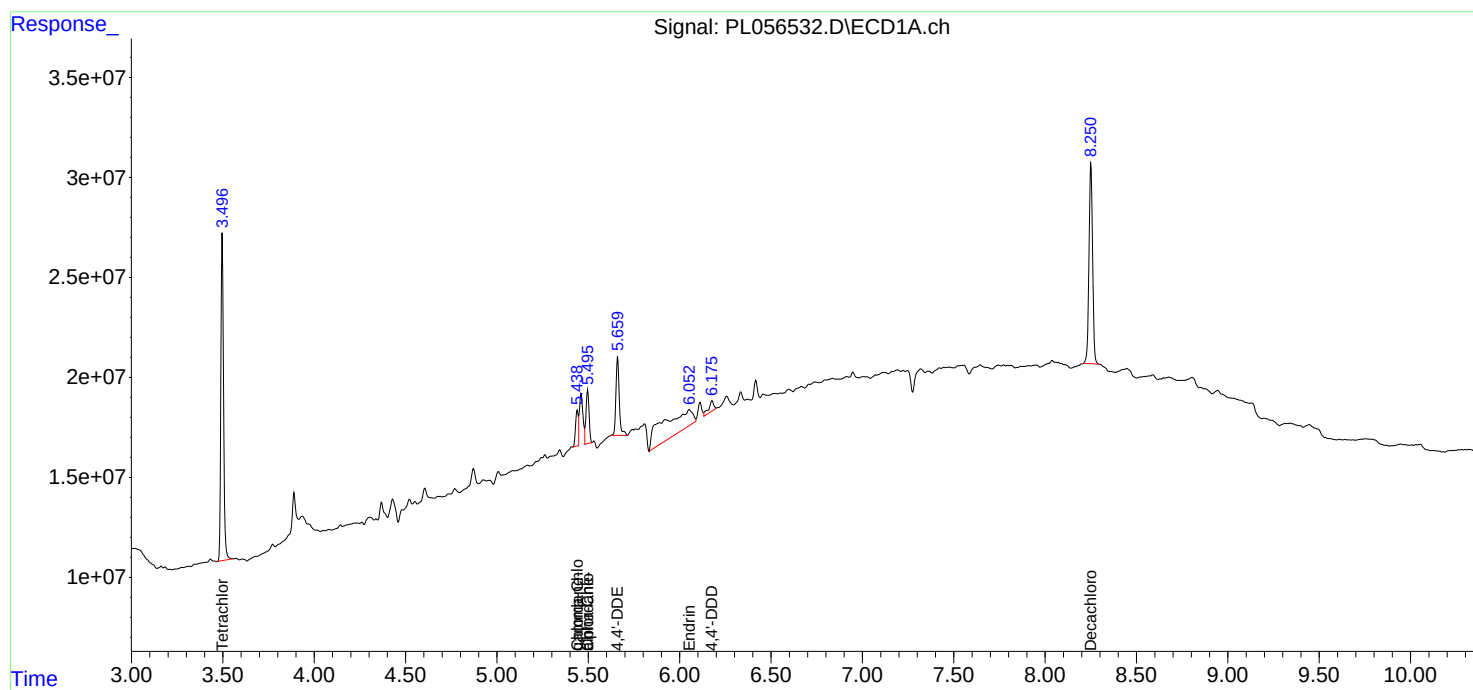


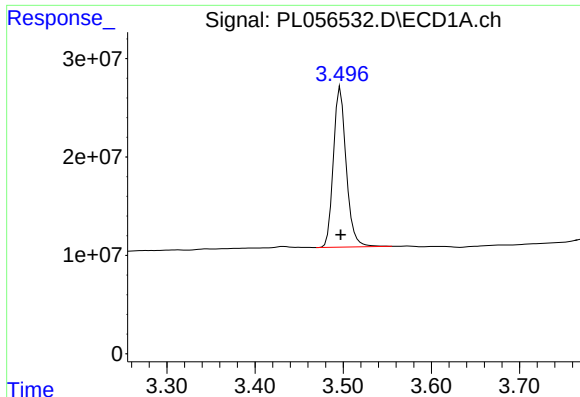

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 164424247
Conc: 18.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

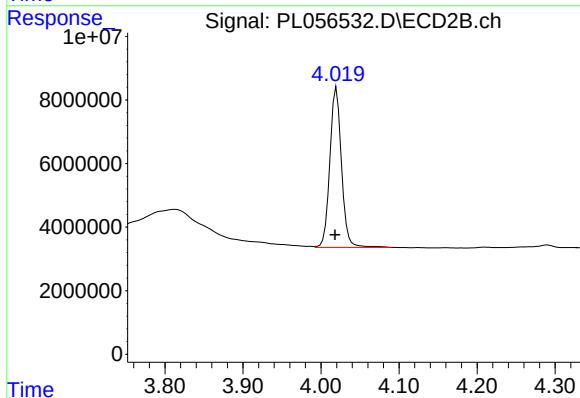


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.002 min
Response: 52118535
Conc: 19.16 ng/ml

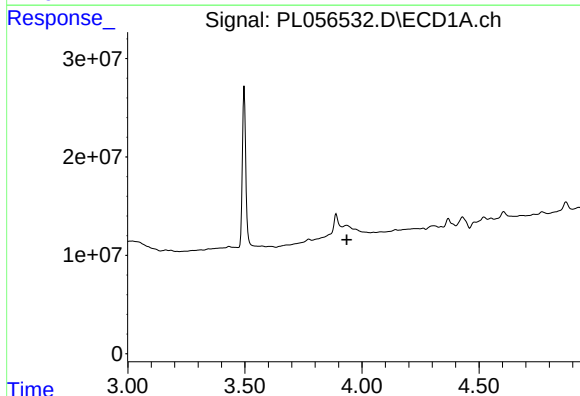


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.935 min
Response: 0
Conc: N.D.

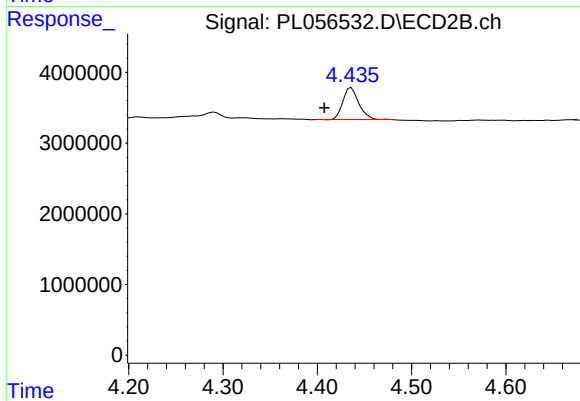

#2 alpha-BHC


R.T.: 4.436 min
Delta R.T.: 0.029 min
Response: 5317989
Conc: 1.31 ng/ml

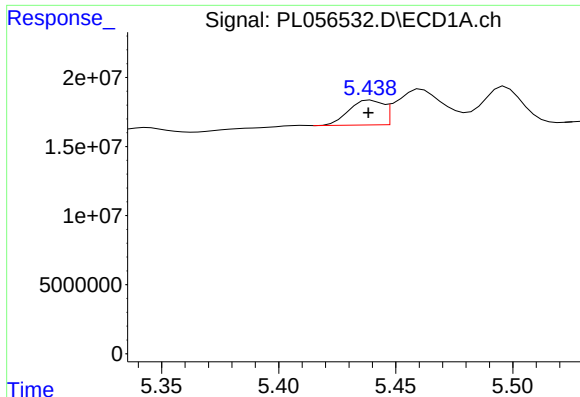

#10 gamma-Chlordane


R.T.: 5.439 min
Delta R.T.: 0.001 min
Response: 18057254
Conc: 1.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

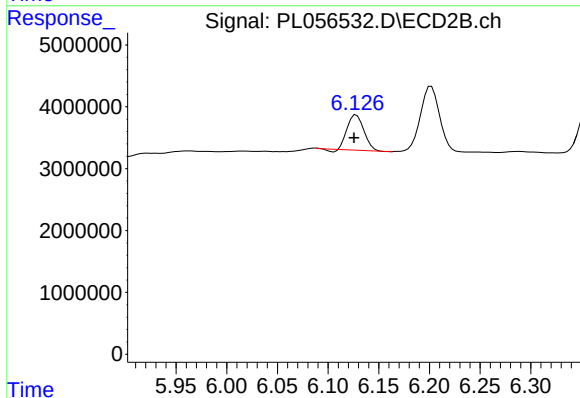


#10 gamma-Chlordane

R.T.: 6.128 min
Delta R.T.: 0.002 min
Response: 6380251
Conc: 2.18 ng/ml

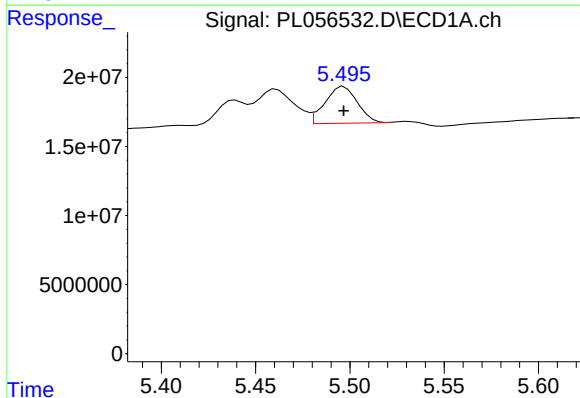


#11 alpha-Chlordane

R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 31644887
Conc: 2.32 ng/ml

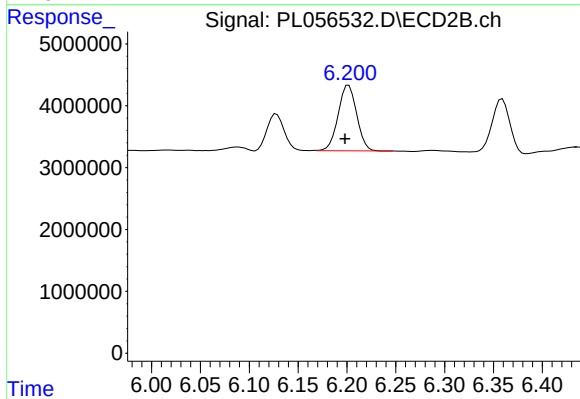

#11 alpha-Chlordane


R.T.: 6.202 min
Delta R.T.: 0.004 min
Response: 14025340
Conc: 4.77 ng/ml

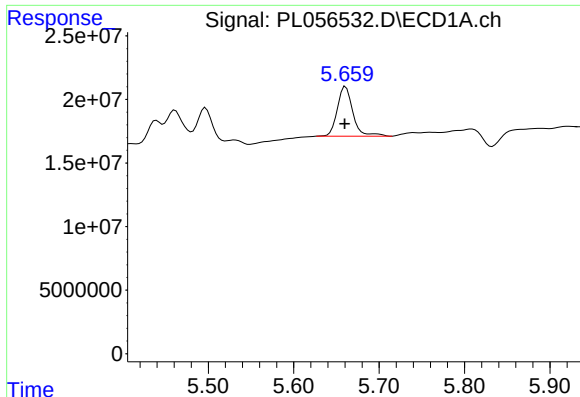

#12 4,4'-DDE


R.T.: 5.661 min
Delta R.T.: 0.001 min
Response: 49904021
Conc: 3.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

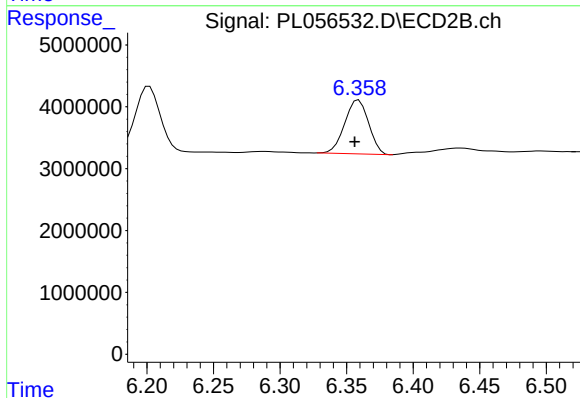


#12 4,4'-DDE

R.T.: 6.359 min
Delta R.T.: 0.003 min
Response: 10920026
Conc: 3.90 ng/ml

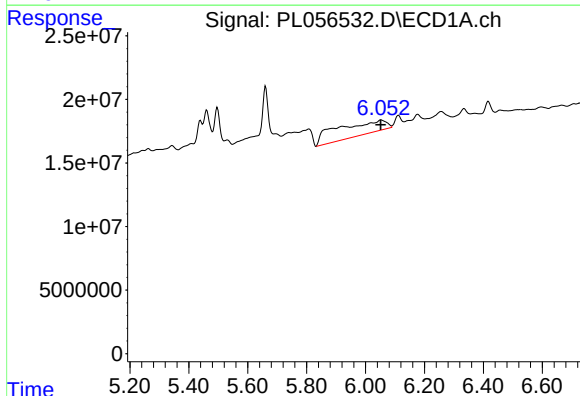


#14 Endrin

R.T.: 6.053 min
Delta R.T.: 0.002 min
Response: 123529232
Conc: 10.55 ng/ml

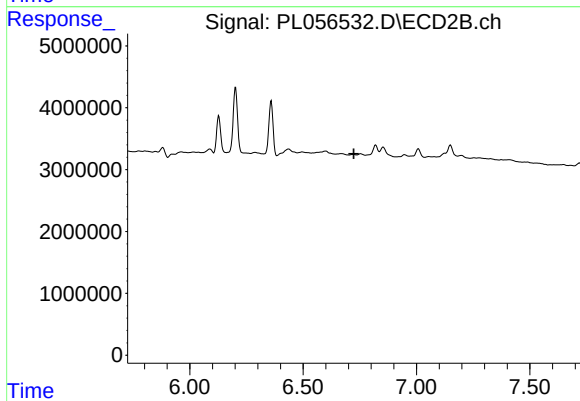

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.724 min
Response: 0
Conc: N.D.

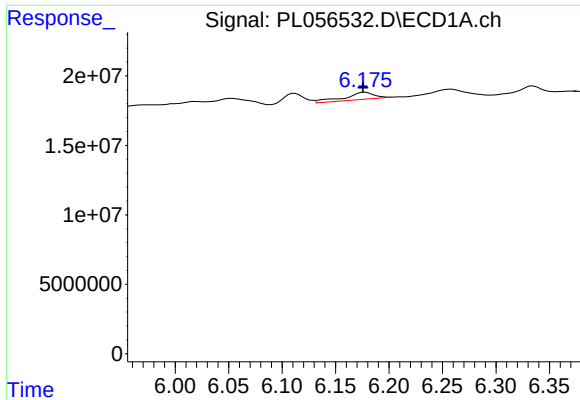

#16 4,4'-DDD


R.T.: 6.178 min
Delta R.T.: 0.002 min
Response: 10046362
Conc: 1.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

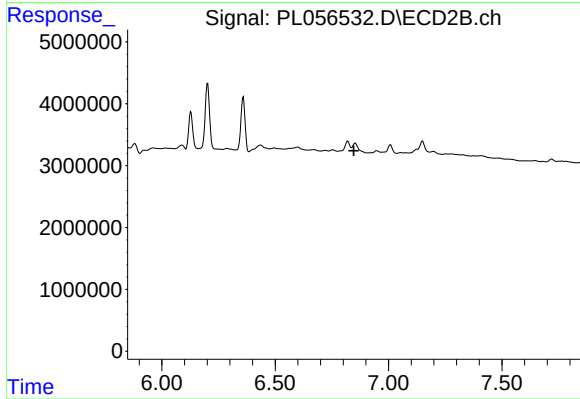


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.847 min
Response: 0
Conc: N.D.

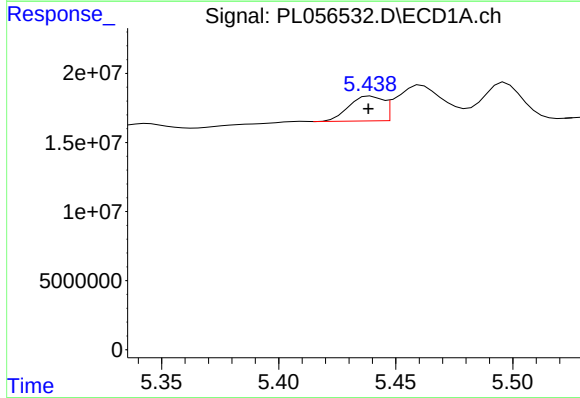


#25 Chlordane-3

R.T.: 5.439 min
Delta R.T.: 0.001 min
Response: 18057254
Conc: 13.75 ng/ml

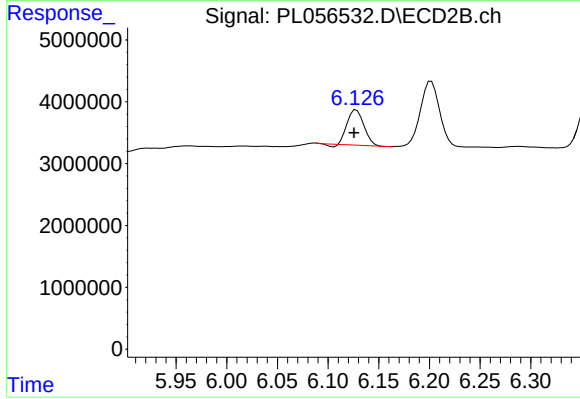

#25 Chlordane-3


R.T.: 6.128 min
Delta R.T.: 0.002 min
Response: 6380251
Conc: 16.46 ng/ml

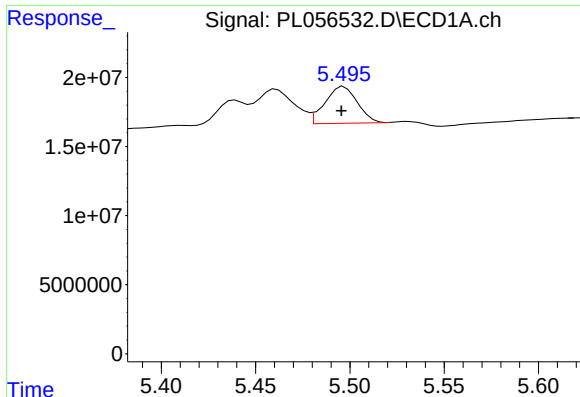

#26 Chlordane-4


R.T.: 5.497 min
Delta R.T.: 0.001 min
Response: 31644887
Conc: 29.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

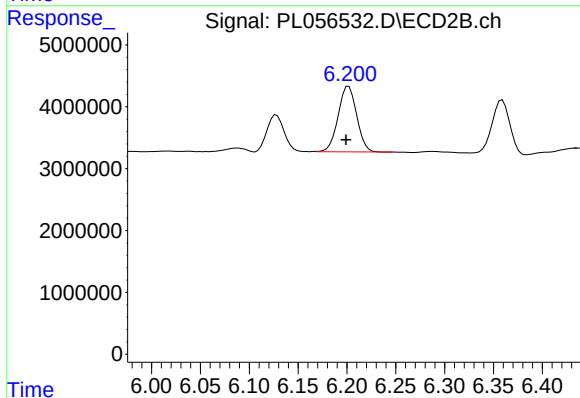


#26 Chlordane-4

R.T.: 6.202 min
Delta R.T.: 0.003 min
Response: 14025340
Conc: 30.82 ng/ml

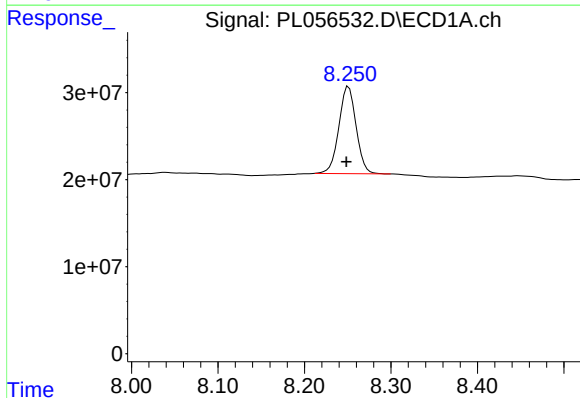

#28 Decachlorobiphenyl

R.T.: 8.251 min
Delta R.T.: 0.002 min
Response: 138013920
Conc: 14.41 ng/ml

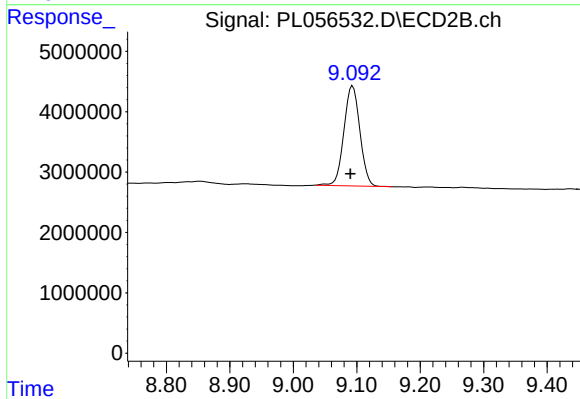

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.004 min
Response: 28964217
Conc: 14.20 ng/ml