

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021320\
 Data File : PL056519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2020 15:53
 Operator : AJ\MA
 Sample : L1505-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-PIT-1

Manual Integrations
 APPROVED

mohammad
 2/14/2020 2:40:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:17:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 13 05:32:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.020	204.0E6	61831915	23.116	22.729
28)	SA Decachlor...	8.252	9.094	214.7E6	33932065	22.409	16.635m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021320\
Data File : PL056519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2020 15:53
Operator : AJ\MA
Sample : L1505-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1


Manual Integrations
APPROVED

mohammad
2/14/2020 2:40:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:17:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
Quant Title : GC Extractables
QLast Update : Thu Feb 13 05:32:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

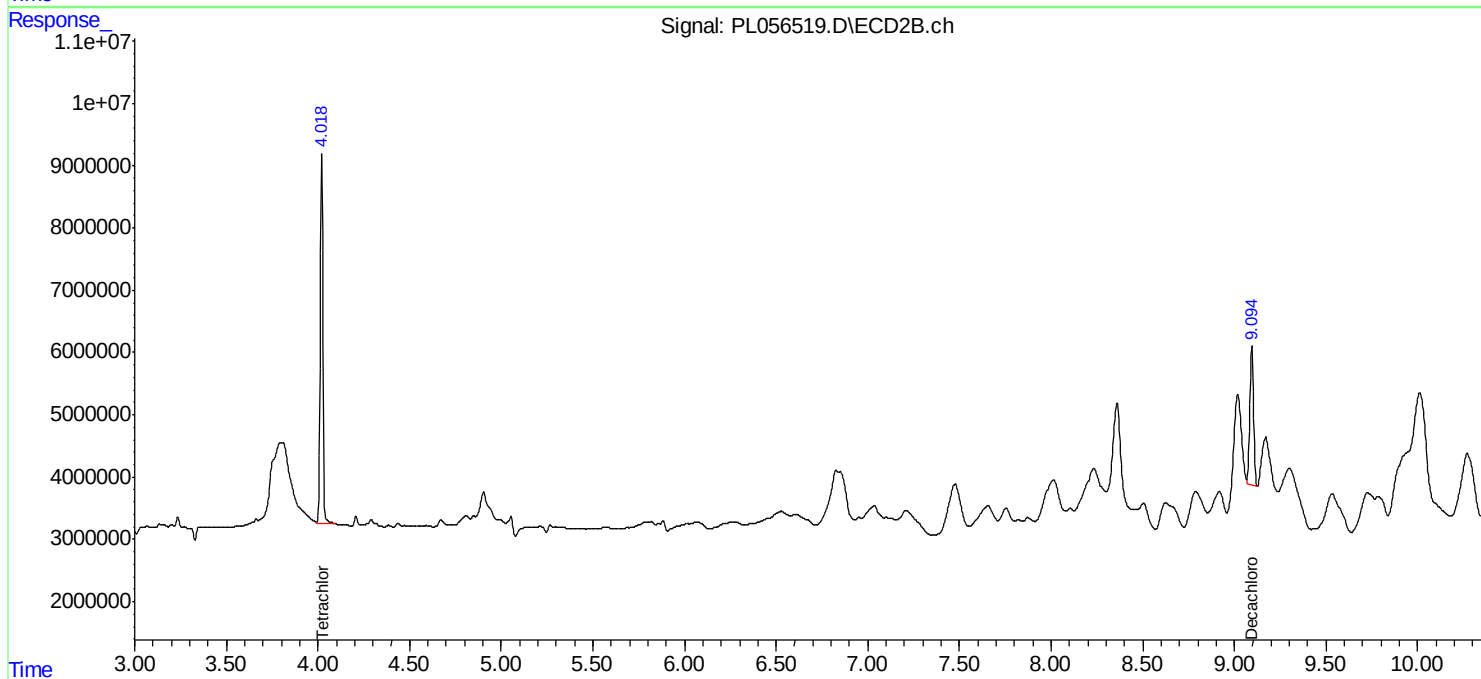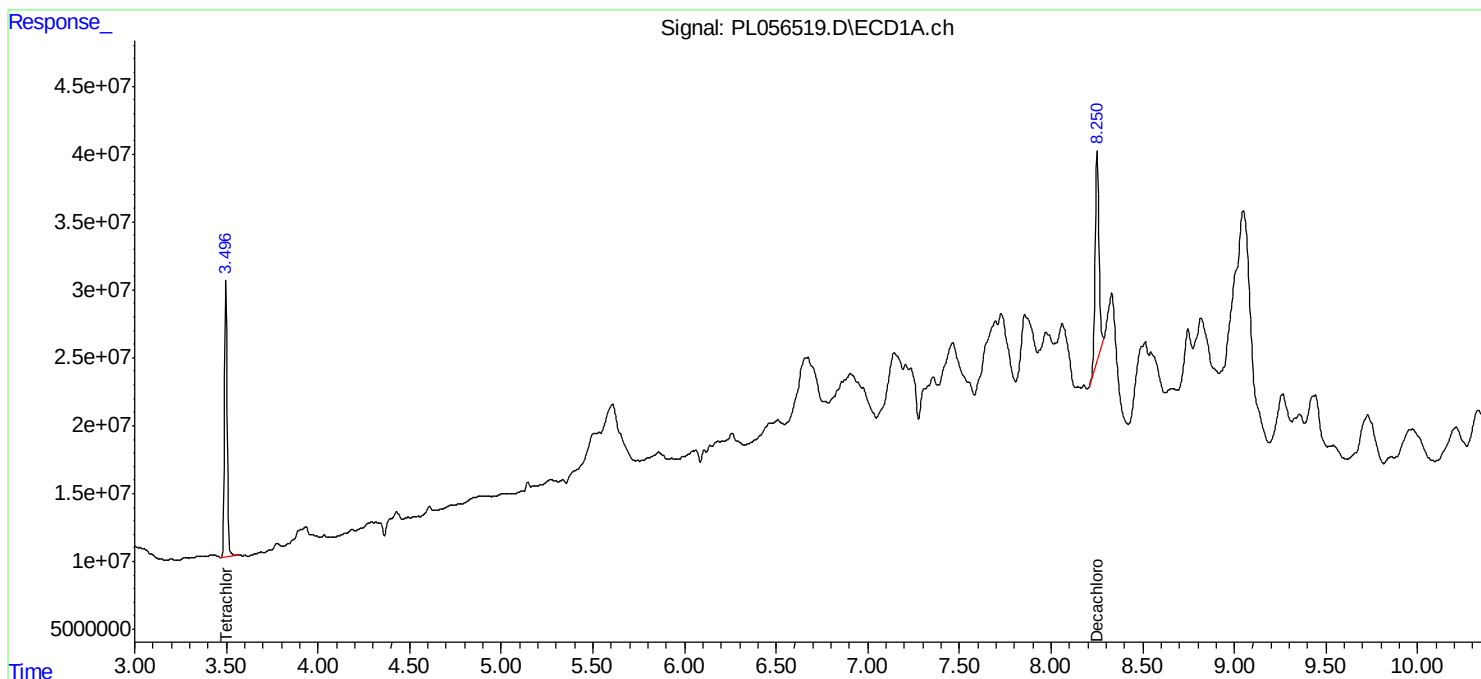

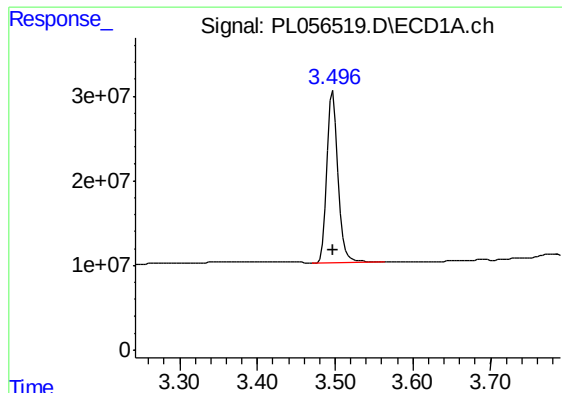


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 203961757
Conc: 23.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1


Manual Integrations
APPROVED

mohammad
2/14/2020 2:40:15 PM

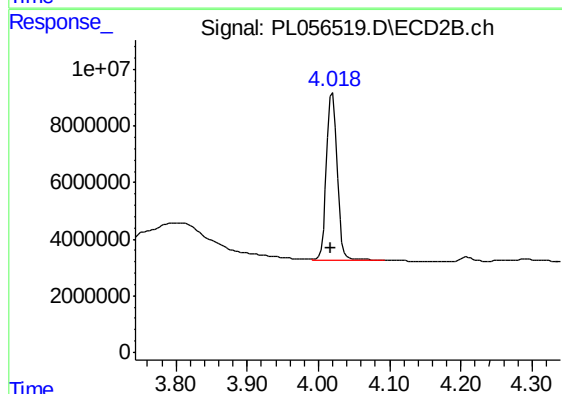


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.002 min
Response: 61831915
Conc: 22.73 ng/ml

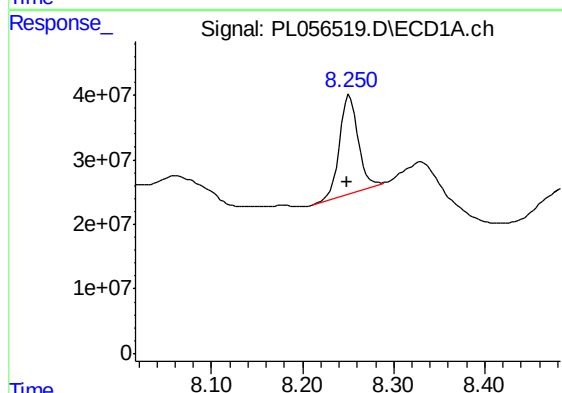

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.003 min
Response: 214663433
Conc: 22.41 ng/ml

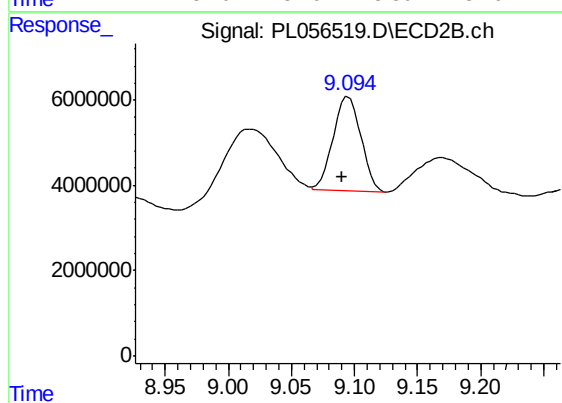

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.004 min
Response: 33932065
Conc: 16.64 ng/ml m