

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021323\
 Data File : PL080887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2023 14:17
 Operator : AR\AJ
 Sample : 01526-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PL-01-021023

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/14/2023
 Supervised By :Ankita Jodhani 02/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 20:09:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.355	2.686	21622554	21762496	10.081m	9.908m
28) SA Decachlor...	8.798	7.838	23826946	26633712	13.610	11.179
Target Compounds						
11) B alpha-Chl...	5.819	4.952	7477021	2461538	2.962m	0.859m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021323\
Data File : PL080887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2023 14:17
Operator : AR\AJ
Sample : 01526-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PL-01-021023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/14/2023
Supervised By : Ankita Jodhani 02/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 20:09:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

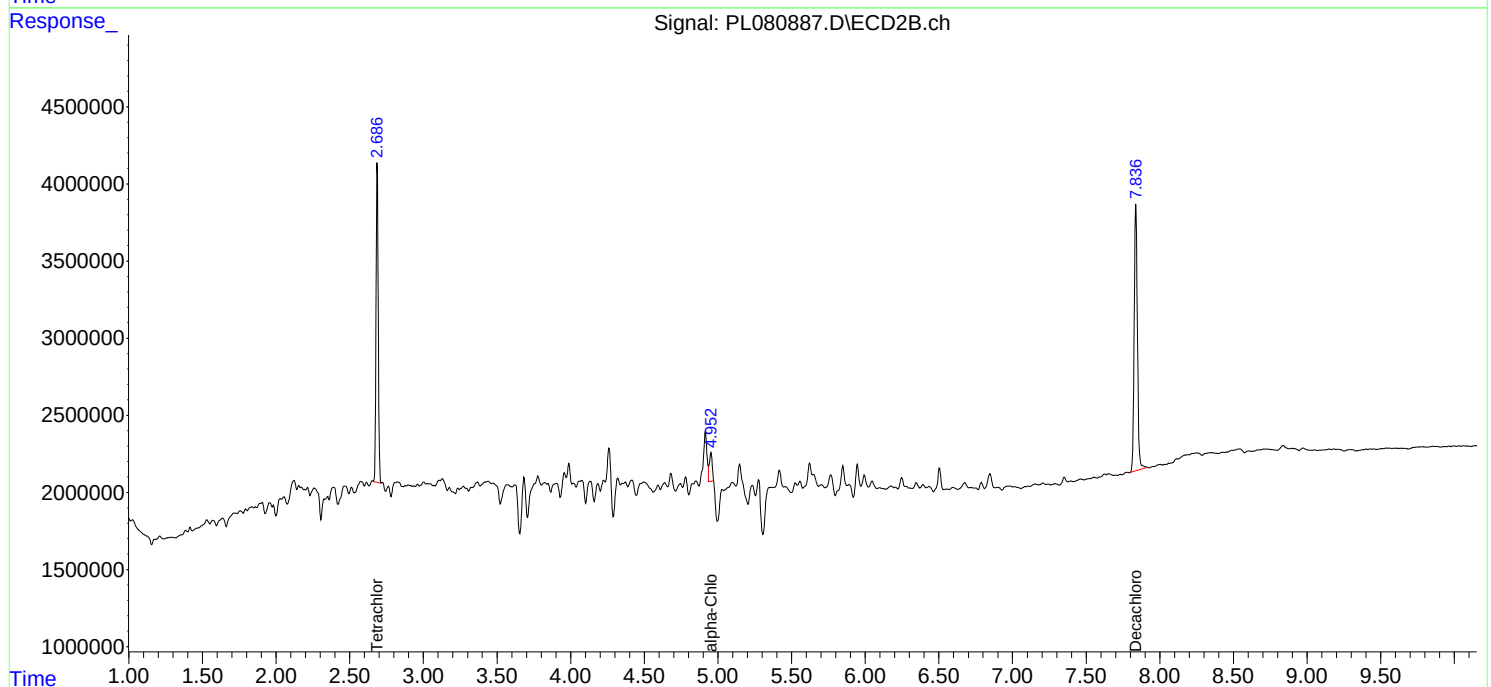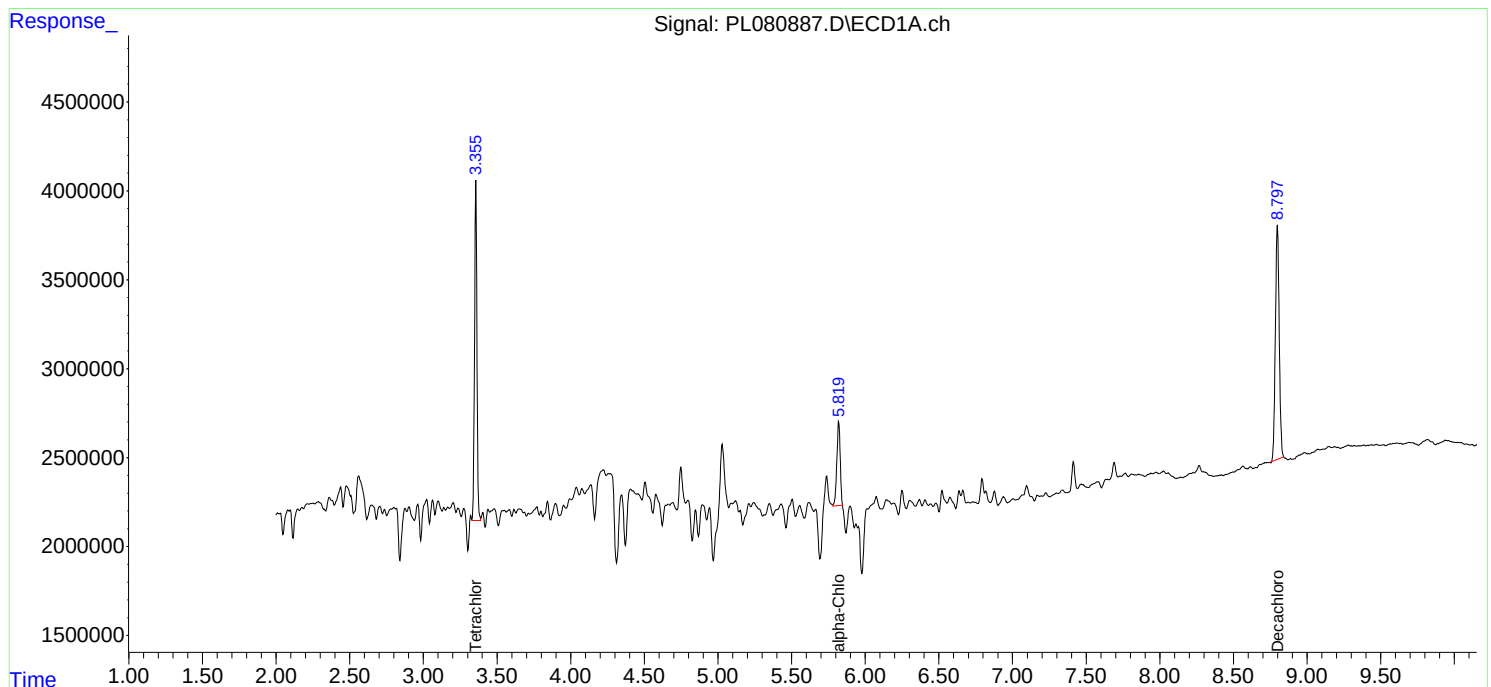

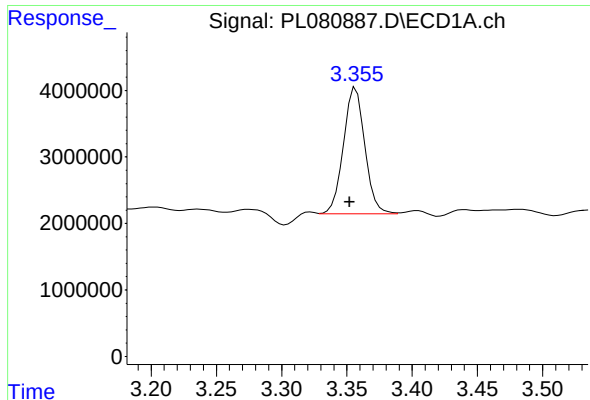


#1 Tetrachloro-m-xylene

R.T.: 3.355 min
Delta R.T.: 0.003 min
Response: 21622554
Conc: 10.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-01-021023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/14/2023
Supervised By :Ankita Jodhani 02/14/2023

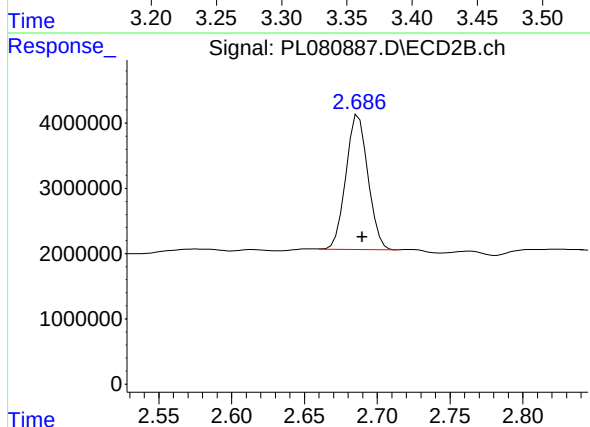


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: -0.004 min
Response: 21762496
Conc: 9.91 ng/ml

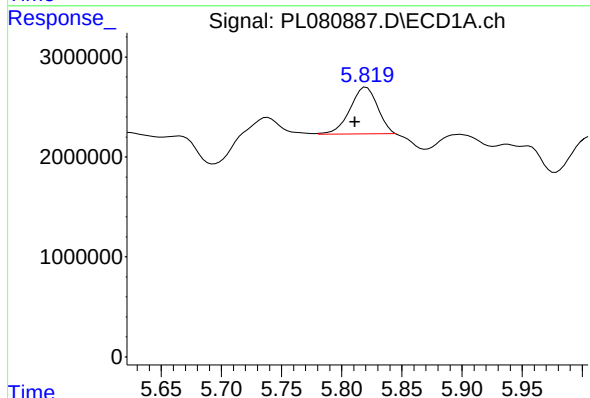


#11 alpha-Chlordane

R.T.: 5.819 min
Delta R.T.: 0.008 min
Response: 7477021
Conc: 2.96 ng/ml

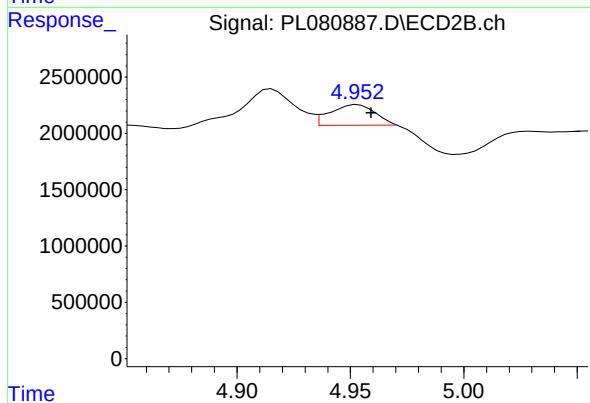

#11 alpha-Chlordane

R.T.: 4.952 min
Delta R.T.: -0.007 min
Response: 2461538
Conc: 0.86 ng/ml

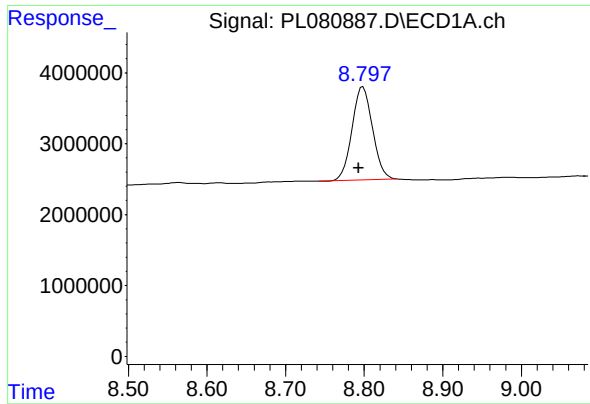


#28 Decachlorobiphenyl

R.T.: 8.798 min
Delta R.T.: 0.005 min
Response: 23826946
Conc: 13.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-01-021023

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/14/2023
Supervised By :Ankita Jodhani 02/14/2023

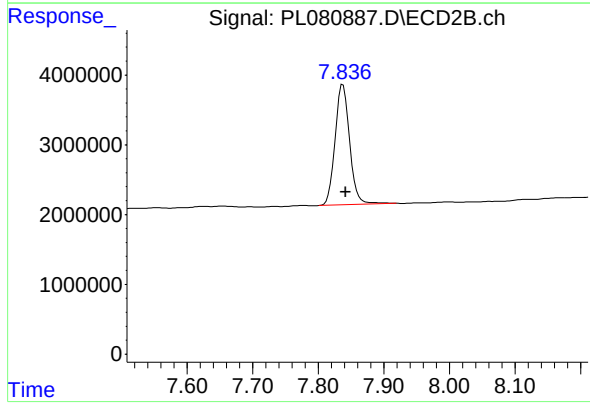

#28 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: -0.004 min
Response: 26633712
Conc: 11.18 ng/ml