

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021323\
 Data File : PL080894.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2023 15:54
 Operator : AR\AJ
 Sample : 01529-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-01-5.0-7.0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/14/2023
 Supervised By : Ankita Jodhani 02/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 20:16:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.350	2.688	36219043	36464484	16.887m	16.602
28) SA Decachlor...	8.790	7.836	14255313	39108655	8.142m	16.415m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021323\
Data File : PL080894.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2023 15:54
Operator : AR\AJ
Sample : 01529-05
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-01-5.0-7.0


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/14/2023
Supervised By : Ankita Jodhani 02/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 20:16:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

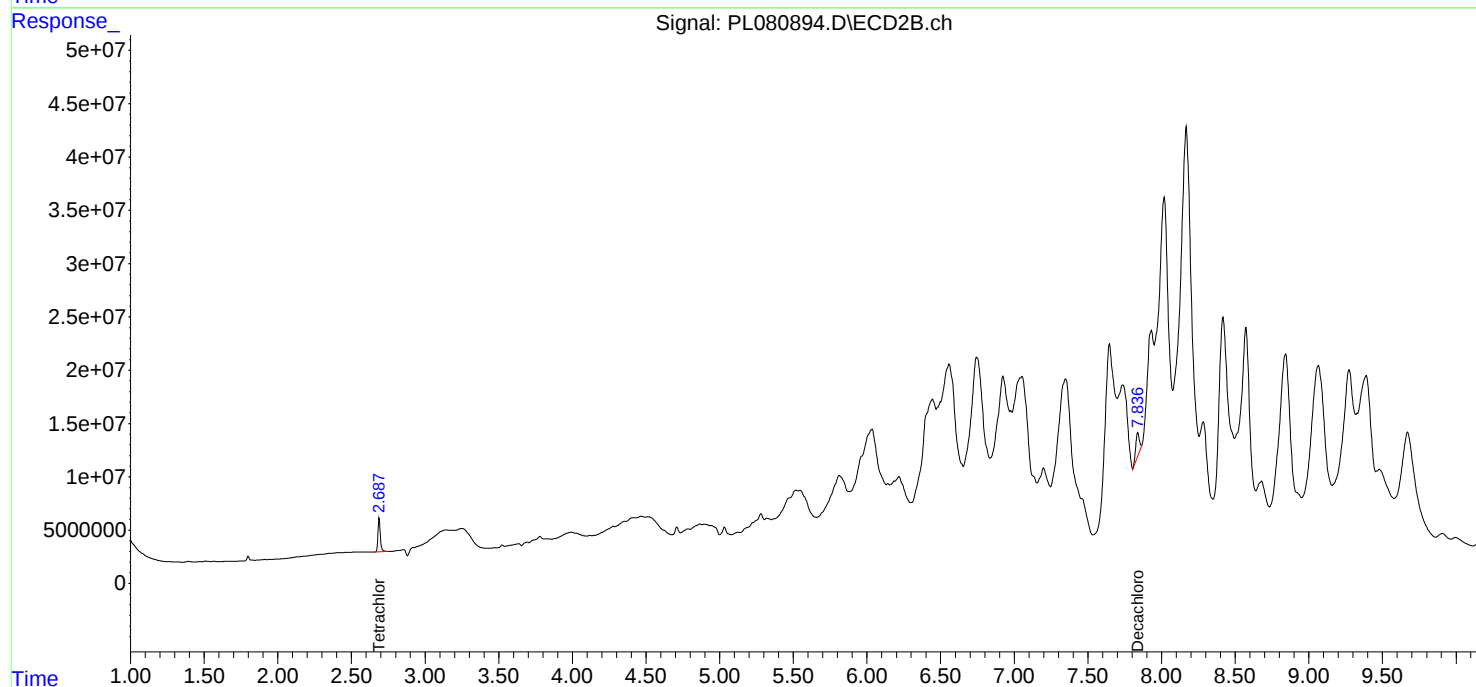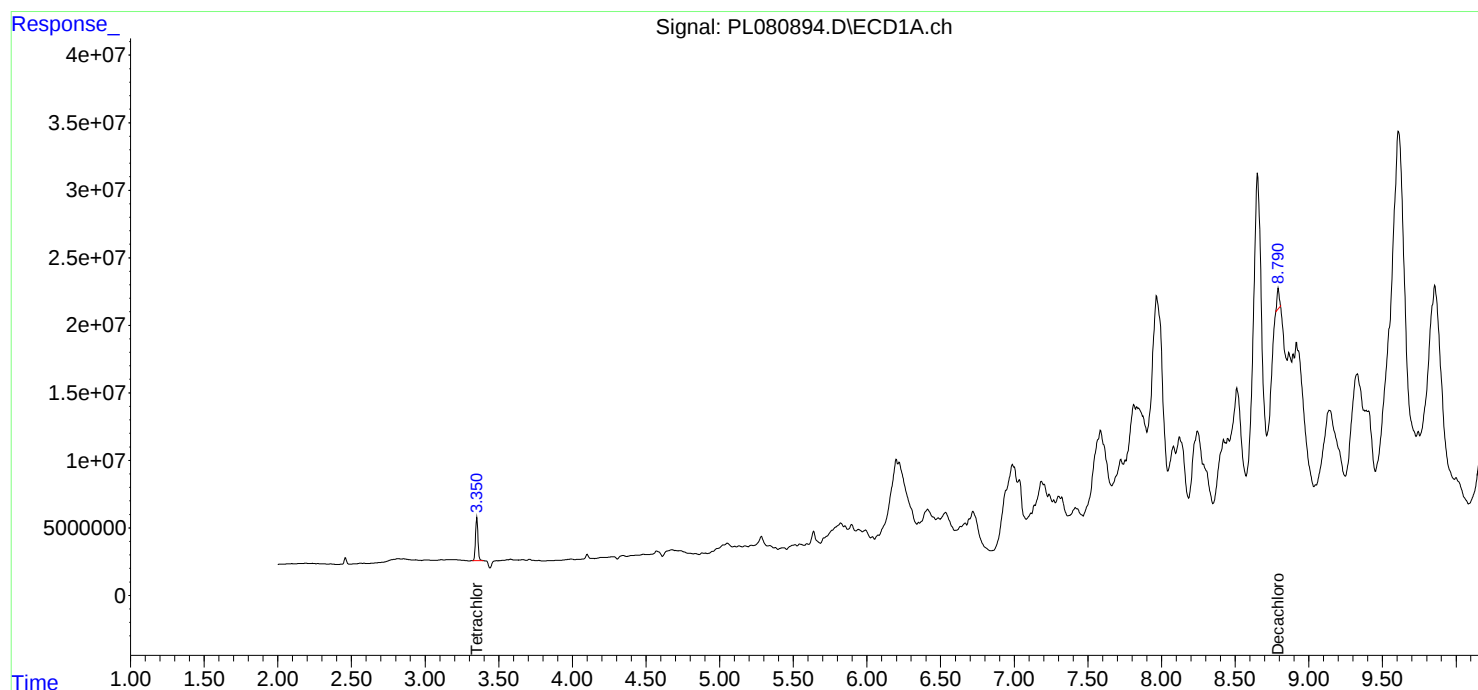

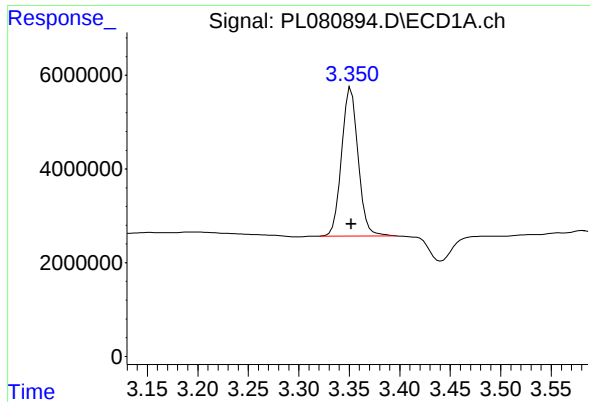


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.002 min
Response: 36219043
Conc: 16.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-01-5.0-7.0


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/14/2023
Supervised By :Ankita Jodhani 02/14/2023

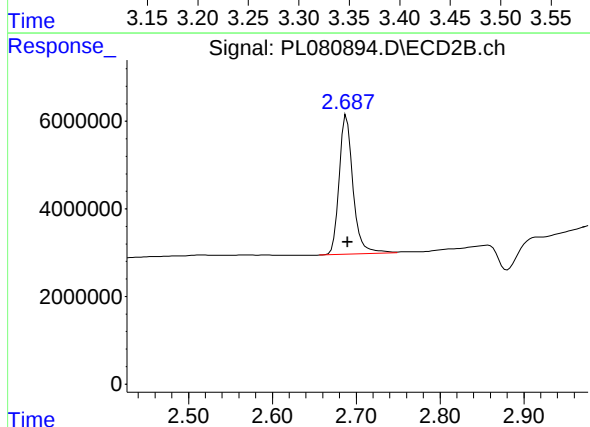


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: -0.001 min
Response: 36464484
Conc: 16.60 ng/ml

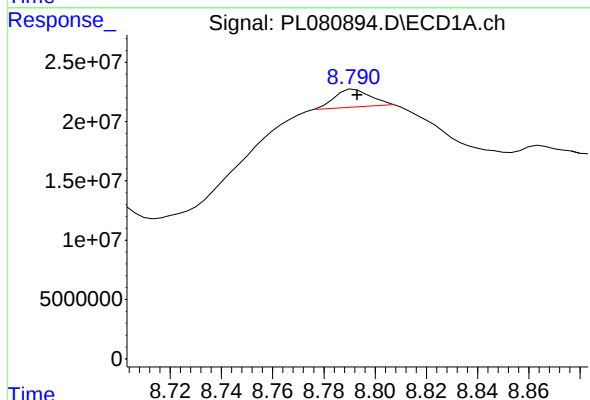

#28 Decachlorobiphenyl

R.T.: 8.790 min
Delta R.T.: -0.003 min
Response: 14255313
Conc: 8.14 ng/ml m

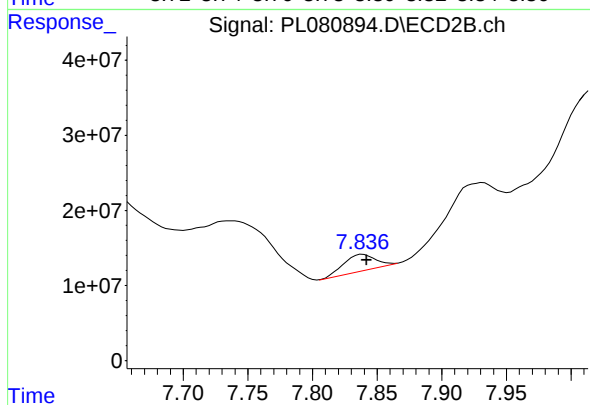

#28 Decachlorobiphenyl

R.T.: 7.836 min
Delta R.T.: -0.005 min
Response: 39108655
Conc: 16.41 ng/ml m