

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021420\
 Data File : PL056551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2020 12:27
 Operator : AJ\MA
 Sample : L1493-06DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 21:52:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 13 05:32:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.501	4.019	18559059	6244188	2.103	2.295
28)	SA Decachlor...	8.254	0.000	33081989	0	3.454	N.D. #
Target Compounds							
8)	B Heptachlo...	0.000	5.884	0	24489594	N.D.	8.754 #
10)	B gamma-Chl...	5.461f	6.140	43655822	34723587	3.174	11.872 #
12)	B 4,4'-DDE	5.665	6.359	87299244	47790555	6.866	17.055 #
13)	MA Dieldrin	5.791	6.499	262.7E6	17219531	19.693	5.917 #
14)	MA Endrin	6.065	6.721	556.0E6	38538130	47.469	15.821 #
15)	B Endosulfa...	6.315	0.000	71249613	0	6.769	N.D. #
16)	A 4,4'-DDD	0.000	6.854	0	52939334	N.D.	23.407 #
17)	MA 4,4'-DDT	6.418	7.148	463.6E6	21895097	48.912	10.365 #
18)	B Endrin al...	6.512f	0.000	56944431	0	5.934	N.D. #
19)	B Endosulfa...	6.705	0.000	62118733	0	5.835	N.D. #
20)	A Methoxychlor	6.951	0.000	167.5E6	0	34.031	N.D. #
21)	B Endrin ke...	7.226f	0.000	24561707	0	2.054	N.D. #
25)	Chlordane-3	5.461f	6.140	43655822	34723587	33.250	89.604 #
27)	Chlordane-5	6.315f	0.000	71249613	0	166.958	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021420\
Data File : PL056551.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2020 12:27
Operator : AJ\MA
Sample : L1493-06DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 21:52:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
Quant Title : GC Extractables
QLast Update : Thu Feb 13 05:32:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

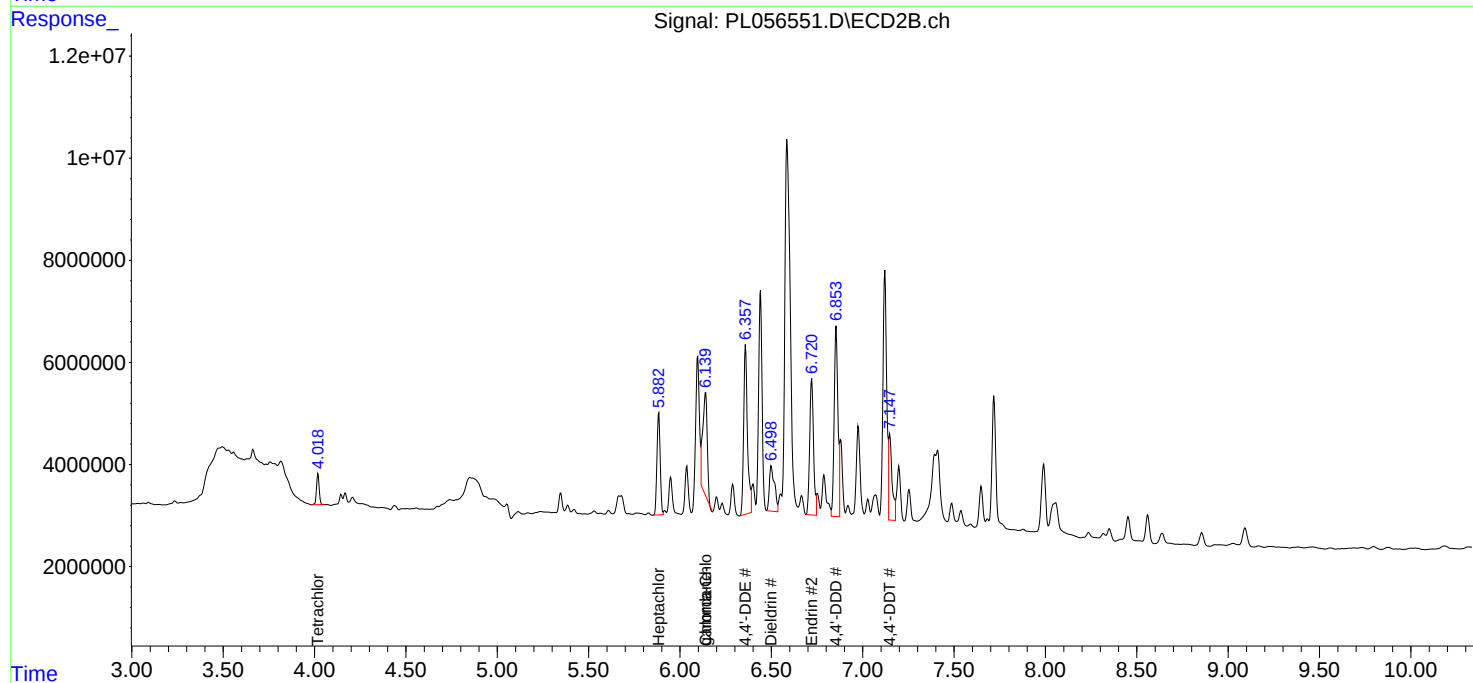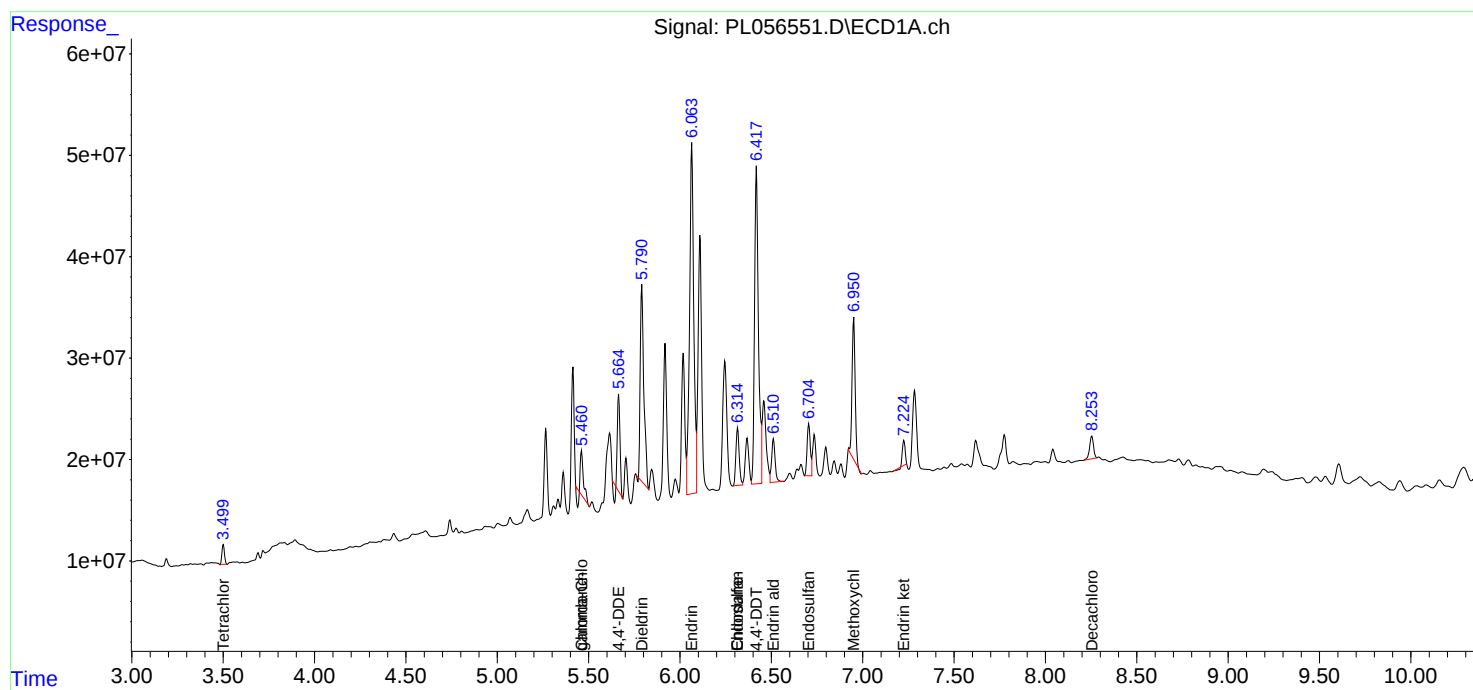


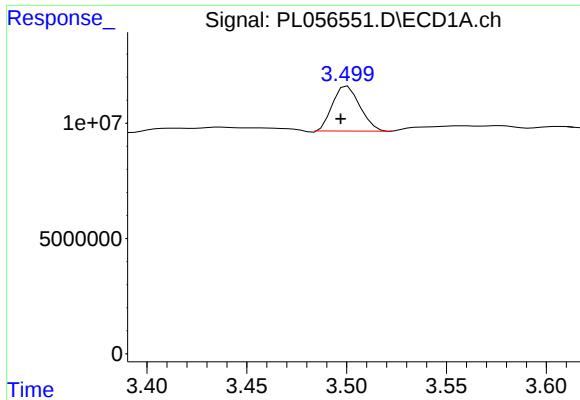

#1 Tetrachloro-m-xylene


R.T.: 3.501 min
Delta R.T.: 0.004 min
Response: 18559059
Conc: 2.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

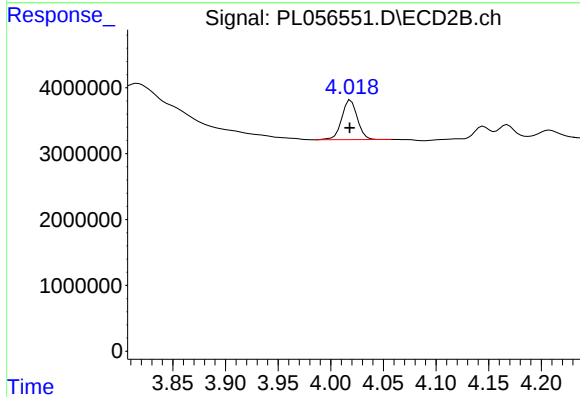


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 6244188
Conc: 2.30 ng/ml

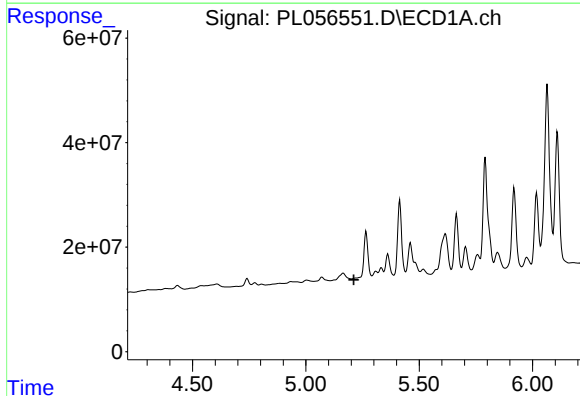


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.211 min
Response: 0
Conc: N.D.

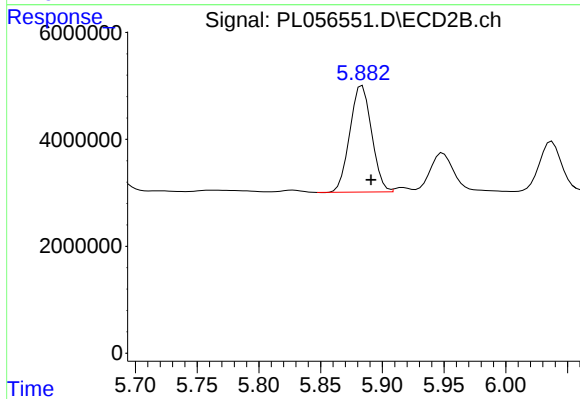

#8 Heptachlor epoxide


R.T.: 5.884 min
Delta R.T.: -0.007 min
Response: 24489594
Conc: 8.75 ng/ml

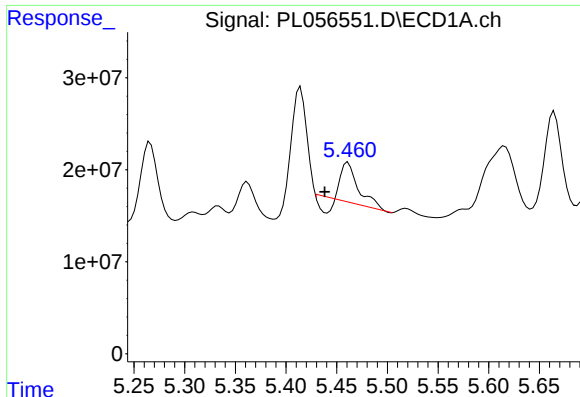

#10 gamma-Chlordane


R.T.: 5.461 min
Delta R.T.: 0.023 min
Response: 43655822
Conc: 3.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

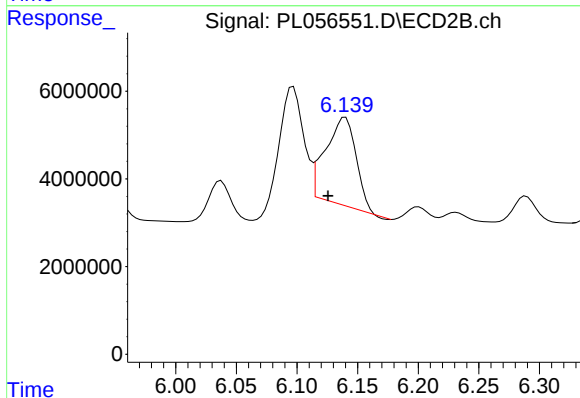


#10 gamma-Chlordane

R.T.: 6.140 min
Delta R.T.: 0.014 min
Response: 34723587
Conc: 11.87 ng/ml

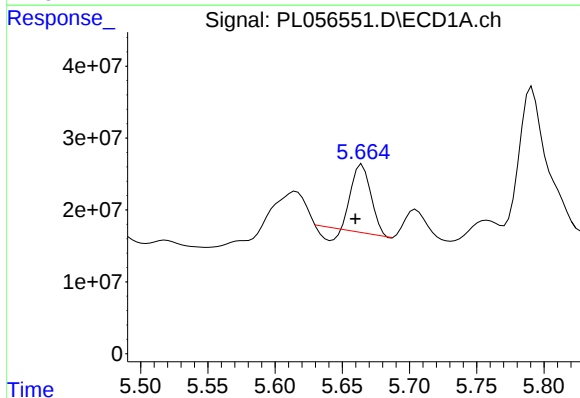


#12 4,4'-DDE

R.T.: 5.665 min
Delta R.T.: 0.005 min
Response: 87299244
Conc: 6.87 ng/ml

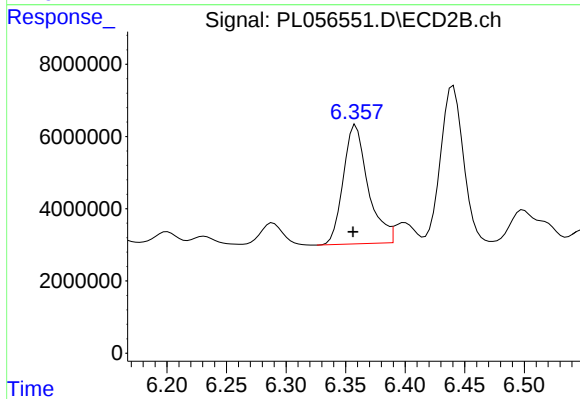

#12 4,4'-DDE


R.T.: 6.359 min
Delta R.T.: 0.003 min
Response: 47790555
Conc: 17.06 ng/ml

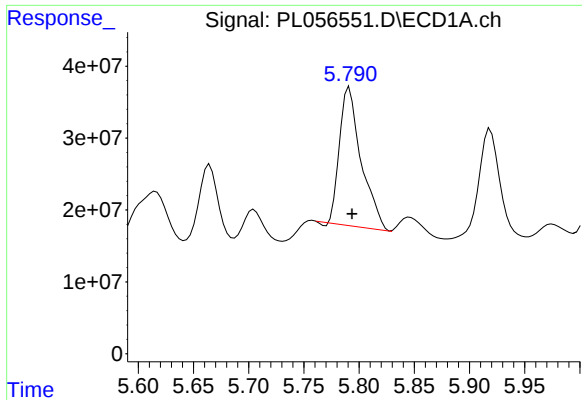

#13 Dieldrin


R.T.: 5.791 min
Delta R.T.: -0.002 min
Response: 262690763
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

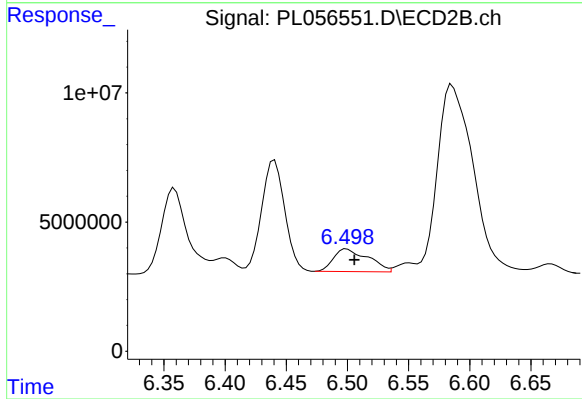


#13 Dieldrin

R.T.: 6.499 min
Delta R.T.: -0.007 min
Response: 17219531
Conc: 5.92 ng/ml

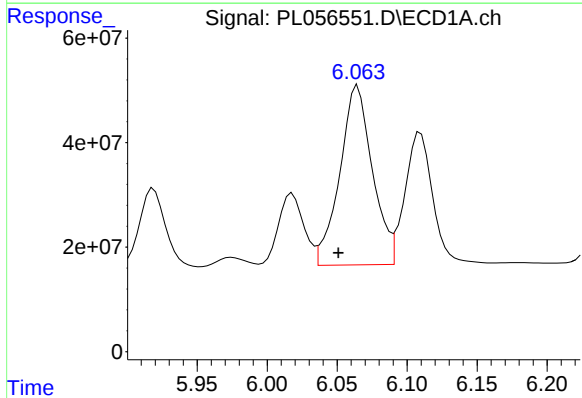


#14 Endrin

R.T.: 6.065 min
Delta R.T.: 0.014 min
Response: 555996569
Conc: 47.47 ng/ml

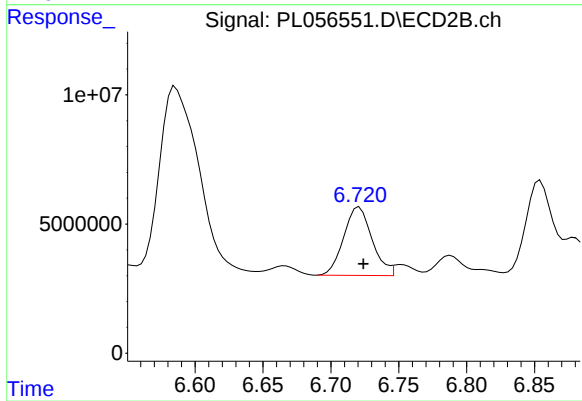

#14 Endrin


R.T.: 6.721 min
Delta R.T.: -0.003 min
Response: 38538130
Conc: 15.82 ng/ml

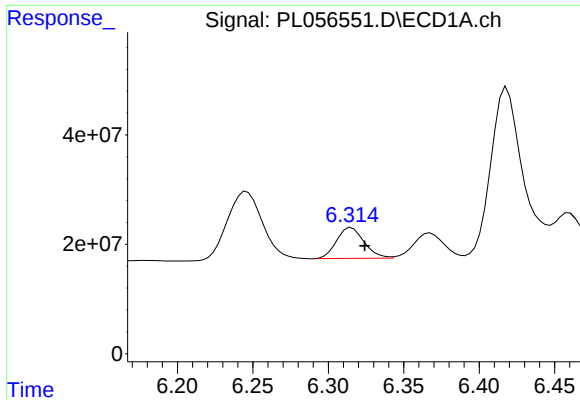

#15 Endosulfan II


R.T.: 6.315 min
Delta R.T.: -0.009 min
Response: 71249613
Conc: 6.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

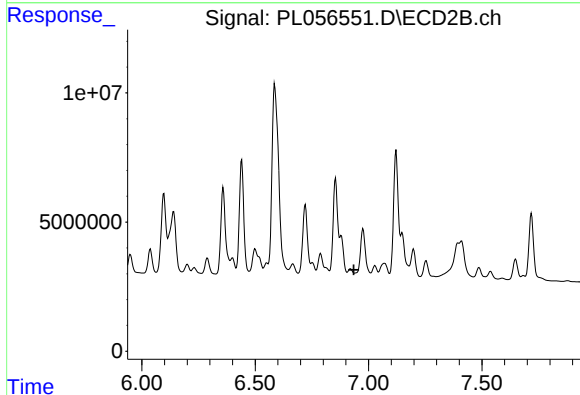


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

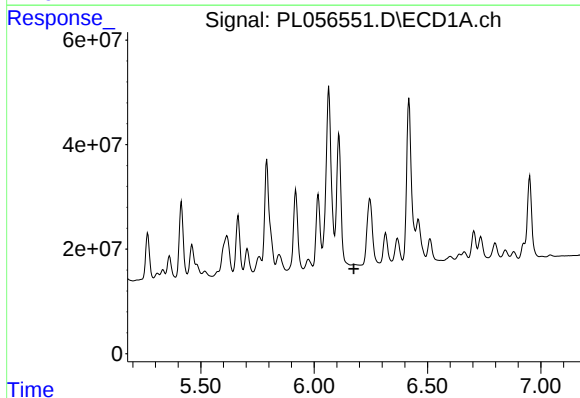


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

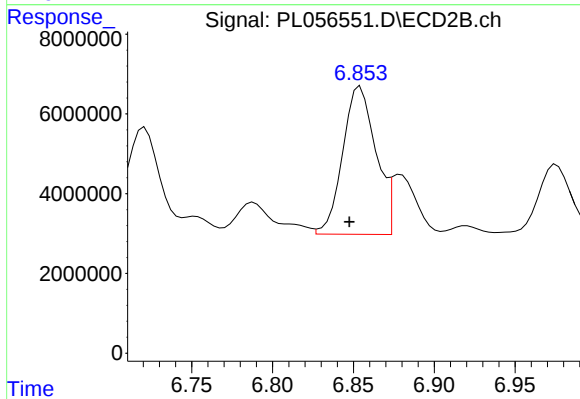

#16 4,4'-DDD


R.T.: 6.854 min
Delta R.T.: 0.007 min
Response: 52939334
Conc: 23.41 ng/ml

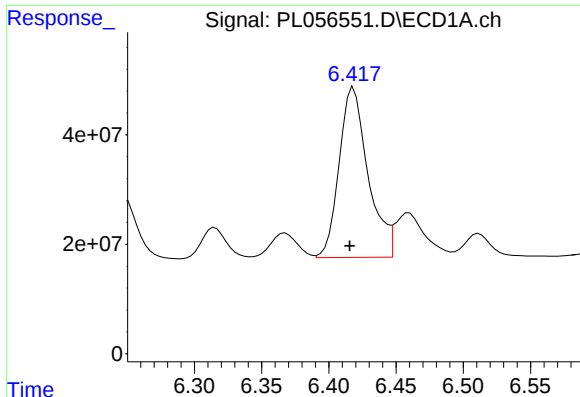

#17 4,4'-DDT


R.T.: 6.418 min
Delta R.T.: 0.003 min
Response: 463552156
Conc: 48.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

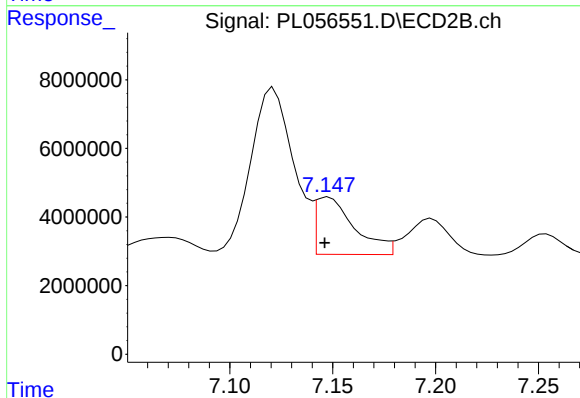


#17 4,4'-DDT

R.T.: 7.148 min
Delta R.T.: 0.002 min
Response: 21895097
Conc: 10.37 ng/ml

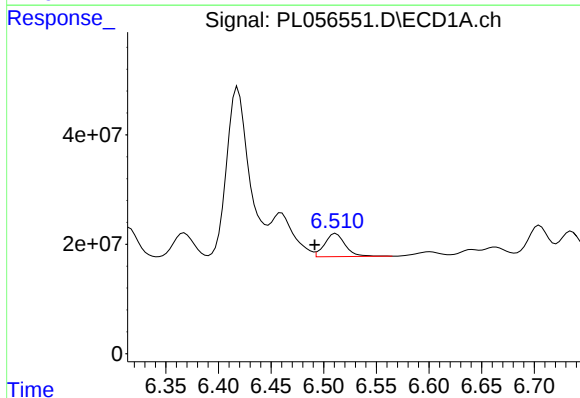


#18 Endrin aldehyde

R.T.: 6.512 min
Delta R.T.: 0.020 min
Response: 56944431
Conc: 5.93 ng/ml

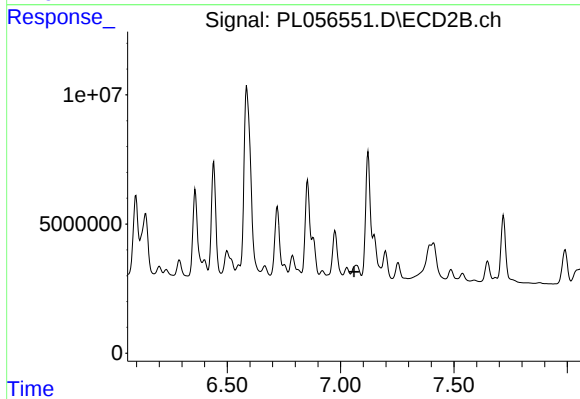

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.059 min
Response: 0
Conc: N.D.

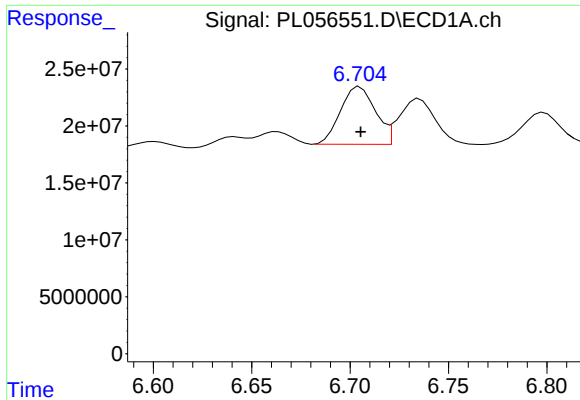

#19 Endosulfan Sulfate


R.T.: 6.705 min
Delta R.T.: 0.000 min
Response: 62118733
Conc: 5.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

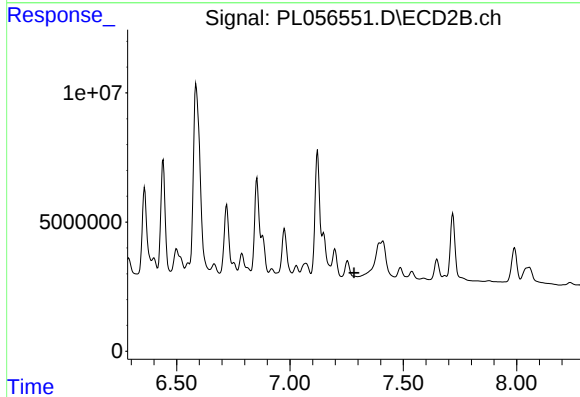


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

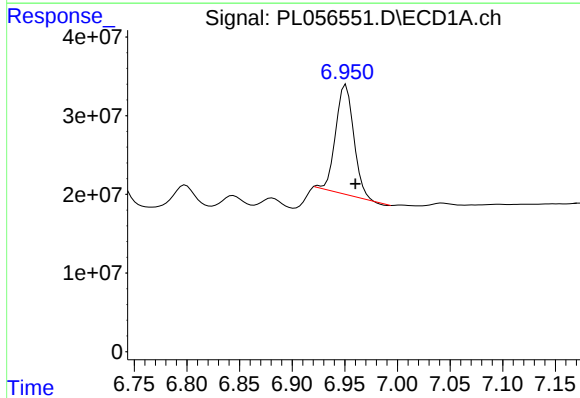


#20 Methoxychlor

R.T.: 6.951 min
Delta R.T.: -0.009 min
Response: 167455558
Conc: 34.03 ng/ml

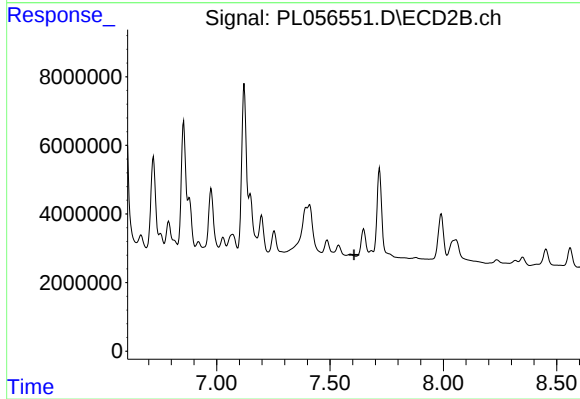

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.606 min
Response: 0
Conc: N.D.

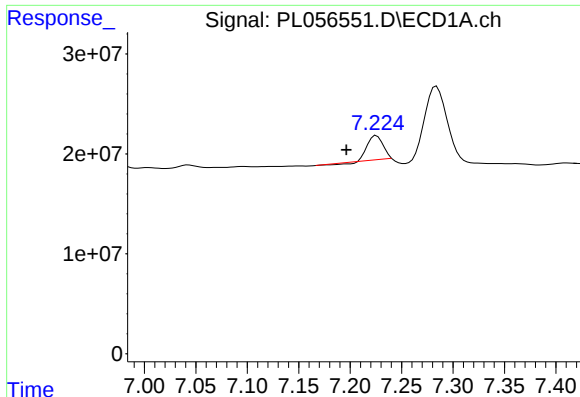

#21 Endrin ketone


R.T.: 7.226 min
Delta R.T.: 0.029 min
Response: 24561707
Conc: 2.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

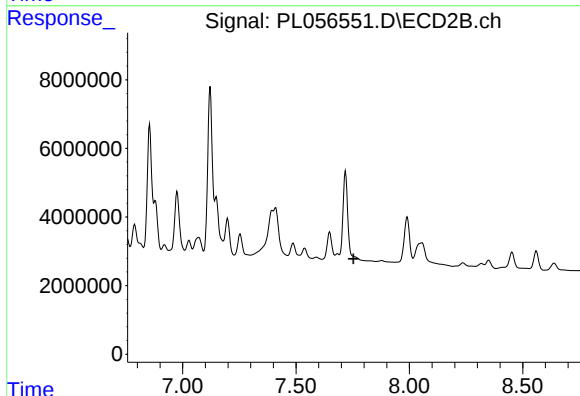


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.754 min
Response: 0
Conc: N.D.

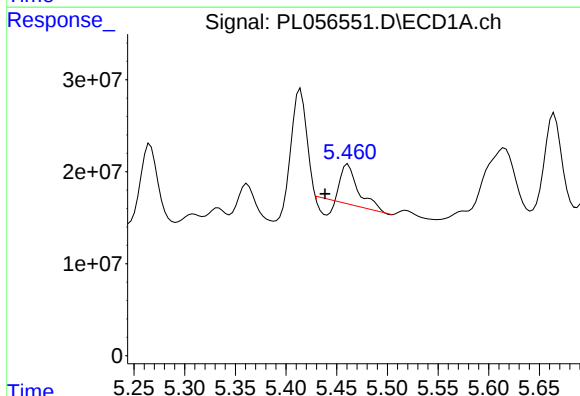


#25 Chlordane-3

R.T.: 5.461 min
Delta R.T.: 0.023 min
Response: 43655822
Conc: 33.25 ng/ml

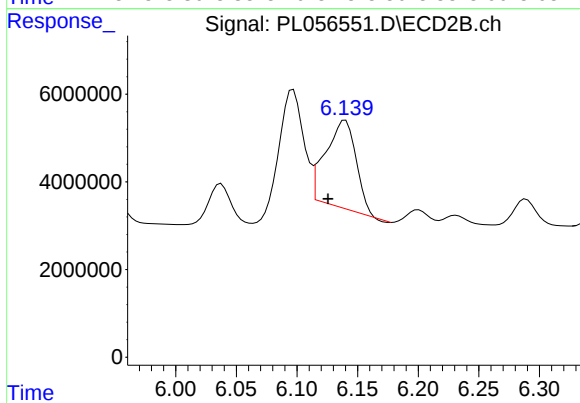

#25 Chlordane-3


R.T.: 6.140 min
Delta R.T.: 0.014 min
Response: 34723587
Conc: 89.60 ng/ml

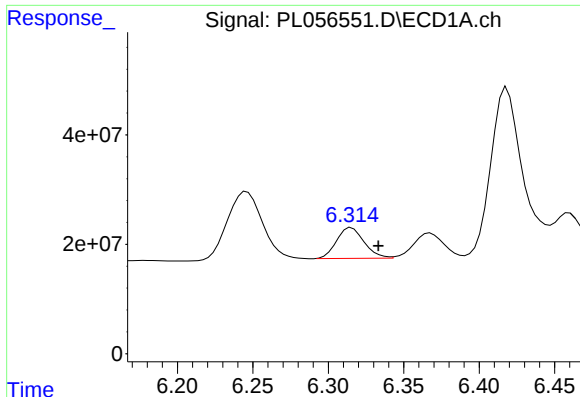

#27 Chlordane-5


R.T.: 6.315 min
Delta R.T.: -0.018 min
Response: 71249613
Conc: 166.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

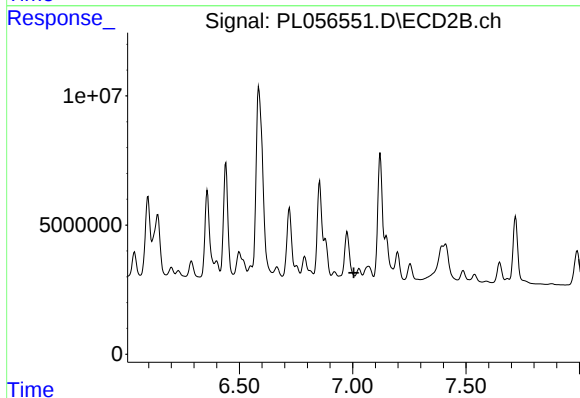


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.006 min
Response: 0
Conc: N.D.

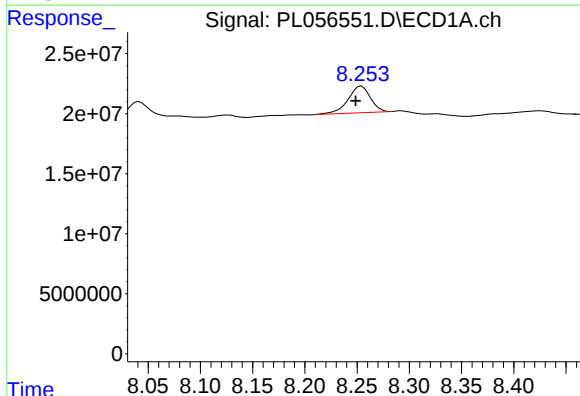

#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: 0.006 min
Response: 33081989
Conc: 3.45 ng/ml

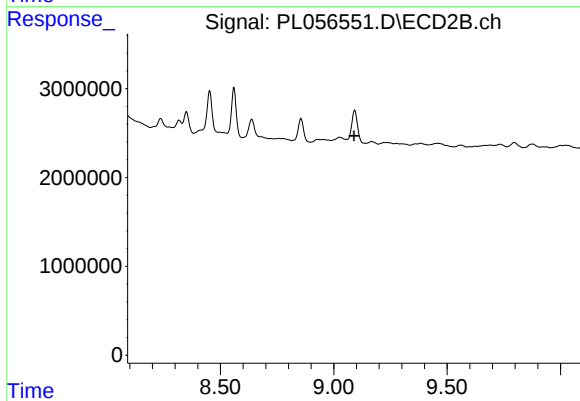

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.090 min
Response: 0
Conc: N.D.