

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021420\
 Data File : PL056558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2020 14:31
 Operator : AJ\MA
 Sample : L1015-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 21:53:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 13 05:32:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.019	209.9E6	61029752	23.790	22.434
28)	SA Decachlor...	8.247	9.090	187.6E6	51709433	19.587	25.351 #
Target Compounds							
9)	A Endosulfan I	5.574f	0.000	132.3E6	0	10.545	N.D. #
10)	B gamma-Chl...	0.000	6.122	0	30518263	N.D.	10.434 #
13)	MA Dieldrin	5.796	0.000	67625018	0	5.070	N.D. #
14)	MA Endrin	6.046	0.000	165.4E6	0	14.118	N.D. #
15)	B Endosulfa...	6.327	0.000	64922172	0	6.168	N.D. #
16)	A 4,4'-DDD	6.188	6.850	68364255	7553082	7.224	3.340 #
18)	B Endrin al...	6.505	0.000	45674785	0	4.760	N.D. #
19)	B Endosulfa...	6.724f	0.000	22610396	0	2.124	N.D. #
25)	Chlordane-3	0.000	6.122	0	30518263	N.D.	78.753 #
27)	Chlordane-5	6.327	0.000	64922172	0	152.131	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021420\
Data File : PL056558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2020 14:31
Operator : AJ\MA
Sample : L1015-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 21:53:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
Quant Title : GC Extractables
QLast Update : Thu Feb 13 05:32:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

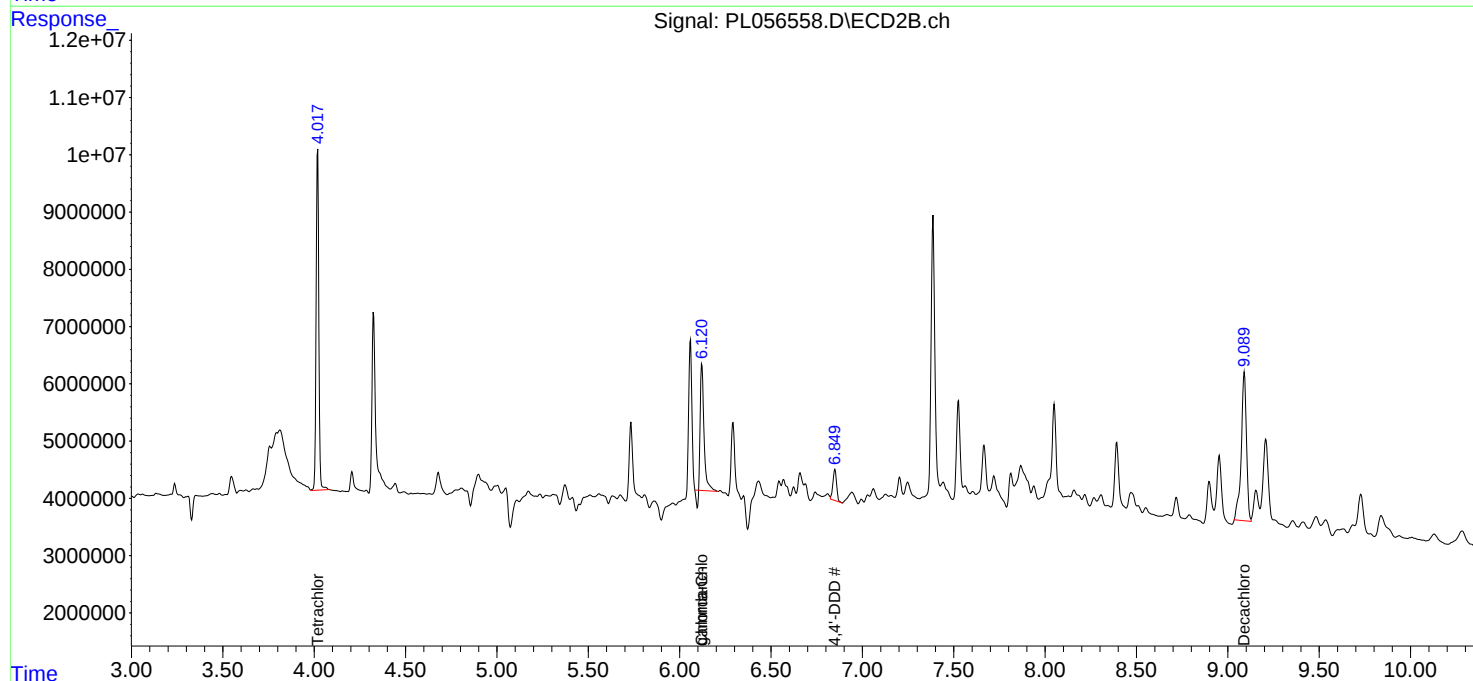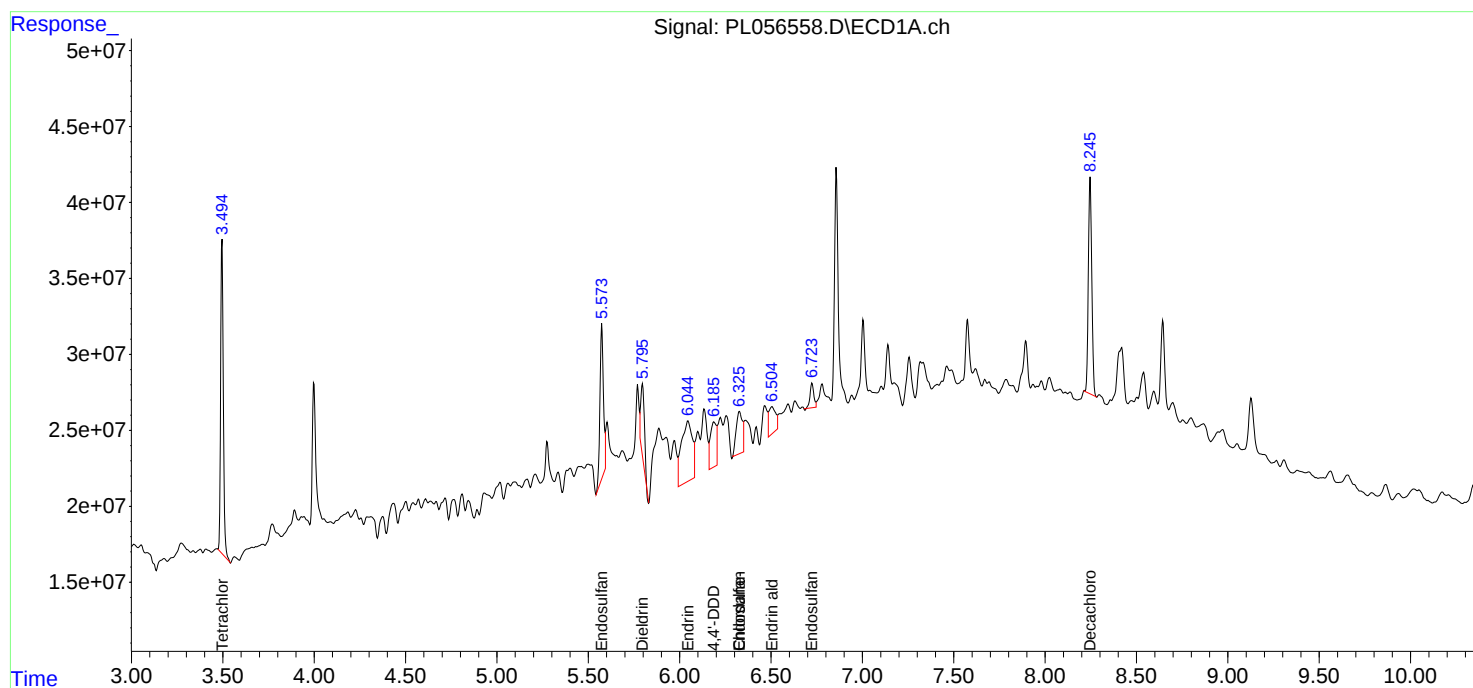


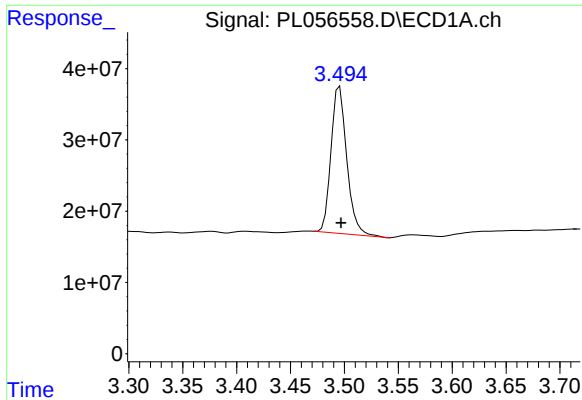

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: -0.001 min
Response: 209909056
Conc: 23.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

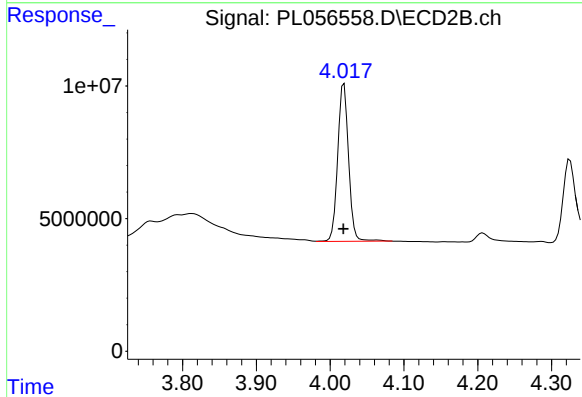


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 61029752
Conc: 22.43 ng/ml

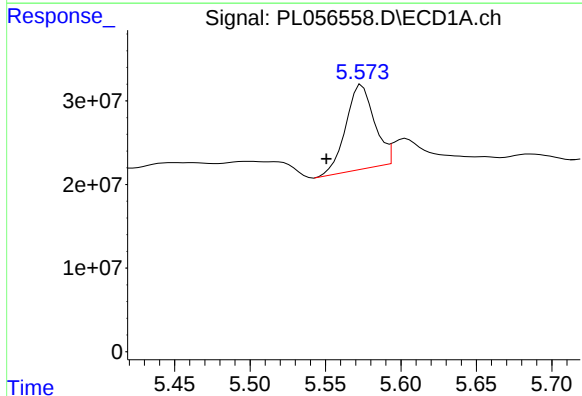


#9 Endosulfan I

R.T.: 5.574 min
Delta R.T.: 0.024 min
Response: 132315250
Conc: 10.55 ng/ml

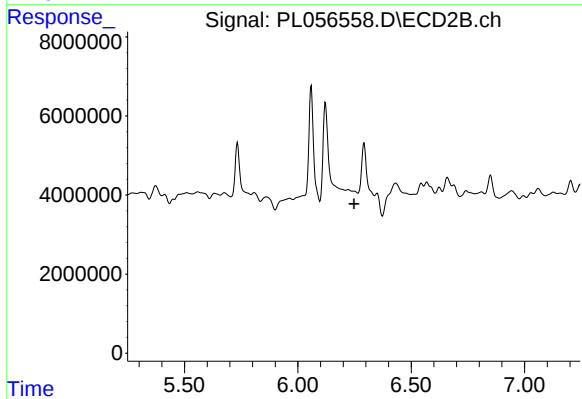

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.248 min
Response: 0
Conc: N.D.

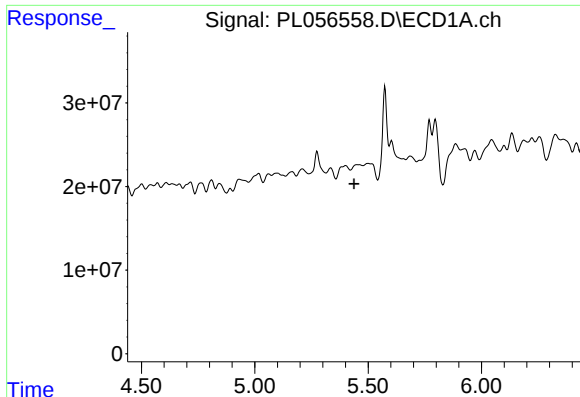

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

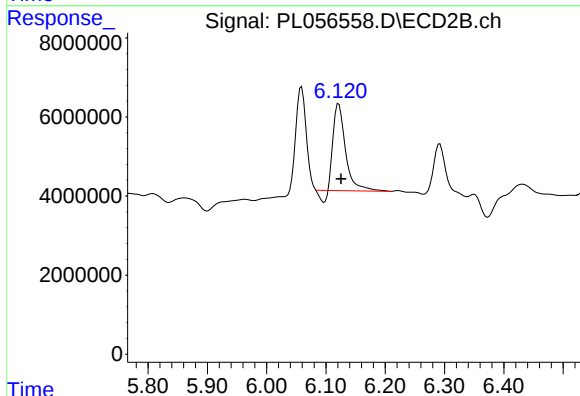


#10 gamma-Chlordane

R.T.: 6.122 min
Delta R.T.: -0.004 min
Response: 30518263
Conc: 10.43 ng/ml

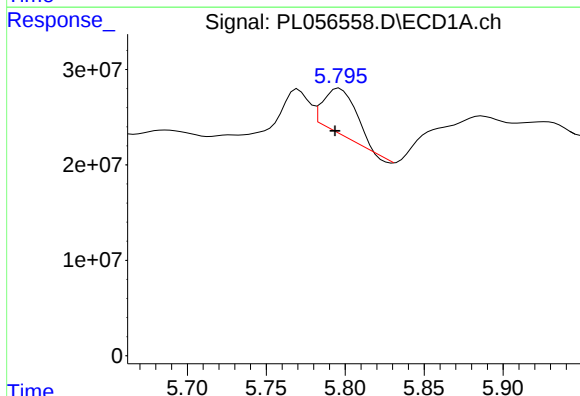


#13 Dieldrin

R.T.: 5.796 min
Delta R.T.: 0.003 min
Response: 67625018
Conc: 5.07 ng/ml

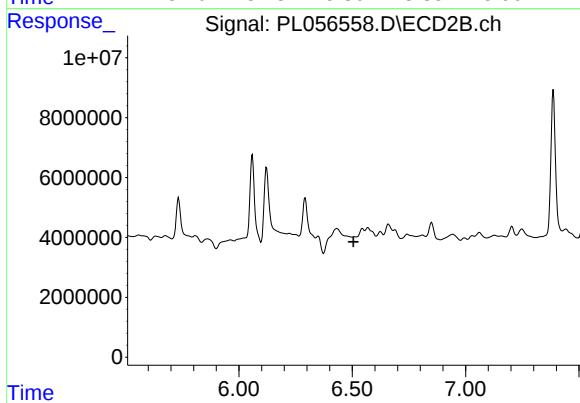

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.506 min
Response: 0
Conc: N.D.

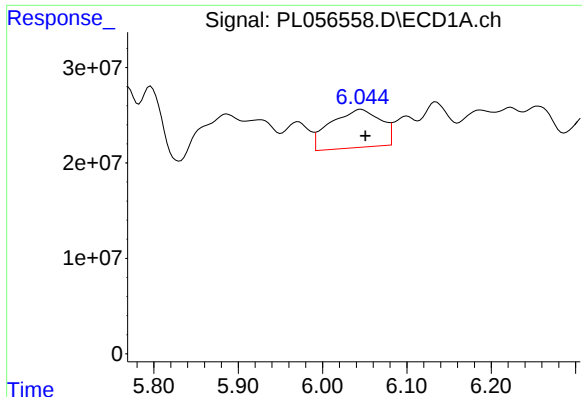

#14 Endrin


R.T.: 6.046 min
Delta R.T.: -0.005 min
Response: 165354673
Conc: 14.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

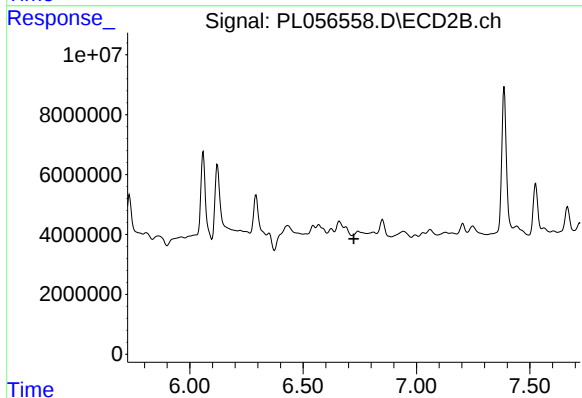


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.724 min
Response: 0
Conc: N.D.

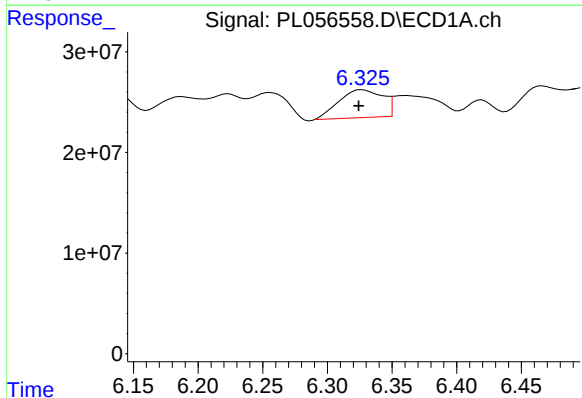


#15 Endosulfan II

R.T.: 6.327 min
Delta R.T.: 0.003 min
Response: 64922172
Conc: 6.17 ng/ml

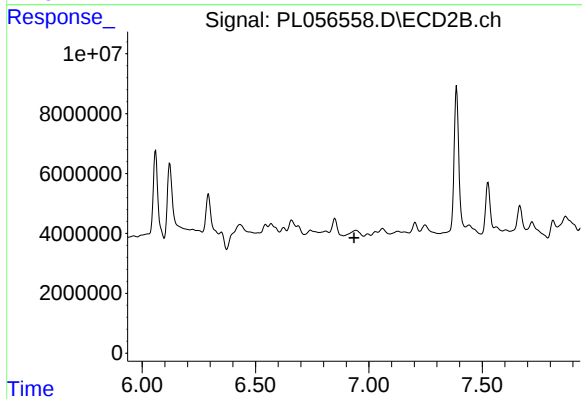

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

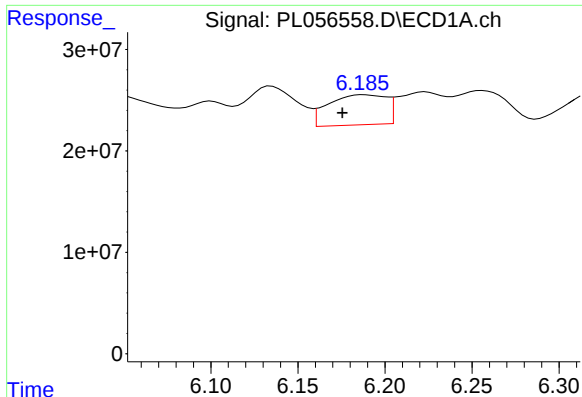

#16 4,4'-DDD


R.T.: 6.188 min
Delta R.T.: 0.012 min
Response: 68364255
Conc: 7.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

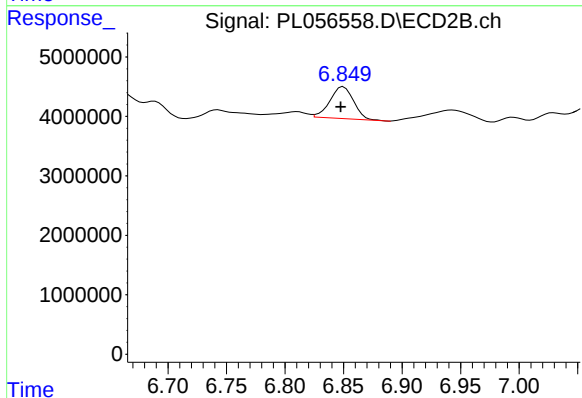


#16 4,4'-DDD

R.T.: 6.850 min
Delta R.T.: 0.002 min
Response: 7553082
Conc: 3.34 ng/ml

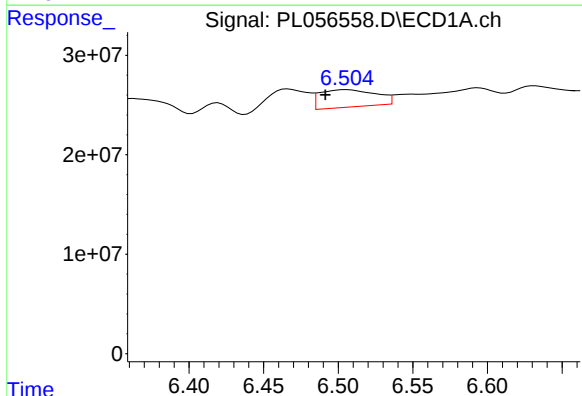


#18 Endrin aldehyde

R.T.: 6.505 min
Delta R.T.: 0.014 min
Response: 45674785
Conc: 4.76 ng/ml

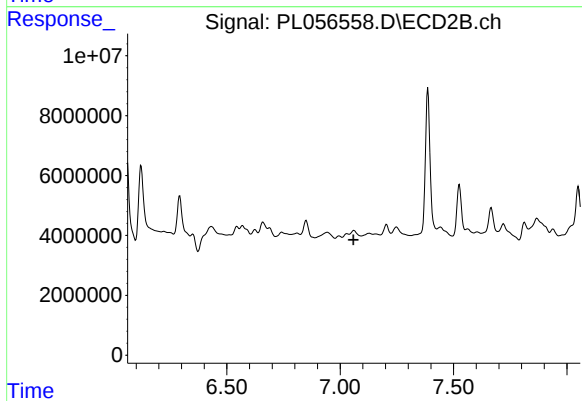

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.059 min
Response: 0
Conc: N.D.

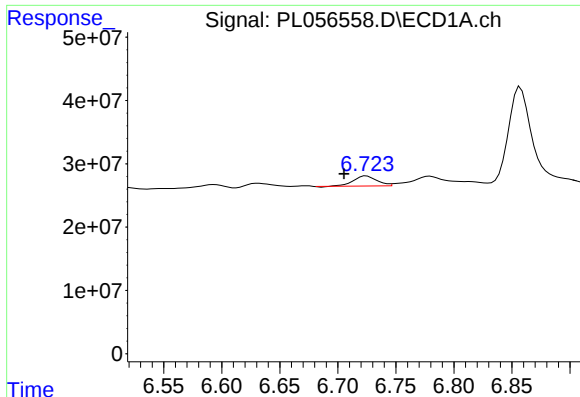

#19 Endosulfan Sulfate


R.T.: 6.724 min
Delta R.T.: 0.019 min
Response: 22610396
Conc: 2.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

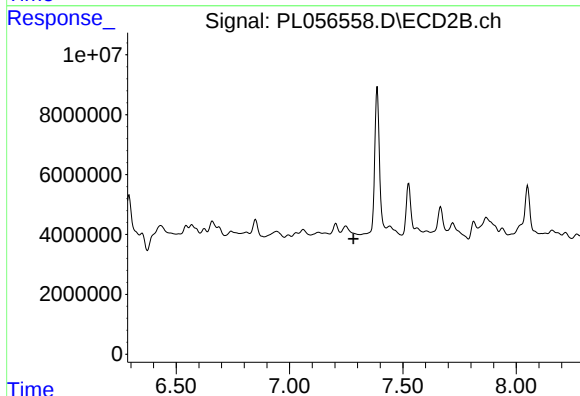


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

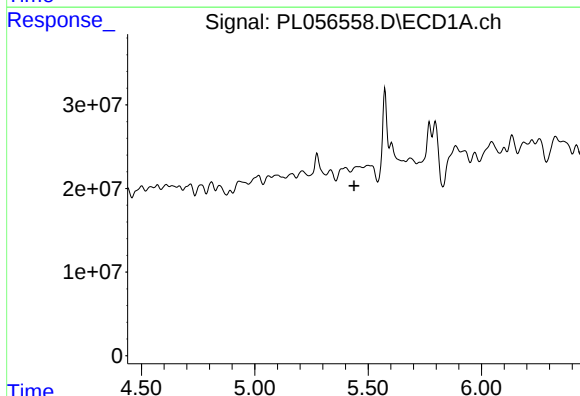


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.438 min
Response: 0
Conc: N.D.

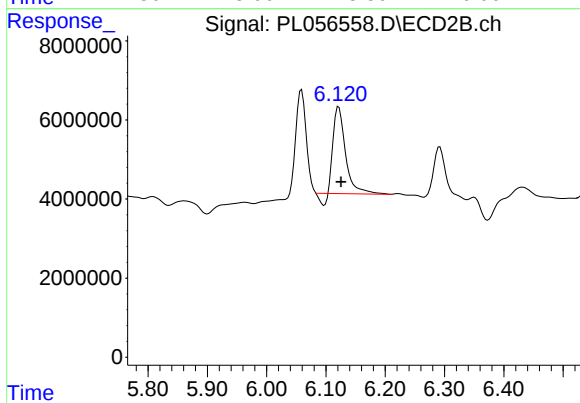

#25 Chlordane-3


R.T.: 6.122 min
Delta R.T.: -0.004 min
Response: 30518263
Conc: 78.75 ng/ml

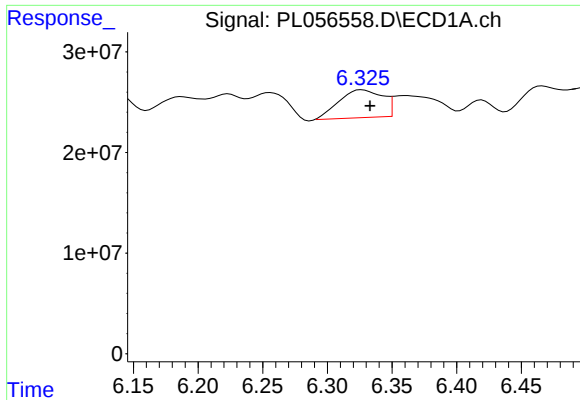

#27 Chlordane-5


R.T.: 6.327 min
Delta R.T.: -0.006 min
Response: 64922172
Conc: 152.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

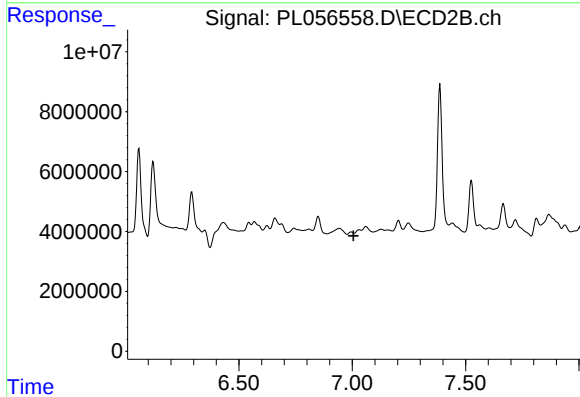


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.006 min
Response: 0
Conc: N.D.

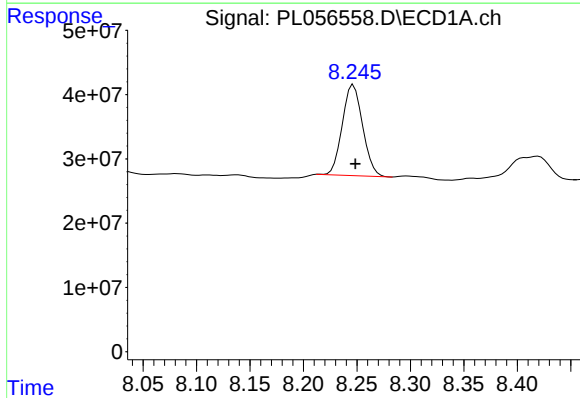

#28 Decachlorobiphenyl

R.T.: 8.247 min
Delta R.T.: -0.002 min
Response: 187631432
Conc: 19.59 ng/ml

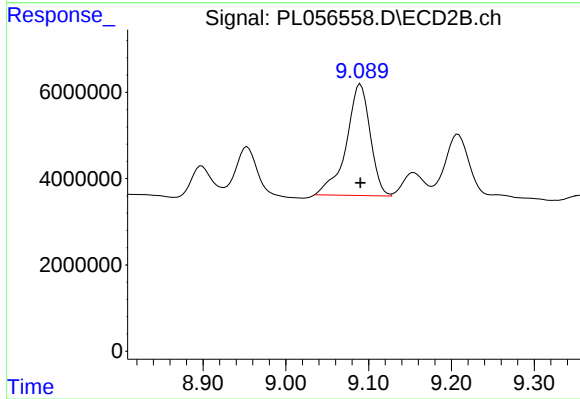

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 51709433
Conc: 25.35 ng/ml