

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021420\
 Data File : PL056571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2020 17:34
 Operator : AJ\MA
 Sample : L1484-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 21:56:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 13 05:32:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.018	115.5E6	36994092	13.093	13.599
28)	SA Decachlor...	8.246	9.088	123.5E6	25857529	12.895	12.677
Target Compounds							
4)	MA Heptachlor	0.000	5.220f	0	4532294	N.D.	1.348 #
5)	MB Aldrin	0.000	5.476f	0	7691878	N.D.	2.372 #
10)	B gamma-Chl...	5.459f	6.125	102.3E6	11642938	7.438	3.981 #
11)	B alpha-Chl...	5.494	6.199	54359926	30162443	3.991	10.269 #
23)	Chlordane-1	4.367	5.010	36854203	9011516	97.969	87.451
24)	Chlordane-2	4.868	5.476	26221764	7691878	60.871	74.503
25)	Chlordane-3	5.459f	6.125	102.3E6	11642938	77.920	30.045 #
26)	Chlordane-4	5.494	6.199	54359926	30162443	50.032	66.277 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021420\
Data File : PL056571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2020 17:34
Operator : AJ\MA
Sample : L1484-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 21:56:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021220.M
Quant Title : GC Extractables
QLast Update : Thu Feb 13 05:32:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

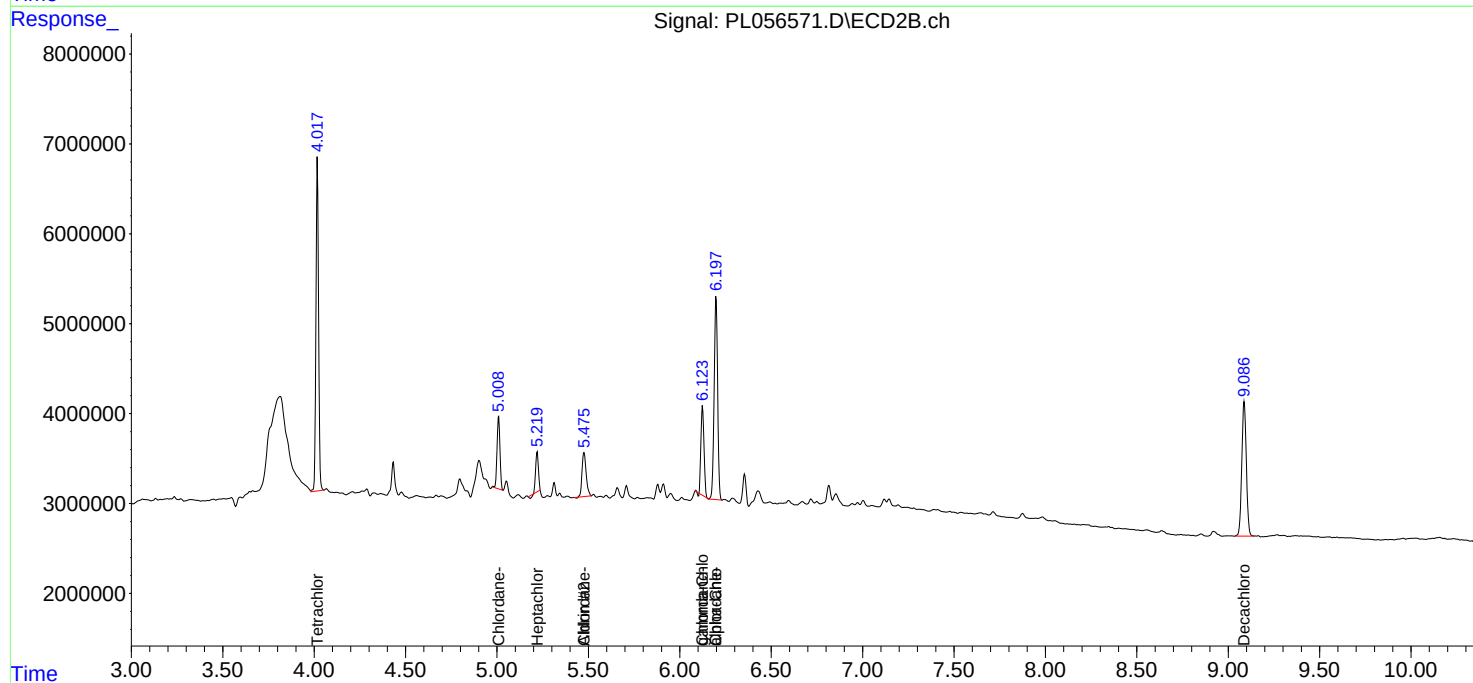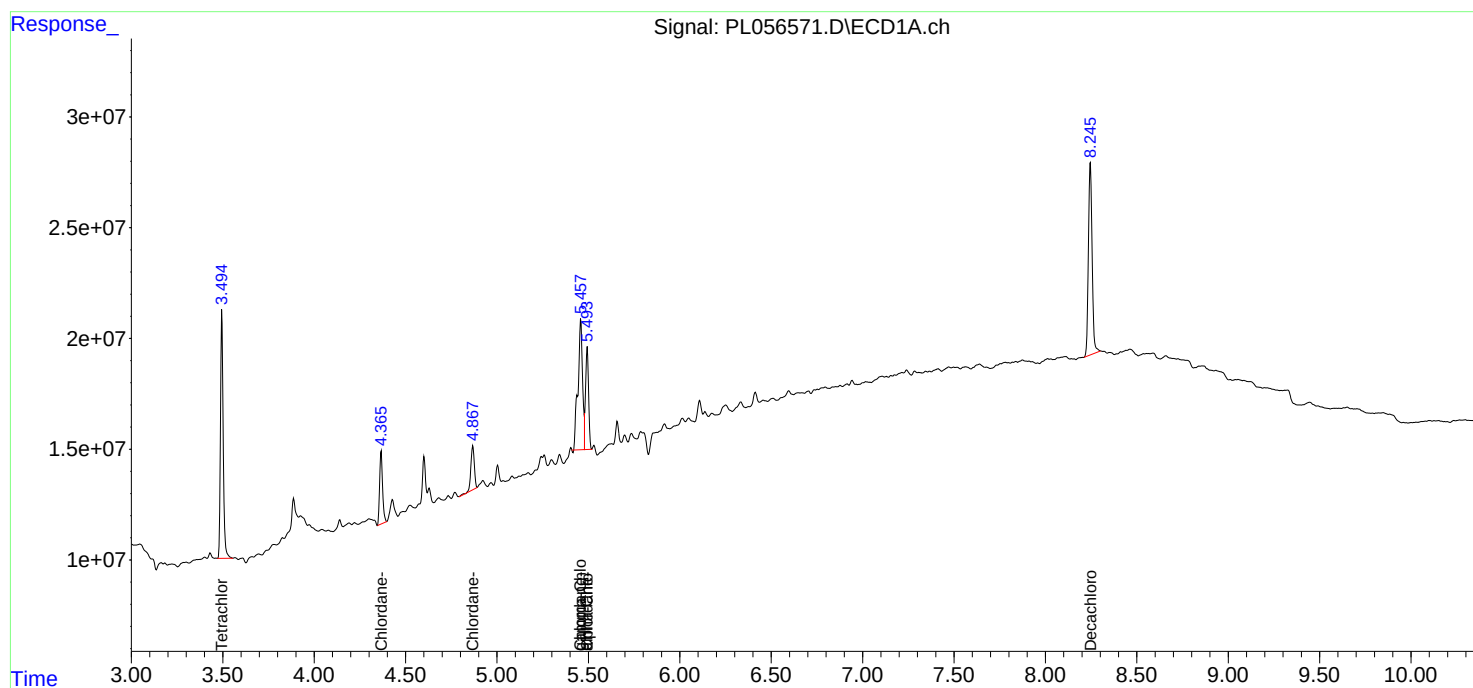


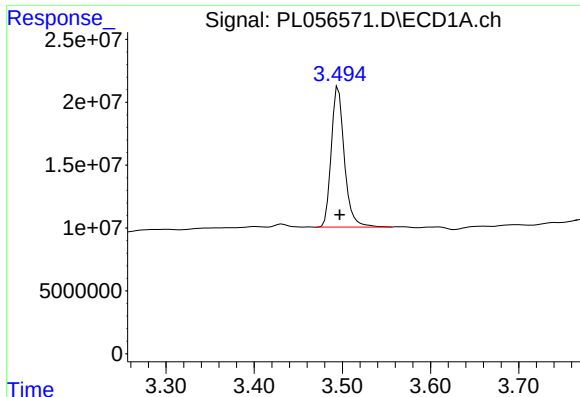

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: -0.002 min
Response: 115527733
Conc: 13.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

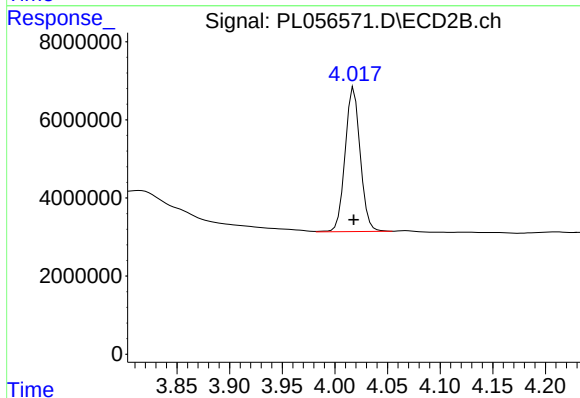


#1 Tetrachloro-m-xylene

R.T.: 4.018 min
Delta R.T.: 0.000 min
Response: 36994092
Conc: 13.60 ng/ml

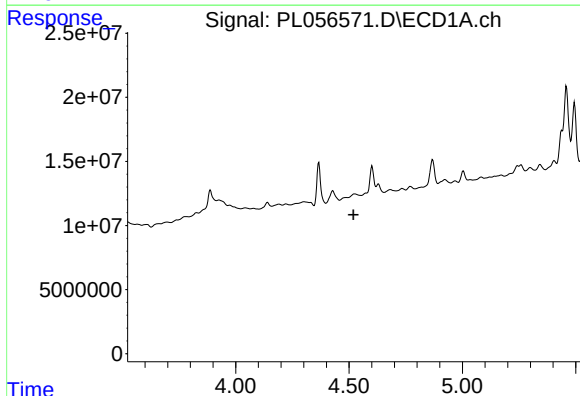


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.520 min
Response: 0
Conc: N.D.

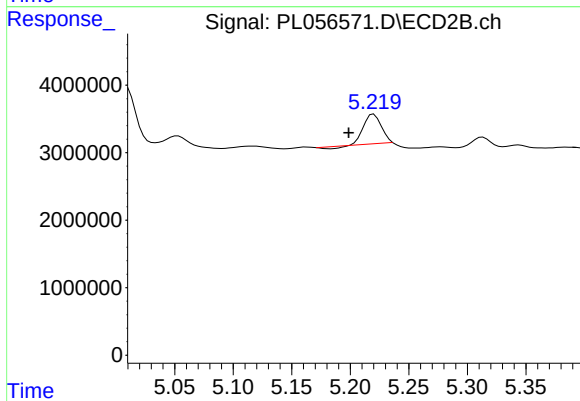

#4 Heptachlor


R.T.: 5.220 min
Delta R.T.: 0.021 min
Response: 4532294
Conc: 1.35 ng/ml

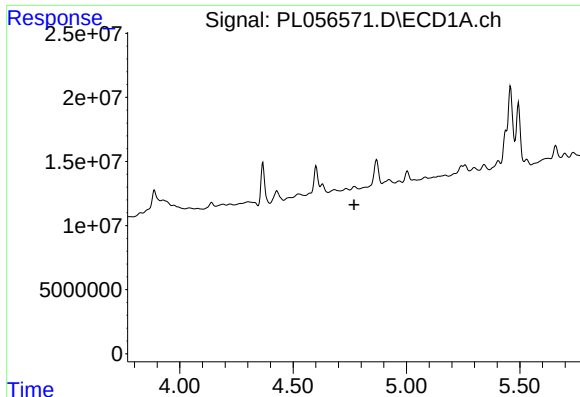

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.769 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

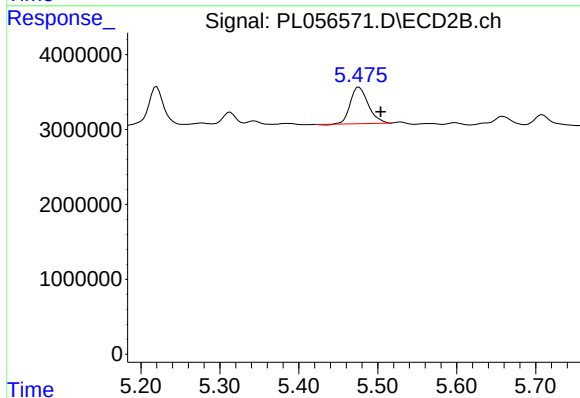


#5 Aldrin

R.T.: 5.476 min
Delta R.T.: -0.027 min
Response: 7691878
Conc: 2.37 ng/ml

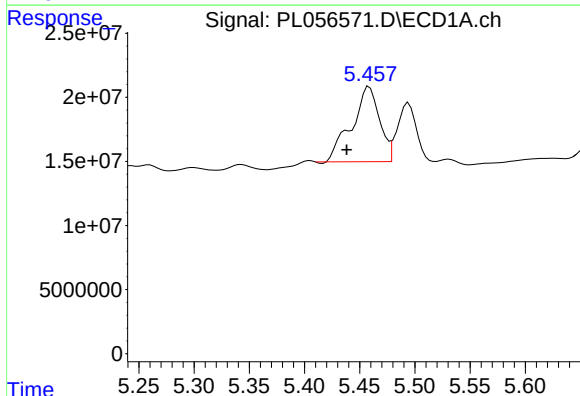


#10 gamma-Chlordane

R.T.: 5.459 min
Delta R.T.: 0.020 min
Response: 102306430
Conc: 7.44 ng/ml

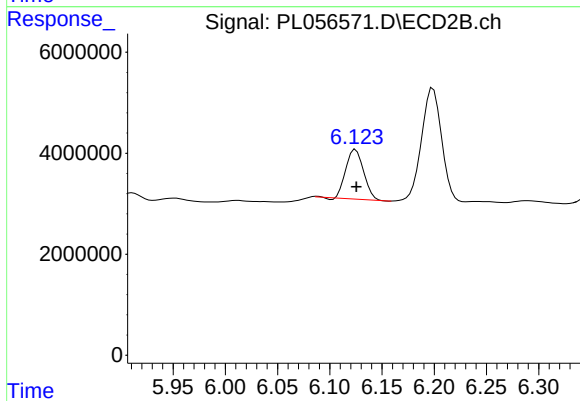

#10 gamma-Chlordane


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 11642938
Conc: 3.98 ng/ml

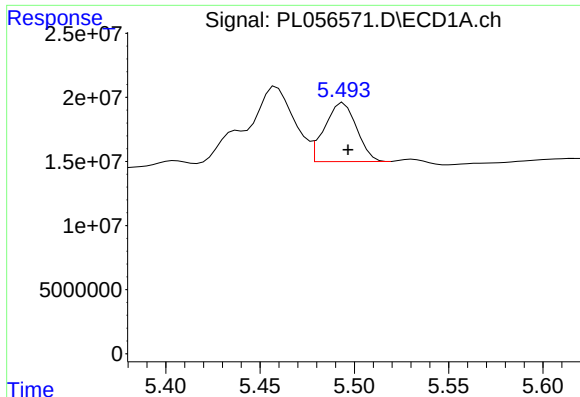

#11 alpha-Chlordane


R.T.: 5.494 min
Delta R.T.: -0.002 min
Response: 54359926
Conc: 3.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

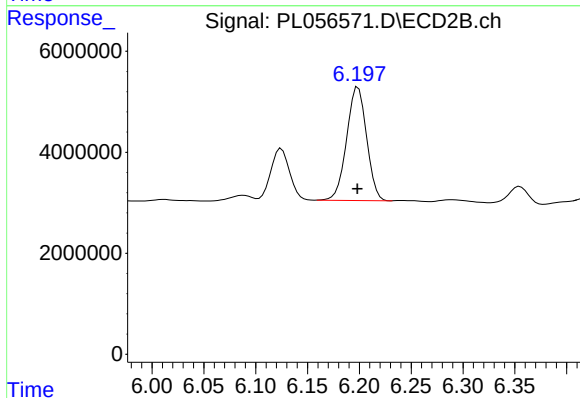


#11 alpha-Chlordane

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 30162443
Conc: 10.27 ng/ml

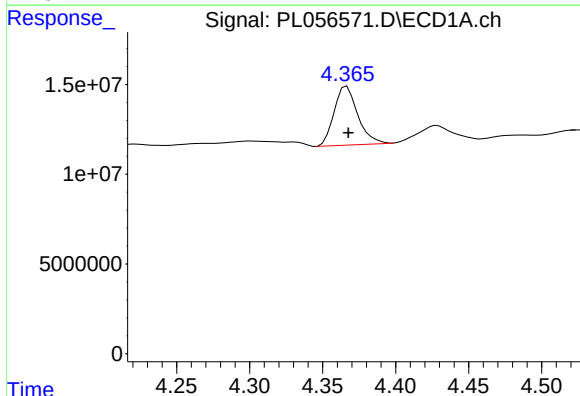


#23 Chlordane-1

R.T.: 4.367 min
Delta R.T.: 0.000 min
Response: 36854203
Conc: 97.97 ng/ml

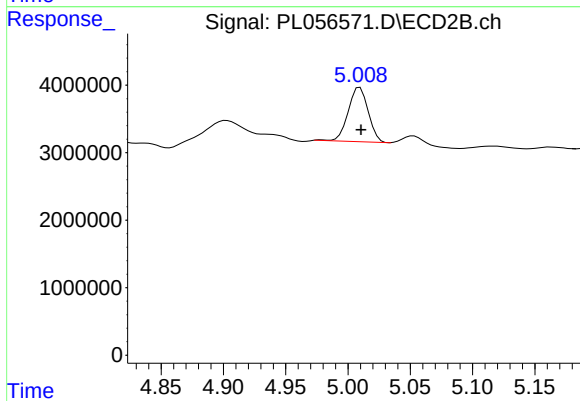

#23 Chlordane-1


R.T.: 5.010 min
Delta R.T.: 0.000 min
Response: 9011516
Conc: 87.45 ng/ml

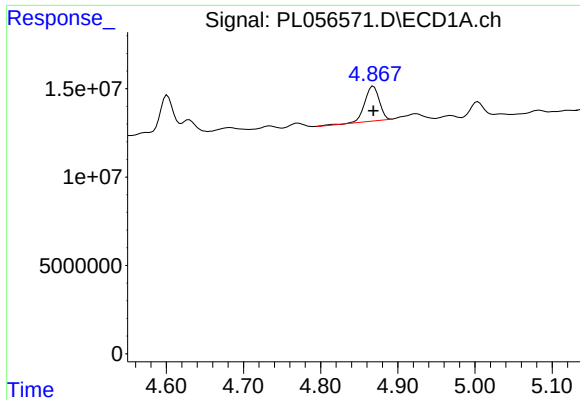

#24 Chlordane-2


R.T.: 4.868 min
Delta R.T.: 0.000 min
Response: 26221764
Conc: 60.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

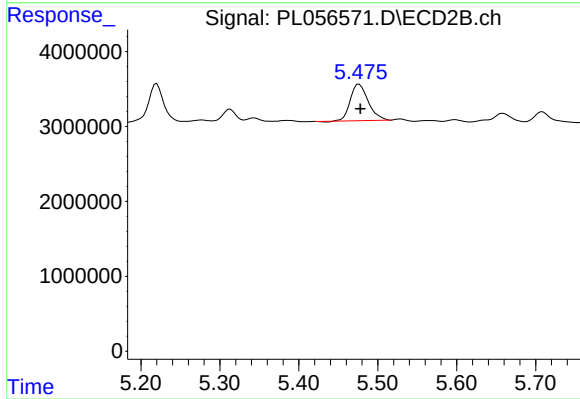


#24 Chlordane-2

R.T.: 5.476 min
Delta R.T.: -0.002 min
Response: 7691878
Conc: 74.50 ng/ml

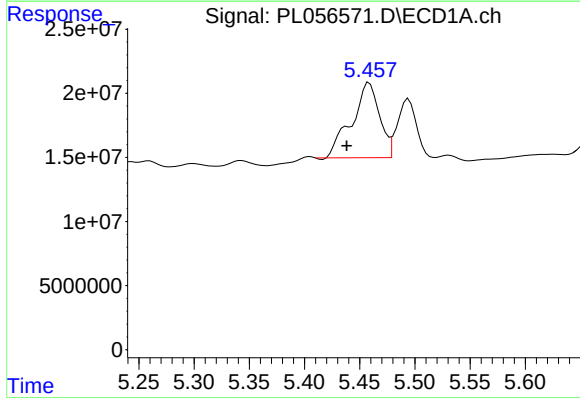


#25 Chlordane-3

R.T.: 5.459 min
Delta R.T.: 0.020 min
Response: 102306430
Conc: 77.92 ng/ml

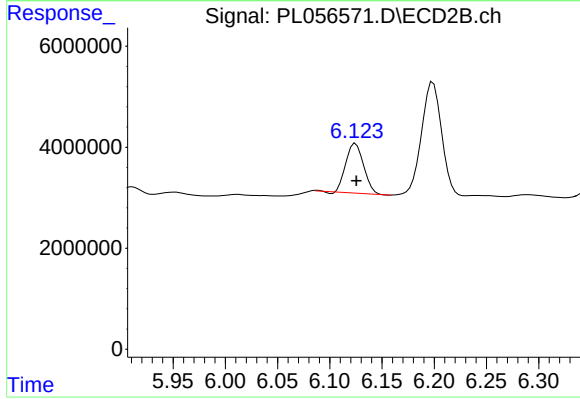

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 11642938
Conc: 30.04 ng/ml

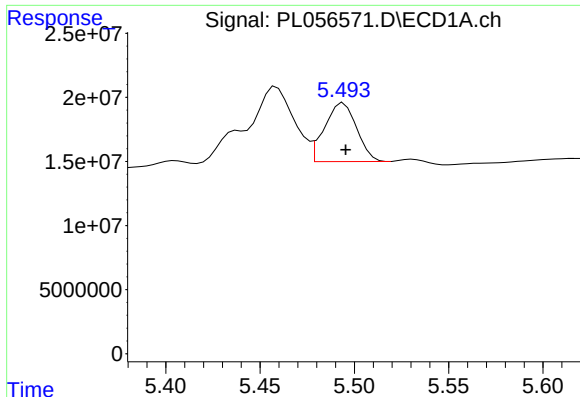

#26 Chlordane-4


R.T.: 5.494 min
Delta R.T.: -0.001 min
Response: 54359926
Conc: 50.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

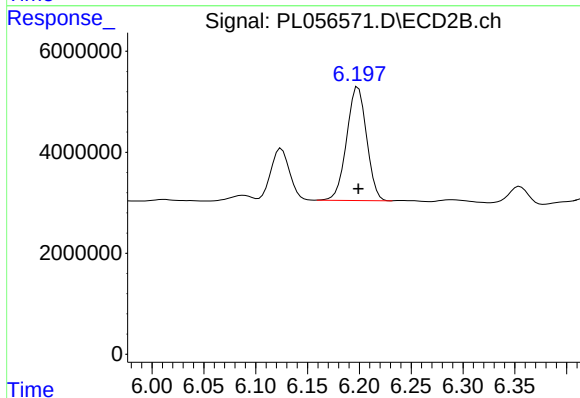


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 30162443
Conc: 66.28 ng/ml

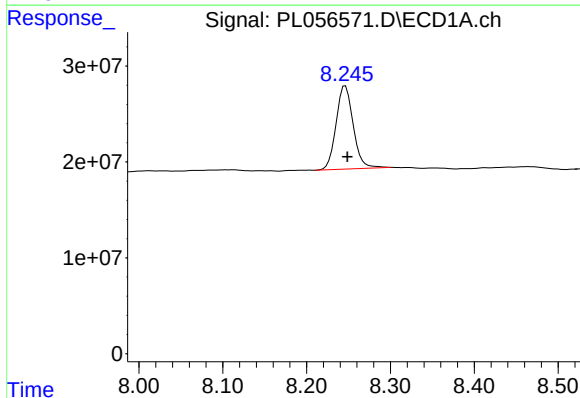

#28 Decachlorobiphenyl

R.T.: 8.246 min
Delta R.T.: -0.002 min
Response: 123523543
Conc: 12.89 ng/ml

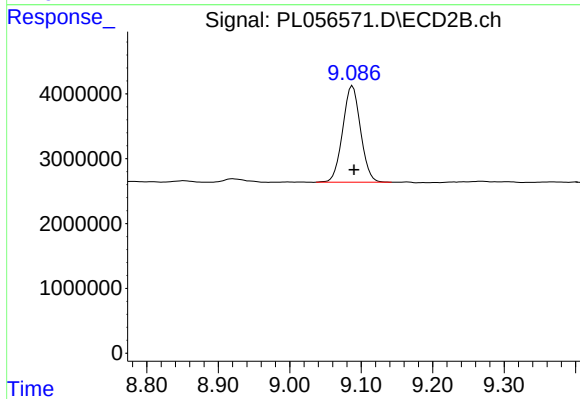

#28 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: -0.002 min
Response: 25857529
Conc: 12.68 ng/ml