

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021422\
 Data File : PL072654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2022 14:37
 Operator : AR\AJ
 Sample : N1470-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CTY2-WC-ROLLOFF

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/15/2022
 Supervised By :Ankita Jodhani 02/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 03:45:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 05:14:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.490	9990526	34298071	20.748	19.855
28)	SA Decachlor...	10.316	11.383	17459385	35529679	23.062	22.405
Target Compounds							
11)	B alpha-Chl...	7.335	8.303	219069	714823	0.344m	0.376

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021422\
Data File : PL072654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2022 14:37
Operator : AR\AJ
Sample : N1470-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CTY2-WC-ROLLOFF


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/15/2022
Supervised By : Ankita Jodhani 02/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 03:45:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 05:14:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

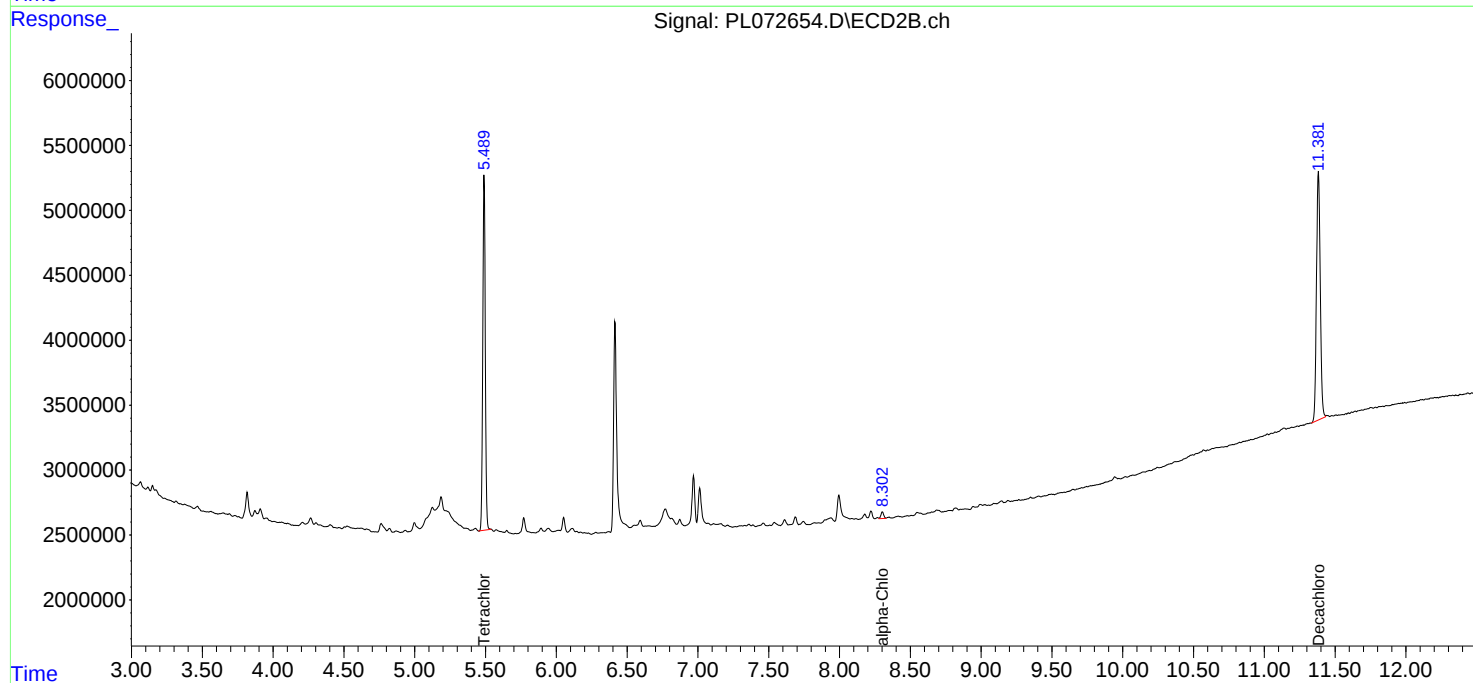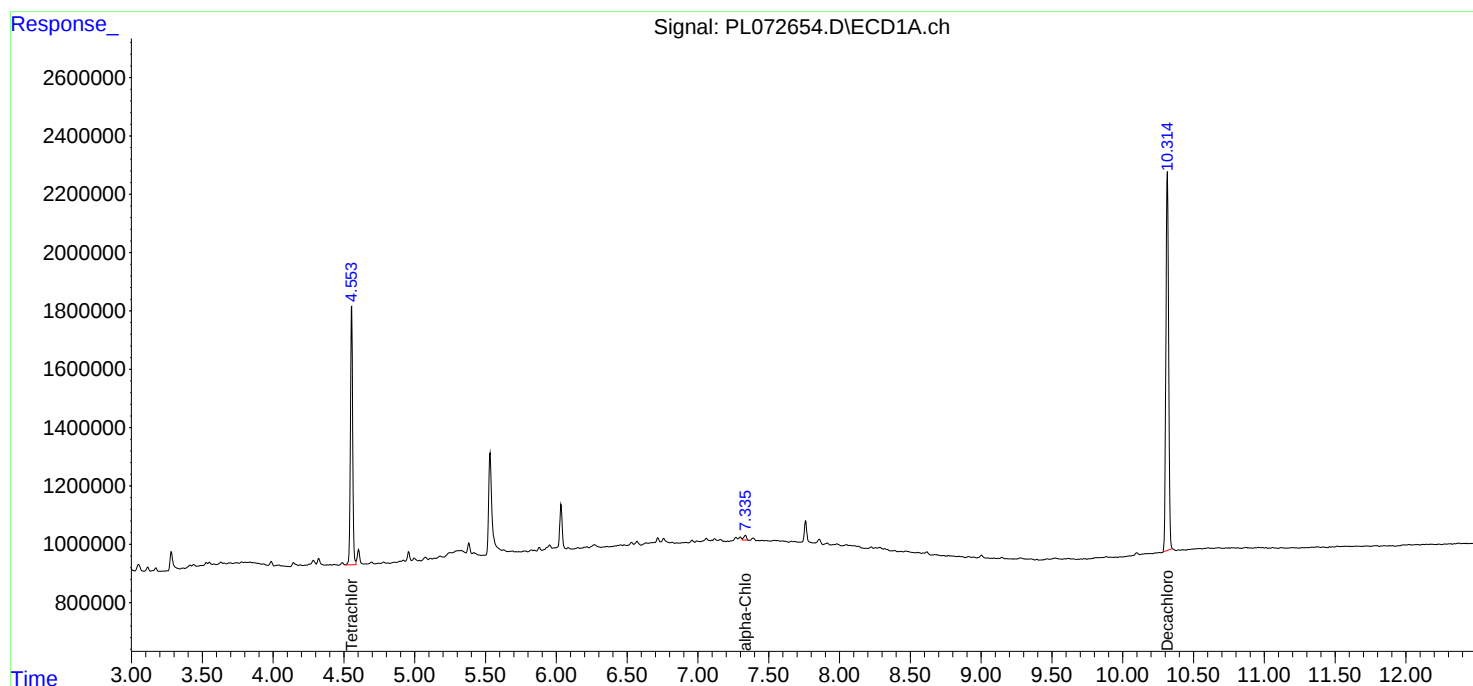

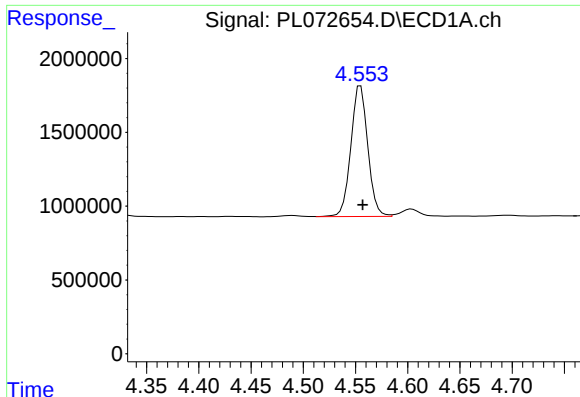


#1 Tetrachloro-m-xylene

R.T.: 4.555 min
Delta R.T.: -0.002 min
Response: 9990526
Conc: 20.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
CTY2-WC-ROLLOFF


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/15/2022
Supervised By :Ankita Jodhani 02/15/2022

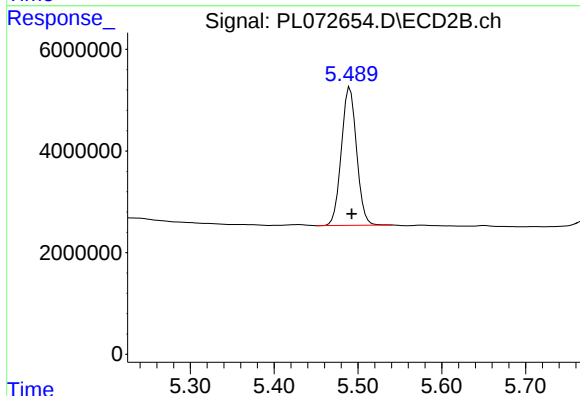


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.002 min
Response: 34298071
Conc: 19.86 ng/ml

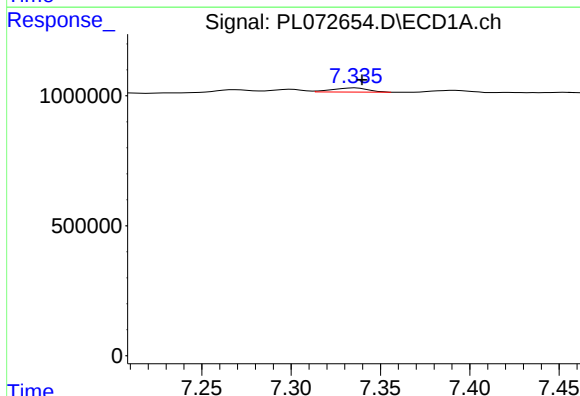


#11 alpha-Chlordane

R.T.: 7.335 min
Delta R.T.: -0.005 min
Response: 219069
Conc: 0.34 ng/ml m

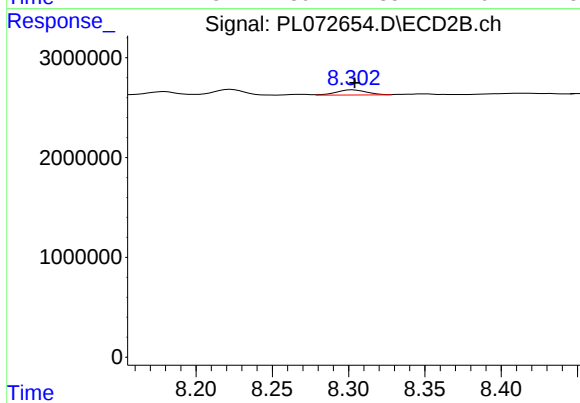

#11 alpha-Chlordane

R.T.: 8.303 min
Delta R.T.: -0.001 min
Response: 714823
Conc: 0.38 ng/ml

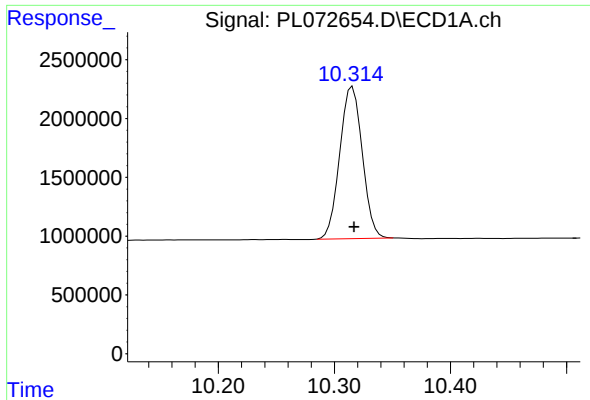


#28 Decachlorobiphenyl

R.T.: 10.316 min
Delta R.T.: -0.001 min
Response: 17459385
Conc: 23.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
CTY2-WC-ROLLOFF

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/15/2022
Supervised By :Ankita Jodhani 02/15/2022

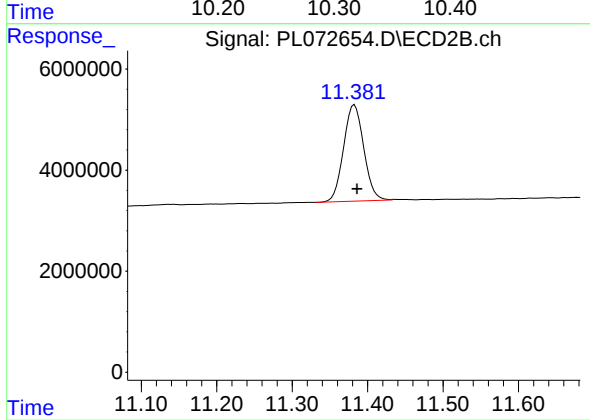

#28 Decachlorobiphenyl

R.T.: 11.383 min
Delta R.T.: -0.003 min
Response: 35529679
Conc: 22.41 ng/ml