

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021422\
 Data File : PL072681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2022 01:13
 Operator : AR\AJ
 Sample : N1524-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/15/2022
 Supervised By : Ankita Jodhani 02/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 04:56:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 05:14:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.554	5.490	9828937	34429966	20.413	19.932
2)	SA Decachlor...	10.312	11.380	15741908	33797380	20.794	21.313

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021422\
Data File : PL072681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2022 01:13
Operator : AR\AJ
Sample : N1524-01
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/15/2022
Supervised By : Ankita Jodhani 02/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 04:56:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 05:14:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

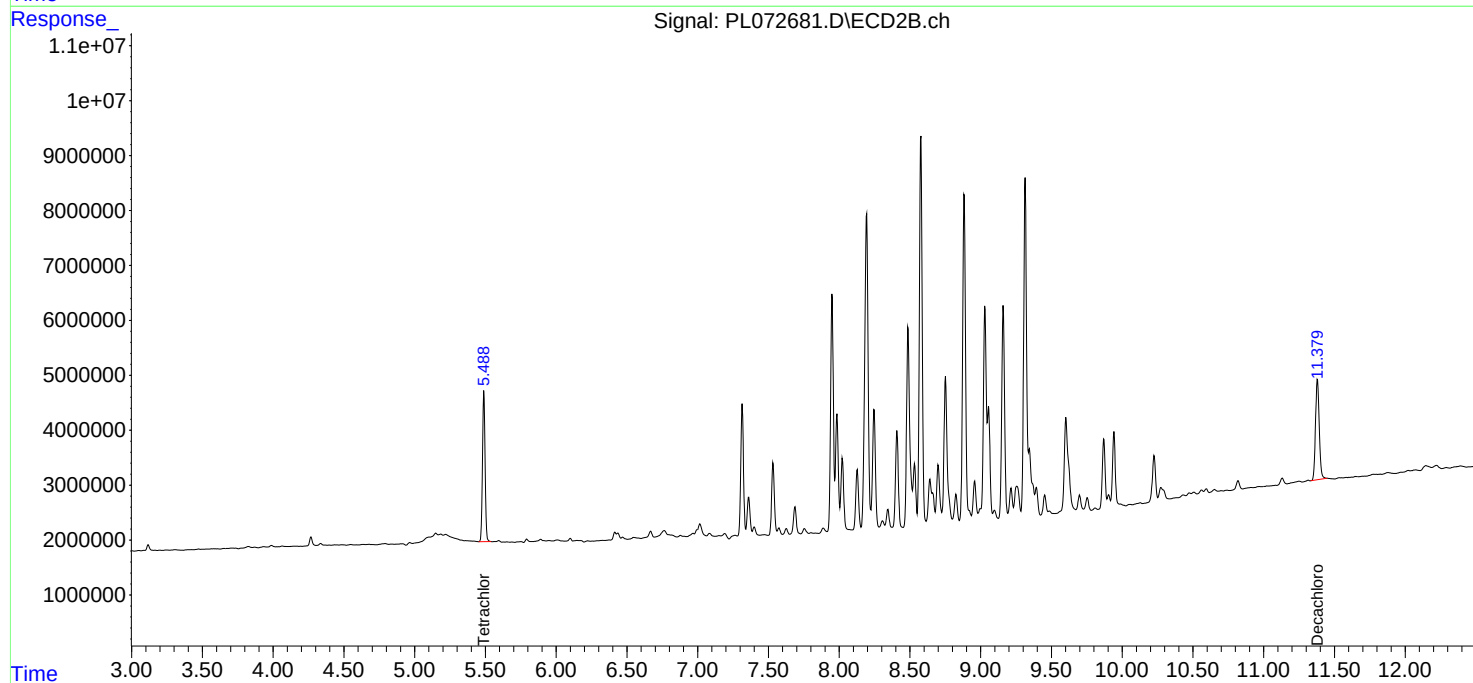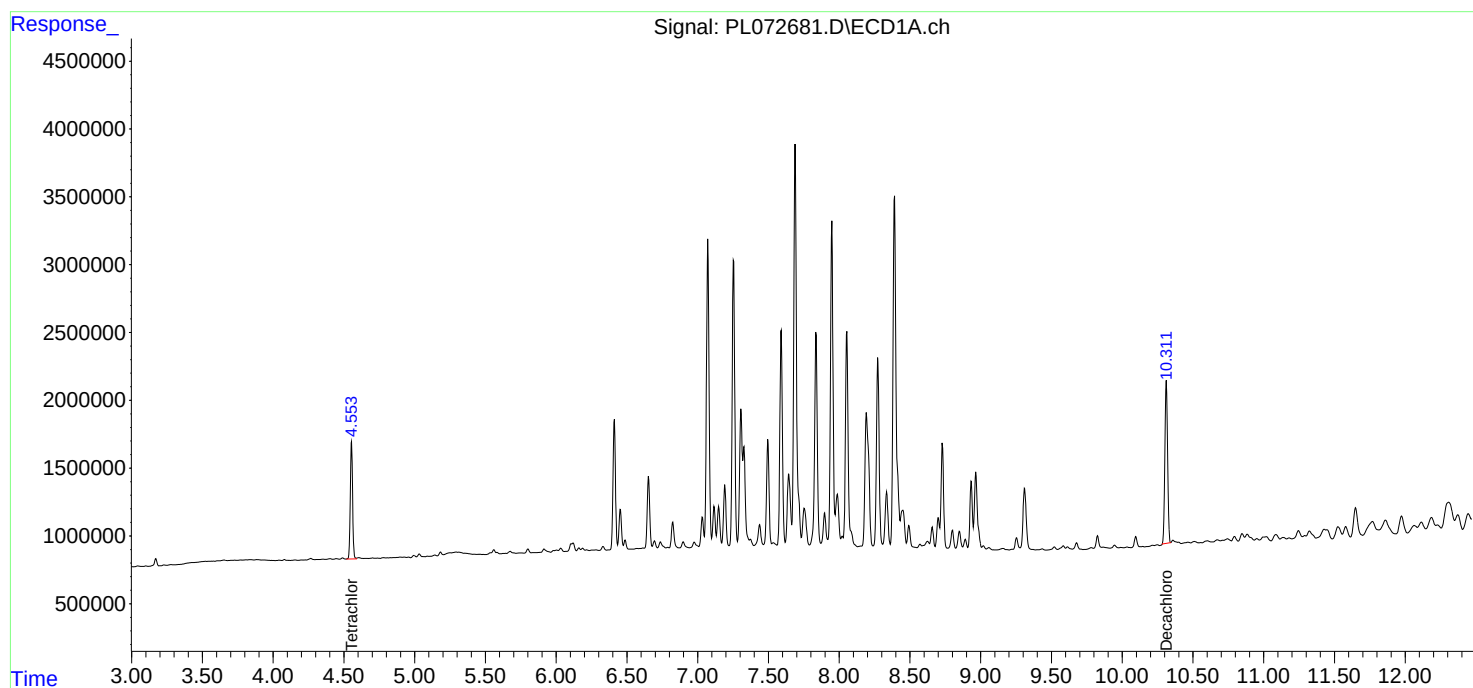

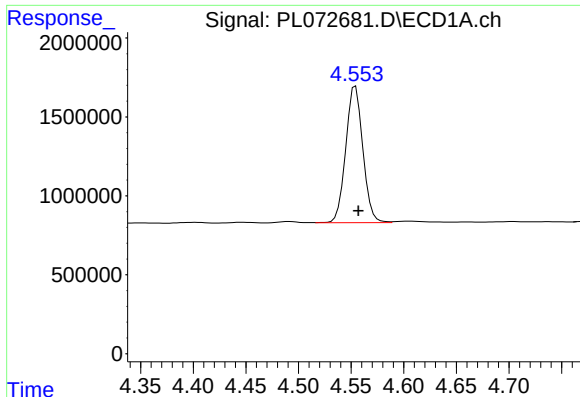


#1 Tetrachloro-m-xylene

R.T.: 4.554 min
Delta R.T.: -0.003 min
Response: 9828937
Conc: 20.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/15/2022
Supervised By :Ankita Jodhani 02/15/2022

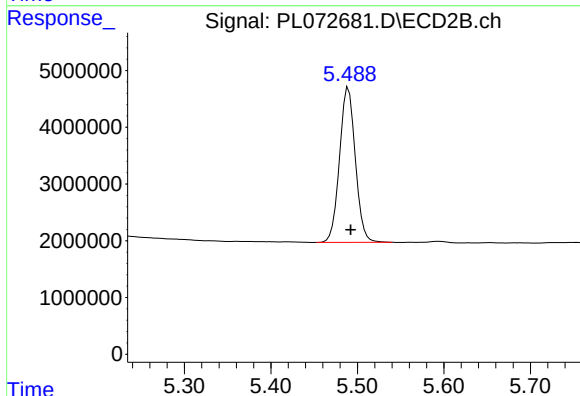


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.003 min
Response: 34429966
Conc: 19.93 ng/ml

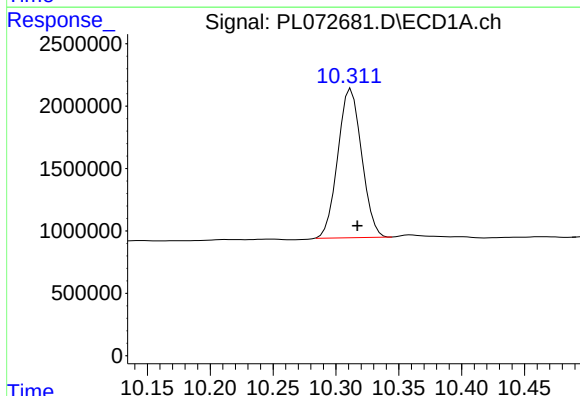

#28 Decachlorobiphenyl

R.T.: 10.312 min
Delta R.T.: -0.005 min
Response: 15741908
Conc: 20.79 ng/ml

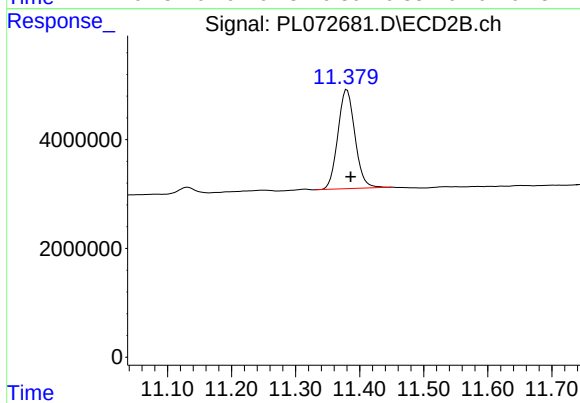

#28 Decachlorobiphenyl

R.T.: 11.380 min
Delta R.T.: -0.006 min
Response: 33797380
Conc: 21.31 ng/ml