

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021423\
 Data File : PL080903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2023 10:25
 Operator : AR\AJ
 Sample : 01529-07RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-05-0-2.0RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/16/2023
 Supervised By :Ankita Jodhani 02/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 20:27:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.357	2.686	19353140	19314095	9.023	8.793
2) SA Decachlor...	8.796	7.832	88989717	85024295	50.829m	35.686 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021423\
Data File : PL080903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2023 10:25
Operator : AR\AJ
Sample : 01529-07RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-05-0-2.0RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/16/2023
Supervised By : Ankita Jodhani 02/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 20:27:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

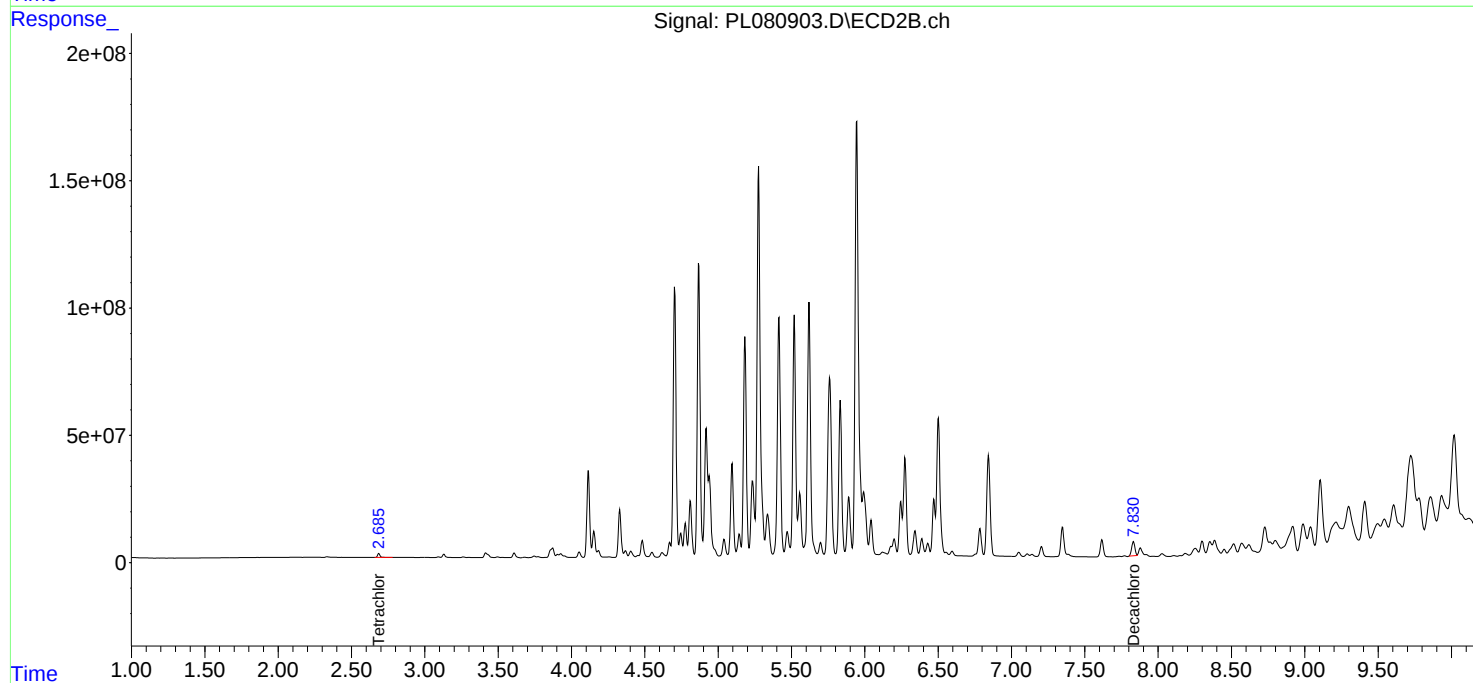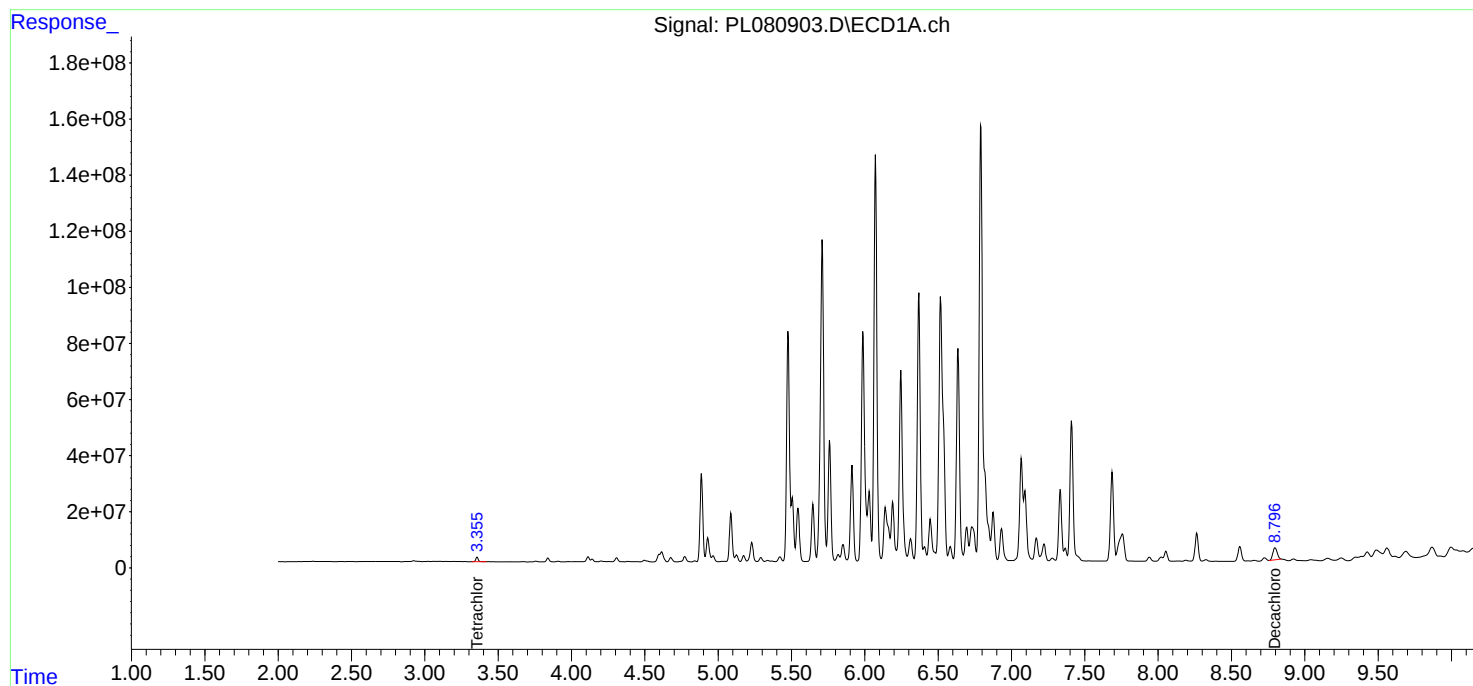

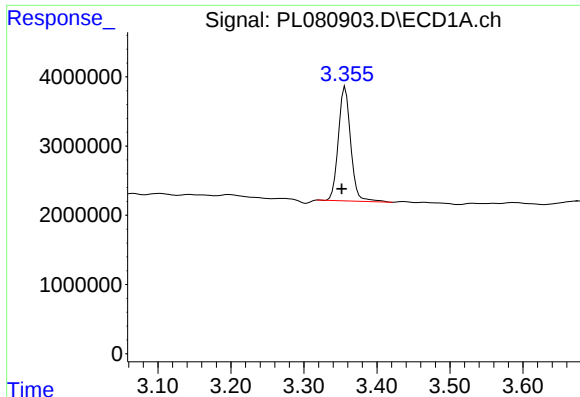


#1 Tetrachloro-m-xylene

R.T.: 3.357 min
Delta R.T.: 0.005 min
Response: 19353140
Conc: 9.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-05-0-2.0RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/16/2023
Supervised By :Ankita Jodhani 02/16/2023

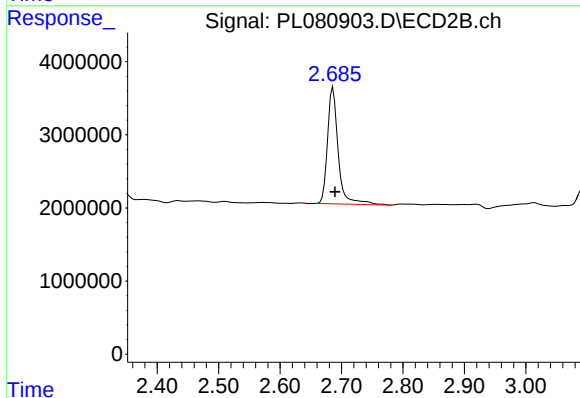


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: -0.004 min
Response: 19314095
Conc: 8.79 ng/ml

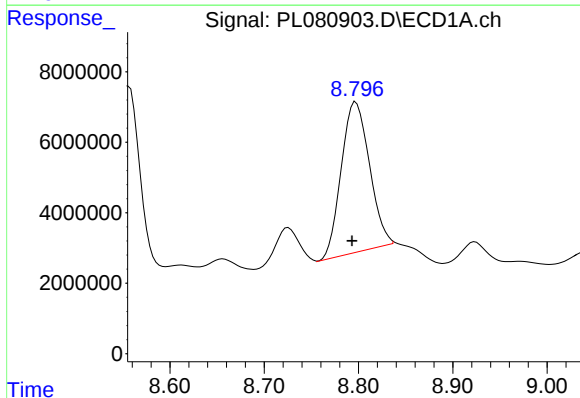

#28 Decachlorobiphenyl

R.T.: 8.796 min
Delta R.T.: 0.003 min
Response: 88989717
Conc: 50.83 ng/ml m

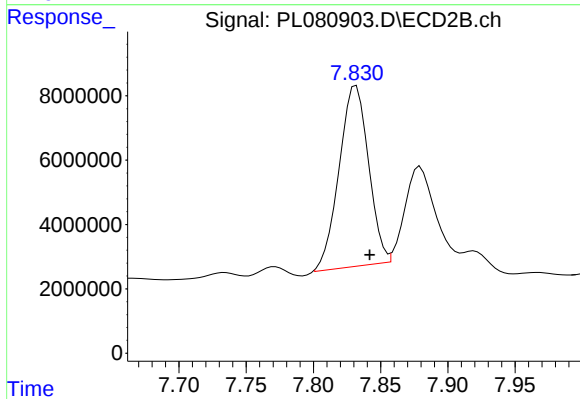

#28 Decachlorobiphenyl

R.T.: 7.832 min
Delta R.T.: -0.010 min
Response: 85024295
Conc: 35.69 ng/ml