

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021423\
 Data File : PL080904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2023 10:52
 Operator : AR\AJ
 Sample : 01529-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-01-5.0-7.0

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/15/2023
 Supervised By :Ankita Jodhani 02/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 20:27:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.350	2.688	36268029	36481547	16.909m	16.609
2) SA Decachlor...	8.786	7.830	14612142	9024981	8.346m	3.788m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021423\
Data File : PL080904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2023 10:52
Operator : AR\AJ
Sample : 01529-05
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-01-5.0-7.0


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/15/2023
Supervised By : Ankita Jodhani 02/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 20:27:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

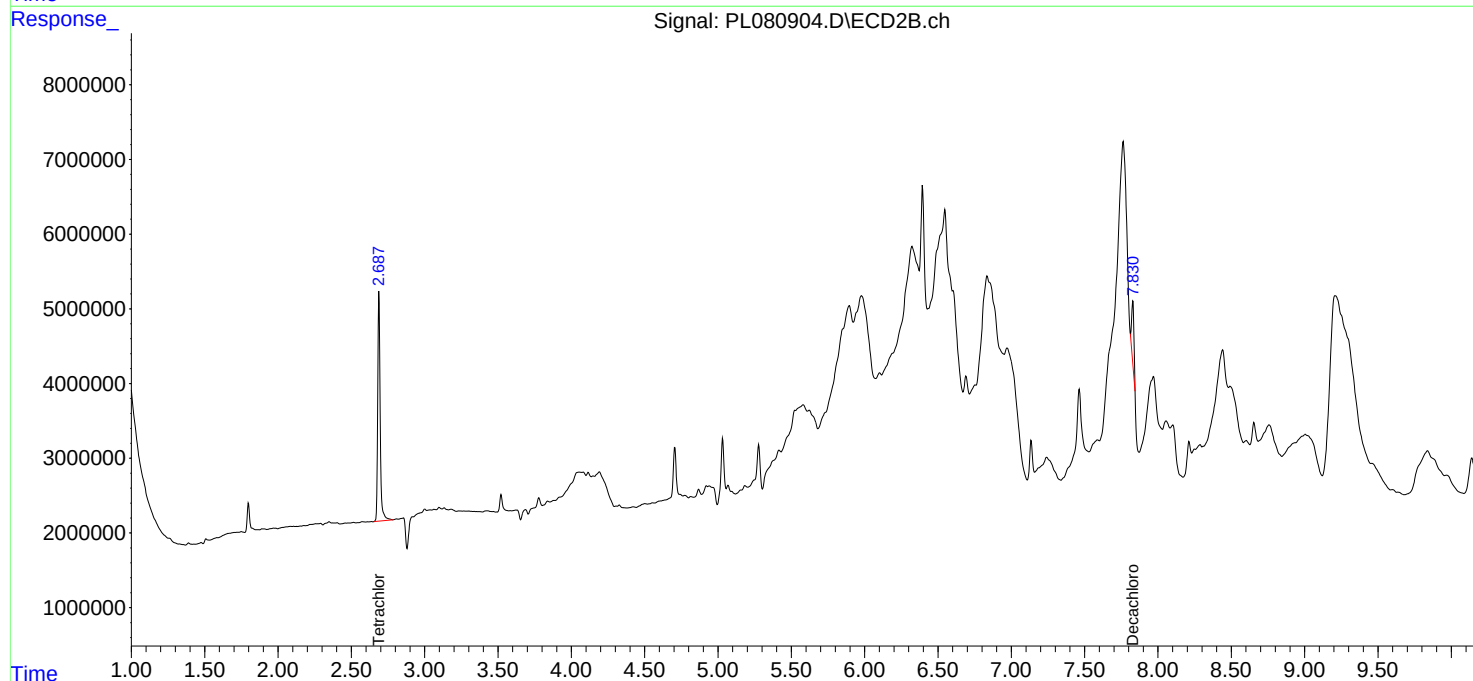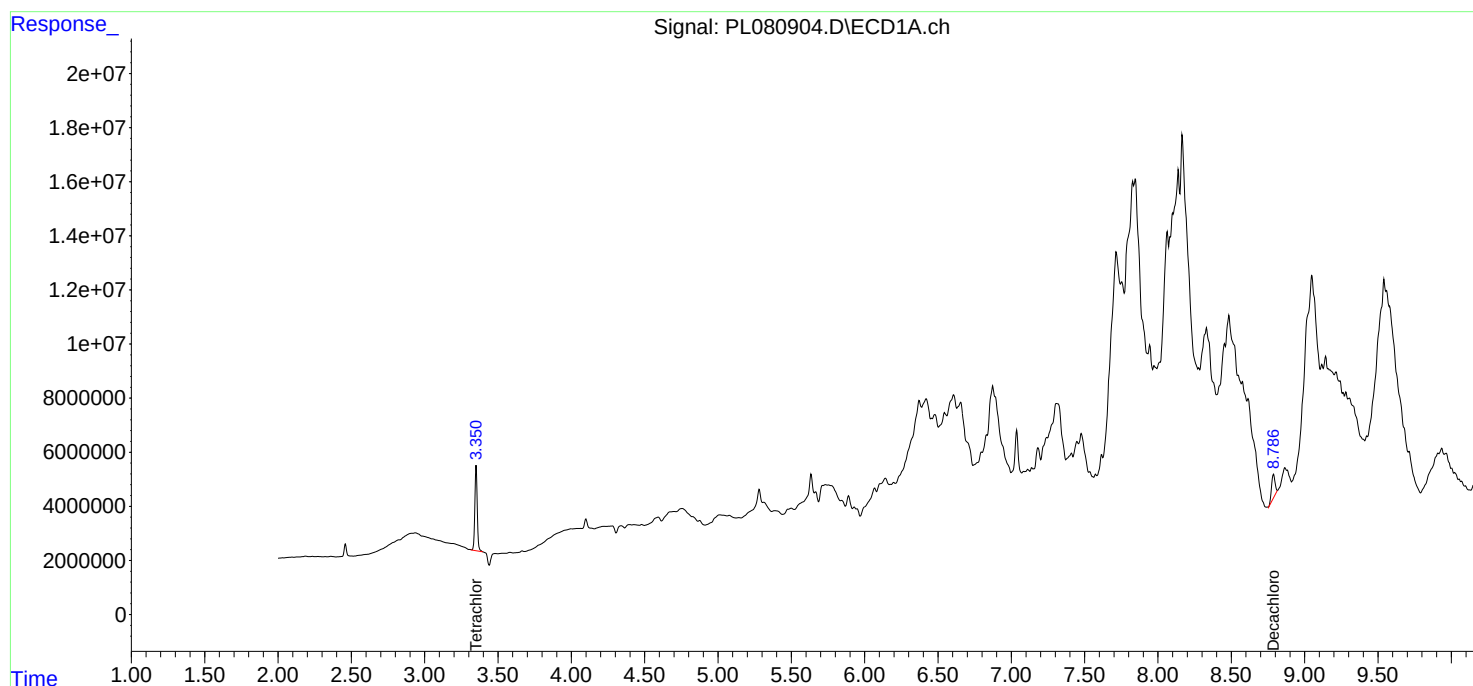

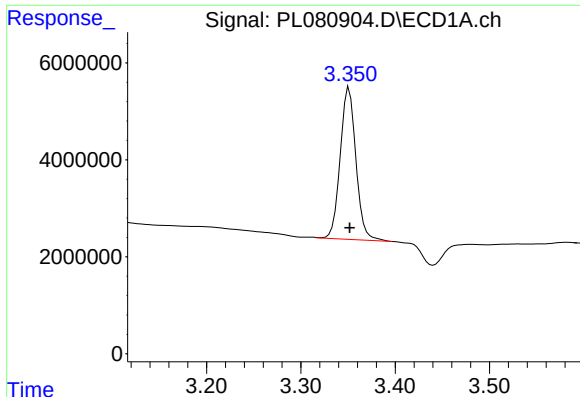


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.002 min
Response: 36268029
Conc: 16.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-01-5.0-7.0


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/15/2023
Supervised By :Ankita Jodhani 02/15/2023

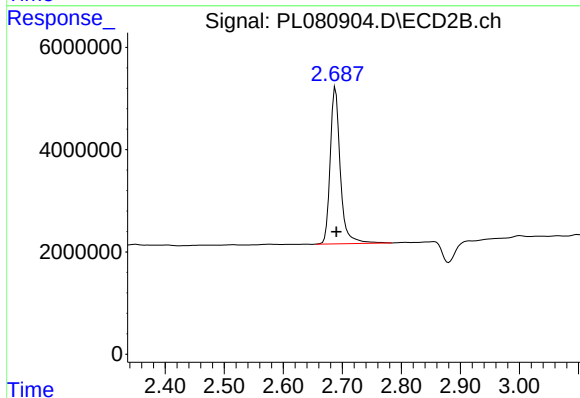


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: -0.001 min
Response: 36481547
Conc: 16.61 ng/ml

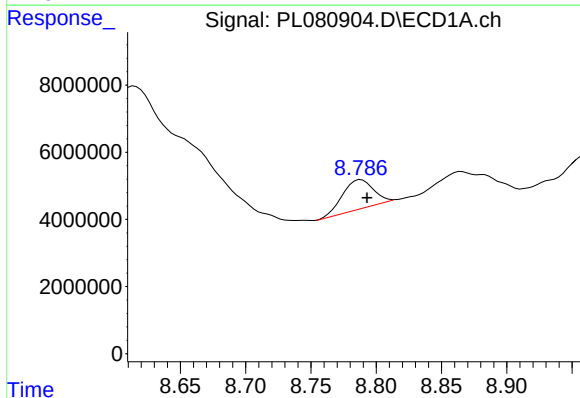

#28 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 14612142
Conc: 8.35 ng/ml m

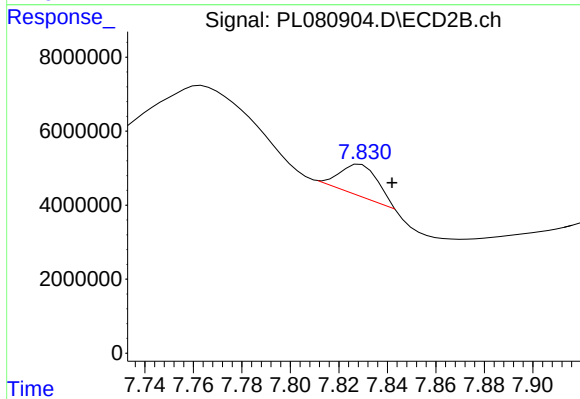

#28 Decachlorobiphenyl

R.T.: 7.830 min
Delta R.T.: -0.012 min
Response: 9024981
Conc: 3.79 ng/ml m