

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021423\
Data File : PL080911.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2023 15:13
Operator : AR\AJ
Sample : 01537-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1-(TP1)-COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 20:33:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.356	2.687	21489896	21720080	10.019	9.889
28)	SA Decachlor...	8.792	7.834	18526003	24302150	10.582	10.200

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021423\
Data File : PL080911.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2023 15:13
Operator : AR\AJ
Sample : 01537-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1-(TP1)-COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 20:33:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

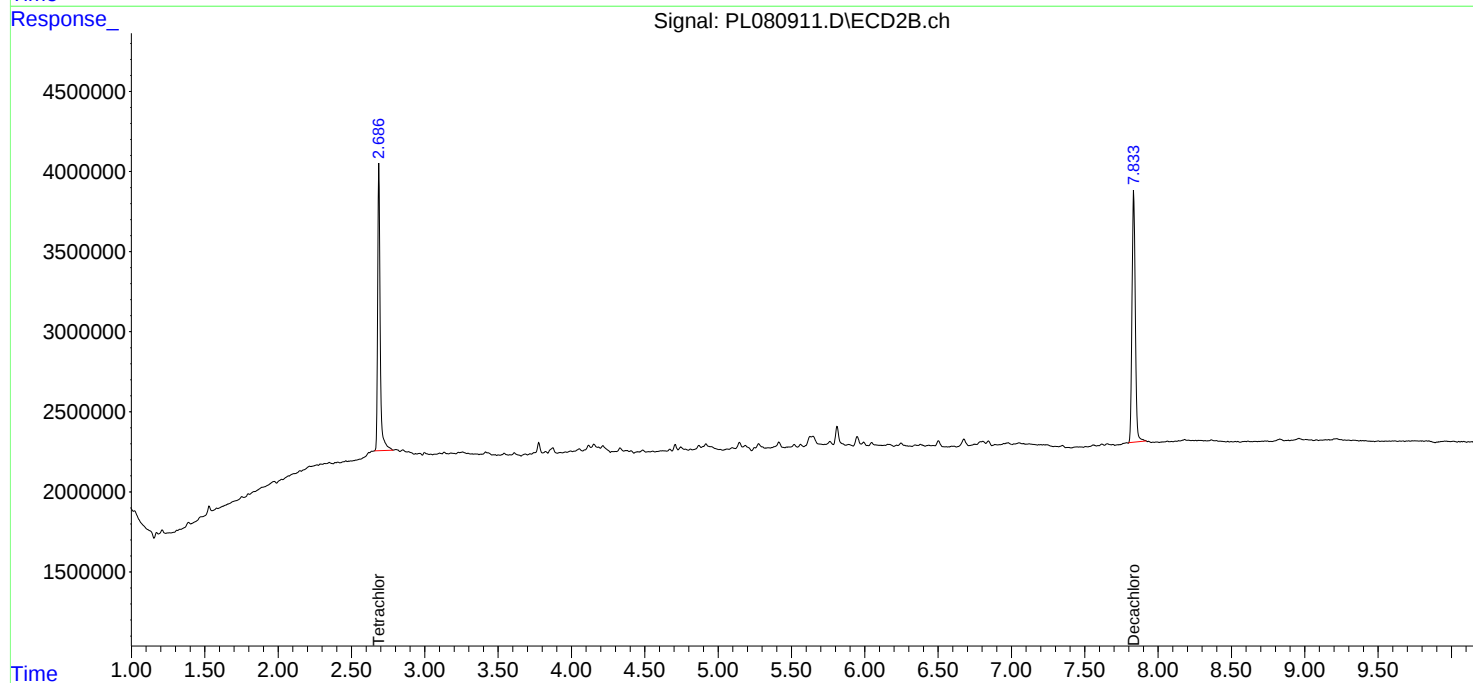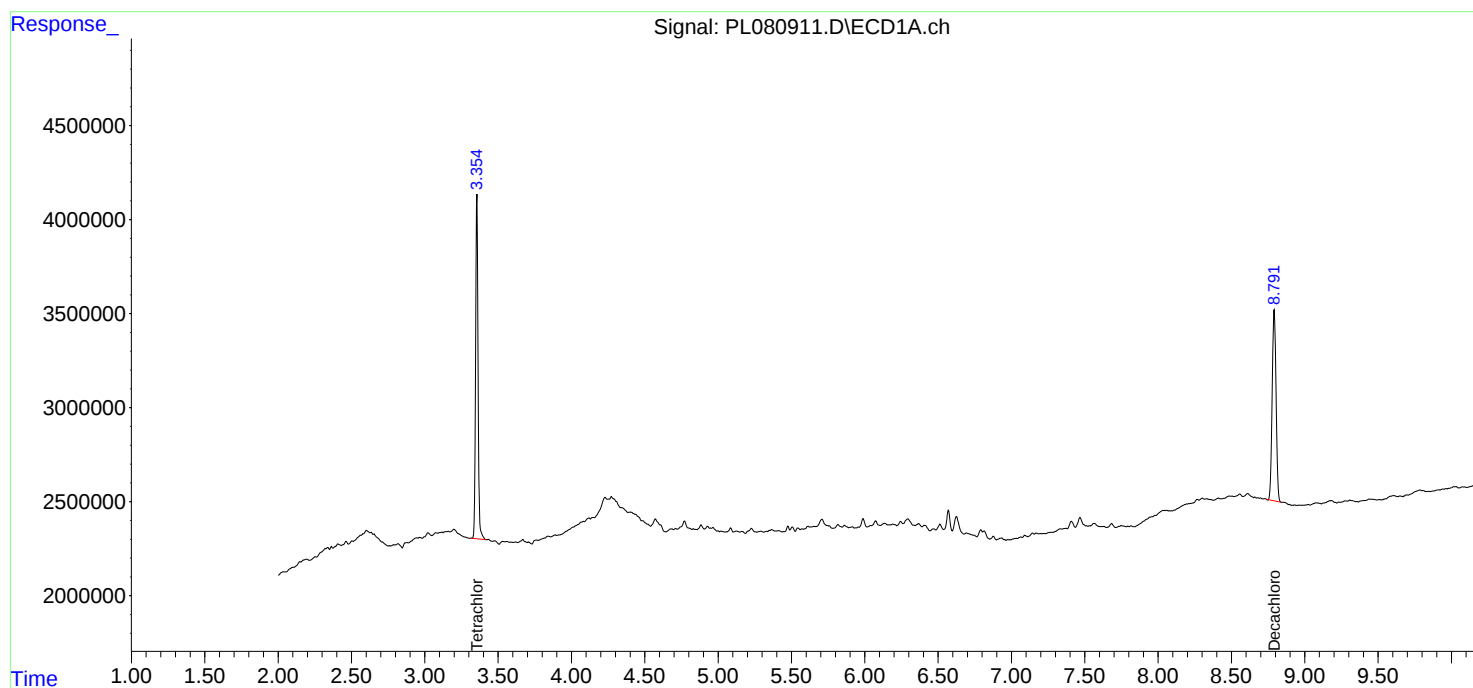


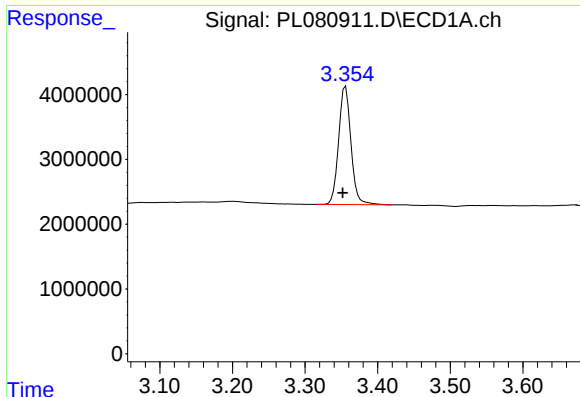

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: 0.004 min
Response: 21489896
Conc: 10.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1-(TP1)-COMP-1

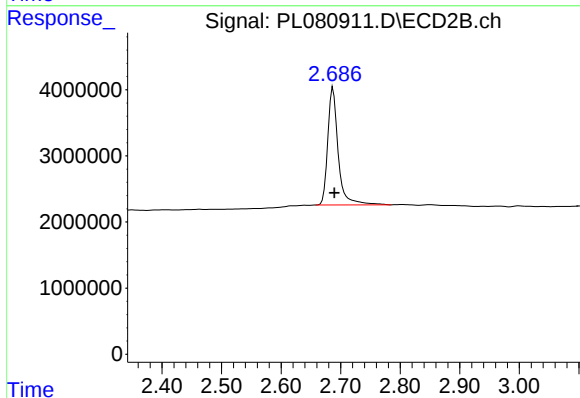


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: -0.002 min
Response: 21720080
Conc: 9.89 ng/ml

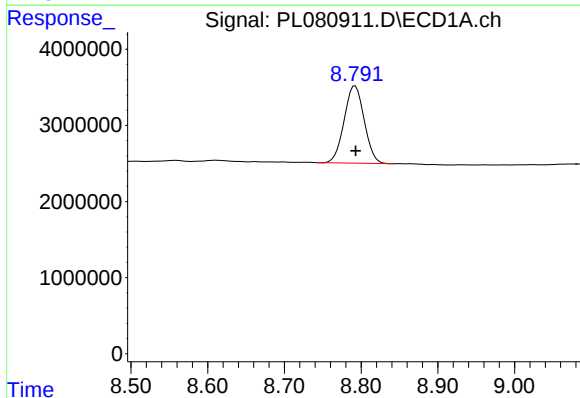

#28 Decachlorobiphenyl

R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 18526003
Conc: 10.58 ng/ml

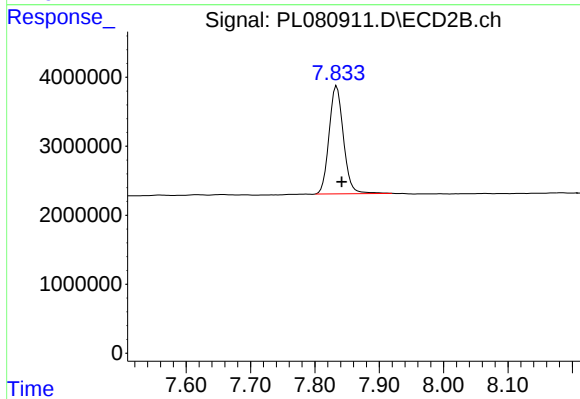

#28 Decachlorobiphenyl

R.T.: 7.834 min
Delta R.T.: -0.008 min
Response: 24302150
Conc: 10.20 ng/ml