

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021423\
 Data File : PL080915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2023 16:08
 Operator : AR\AJ
 Sample : 01538-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-PIT-5-(TP5)-COMP-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 20:36:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.687	21966644	21863827	10.242	9.954
28)	SA Decachlor...	8.786	7.831	19493150	24536447	11.134	10.298

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021423\
Data File : PL080915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2023 16:08
Operator : AR\AJ
Sample : 01538-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-5-(TP5)-COMP-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 20:36:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

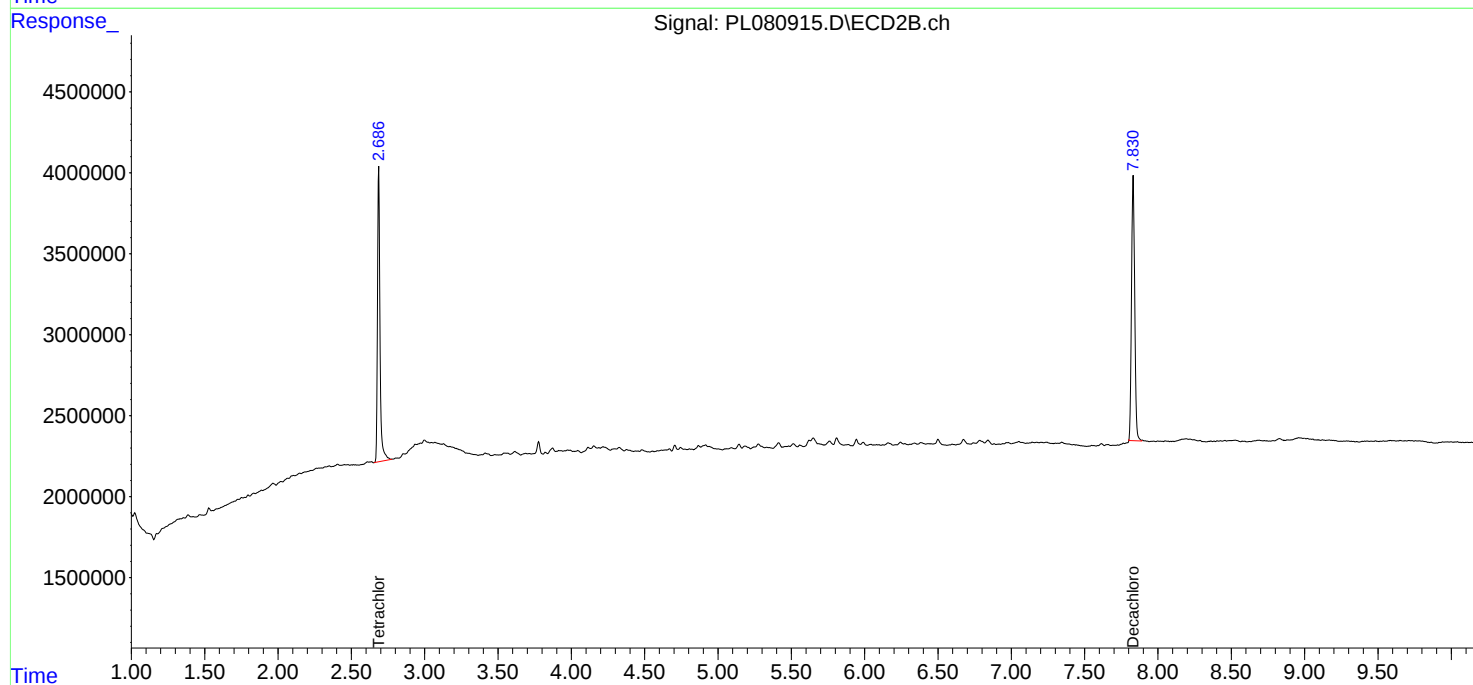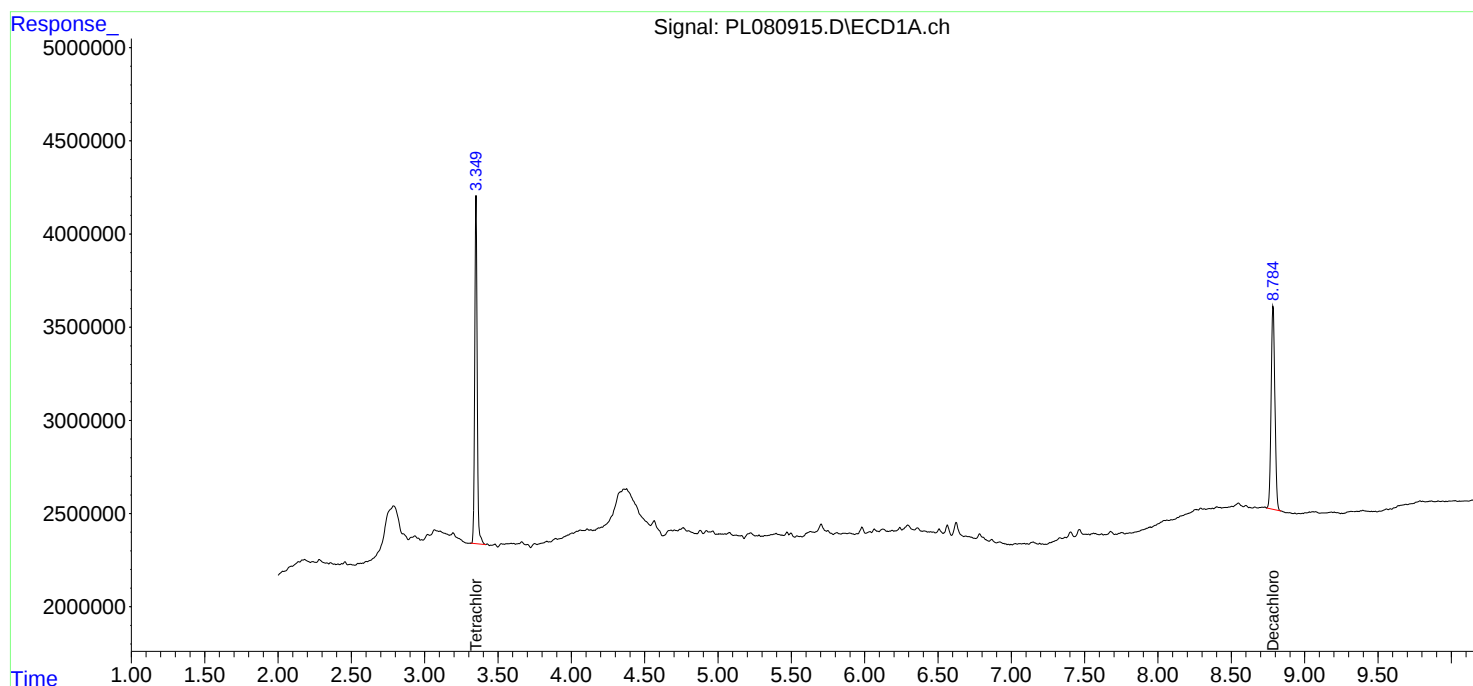


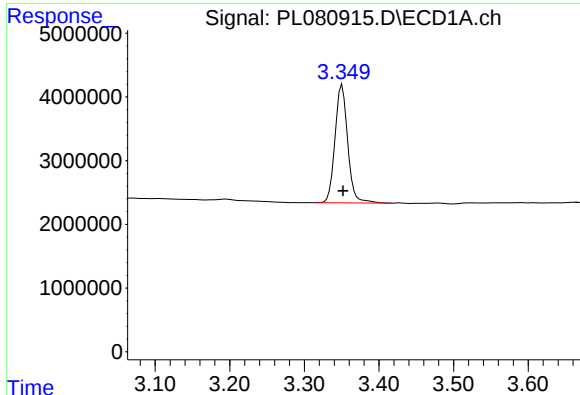

#1 Tetrachloro-m-xylene


R.T.: 3.351 min
Delta R.T.: -0.001 min
Response: 21966644
Conc: 10.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-5-(TP5)-COMP-5

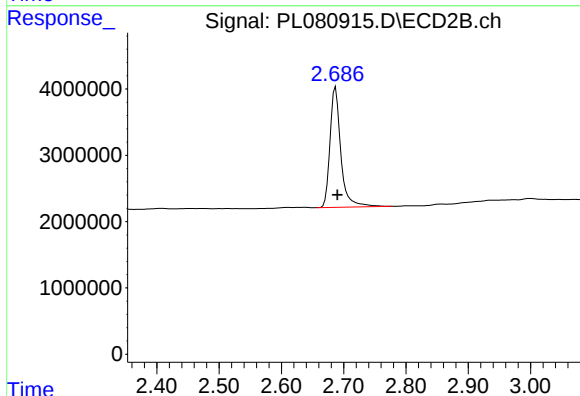


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: -0.003 min
Response: 21863827
Conc: 9.95 ng/ml

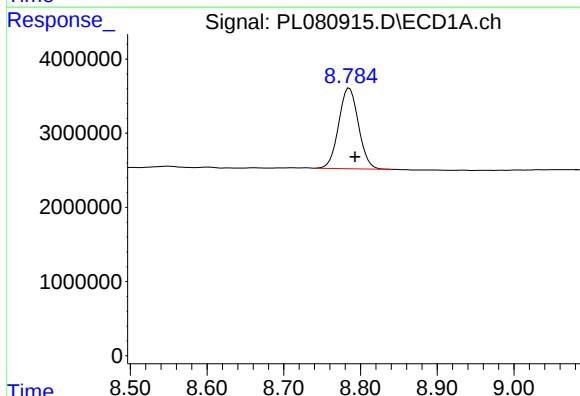

#28 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: -0.008 min
Response: 19493150
Conc: 11.13 ng/ml

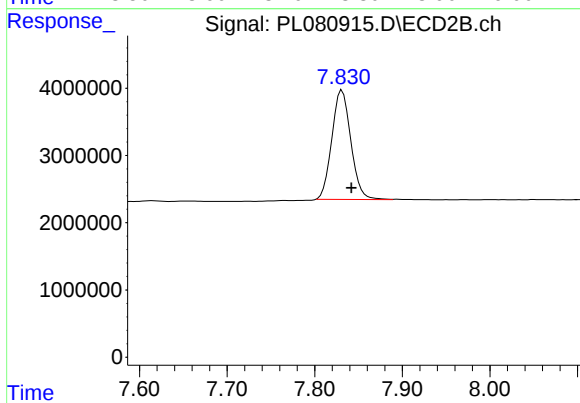

#28 Decachlorobiphenyl

R.T.: 7.831 min
Delta R.T.: -0.011 min
Response: 24536447
Conc: 10.30 ng/ml