

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021519\
 Data File : PL044842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2019 14:25
 Operator : AJ\SJ
 Sample : K1346-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-021419-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 21:59:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.984	71354379	24144879	10.028	10.278
28)	SA Decachlor...	8.052	9.047	85939206	26135751	11.783	11.800
Target Compounds							
10)	B gamma-Chl...	5.284f	6.093	14613079	2242946	1.514	0.808 #
11)	B alpha-Chl...	5.319	6.167	9876160	7345464	1.033	2.651 #
12)	B 4,4'-DDE	5.487	6.322	6160581	2576482	0.710	1.079 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021519\
Data File : PL044842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2019 14:25
Operator : AJ\SJ
Sample : K1346-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-01-021419-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 21:59:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

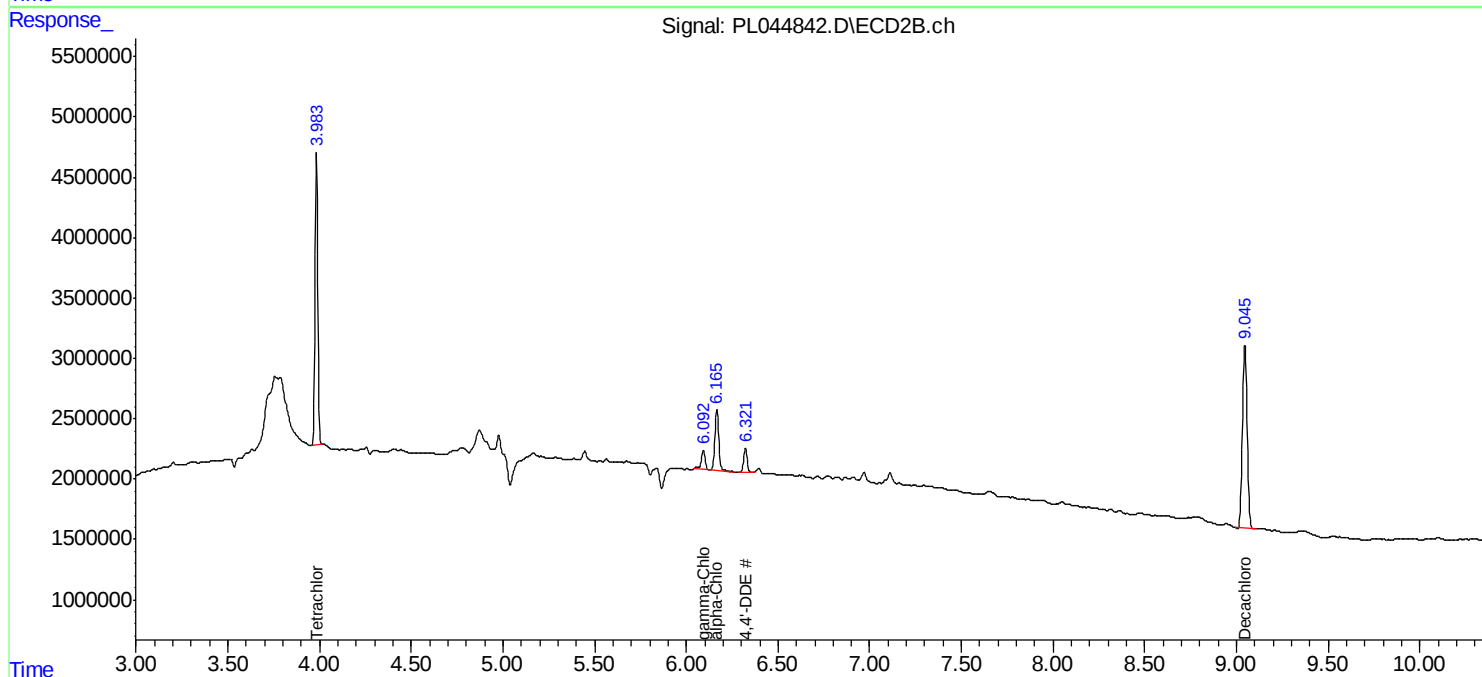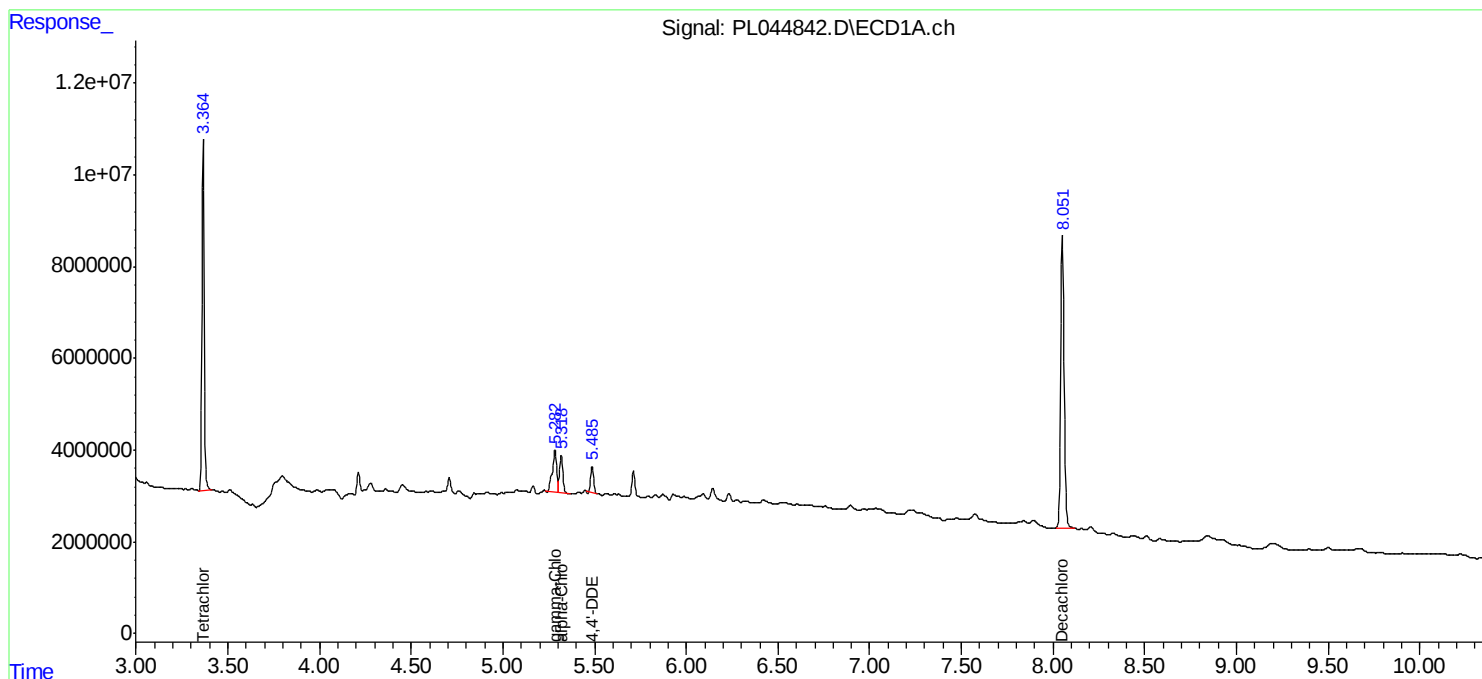


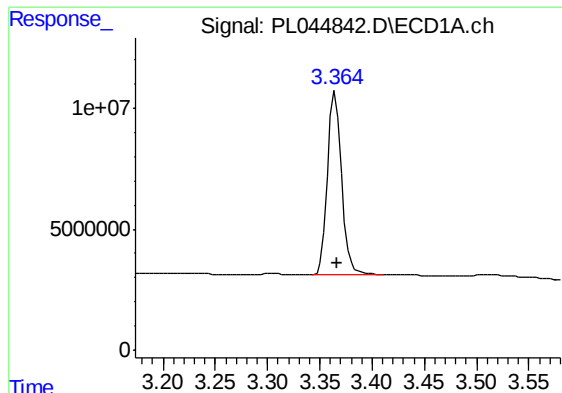

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 71354379
Conc: 10.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-021419-E

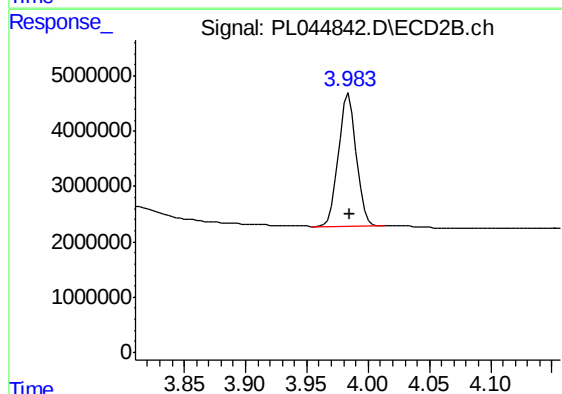


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 24144879
Conc: 10.28 ng/ml

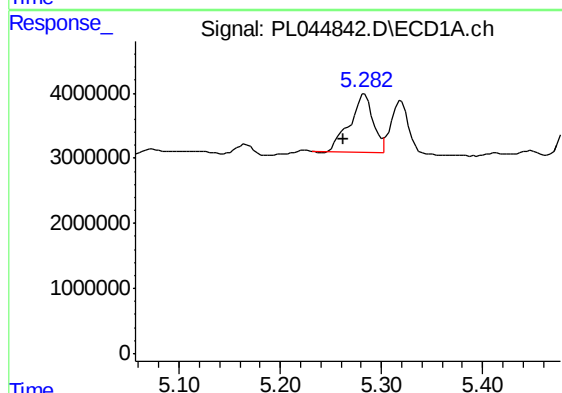


#10 gamma-Chlordane

R.T.: 5.284 min
Delta R.T.: 0.021 min
Response: 14613079
Conc: 1.51 ng/ml

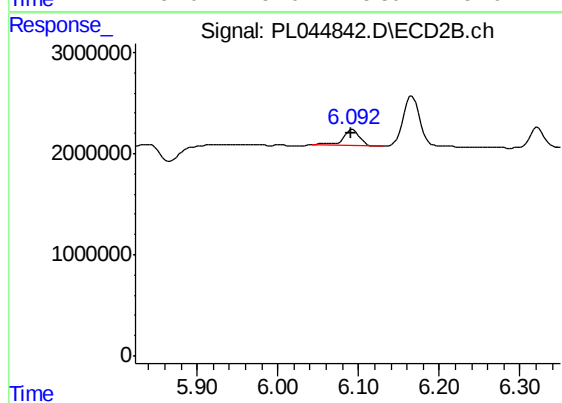

#10 gamma-Chlordane


R.T.: 6.093 min
Delta R.T.: 0.002 min
Response: 2242946
Conc: 0.81 ng/ml

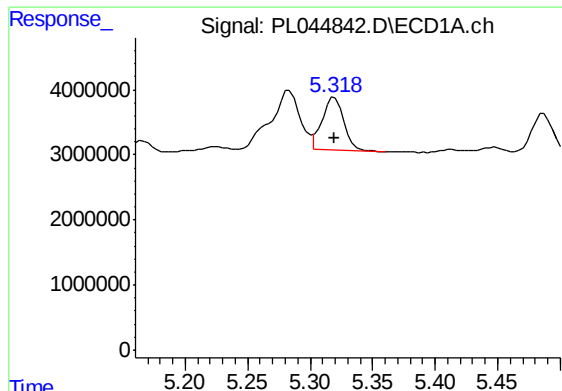

#11 alpha-Chlordane


R.T.: 5.319 min
Delta R.T.: 0.000 min
Response: 9876160
Conc: 1.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-021419-E

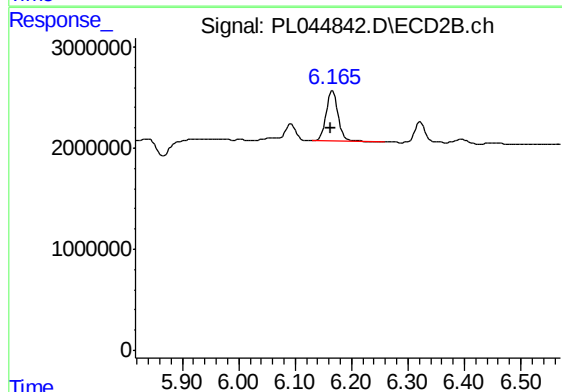


#11 alpha-Chlordane

R.T.: 6.167 min
Delta R.T.: 0.003 min
Response: 7345464
Conc: 2.65 ng/ml

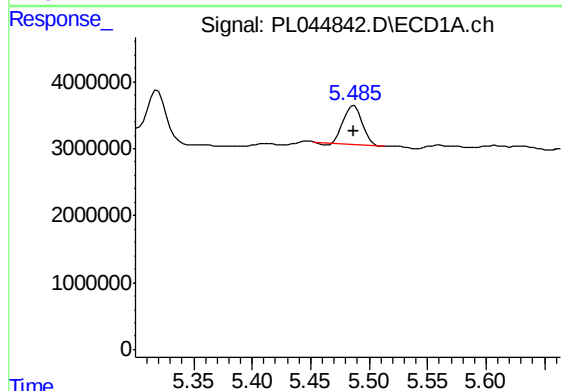


#12 4,4'-DDE

R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 6160581
Conc: 0.71 ng/ml

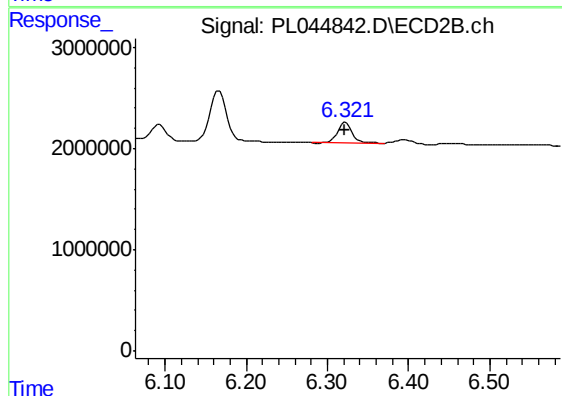

#12 4,4'-DDE


R.T.: 6.322 min
Delta R.T.: 0.001 min
Response: 2576482
Conc: 1.08 ng/ml

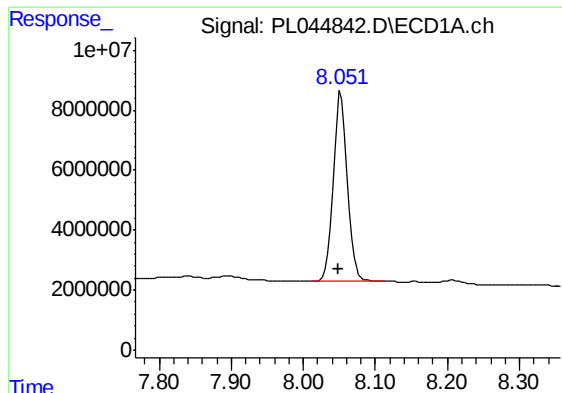

#28 Decachlorobiphenyl

R.T.: 8.052 min
Delta R.T.: 0.003 min
Response: 85939206
Conc: 11.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-021419-E

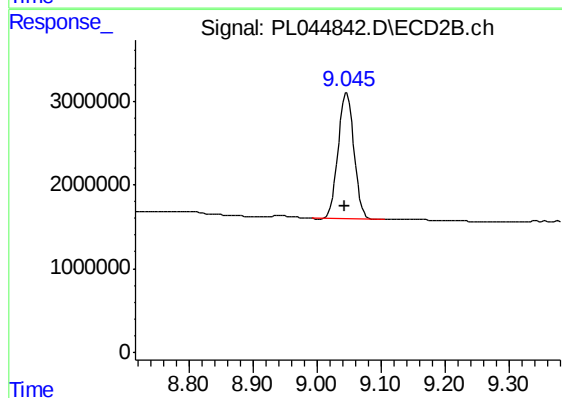

#28 Decachlorobiphenyl

R.T.: 9.047 min
Delta R.T.: 0.004 min
Response: 26135751
Conc: 11.80 ng/ml