

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021519\
 Data File : PL044849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2019 16:04
 Operator : AJ\SJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 22:02:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.985	367.1E6	120.9E6	51.585	51.468
28)	SA Decachlor...	8.052	9.047	368.6E6	110.3E6	50.535	49.788
Target Compounds							
2)	A alpha-BHC	3.796	4.375	564.4E6	162.5E6	52.849	53.335
3)	MA gamma-BHC...	4.073	4.660	520.3E6	152.1E6	52.882	52.498
4)	MA Heptachlor	4.362	5.168	532.2E6	155.9E6	51.658	51.178
5)	MB Aldrin	4.603	5.472	512.2E6	142.9E6	53.210	51.572
6)	B beta-BHC	4.326	4.831	215.7E6	68447499	51.049	51.658
7)	B delta-BHC	4.523	5.048	433.8E6	103.3E6	53.891	56.485
8)	B Heptachlo...	5.040	5.858	475.6E6	125.9E6	51.108	50.333
9)	A Endosulfan I	5.373	6.215	445.8E6	127.0E6	51.081	50.204
10)	B gamma-Chl...	5.264	6.093	492.7E6	140.2E6	51.051	50.508
11)	B alpha-Chl...	5.320	6.165	482.8E6	138.6E6	50.500	50.014
12)	B 4,4'-DDE	5.488	6.323	445.9E6	122.7E6	51.417	51.374
13)	MA Dieldrin	5.613	6.472	483.6E6	132.2E6	51.529	51.230
14)	MA Endrin	5.867	6.690	422.3E6	108.1E6	48.210	48.100
15)	B Endosulfa...	6.141	6.899	414.5E6	118.0E6	49.024	51.222
16)	A 4,4'-DDD	5.999	6.813	373.7E6	101.2E6	51.653	52.708
17)	MA 4,4'-DDT	6.235	7.112	346.5E6	97287187	48.321	49.590
18)	B Endrin al...	6.308	7.023	347.5E6	101.6E6	49.563	50.057
19)	B Endosulfa...	6.519	7.246	368.3E6	106.2E6	50.680	50.309
20)	A Methoxychlor	6.780	7.570	195.3E6	57440120	48.672	48.078
21)	B Endrin ke...	7.003	7.716	458.1E6	119.8E6	55.064	52.797



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021519\
Data File : PL044849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2019 16:04
Operator : AJ\SJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 22:02:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

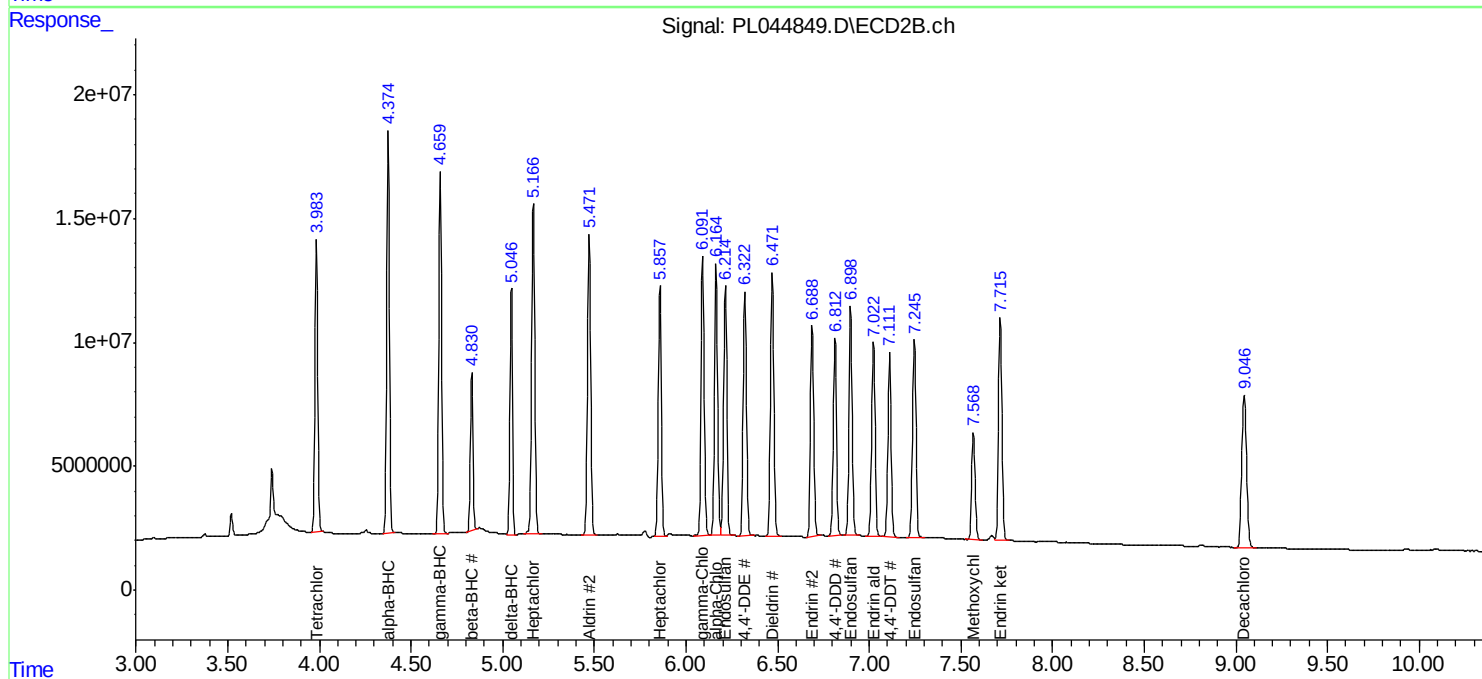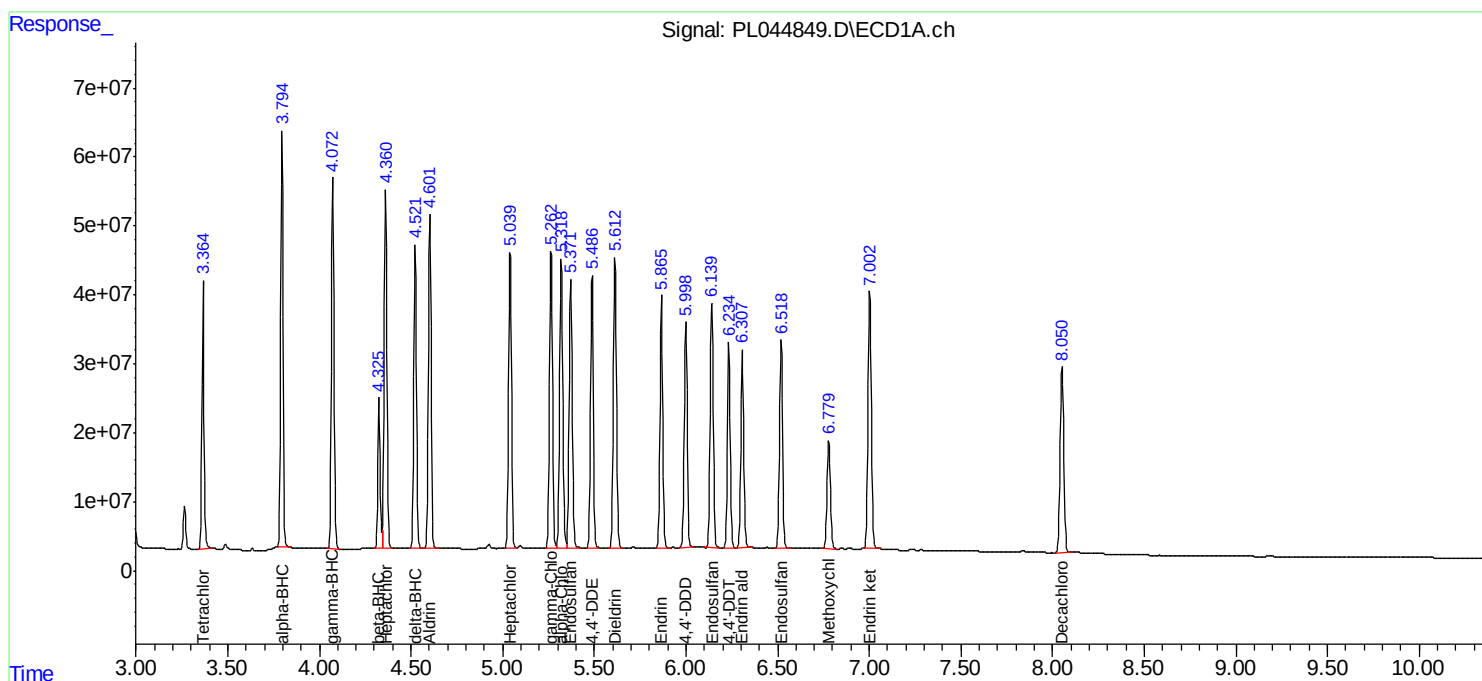




#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 367072455
Conc: 51.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

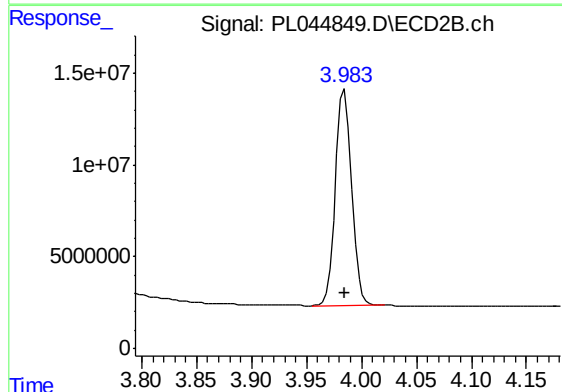


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 120907000
Conc: 51.47 ng/ml

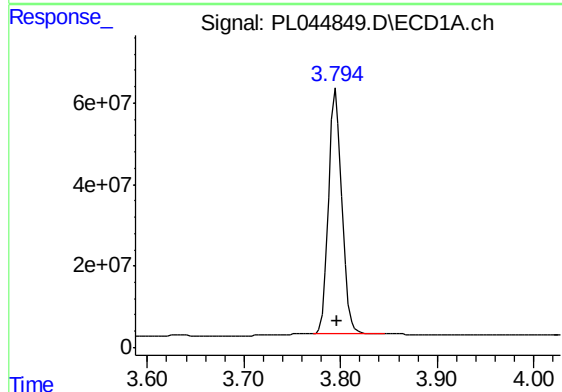


#2 alpha-BHC

R.T.: 3.796 min
Delta R.T.: 0.000 min
Response: 564436616
Conc: 52.85 ng/ml

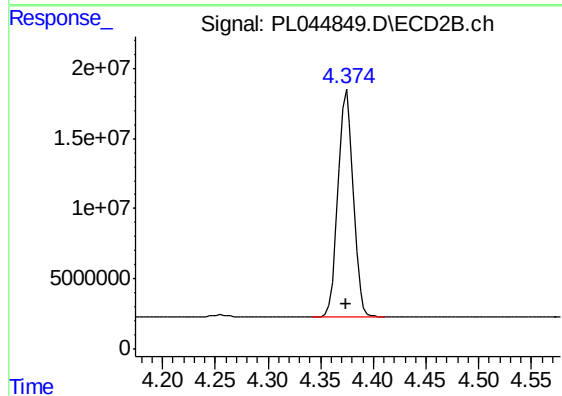

#2 alpha-BHC


R.T.: 4.375 min
Delta R.T.: 0.001 min
Response: 162465397
Conc: 53.34 ng/ml



#3 gamma-BHC (Lindane)


R.T.: 4.073 min
Delta R.T.: 0.000 min
Response: 520287985
Conc: 52.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

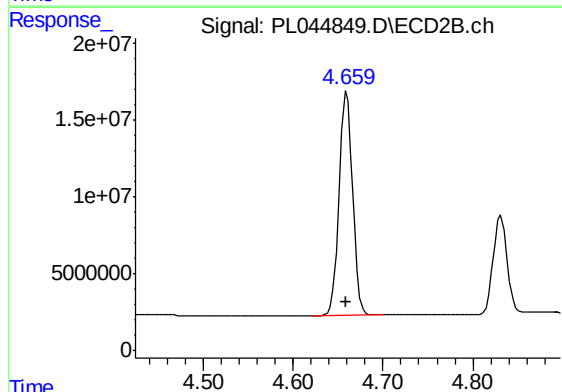


#3 gamma-BHC (Lindane)

R.T.: 4.660 min
Delta R.T.: 0.001 min
Response: 152095125
Conc: 52.50 ng/ml




#4 Heptachlor

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 532155929
Conc: 51.66 ng/ml

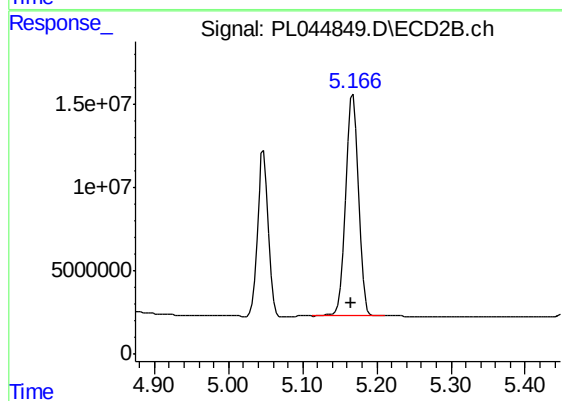

#4 Heptachlor


R.T.: 5.168 min
Delta R.T.: 0.002 min
Response: 155892132
Conc: 51.18 ng/ml

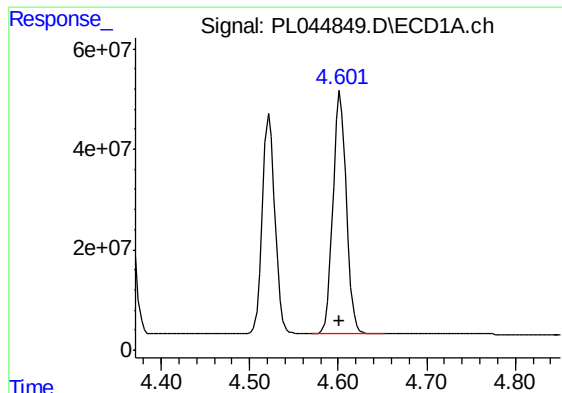

#5 Aldrin


R.T.: 4.603 min
Delta R.T.: 0.000 min
Response: 512180669
Conc: 53.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

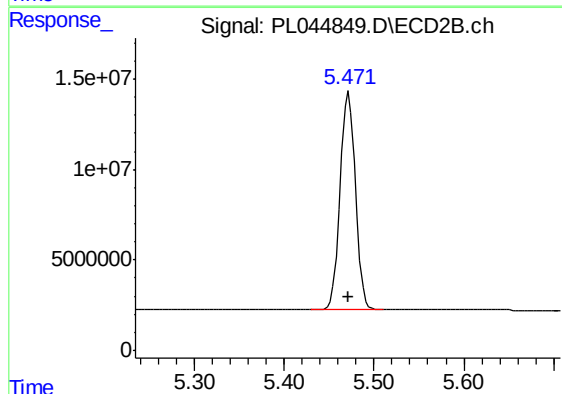


#5 Aldrin

R.T.: 5.472 min
Delta R.T.: 0.001 min
Response: 142908631
Conc: 51.57 ng/ml




#6 beta-BHC

R.T.: 4.326 min
Delta R.T.: 0.000 min
Response: 215709810
Conc: 51.05 ng/ml

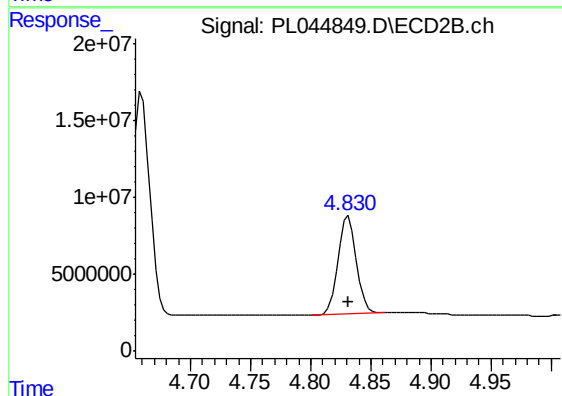

#6 beta-BHC


R.T.: 4.831 min
Delta R.T.: 0.000 min
Response: 68447499
Conc: 51.66 ng/ml



#7 delta-BHC


R.T.: 4.523 min
Delta R.T.: 0.000 min
Response: 433824369
Conc: 53.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

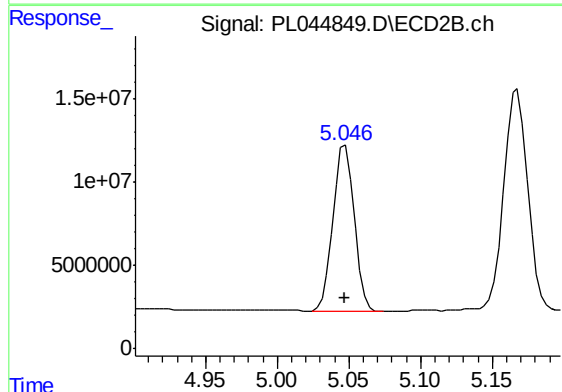


#7 delta-BHC

R.T.: 5.048 min
Delta R.T.: 0.000 min
Response: 103285878
Conc: 56.48 ng/ml

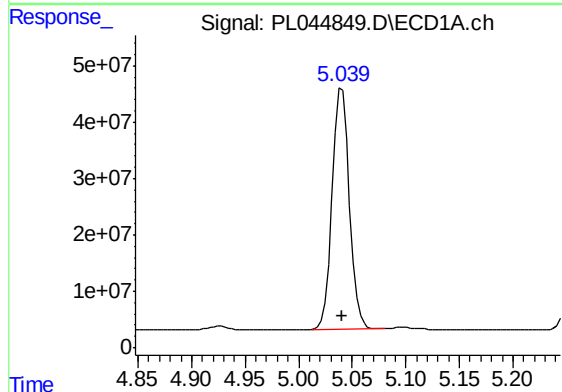


#8 Heptachlor epoxide

R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 475556046
Conc: 51.11 ng/ml

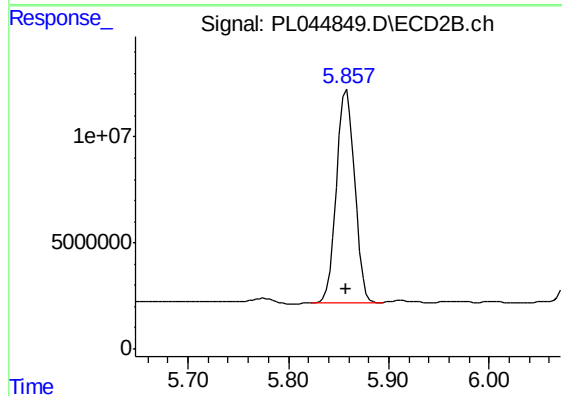

#8 Heptachlor epoxide


R.T.: 5.858 min
Delta R.T.: 0.001 min
Response: 125860662
Conc: 50.33 ng/ml

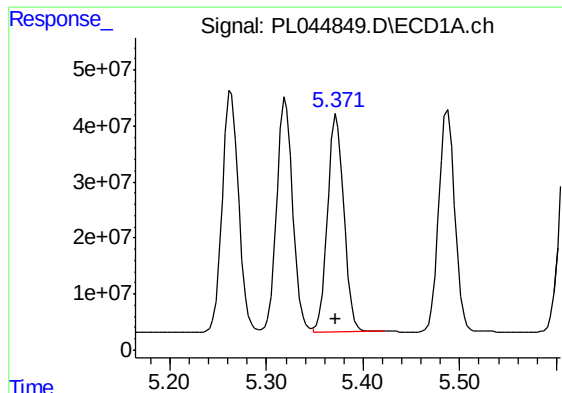

#9 Endosulfan I


R.T.: 5.373 min
Delta R.T.: 0.000 min
Response: 445783957
Conc: 51.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

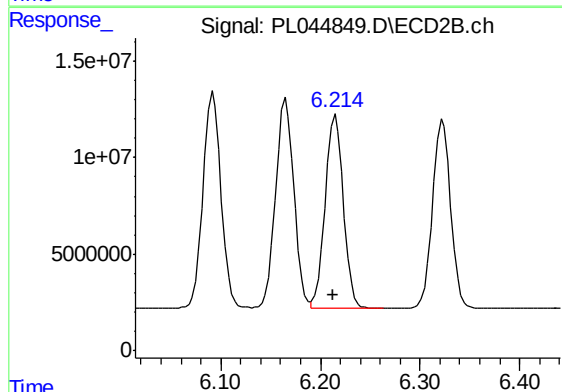


#9 Endosulfan I

R.T.: 6.215 min
Delta R.T.: 0.002 min
Response: 127007846
Conc: 50.20 ng/ml

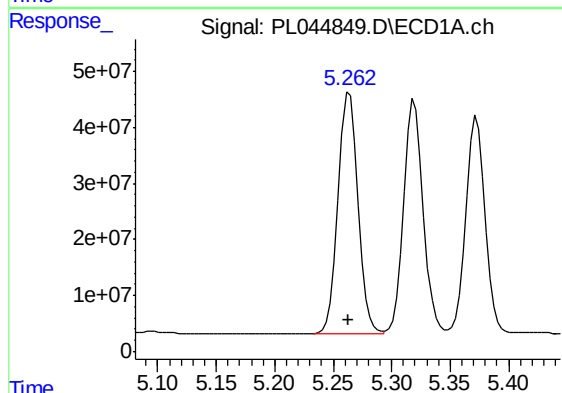


#10 gamma-Chlordane

R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 492700448
Conc: 51.05 ng/ml

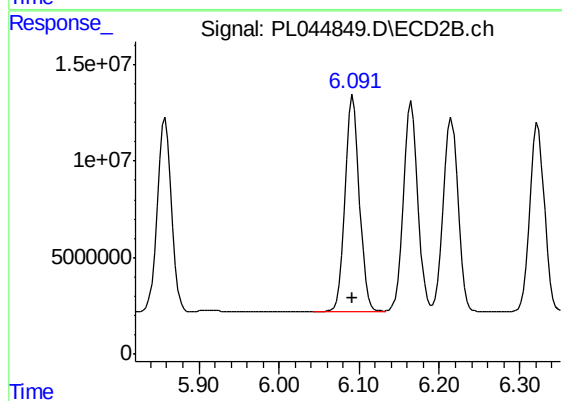

#10 gamma-Chlordane


R.T.: 6.093 min
Delta R.T.: 0.002 min
Response: 140214506
Conc: 50.51 ng/ml

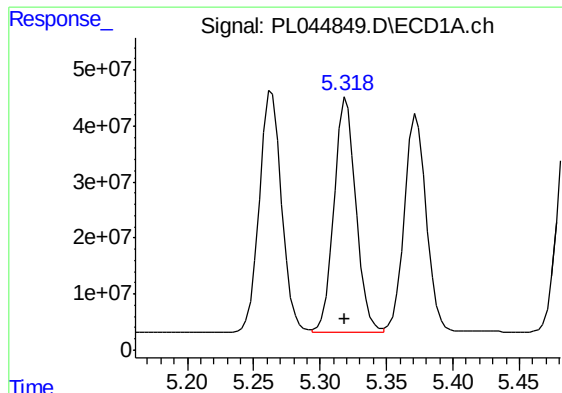

#11 alpha-Chlordane


R.T.: 5.320 min
Delta R.T.: 0.000 min
Response: 482843832
Conc: 50.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

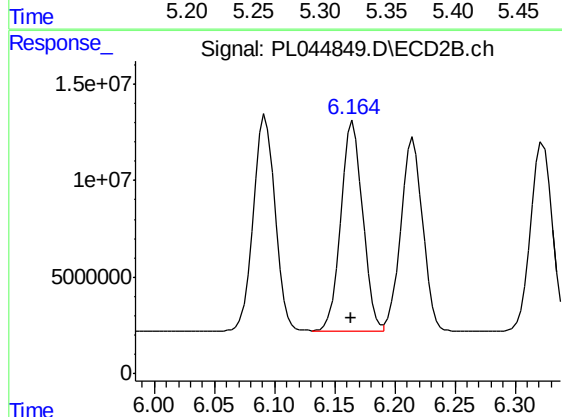


#11 alpha-Chlordane

R.T.: 6.165 min
Delta R.T.: 0.001 min
Response: 138578549
Conc: 50.01 ng/ml

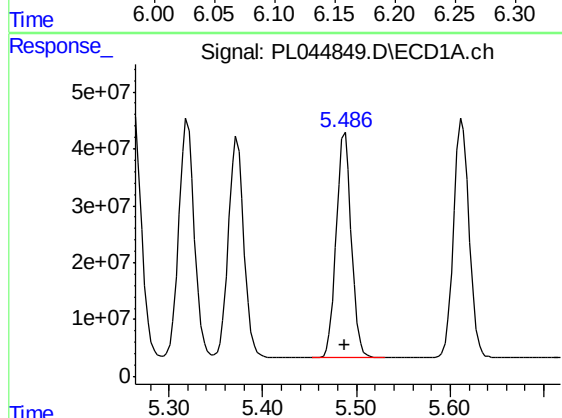


#12 4,4'-DDE

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 445893788
Conc: 51.42 ng/ml

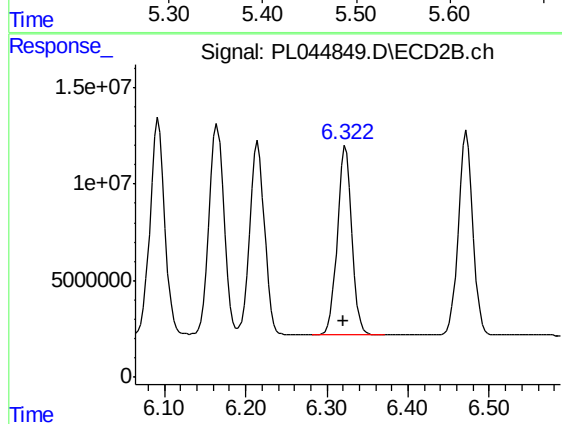

#12 4,4'-DDE


R.T.: 6.323 min
Delta R.T.: 0.002 min
Response: 122663591
Conc: 51.37 ng/ml



#13 Dielldrin


R.T.: 5.613 min
Delta R.T.: 0.001 min
Response: 483635213
Conc: 51.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

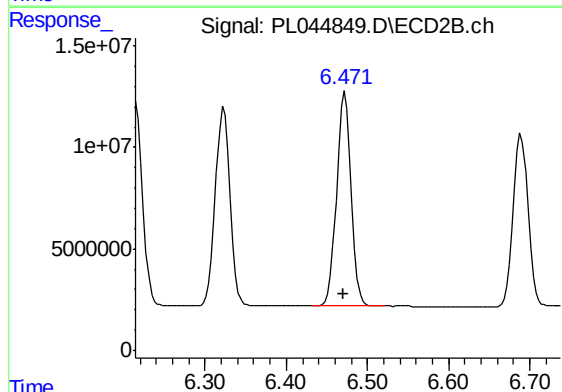


#13 Dielldrin

R.T.: 6.472 min
Delta R.T.: 0.002 min
Response: 132166570
Conc: 51.23 ng/ml




#14 Endrin

R.T.: 5.867 min
Delta R.T.: 0.002 min
Response: 422324935
Conc: 48.21 ng/ml

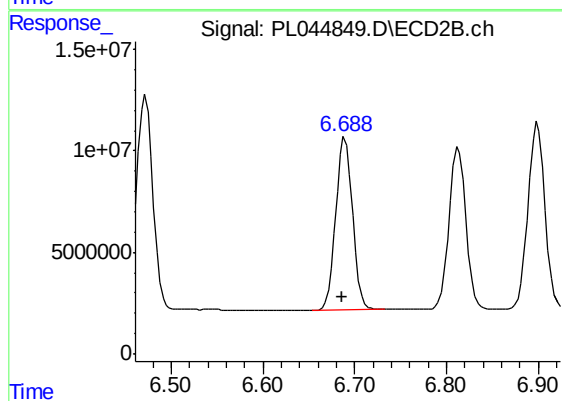

#14 Endrin


R.T.: 6.690 min
Delta R.T.: 0.003 min
Response: 108076839
Conc: 48.10 ng/ml



#15 Endosulfan II


R.T.: 6.141 min
Delta R.T.: 0.002 min
Response: 414528683
Conc: 49.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

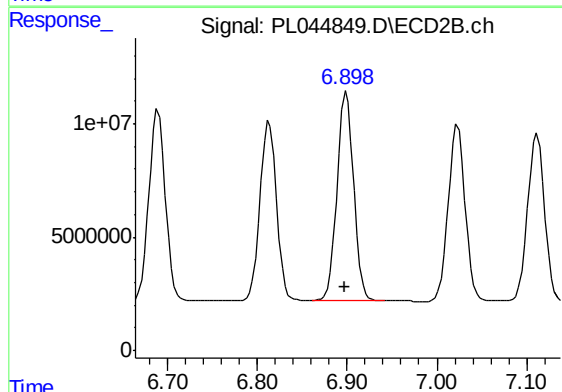


#15 Endosulfan II

R.T.: 6.899 min
Delta R.T.: 0.002 min
Response: 117976492
Conc: 51.22 ng/ml




#16 4,4'-DDD

R.T.: 5.999 min
Delta R.T.: 0.001 min
Response: 373666881
Conc: 51.65 ng/ml

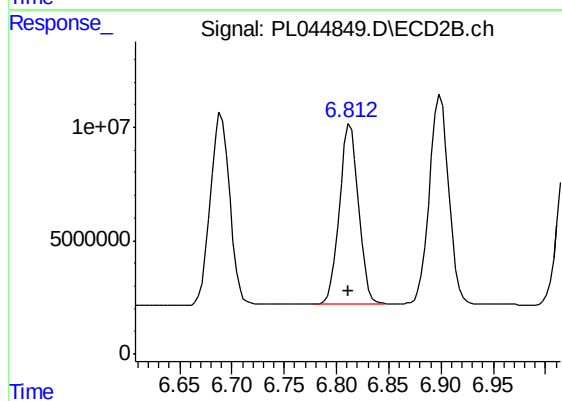

#16 4,4'-DDD


R.T.: 6.813 min
Delta R.T.: 0.002 min
Response: 101208845
Conc: 52.71 ng/ml



#17 4,4'-DDT


R.T.: 6.235 min
Delta R.T.: 0.000 min
Response: 346522588
Conc: 48.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

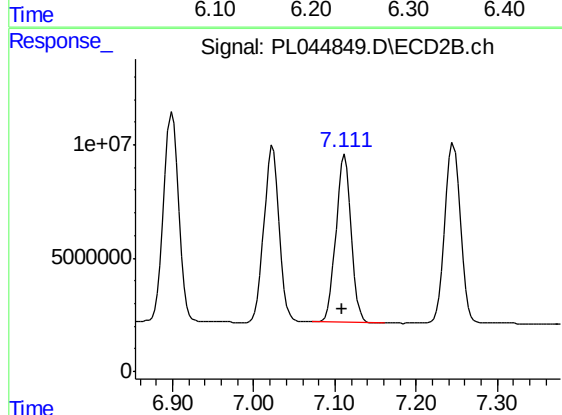


#17 4,4'-DDT

R.T.: 7.112 min
Delta R.T.: 0.003 min
Response: 97287187
Conc: 49.59 ng/ml

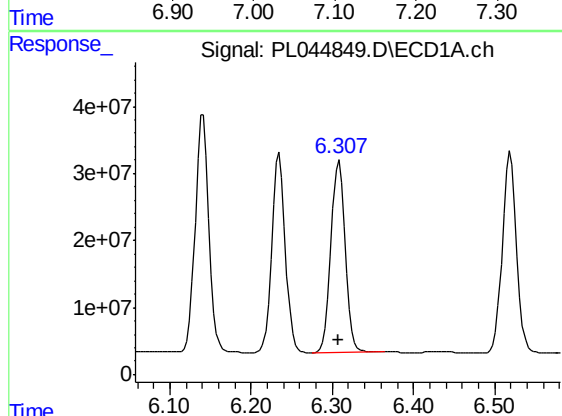


#18 Endrin aldehyde

R.T.: 6.308 min
Delta R.T.: 0.001 min
Response: 347459557
Conc: 49.56 ng/ml

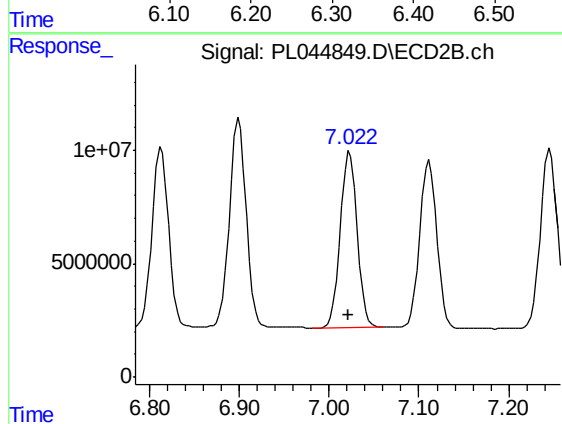

#18 Endrin aldehyde


R.T.: 7.023 min
Delta R.T.: 0.002 min
Response: 101560868
Conc: 50.06 ng/ml



#19 Endosulfan Sulfate


R.T.: 6.519 min
Delta R.T.: 0.002 min
Response: 368331836
Conc: 50.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

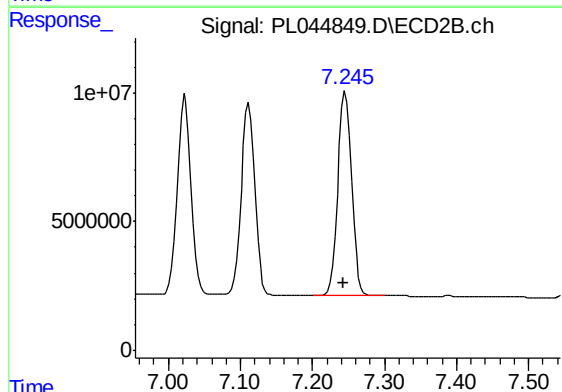


#19 Endosulfan Sulfate

R.T.: 7.246 min
Delta R.T.: 0.003 min
Response: 106150145
Conc: 50.31 ng/ml




#20 Methoxychlor

R.T.: 6.780 min
Delta R.T.: 0.001 min
Response: 195324197
Conc: 48.67 ng/ml

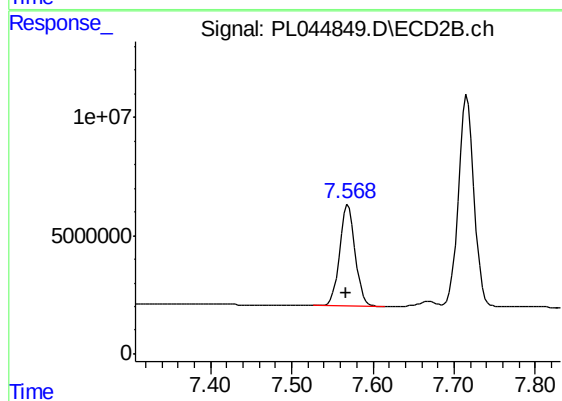

#20 Methoxychlor


R.T.: 7.570 min
Delta R.T.: 0.003 min
Response: 57440120
Conc: 48.08 ng/ml

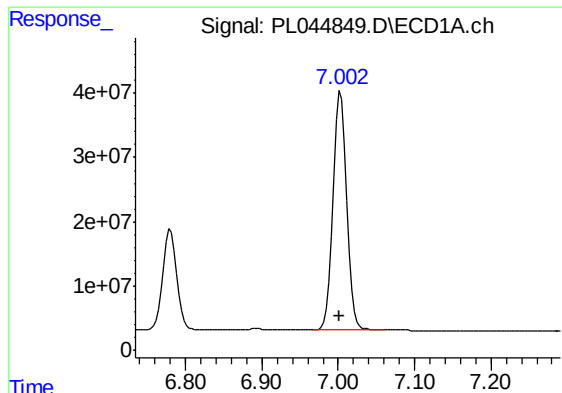

#21 Endrin ketone


R.T.: 7.003 min
Delta R.T.: 0.002 min
Response: 458142632
Conc: 55.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

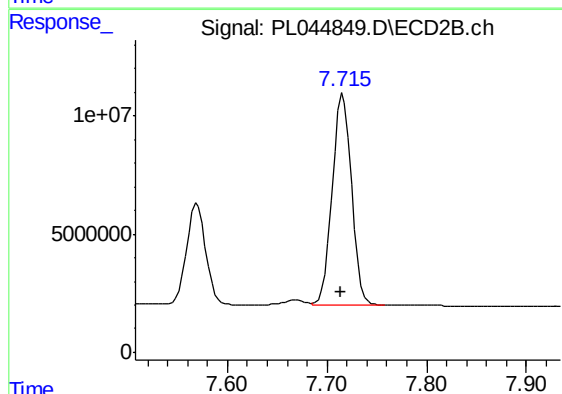


#21 Endrin ketone

R.T.: 7.716 min
Delta R.T.: 0.002 min
Response: 119826206
Conc: 52.80 ng/ml

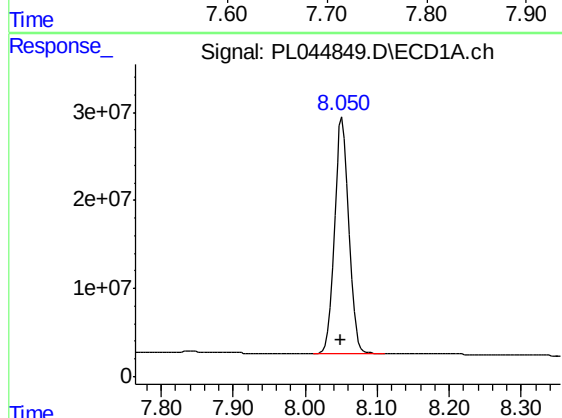

#28 Decachlorobiphenyl

R.T.: 8.052 min
Delta R.T.: 0.003 min
Response: 368579603
Conc: 50.54 ng/ml

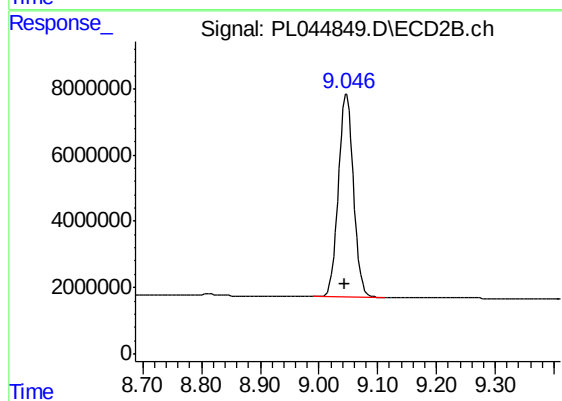

#28 Decachlorobiphenyl

R.T.: 9.047 min
Delta R.T.: 0.004 min
Response: 110273340
Conc: 49.79 ng/ml