

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021519\
 Data File : PL044856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2019 17:44
 Operator : AJ\SJ
 Sample : K1502-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-1-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 22:04:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.985	154.1E6	50869781	21.651	21.654
28)	SA Decachlor...	8.052	9.048	147.5E6	45585517	20.230	20.582
Target Compounds							
10)	B gamma-Chl...	5.264	6.092	57174740	26817286	5.924m	9.660 #
11)	B alpha-Chl...	5.319	6.167	67911982	51742041	7.103	18.674 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021519\
Data File : PL044856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2019 17:44
Operator : AJ\SJ
Sample : K1502-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RO-1-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 22:04:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

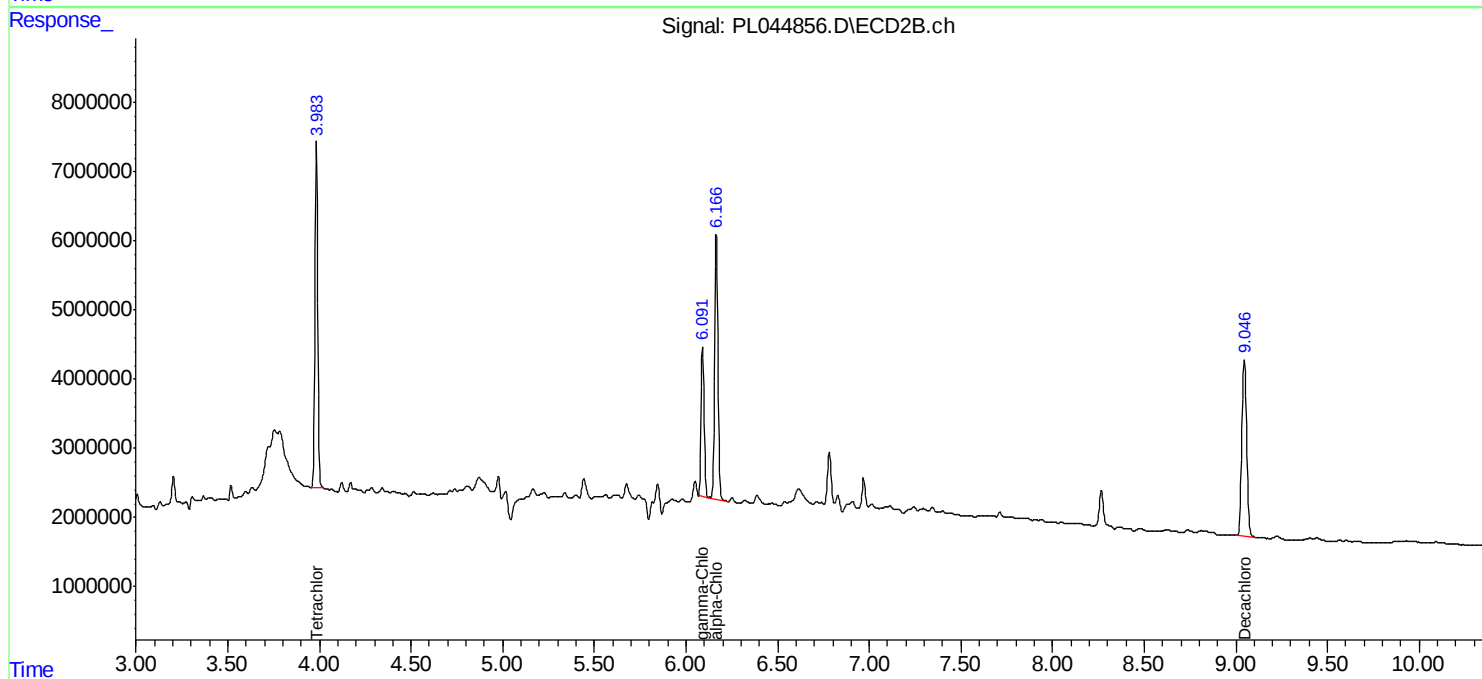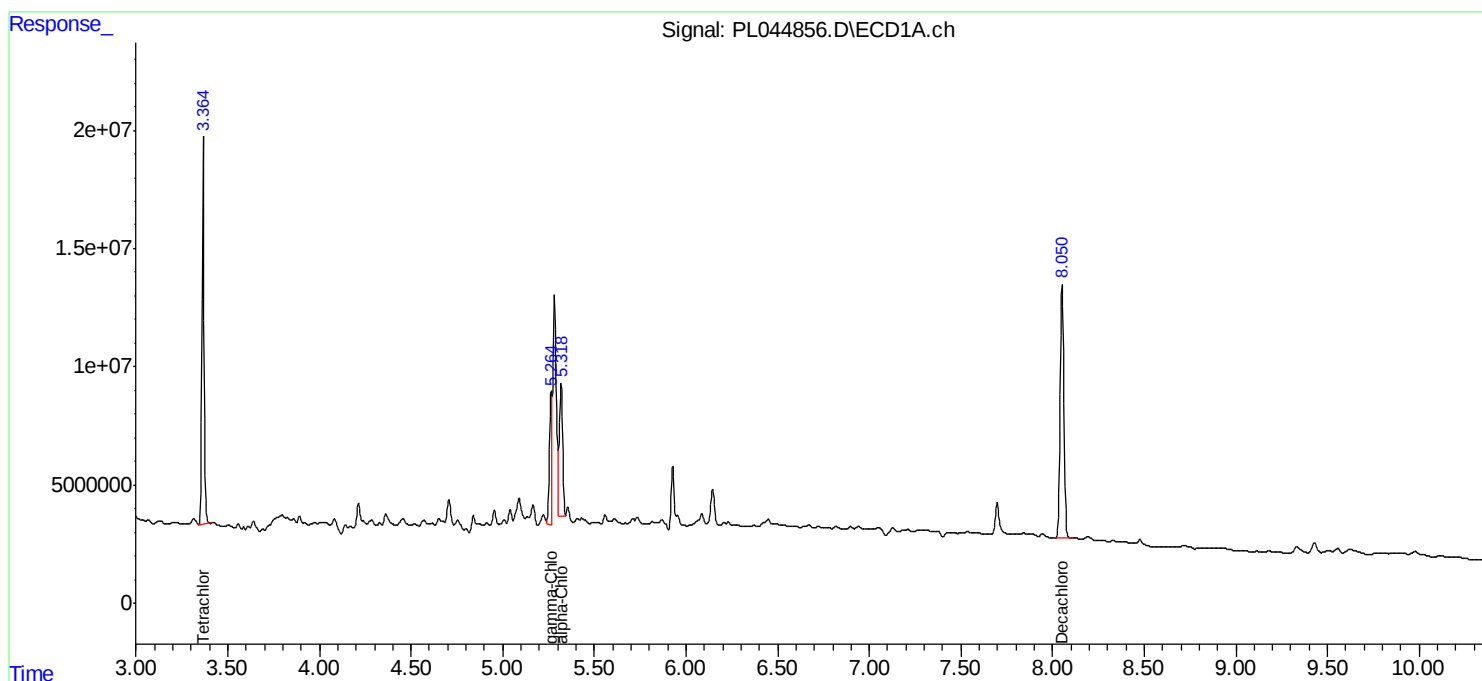


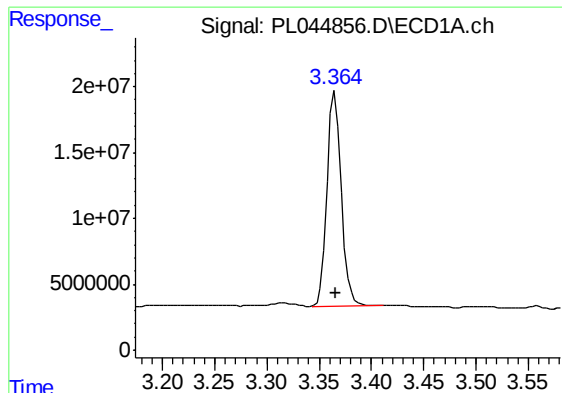

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 154064022
Conc: 21.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-1-4

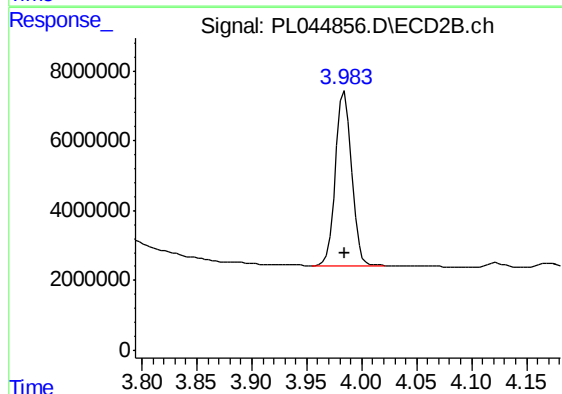


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 50869781
Conc: 21.65 ng/ml

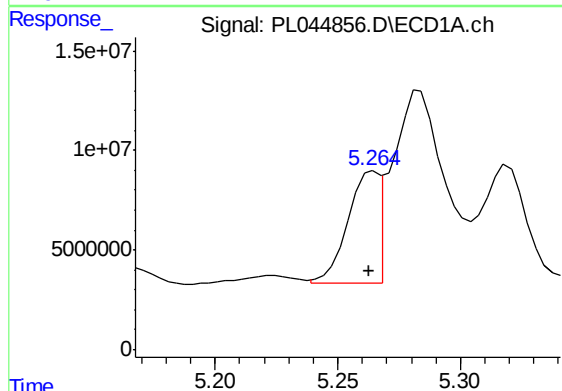


#10 gamma-Chlordane

R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 57174740
Conc: 5.92 ng/ml m

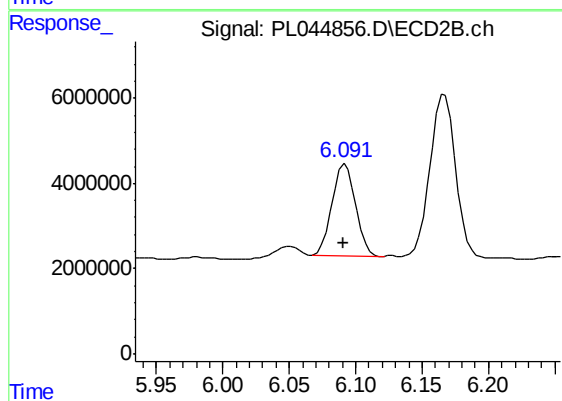

#10 gamma-Chlordane


R.T.: 6.092 min
Delta R.T.: 0.001 min
Response: 26817286
Conc: 9.66 ng/ml

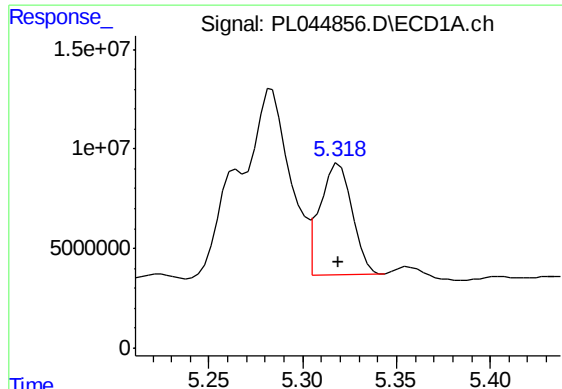

#11 alpha-Chlordane


R.T.: 5.319 min
Delta R.T.: 0.000 min
Response: 67911982
Conc: 7.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-1-4

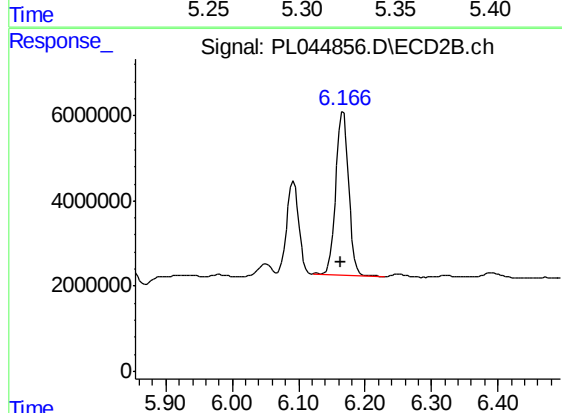


#11 alpha-Chlordane

R.T.: 6.167 min
Delta R.T.: 0.003 min
Response: 51742041
Conc: 18.67 ng/ml

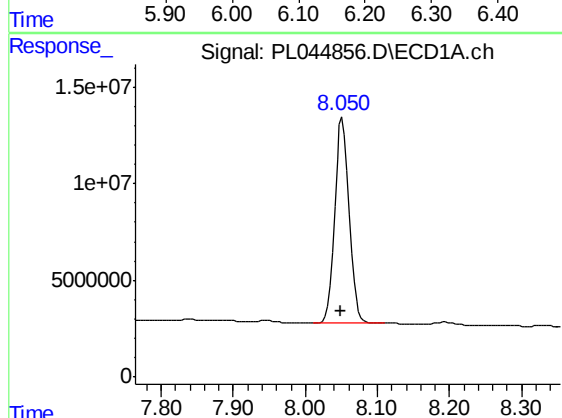

#28 Decachlorobiphenyl

R.T.: 8.052 min
Delta R.T.: 0.003 min
Response: 147549621
Conc: 20.23 ng/ml

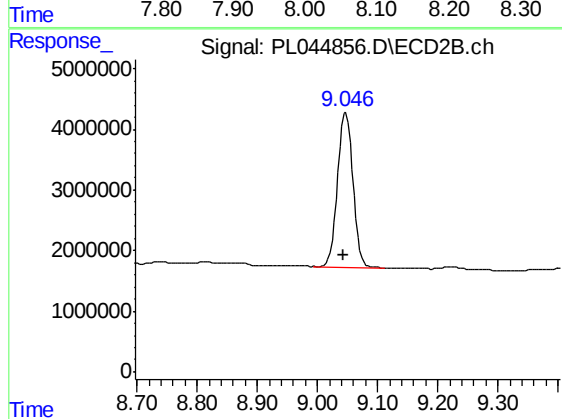

#28 Decachlorobiphenyl

R.T.: 9.048 min
Delta R.T.: 0.005 min
Response: 45585517
Conc: 20.58 ng/ml