

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021521\
 Data File : PL064793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2021 09:11
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 14:40:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.424	4.100	63859213	51713138	22.697	23.939
28)	SA Decachlor...	8.146	9.256	47765129	39289715	21.240	20.686
Target Compounds							
17)	MA 4,4'-DDT	6.317	0.000	1298544	0	0.576	N.D. #
23)	Chlordane-1	4.312f	0.000	2450996	0	21.561	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021521\
Data File : PL064793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2021 09:11
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 14:40:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

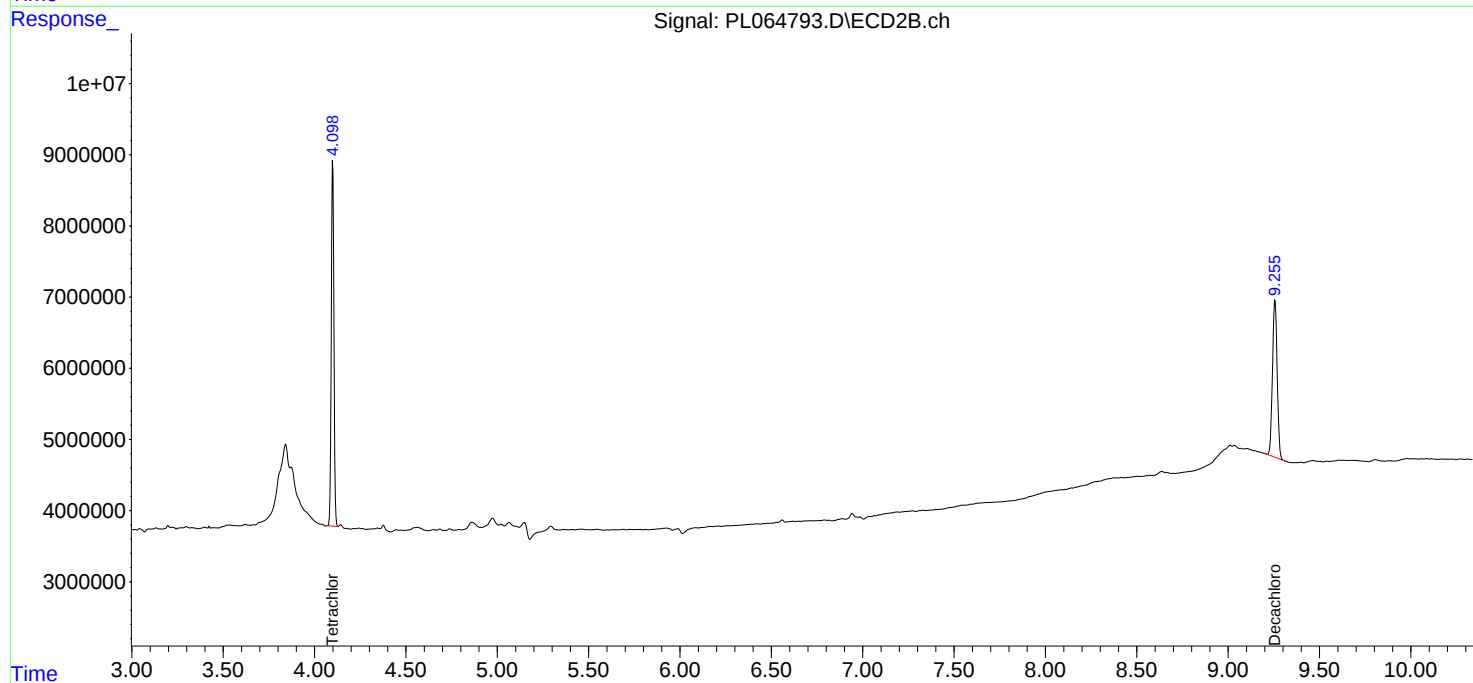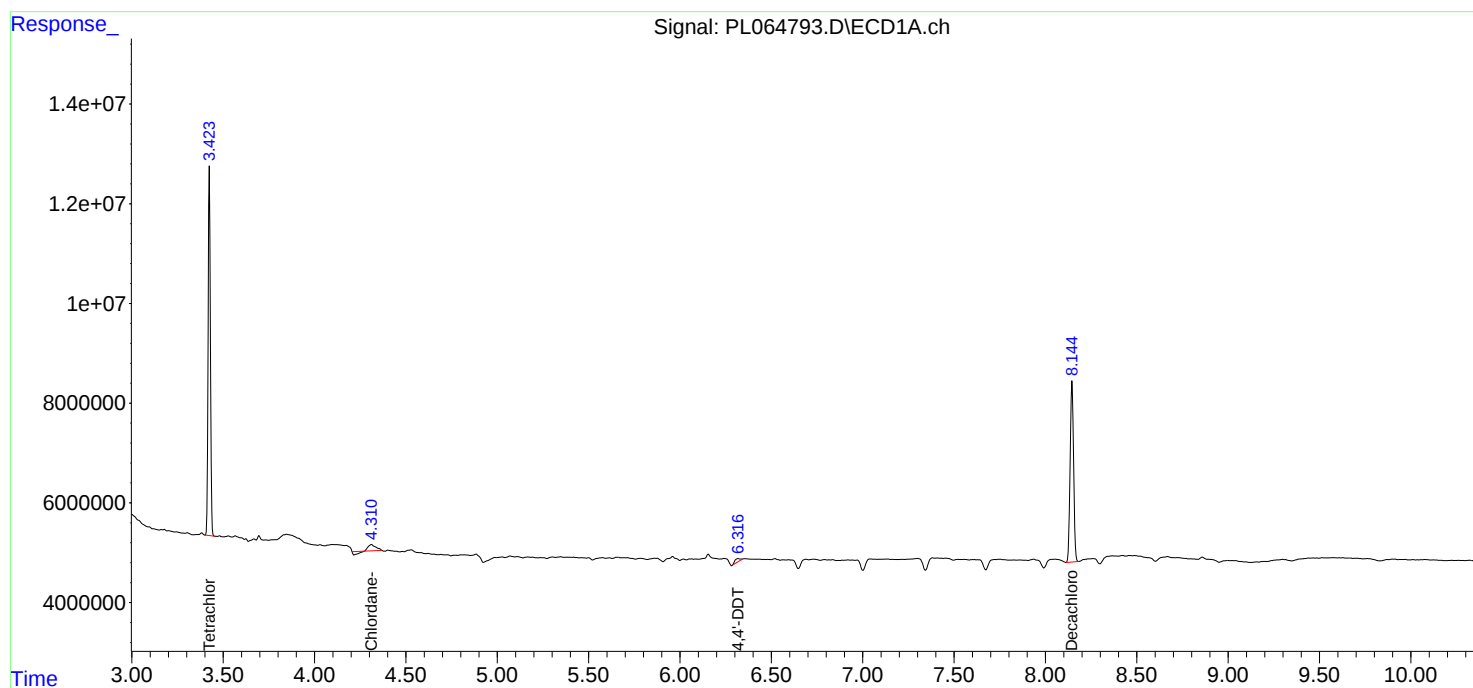


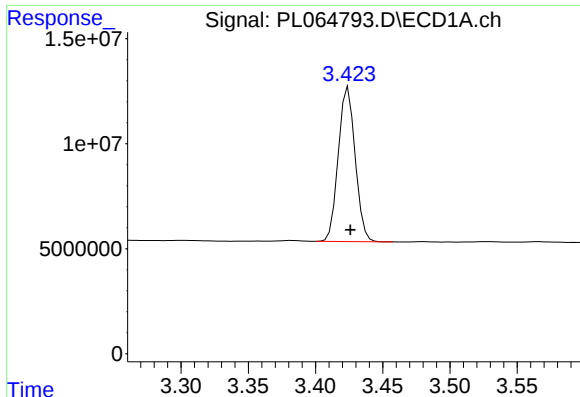

#1 Tetrachloro-m-xylene


R.T.: 3.424 min
Delta R.T.: -0.002 min
Response: 63859213
Conc: 22.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

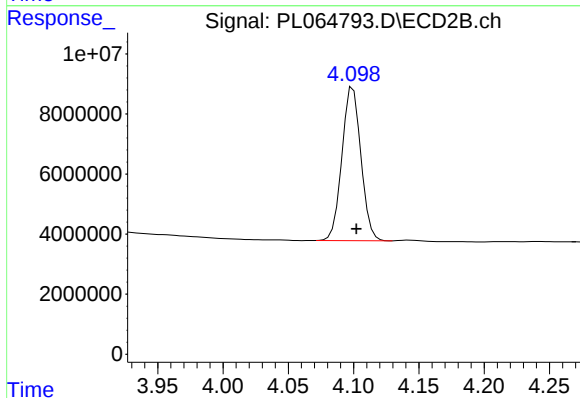


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.003 min
Response: 51713138
Conc: 23.94 ng/ml

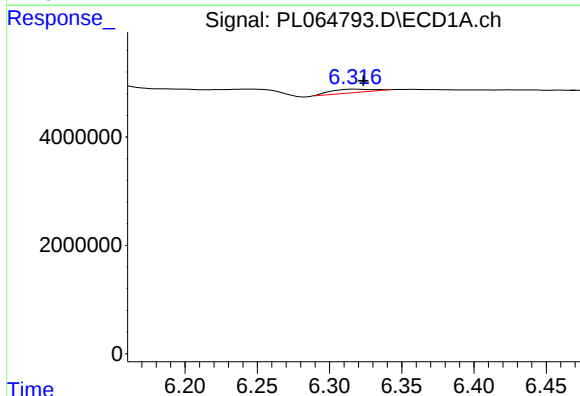


#17 4,4'-DDT

R.T.: 6.317 min
Delta R.T.: -0.006 min
Response: 1298544
Conc: 0.58 ng/ml

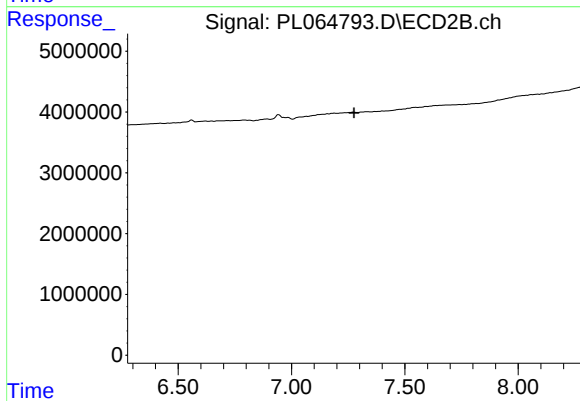

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.276 min
Response: 0
Conc: N.D.

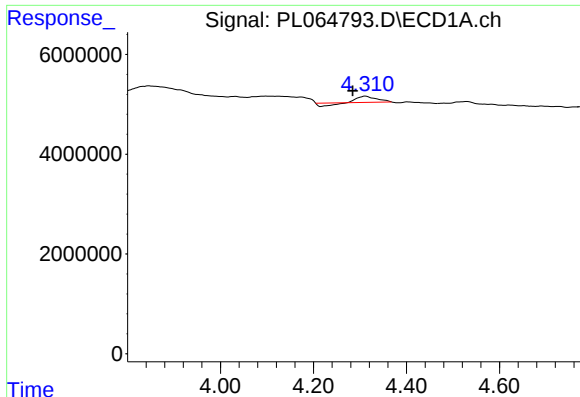

#23 Chlordane-1


R.T.: 4.312 min
Delta R.T.: 0.027 min
Response: 2450996
Conc: 21.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

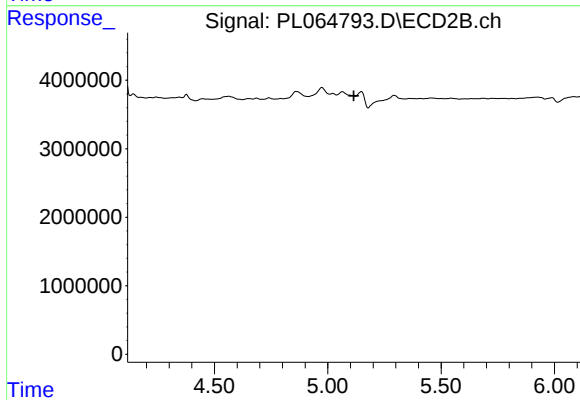


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

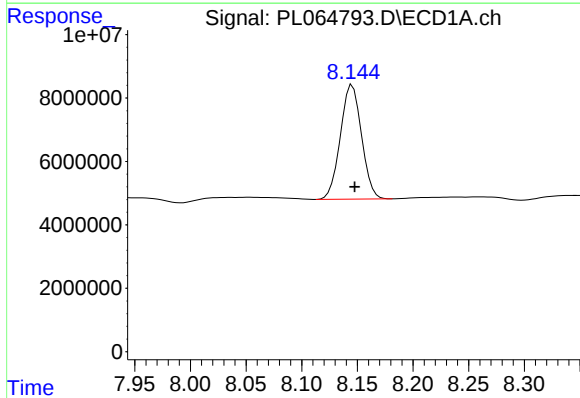

#28 Decachlorobiphenyl

R.T.: 8.146 min
Delta R.T.: -0.002 min
Response: 47765129
Conc: 21.24 ng/ml

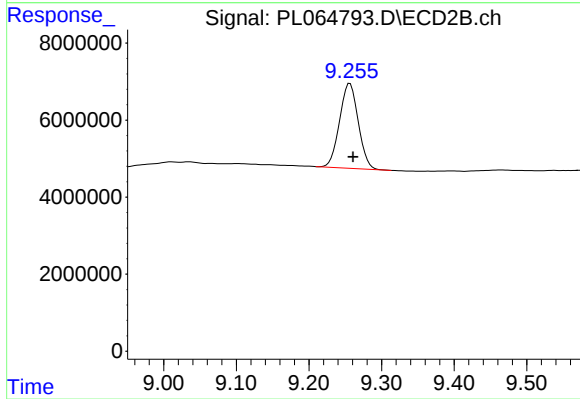

#28 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.004 min
Response: 39289715
Conc: 20.69 ng/ml