

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021521\
 Data File : PL064798.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2021 13:16
 Operator : AR\AJ
 Sample : M1400-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BIN-2

Manual Integrations
 APPROVED

Ankita
 2/16/2021 9:51:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 14:41:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.098	47751205	38023078	16.972m	17.602m
28)	SA Decachlor...	8.151	9.259	29848206	27715294	13.273	14.592

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021521\
Data File : PL064798.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2021 13:16
Operator : AR\AJ
Sample : M1400-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BIN-2


Manual Integrations
APPROVED

Ankita
2/16/2021 9:51:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 14:41:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

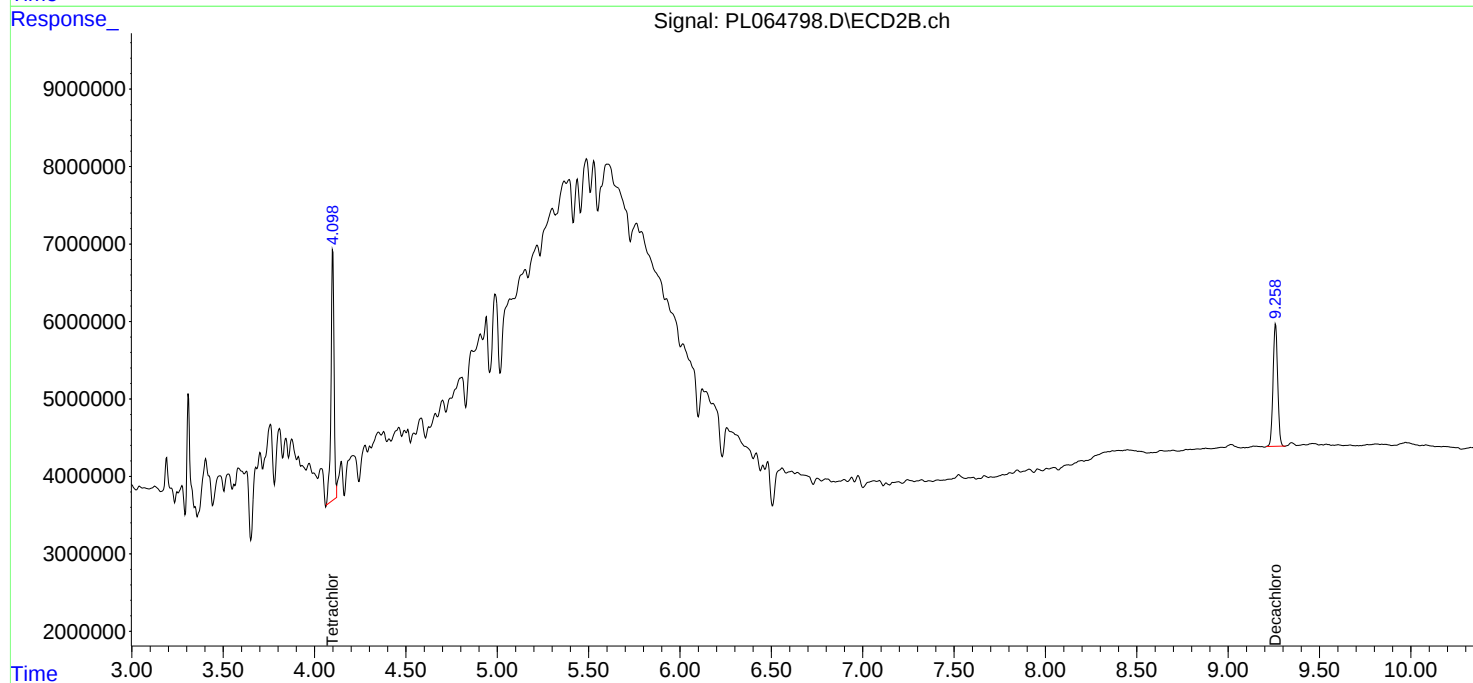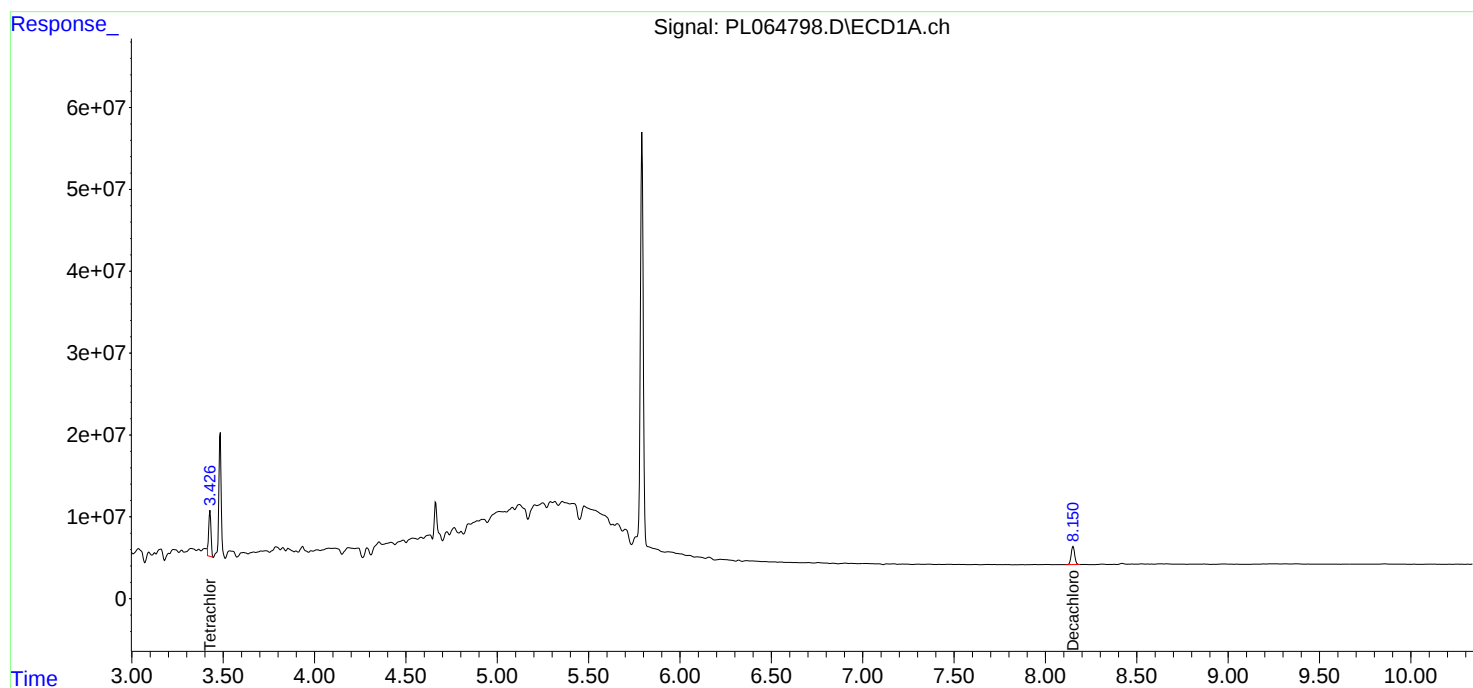

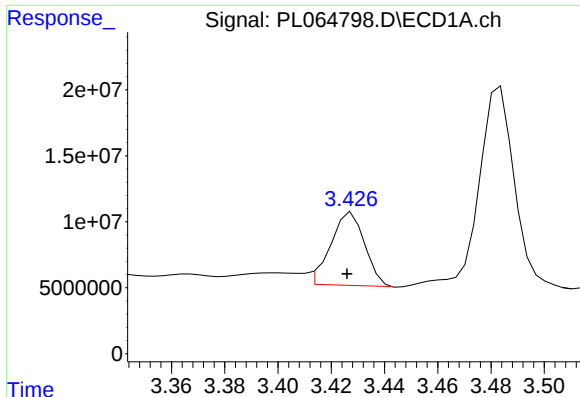


#1 Tetrachloro-m-xylene

R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 47751205
Conc: 16.97 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BIN-2


Manual Integrations
APPROVED

Ankita
2/16/2021 9:51:14 AM

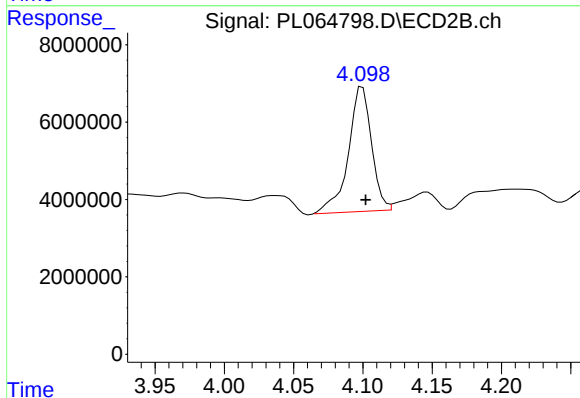


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.004 min
Response: 38023078
Conc: 17.60 ng/ml m

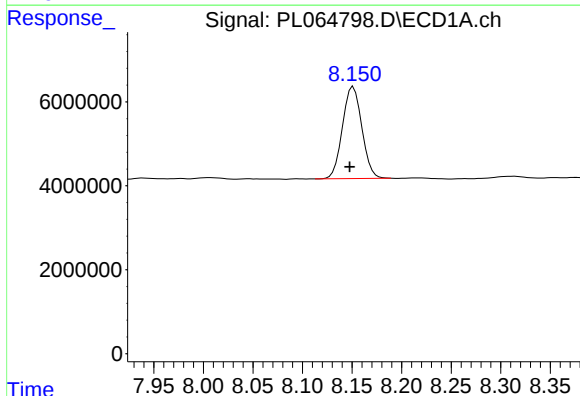

#28 Decachlorobiphenyl

R.T.: 8.151 min
Delta R.T.: 0.003 min
Response: 29848206
Conc: 13.27 ng/ml

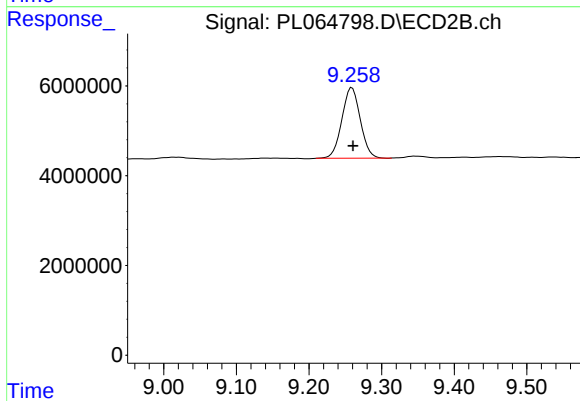

#28 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.001 min
Response: 27715294
Conc: 14.59 ng/ml