

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021521\
 Data File : PL064799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2021 13:30
 Operator : AR\AJ
 Sample : M1402-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-N9994

Manual Integrations
 APPROVED

Ankita
 2/16/2021 9:51:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 14:41:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.425	4.100	57674893	46058717	20.499	21.322
28)	SA Decachlor...	8.146	9.250	28541787	40794365	12.692m	21.478m#
Target Compounds							
12)	B 4,4'-DDE	5.569	6.476	6840166	8630600	2.186m	4.256 #
17)	MA 4,4'-DDT	6.320	7.272	13611493	5526219	6.036	3.625m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021521\
Data File : PL064799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2021 13:30
Operator : AR\AJ
Sample : M1402-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RO-N9994


Manual Integrations
APPROVED

Ankita
2/16/2021 9:51:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 14:41:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

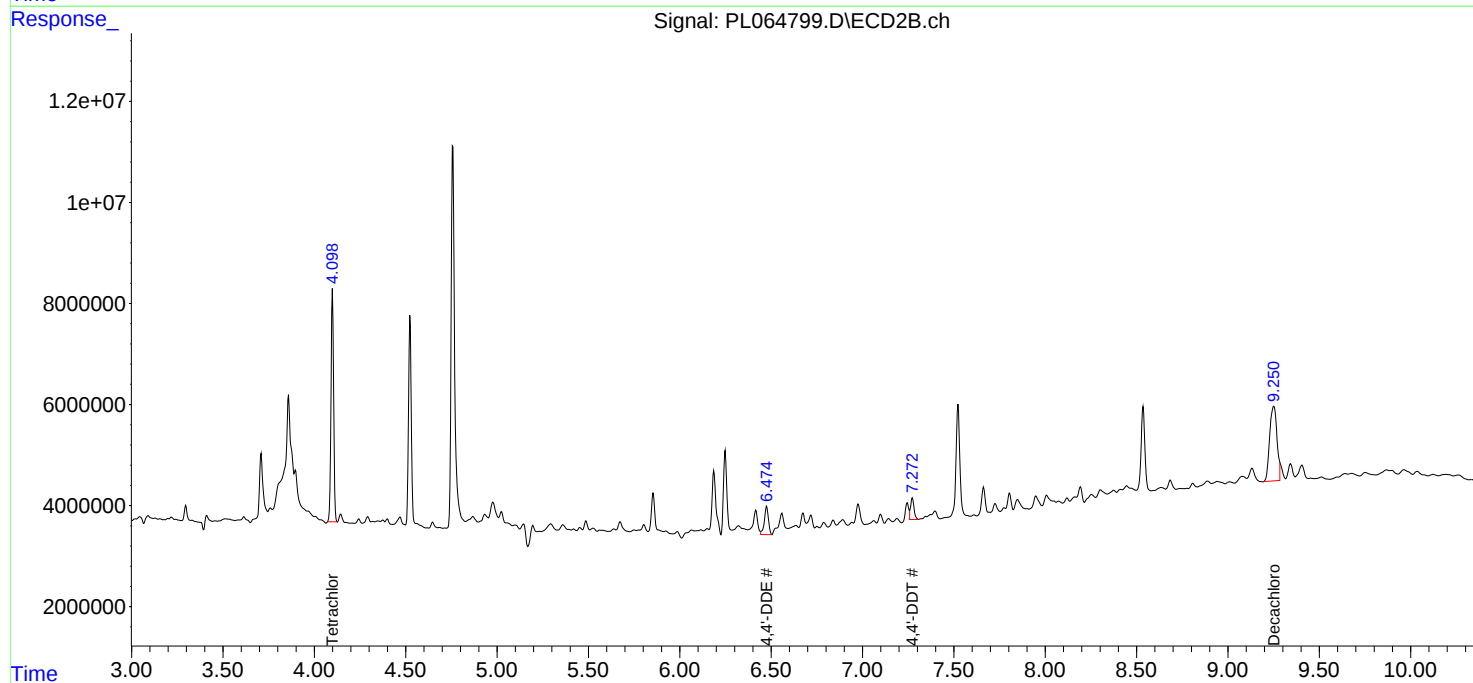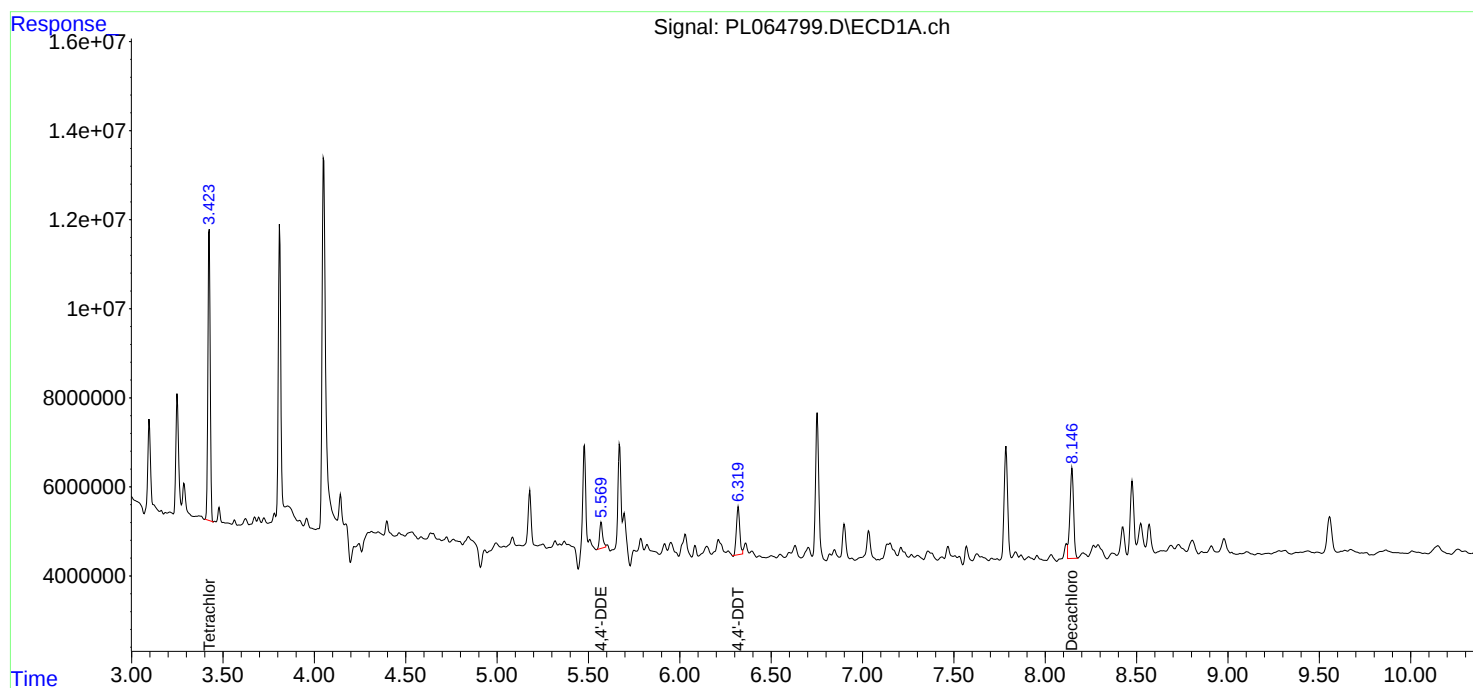

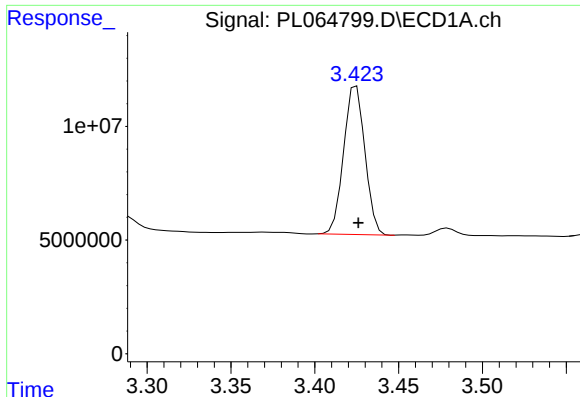


#1 Tetrachloro-m-xylene

R.T.: 3.425 min
Delta R.T.: -0.001 min
Response: 57674893
Conc: 20.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-N9994


Manual Integrations
APPROVED

Ankita
2/16/2021 9:51:17 AM

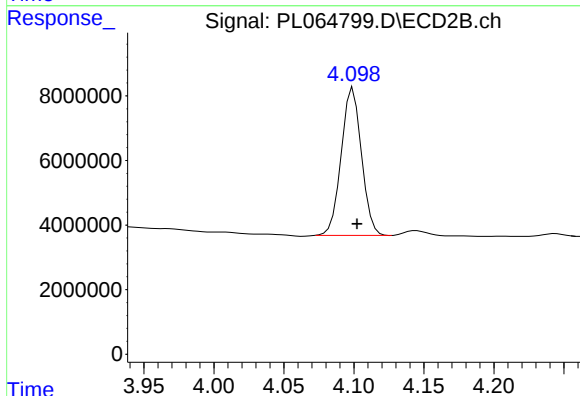


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.003 min
Response: 46058717
Conc: 21.32 ng/ml

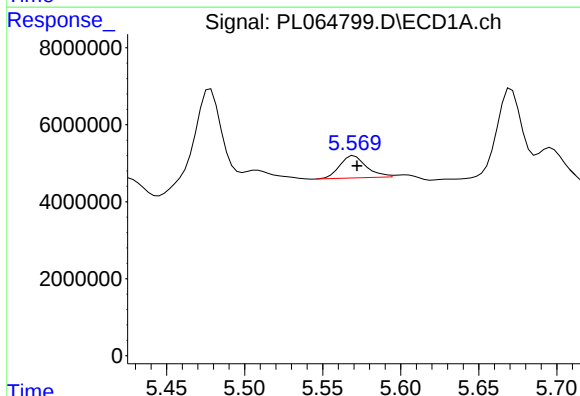


#12 4,4'-DDE

R.T.: 5.569 min
Delta R.T.: -0.003 min
Response: 6840166
Conc: 2.19 ng/ml m

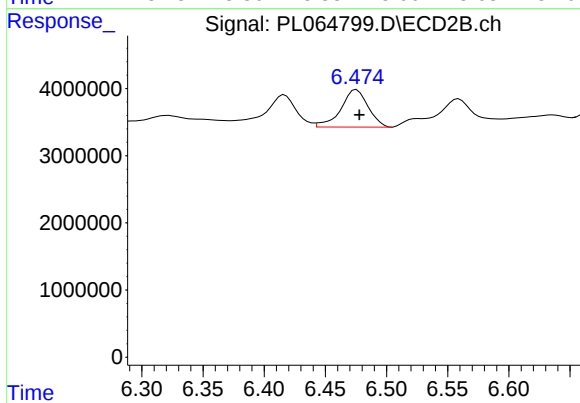

#12 4,4'-DDE

R.T.: 6.476 min
Delta R.T.: -0.002 min
Response: 8630600
Conc: 4.26 ng/ml

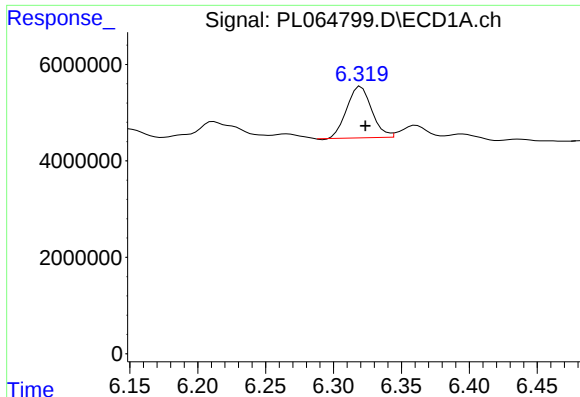


#17 4,4'-DDT

R.T.: 6.320 min
Delta R.T.: -0.003 min
Response: 13611493
Conc: 6.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-N9994


Manual Integrations
APPROVED

Ankita
2/16/2021 9:51:17 AM

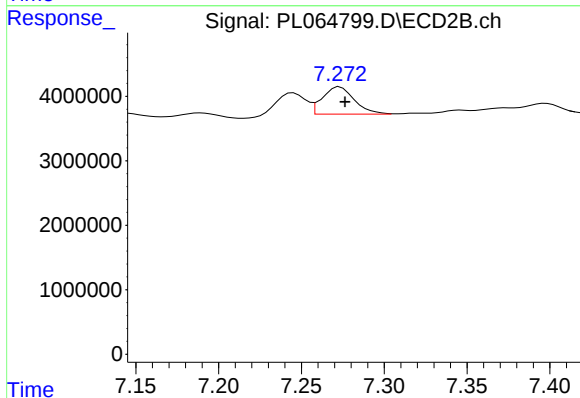


#17 4,4'-DDT

R.T.: 7.272 min
Delta R.T.: -0.004 min
Response: 5526219
Conc: 3.62 ng/ml m

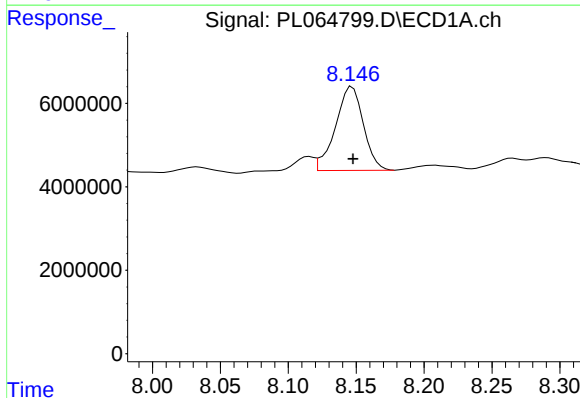

#28 Decachlorobiphenyl

R.T.: 8.146 min
Delta R.T.: -0.002 min
Response: 28541787
Conc: 12.69 ng/ml m

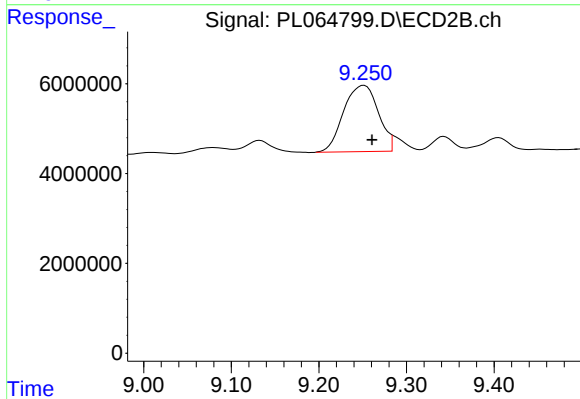

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.010 min
Response: 40794365
Conc: 21.48 ng/ml m