

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021522\
 Data File : PL072727.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Feb 2022 00:00
 Operator : AR\AJ
 Sample : N1477-05
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-COMP-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 02:00:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 05:14:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.553	5.489	9906007	33696316	20.573	19.507
28)	SA Decachlor...	10.310	11.377	11871842	25330941	15.682	15.974

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021522\
Data File : PL072727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Feb 2022 00:00
Operator : AR\AJ
Sample : N1477-05
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACHATE-AMENDED-COMP-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 02:00:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 05:14:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

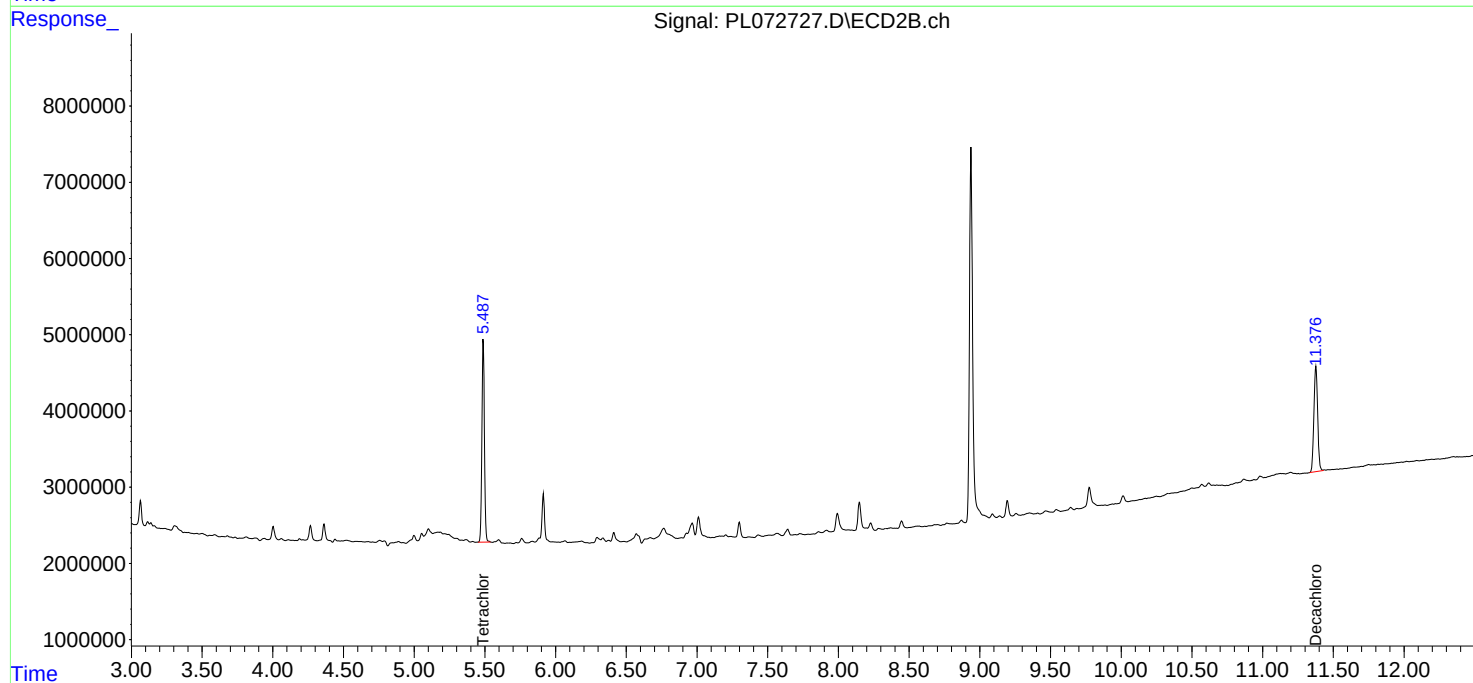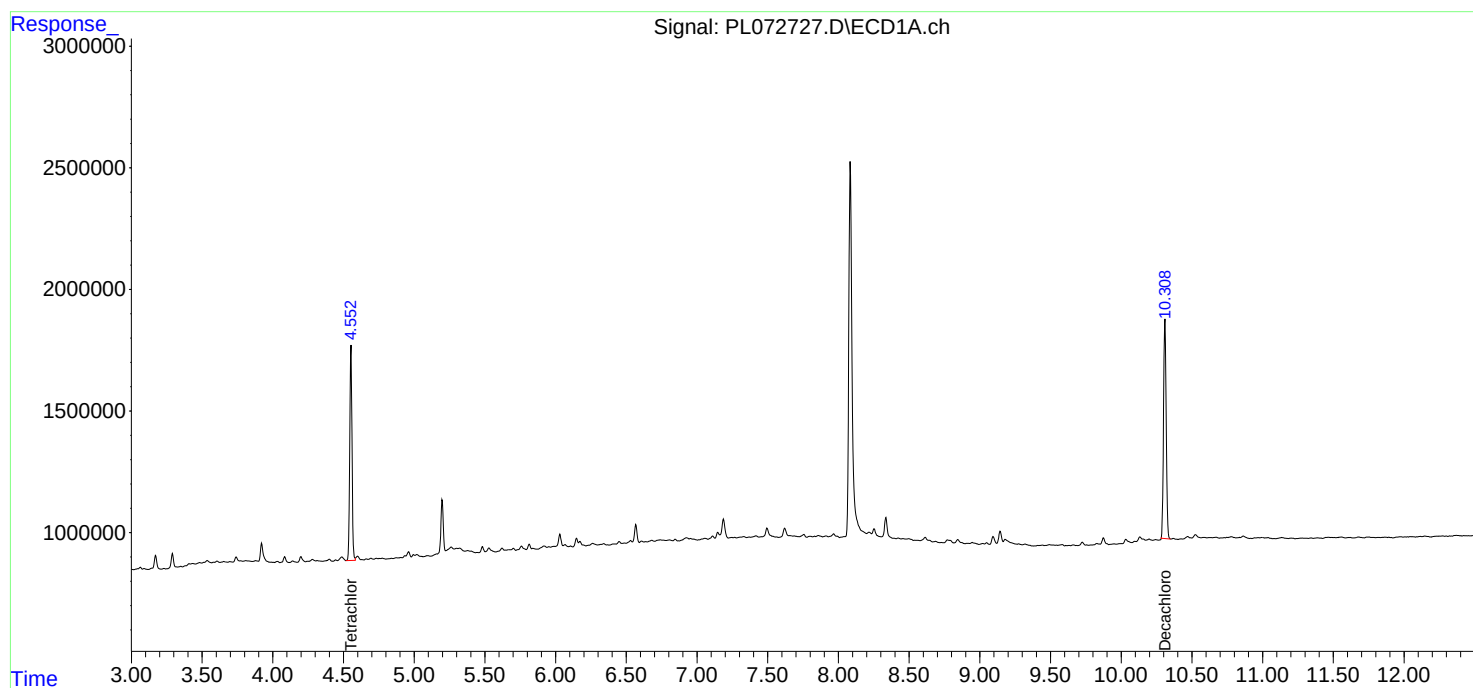


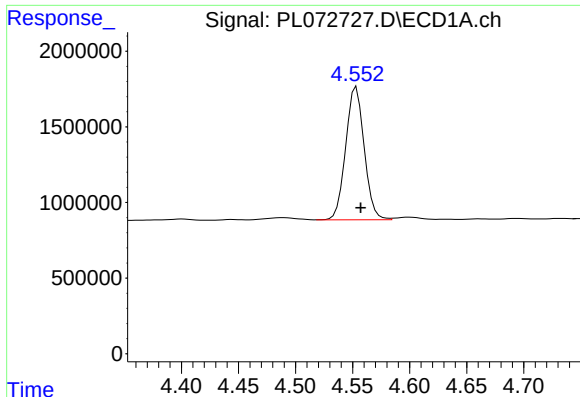

#1 Tetrachloro-m-xylene


R.T.: 4.553 min
Delta R.T.: -0.004 min
Response: 9906007
Conc: 20.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACHATE-AMENDED-COMP-7

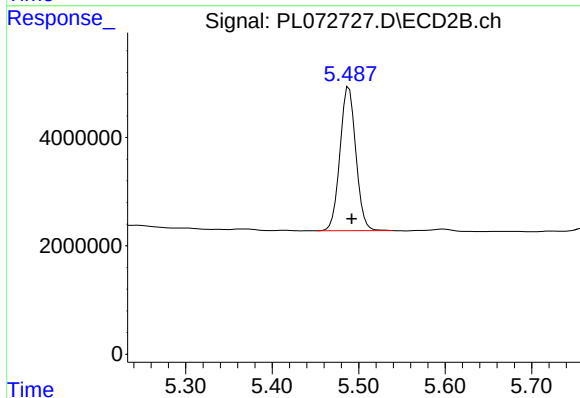


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.003 min
Response: 33696316
Conc: 19.51 ng/ml

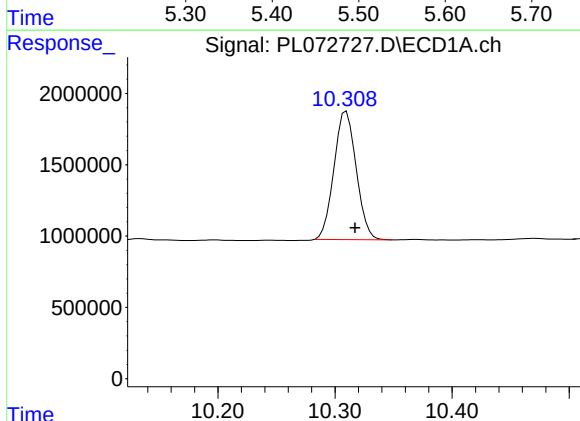

#28 Decachlorobiphenyl

R.T.: 10.310 min
Delta R.T.: -0.007 min
Response: 11871842
Conc: 15.68 ng/ml

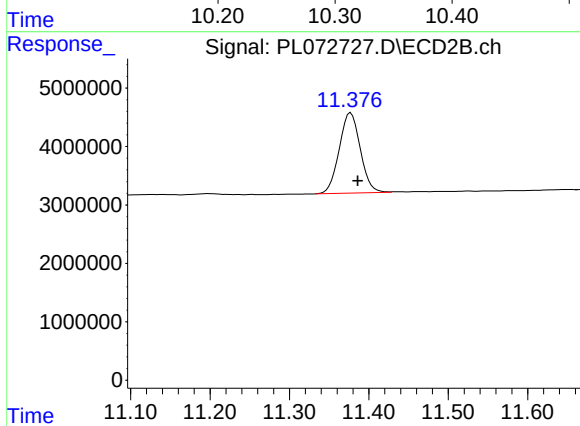

#28 Decachlorobiphenyl

R.T.: 11.377 min
Delta R.T.: -0.009 min
Response: 25330941
Conc: 15.97 ng/ml